

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026101.D
 Acq On : 10 Jun 2022 18:30
 Operator : SY/MD
 Sample : N3247-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	100	rVB	59946	68605	12.00%	1.491%
2	1.580	160	168	178	rBV	72290	83302	14.57%	1.810%
3	2.117	324	335	353	rVB	116638	170733	29.87%	3.710%
4	3.912	883	893	924	rBV2	46836	172929	30.25%	3.758%
5	4.358	1017	1032	1055	rBV	105873	264730	46.31%	5.753%
6	5.056	1232	1249	1281	rBV2	204714	517739	90.57%	11.250%
7	5.622	1414	1425	1450	rBV	197139	406465	71.11%	8.832%
8	5.921	1507	1518	1537	rVB7	15607	37188	6.51%	0.808%
9	6.075	1552	1566	1591	rBV	135533	284470	49.76%	6.182%
10	6.992	1841	1851	1877	rBV	44245	87571	15.32%	1.903%
11	7.320	1940	1953	1978	rBV	195604	354418	62.00%	7.701%
12	7.628	2039	2049	2071	rBV	25623	48184	8.43%	1.047%
13	7.940	2136	2146	2155	rBV	9986	16790	2.94%	0.365%
14	8.091	2183	2193	2234	rBV2	246340	571634	100.00%	12.422%
15	8.853	2417	2430	2457	rBV	304681	503841	88.14%	10.948%
16	9.140	2510	2519	2532	rBV2	16535	28719	5.02%	0.624%
17	10.217	2842	2854	2874	rBV	96153	156615	27.40%	3.403%
18	10.381	2892	2905	2919	rVB	21238	34791	6.09%	0.756%
19	11.249	3164	3175	3195	rBV	273603	426334	74.58%	9.264%
20	11.622	3280	3291	3312	rBV	226012	366894	64.18%	7.973%




Sum of corrected areas: 4601952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026101.D
Acq On : 10 Jun 2022 18:30
Operator : SY/MD
Sample : N3247-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

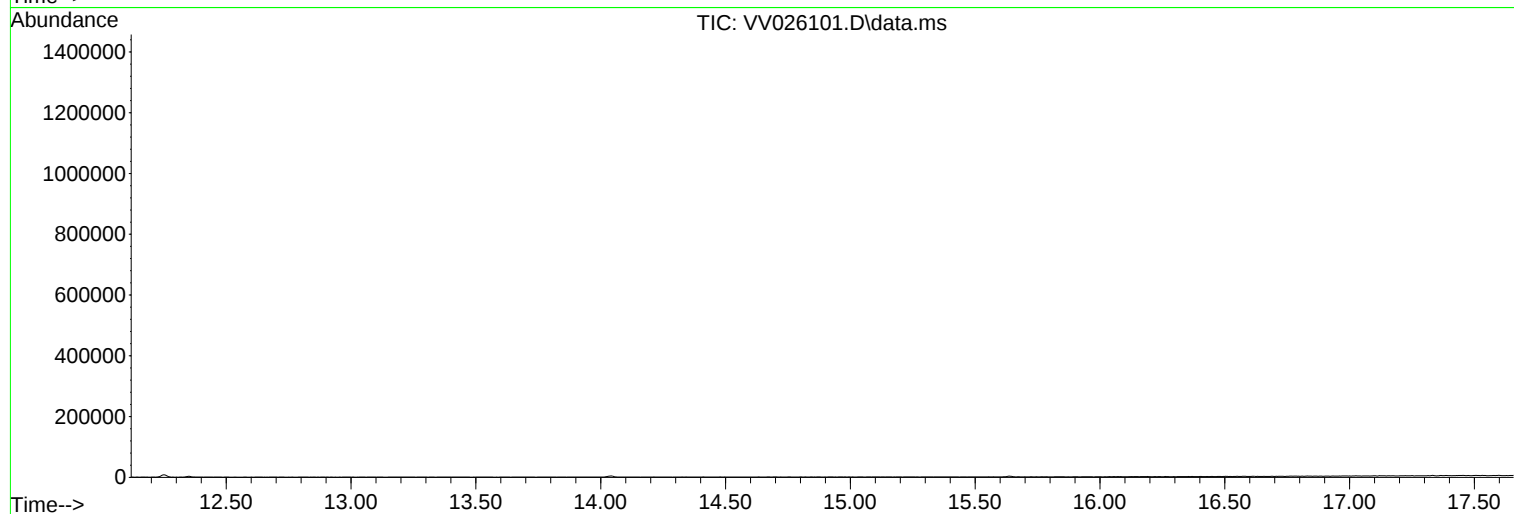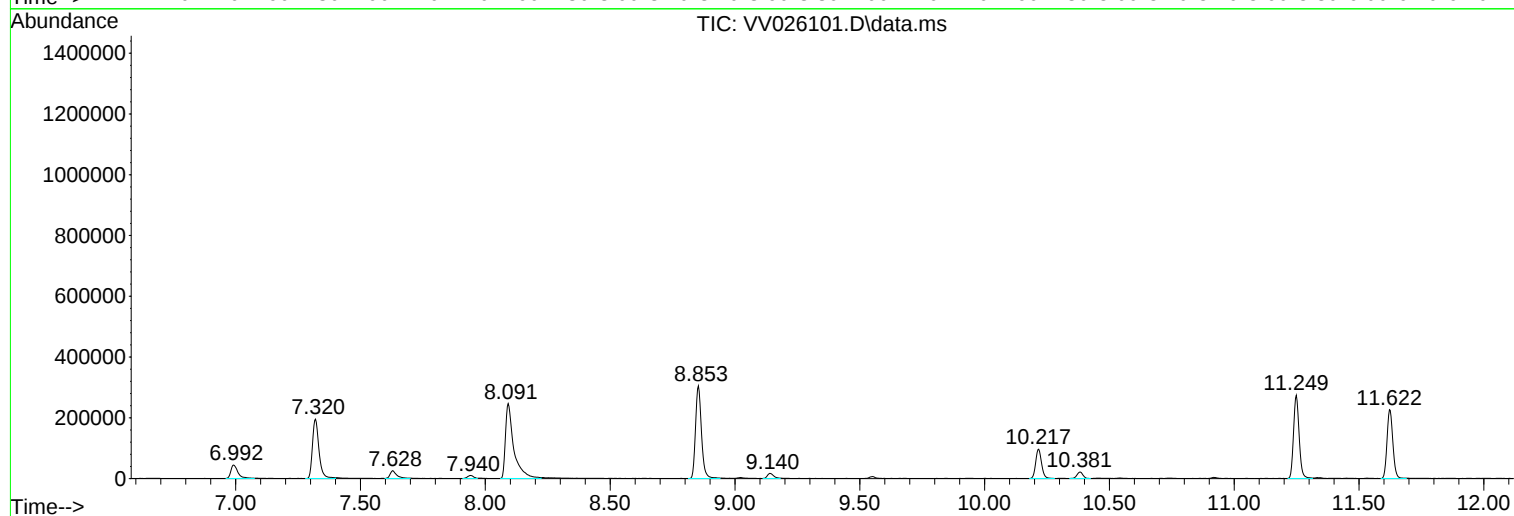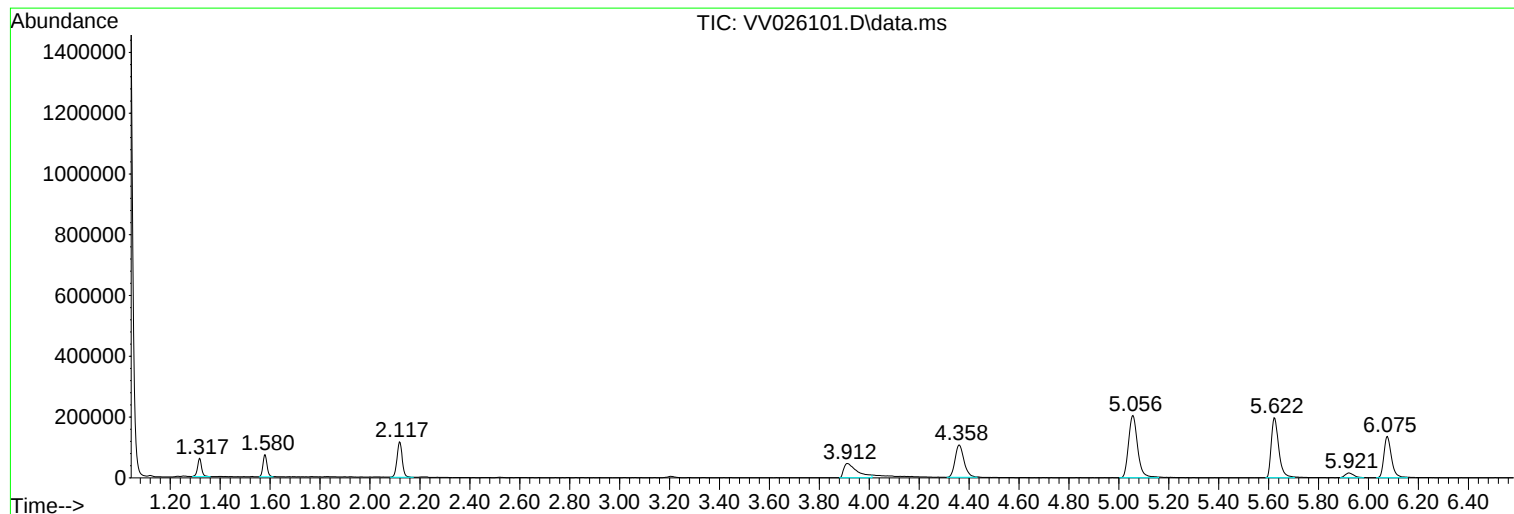

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026101.D
Acq On : 10 Jun 2022 18:30
Operator : SY/MD
Sample : N3247-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026101.D
Acq On : 10 Jun 2022 18:30
Operator : SY/MD
Sample : N3247-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc