

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026102.D
 Acq On : 10 Jun 2022 18:54
 Operator : SY/MD
 Sample : N3247-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	21	25	40	rVB3	11467	16297	2.86%	0.342%
2	1.317	77	86	97	rBV	90604	101150	17.74%	2.123%
3	1.577	159	167	175	rBV	93477	109257	19.16%	2.293%
4	2.118	325	335	353	rVB	170122	254330	44.61%	5.339%
5	3.921	885	896	924	rBV	36644	144148	25.29%	3.026%
6	4.359	1016	1032	1060	rBV	107054	267035	46.84%	5.605%
7	4.616	1094	1112	1129	rBV4	18667	46611	8.18%	0.978%
8	5.053	1231	1248	1273	rBV2	228981	570088	100.00%	11.967%
9	5.622	1412	1425	1448	rBV	195582	403653	70.81%	8.473%
10	5.924	1508	1519	1543	rBV5	22963	52599	9.23%	1.104%
11	6.076	1552	1566	1588	rBV	134676	282728	49.59%	5.935%
12	6.992	1840	1851	1876	rBV2	42361	83145	14.58%	1.745%
13	7.320	1939	1953	1975	rBV	246897	437863	76.81%	9.191%
14	7.629	2038	2049	2065	rBV2	22431	42097	7.38%	0.884%
15	7.937	2133	2145	2150	rBV	12308	18739	3.29%	0.393%
16	7.979	2151	2158	2176	rVB5	19836	36252	6.36%	0.761%
17	8.092	2183	2193	2231	rBV2	204384	447548	78.51%	9.395%
18	8.854	2418	2430	2449	rBV	298982	493652	86.59%	10.362%
19	10.217	2842	2854	2869	rBV	88174	139148	24.41%	2.921%
20	10.381	2894	2905	2919	rVB2	24739	39694	6.96%	0.833%
21	11.249	3161	3175	3193	rBV	275506	424911	74.53%	8.919%
22	11.622	3280	3291	3308	rBV	221794	352953	61.91%	7.409%




Sum of corrected areas: 4763898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026102.D
Acq On : 10 Jun 2022 18:54
Operator : SY/MD
Sample : N3247-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

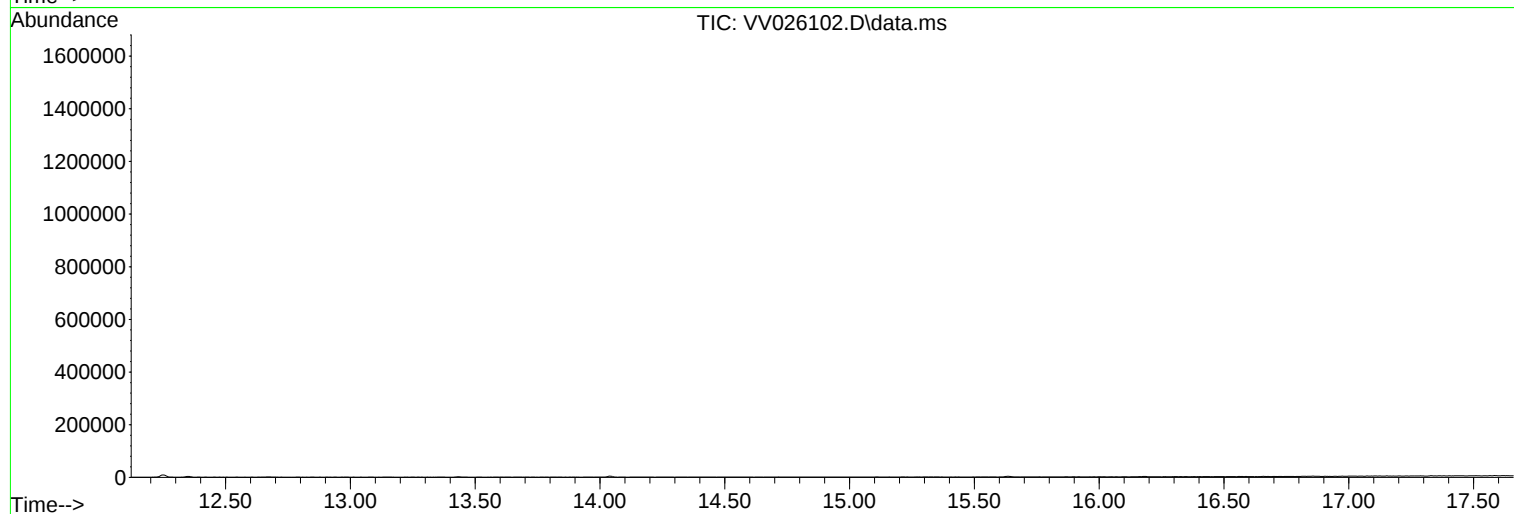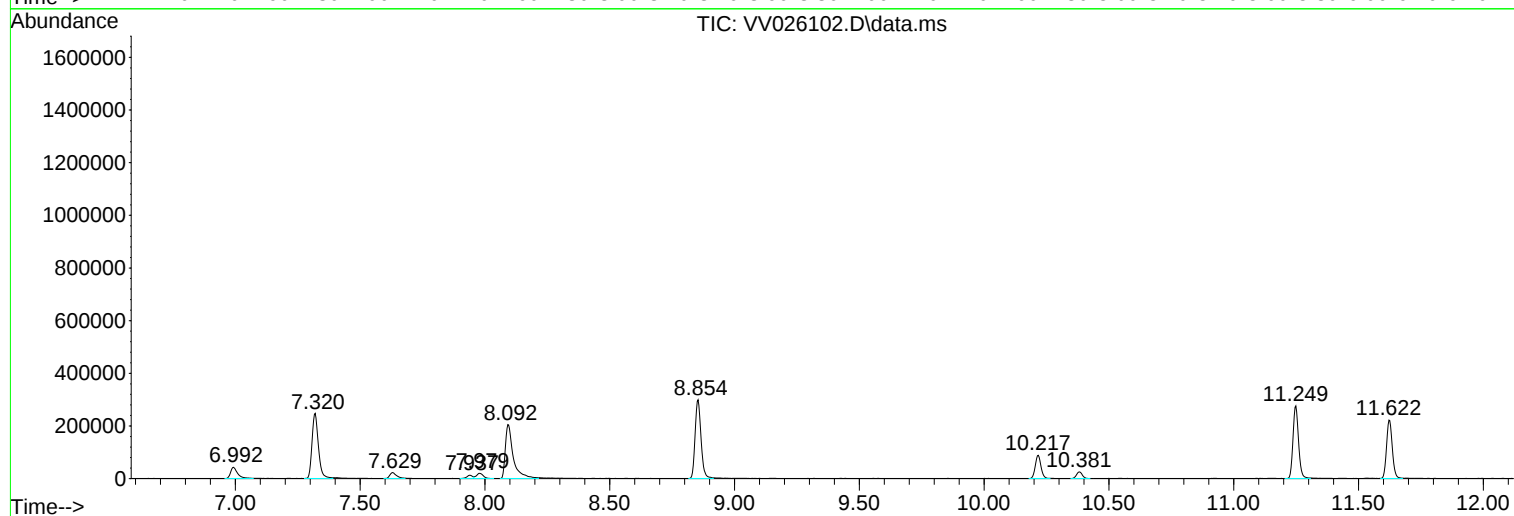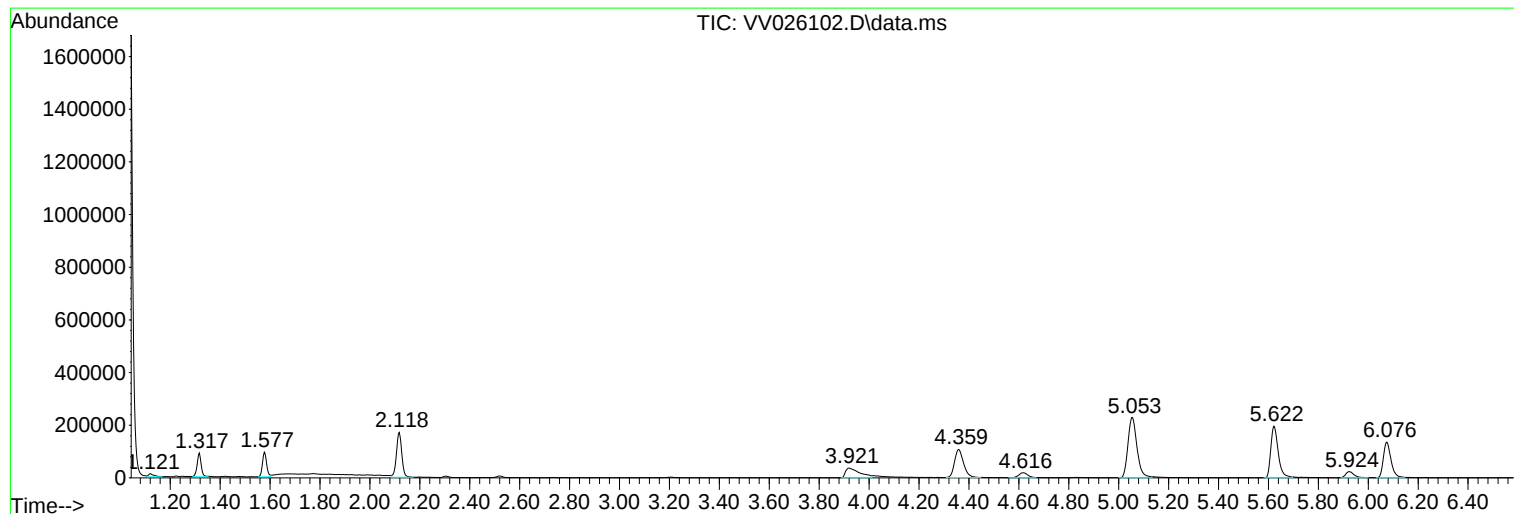

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026102.D
Acq On : 10 Jun 2022 18:54
Operator : SY/MD
Sample : N3247-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026102.D
Acq On : 10 Jun 2022 18:54
Operator : SY/MD
Sample : N3247-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
