

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026104.D
 Acq On : 10 Jun 2022 19:41
 Operator : SY/MD
 Sample : N3247-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYT8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	103	rVB	88280	103788	18.08%	2.133%
2	1.577	159	167	180	rVB	93405	108131	18.83%	2.223%
3	2.117	325	335	352	rVB	172670	254948	44.40%	5.240%
4	3.924	884	897	923	rBV4	64909	217289	37.84%	4.466%
5	4.358	1016	1032	1072	rVB	108757	297615	51.83%	6.117%
6	4.619	1098	1113	1129	rBV4	16863	41323	7.20%	0.849%
7	5.056	1234	1249	1278	rBV2	232604	574193	100.00%	11.802%
8	5.622	1414	1425	1453	rBV	188993	387674	67.52%	7.968%
9	5.921	1505	1518	1539	rBV6	52176	113795	19.82%	2.339%
10	6.075	1554	1566	1589	rBV	136673	283437	49.36%	5.826%
11	6.992	1840	1851	1874	rBV	41648	81833	14.25%	1.682%
12	7.320	1941	1953	1979	rBV	244187	437123	76.13%	8.985%
13	7.628	2040	2049	2074	rBV	23009	44178	7.69%	0.908%
14	7.979	2149	2158	2176	rVB	52517	89523	15.59%	1.840%
15	8.091	2183	2193	2227	rBV	209425	446169	77.70%	9.171%
16	8.853	2419	2430	2456	rBV	287181	476384	82.97%	9.792%
17	10.217	2843	2854	2869	rBV	86320	138238	24.08%	2.841%
18	10.384	2895	2906	2916	rBV2	14166	22732	3.96%	0.467%
19	11.249	3162	3175	3192	rBV	259446	400340	69.72%	8.229%
20	11.622	3278	3291	3308	rBV	217636	346398	60.33%	7.120%




Sum of corrected areas: 4865111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026104.D
Acq On : 10 Jun 2022 19:41
Operator : SY/MD
Sample : N3247-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

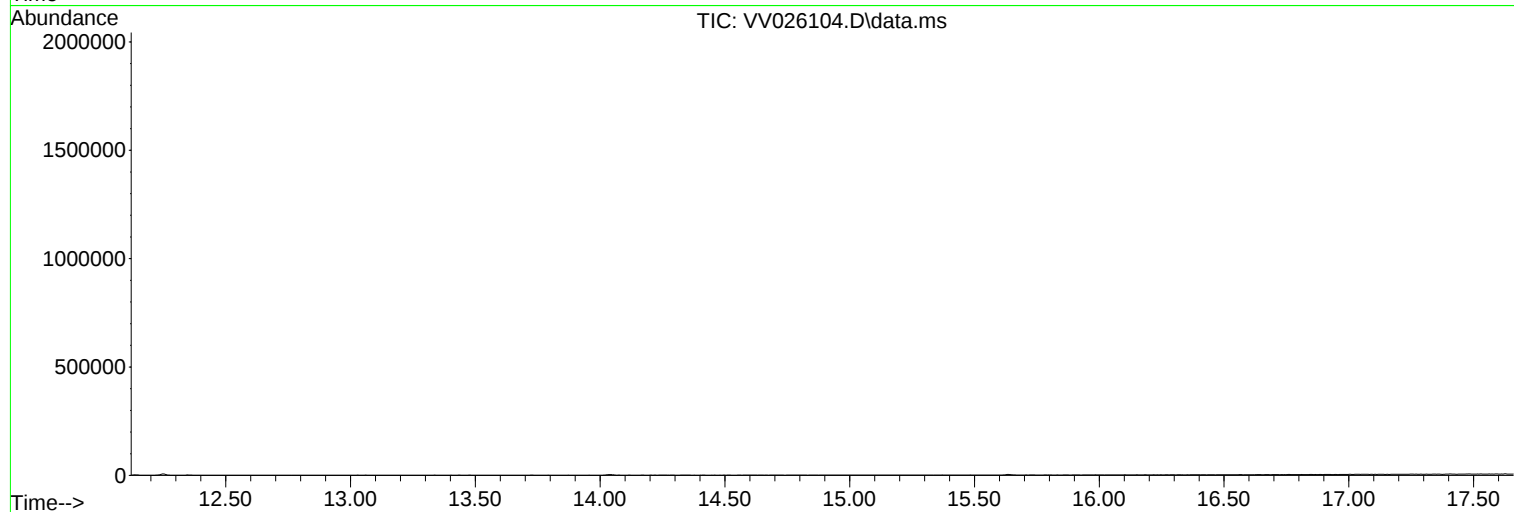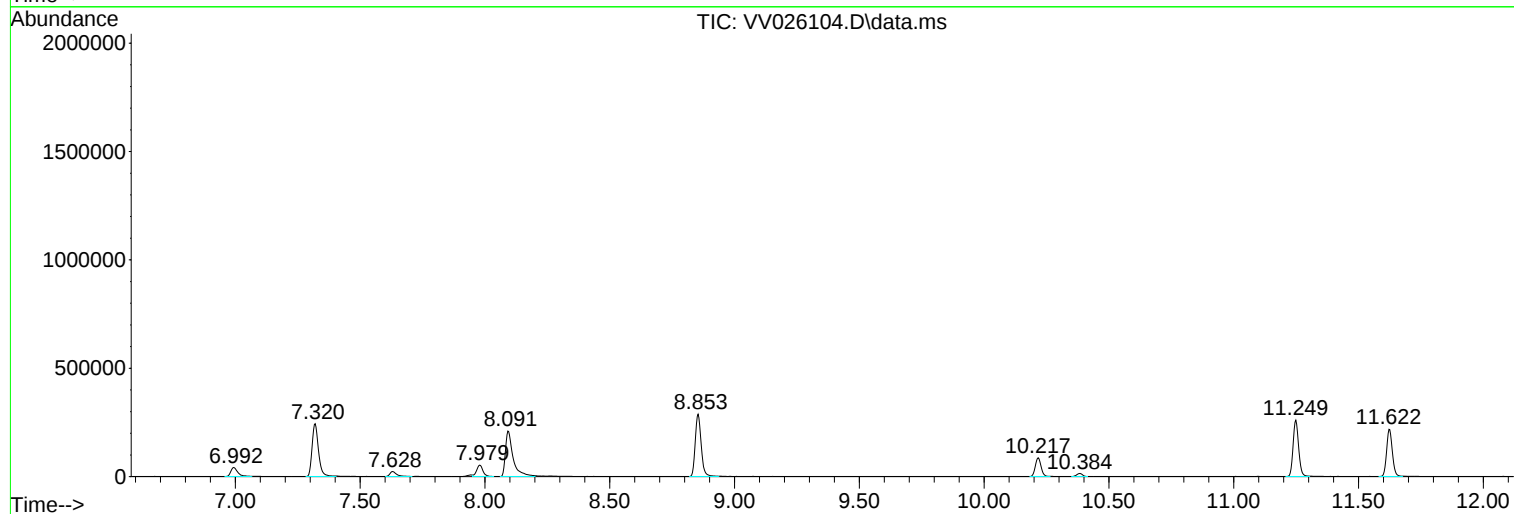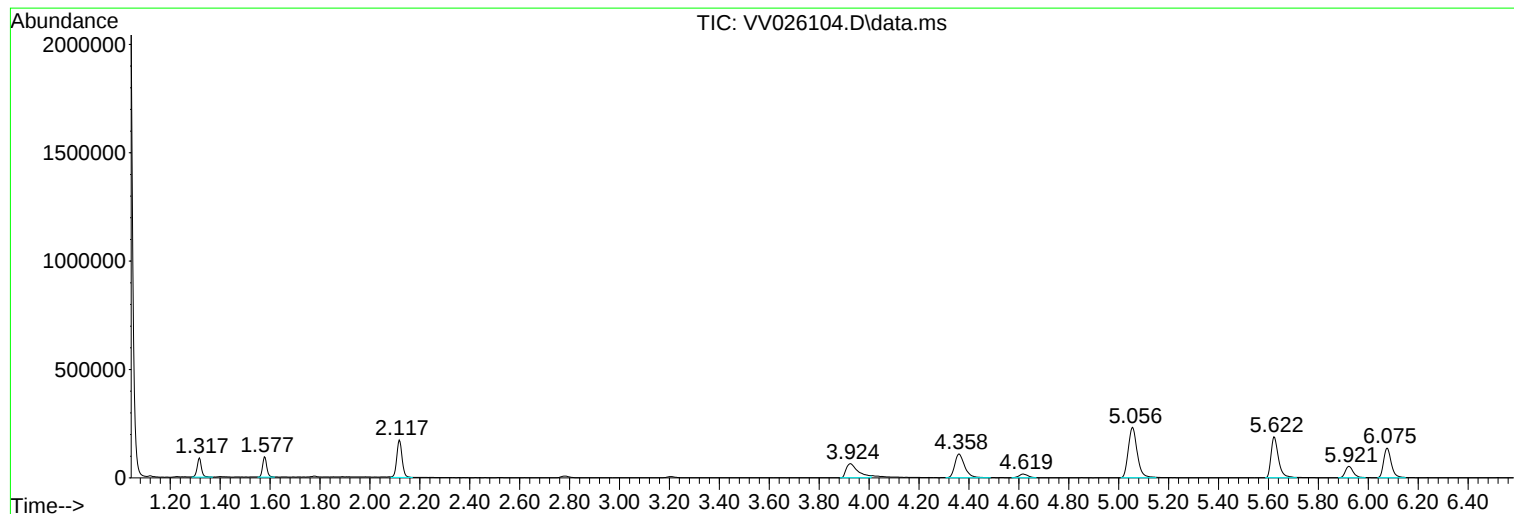

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026104.D
Acq On : 10 Jun 2022 19:41
Operator : SY/MD
Sample : N3247-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026104.D
Acq On : 10 Jun 2022 19:41
Operator : SY/MD
Sample : N3247-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc