

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026105.D
 Acq On : 10 Jun 2022 20:05
 Operator : SY/MD
 Sample : N3272-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B51

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	77	86	101	rBV	83536	90499	15.87%	1.990%
2	1.577	159	167	184	rVB	93423	107504	18.85%	2.363%
3	2.117	323	335	354	rVB	162775	236963	41.54%	5.209%
4	3.915	880	894	930	rBV2	43406	176078	30.87%	3.871%
5	4.359	1016	1032	1060	rBV	106005	267146	46.83%	5.873%
6	5.056	1232	1249	1275	rBV2	228461	570414	100.00%	12.540%
7	5.622	1414	1425	1451	rBV	189118	390614	68.48%	8.587%
8	5.928	1506	1520	1539	rVB6	13913	34245	6.00%	0.753%
9	6.075	1553	1566	1585	rBV	138559	284005	49.79%	6.243%
10	6.992	1841	1851	1874	rBV2	40741	80379	14.09%	1.767%
11	7.320	1941	1953	1982	rBV	238503	427287	74.91%	9.393%
12	7.629	2040	2049	2071	rBV	23402	44859	7.86%	0.986%
13	7.940	2132	2146	2154	rBV2	8646	14445	2.53%	0.318%
14	8.091	2183	2193	2225	rBV	203697	459074	80.48%	10.092%
15	8.854	2419	2430	2458	rBV	281474	468967	82.22%	10.310%
16	10.217	2843	2854	2871	rBV	89874	140983	24.72%	3.099%
17	10.381	2895	2905	2916	rVB2	18411	28982	5.08%	0.637%
18	11.249	3163	3175	3199	rBV	238796	373106	65.41%	8.202%
19	11.622	3279	3291	3314	rBV	217240	341245	59.82%	7.502%
20	12.252	3473	3487	3495	rBV3	7349	12026	2.11%	0.264%




Sum of corrected areas: 4548821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026105.D
Acq On : 10 Jun 2022 20:05
Operator : SY/MD
Sample : N3272-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

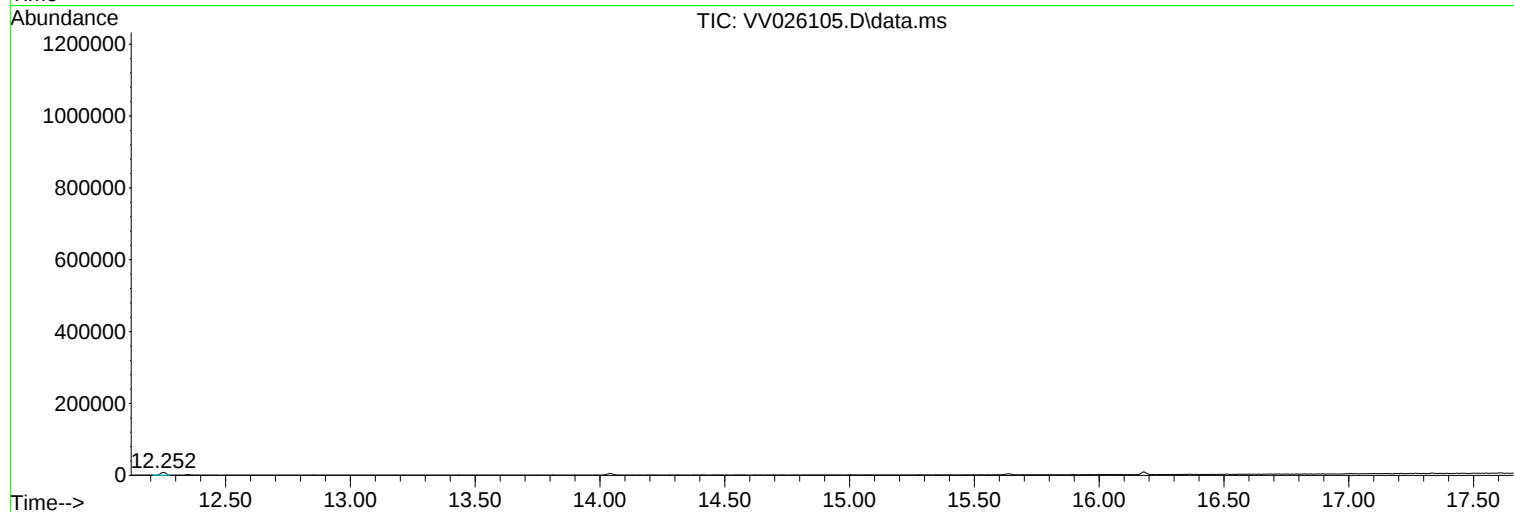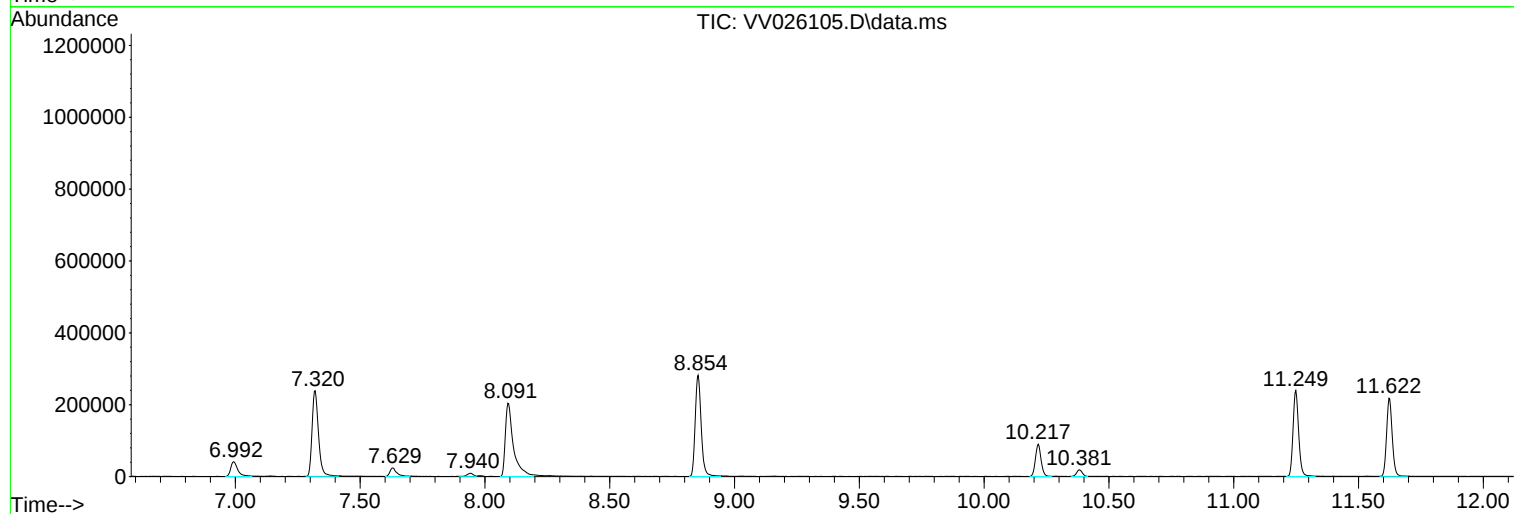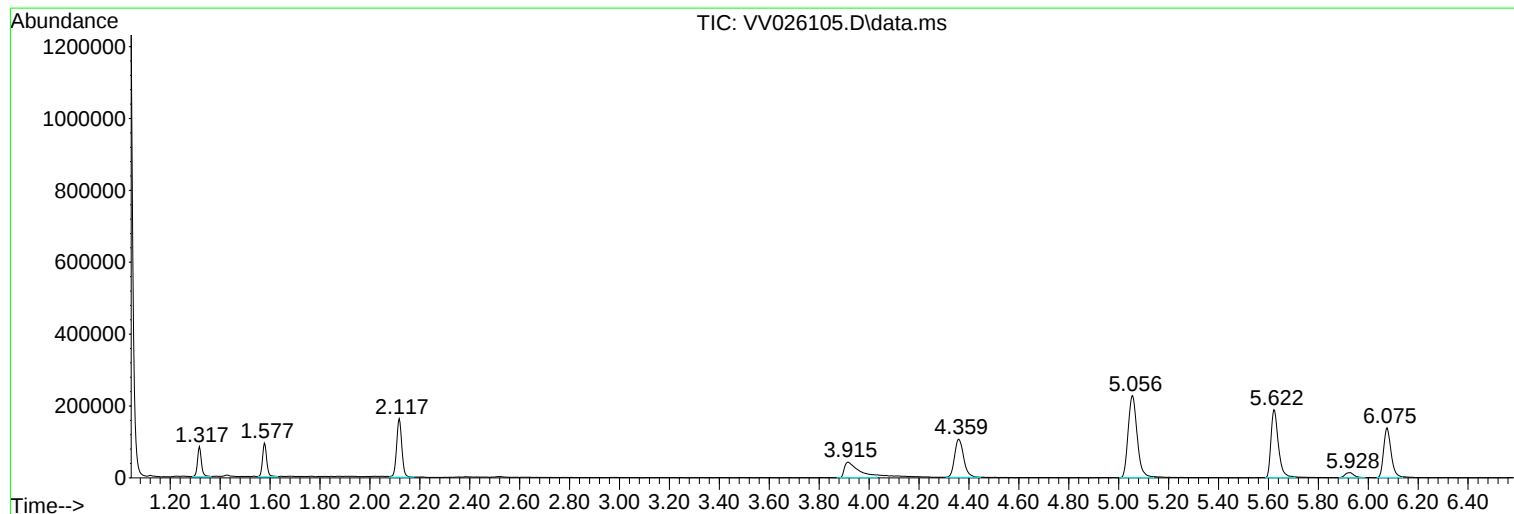

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026105.D
Acq On : 10 Jun 2022 20:05
Operator : SY/MD
Sample : N3272-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026105.D
Acq On : 10 Jun 2022 20:05
Operator : SY/MD
Sample : N3272-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------