

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026106.D
 Acq On : 10 Jun 2022 20:29
 Operator : SY/MD
 Sample : N3272-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	99	rVB	81103	84702	15.11%	1.879%
2	1.577	160	167	182	rVB	92140	106543	19.01%	2.364%
3	2.117	325	335	354	rVB	160782	232770	41.52%	5.164%
4	3.915	884	894	927	rBV	33527	126703	22.60%	2.811%
5	4.359	1017	1032	1063	rVB2	107274	264146	47.12%	5.860%
6	5.056	1229	1249	1281	rBV2	225522	560591	100.00%	12.436%
7	5.622	1414	1425	1451	rBV2	196931	410023	73.14%	9.096%
8	5.924	1507	1519	1533	rBV6	13854	32108	5.73%	0.712%
9	6.075	1553	1566	1598	rBV	132019	276727	49.36%	6.139%
10	6.992	1840	1851	1873	rBV	40850	79233	14.13%	1.758%
11	7.320	1941	1953	1980	rBV	234172	422442	75.36%	9.371%
12	7.628	2040	2049	2070	rBV2	22372	42499	7.58%	0.943%
13	7.944	2134	2147	2158	rBV2	5135	9735	1.74%	0.216%
14	8.091	2183	2193	2232	rBV	180147	428031	76.35%	9.495%
15	8.854	2418	2430	2469	rBV	309666	515866	92.02%	11.444%
16	10.217	2842	2854	2873	rBV	81227	132176	23.58%	2.932%
17	10.384	2896	2906	2918	rVB3	9314	15096	2.69%	0.335%
18	11.249	3164	3175	3197	rBV	258033	410352	73.20%	9.103%
19	11.622	3280	3291	3311	rBV	215638	341384	60.90%	7.573%
20	14.043	4030	4044	4059	rBV2	4617	8174	1.46%	0.181%
21	15.635	4531	4539	4551	rVB2	5787	8457	1.51%	0.188%




Sum of corrected areas: 4507758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026106.D
Acq On : 10 Jun 2022 20:29
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

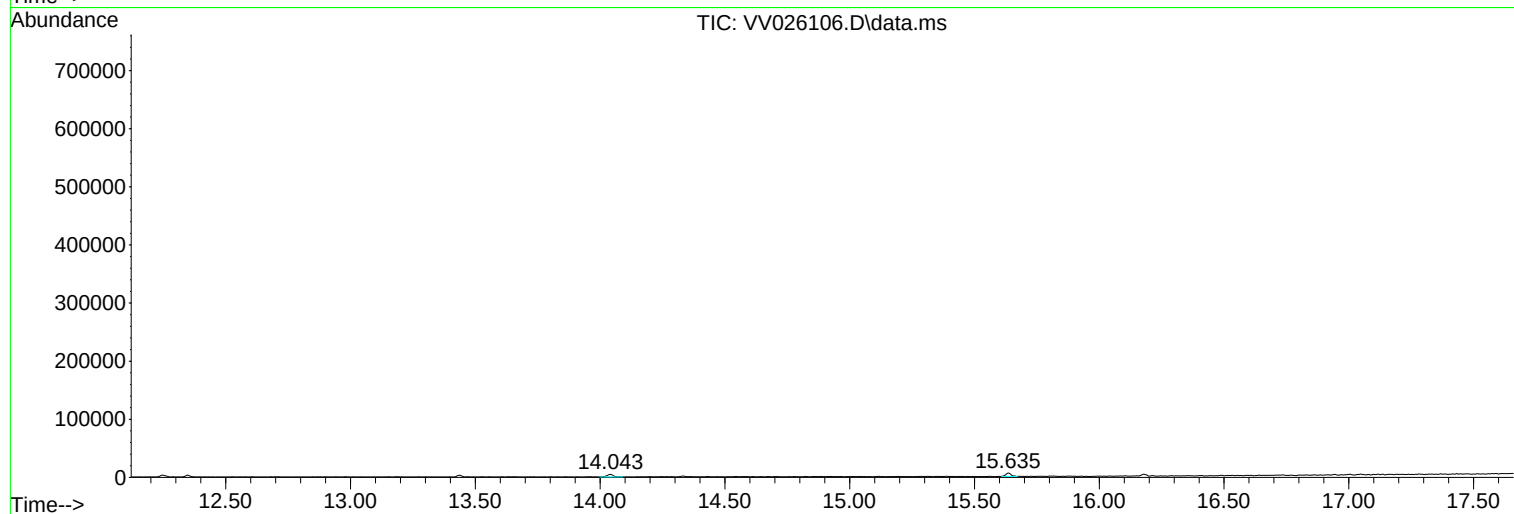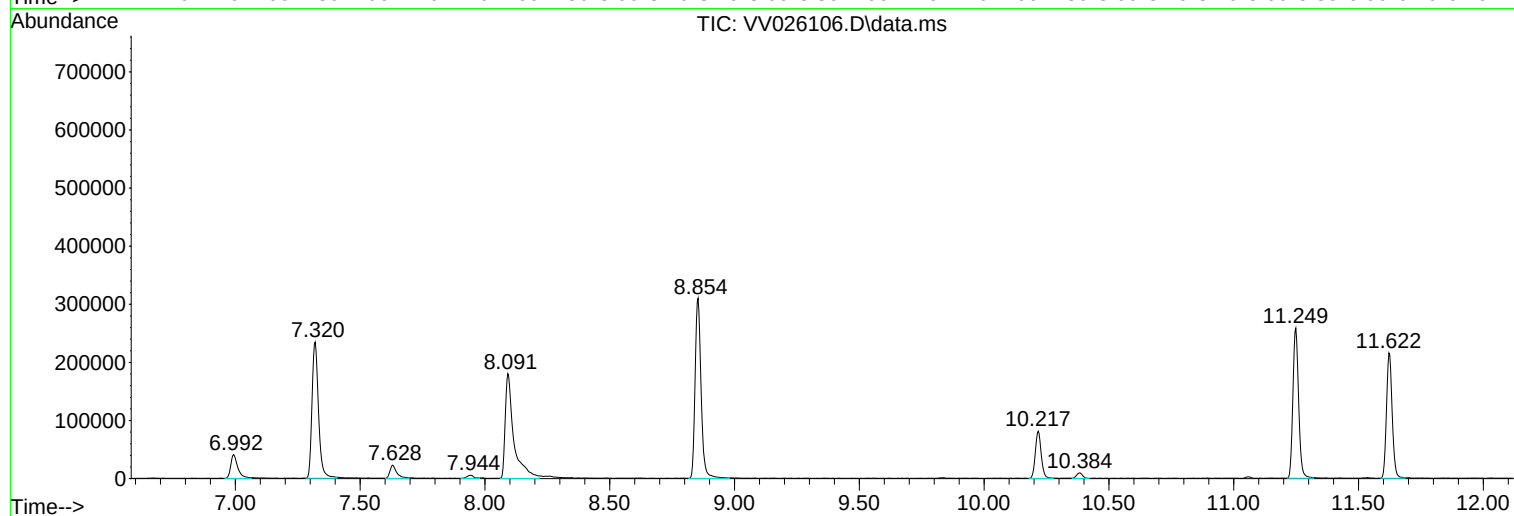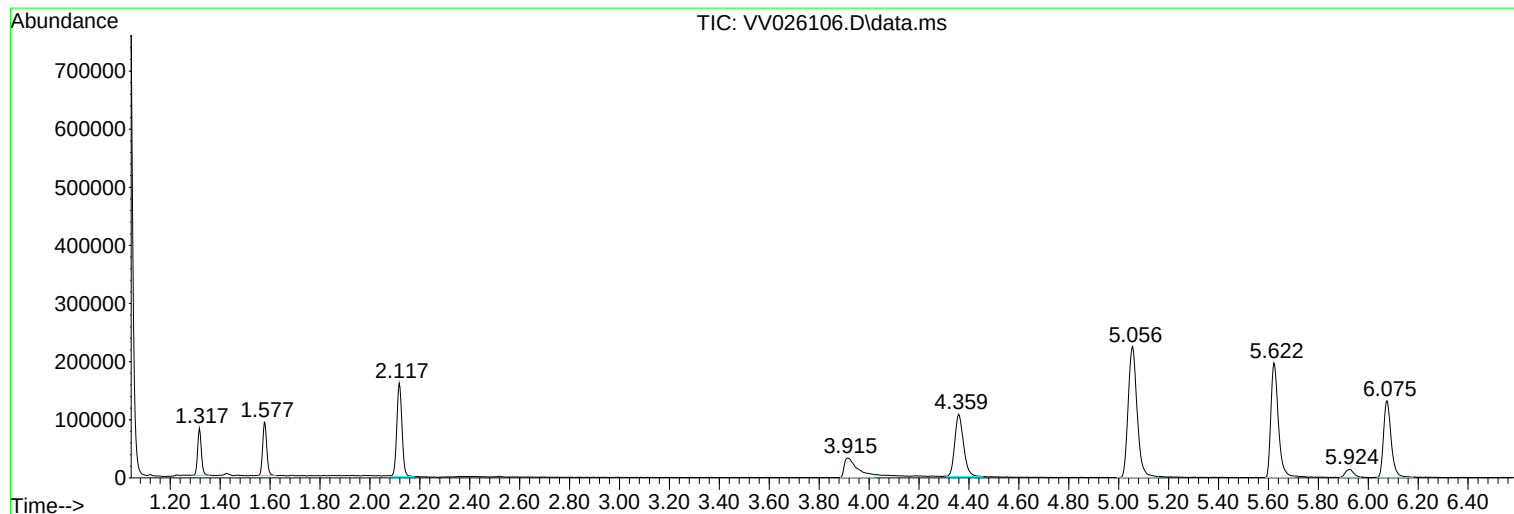

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026106.D
Acq On : 10 Jun 2022 20:29
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026106.D
Acq On : 10 Jun 2022 20:29
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------