

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026110.D
 Acq On : 10 Jun 2022 22:05
 Operator : SY/MD
 Sample : N3272-18
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B63

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	41	rVB	26136	27576	5.03%	0.622%
2	1.317	77	86	98	rBV2	89624	107816	19.66%	2.431%
3	1.430	115	121	129	rVB3	5539	6320	1.15%	0.142%
4	1.581	159	168	179	rBV	93382	104549	19.06%	2.357%
5	1.719	203	211	222	rBV	44214	55055	10.04%	1.241%
6	1.780	222	230	238	rBV5	4677	6884	1.26%	0.155%
7	2.121	325	336	352	rVB	157508	228328	41.63%	5.147%
8	2.217	359	366	377	rVB7	3151	5523	1.01%	0.125%
9	3.931	888	899	931	rBV2	34302	148806	27.13%	3.355%
10	4.362	1017	1033	1061	rVB	102420	255661	46.61%	5.763%
11	5.056	1233	1249	1284	rBV2	219005	548486	100.00%	12.365%
12	5.625	1413	1426	1451	rBV	177855	365425	66.62%	8.238%
13	5.925	1507	1519	1536	rVB7	12922	28790	5.25%	0.649%
14	6.076	1554	1566	1592	rBV	129706	272369	49.66%	6.140%
15	6.992	1842	1851	1872	rBV	38894	76806	14.00%	1.731%
16	7.320	1940	1953	1973	rBV	227620	403907	73.64%	9.105%
17	7.632	2037	2050	2072	rBV	21987	42567	7.76%	0.960%
18	7.941	2133	2146	2153	rBV2	5322	9410	1.72%	0.212%
19	8.095	2182	2194	2232	rBV2	195670	431238	78.62%	9.722%
20	8.854	2419	2430	2457	rBV	271211	454912	82.94%	10.255%
21	10.217	2841	2854	2874	rBV	81797	130939	23.87%	2.952%
22	10.381	2895	2905	2916	rBV3	10498	17205	3.14%	0.388%
23	11.249	3164	3175	3195	rBV	237157	368765	67.23%	8.313%
24	11.622	3280	3291	3314	rBV	203662	326516	59.53%	7.361%
25	12.252	3472	3487	3494	rBV4	3589	6422	1.17%	0.145%
26	15.635	4529	4539	4548	rBV2	3585	5635	1.03%	0.127%




Sum of corrected areas: 4435910

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026110.D
Acq On : 10 Jun 2022 22:05
Operator : SY/MD
Sample : N3272-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

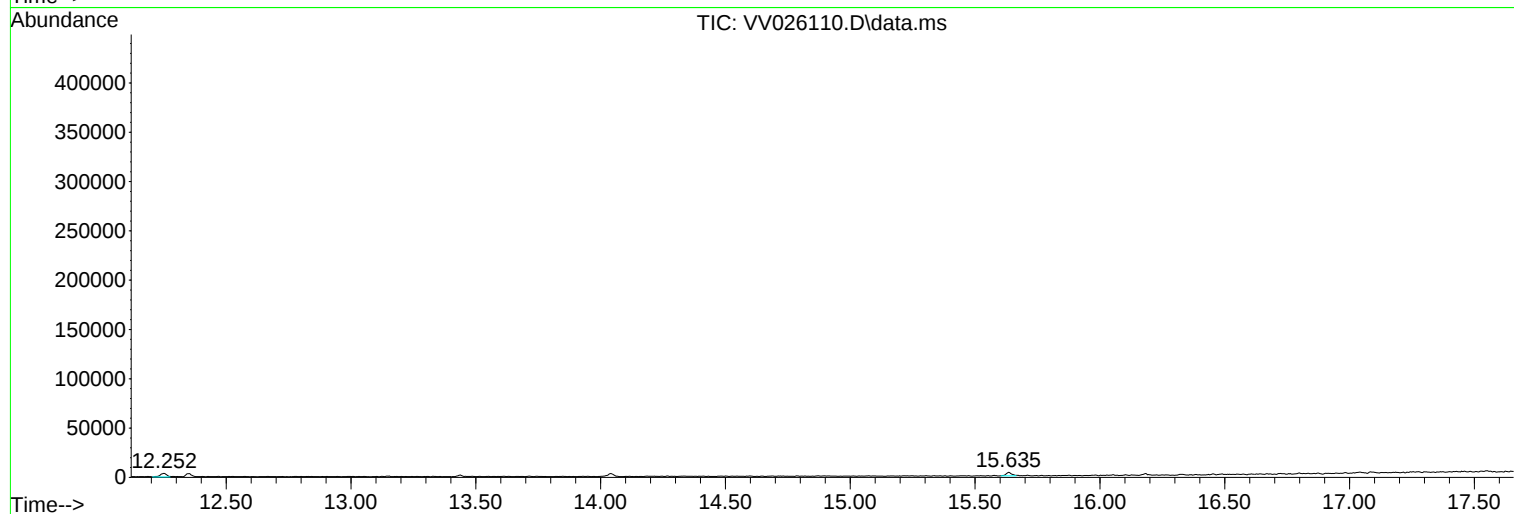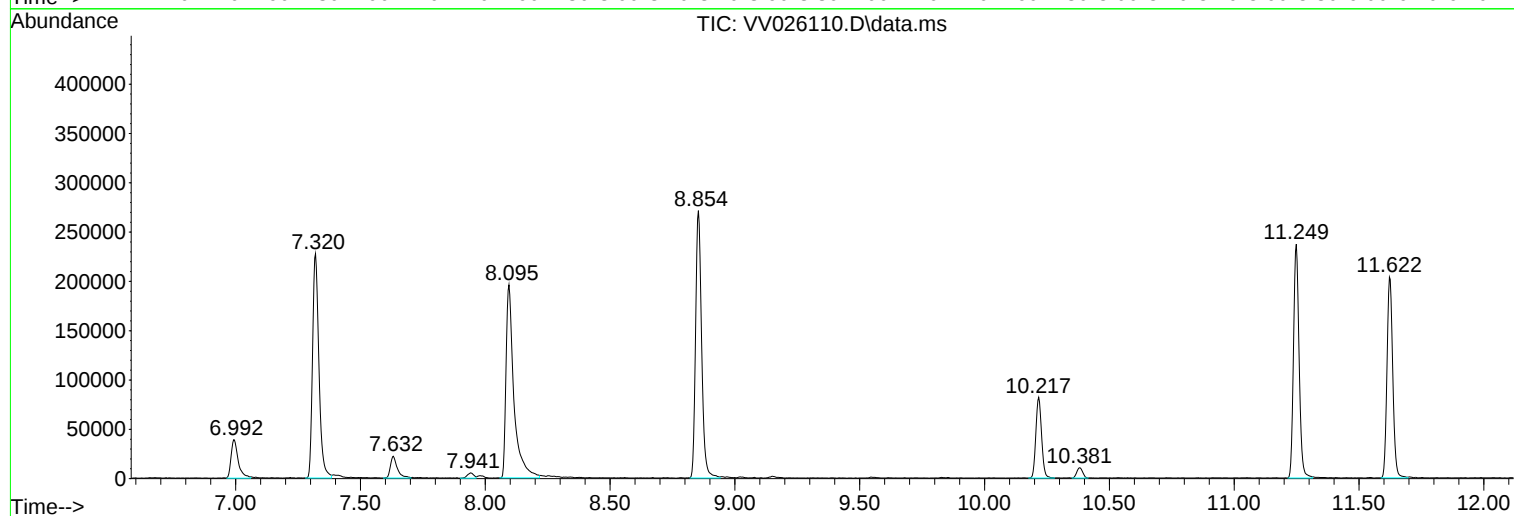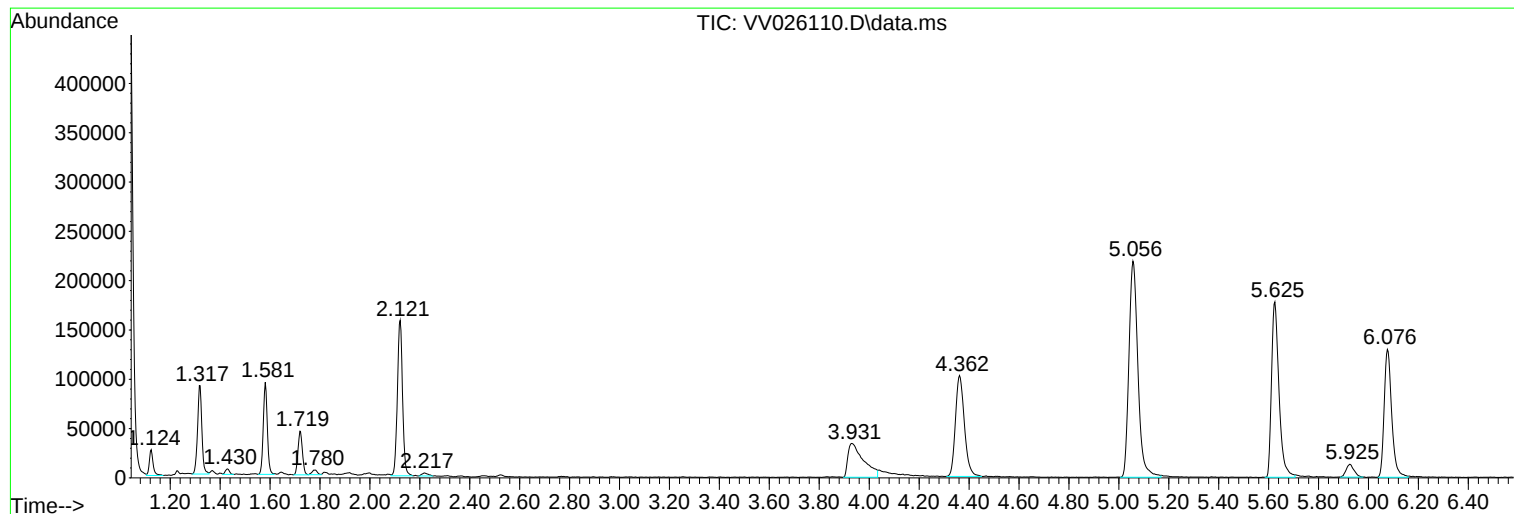

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026110.D
Acq On : 10 Jun 2022 22:05
Operator : SY/MD
Sample : N3272-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.719	0.75 ug/L	55055	1,4-Difluorobenzene	5.625

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	4
5			Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	4

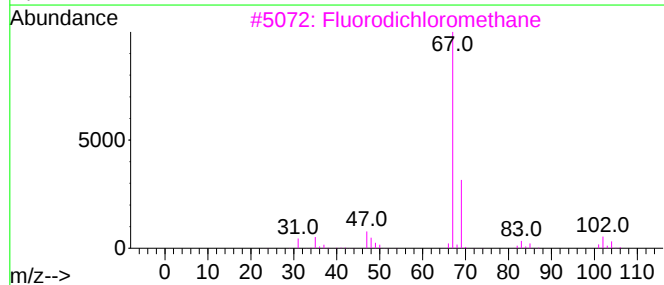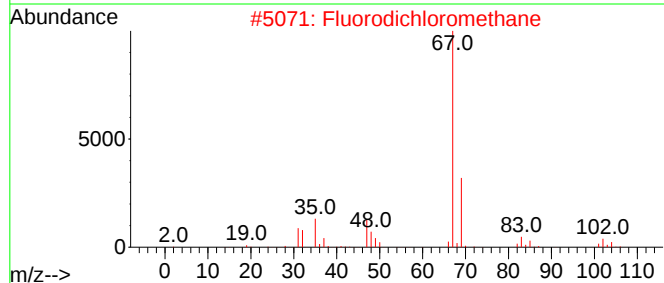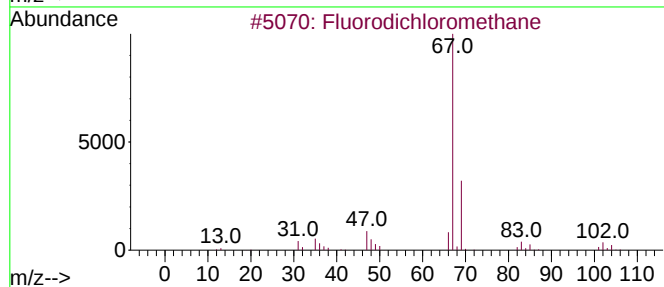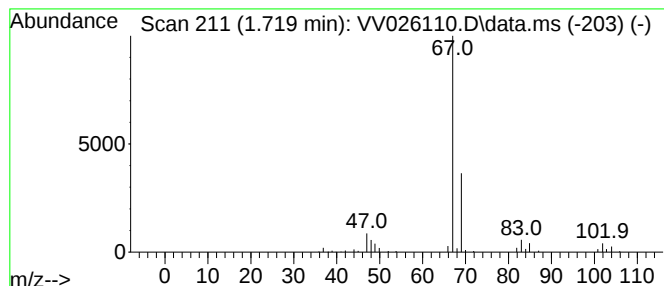

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026110.D
Acq On : 10 Jun 2022 22:05
Operator : SY/MD
Sample : N3272-18
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	1.719	0.8	ug/L	55055	1	5.625	365425	5.0