

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026111.D
 Acq On : 10 Jun 2022 22:29
 Operator : SY/MD
 Sample : N3272-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	104	rVB	80801	85855	15.76%	1.987%
2	1.581	161	168	181	rVB	88349	100366	18.42%	2.323%
3	2.121	325	336	352	rVB	154478	223683	41.06%	5.178%
4	3.931	887	899	935	rBV	35072	158491	29.09%	3.669%
5	4.362	1017	1033	1057	rBV	101711	255796	46.96%	5.921%
6	5.056	1233	1249	1279	rBV2	220910	544750	100.00%	12.610%
7	5.625	1415	1426	1452	rBV	169965	347810	63.85%	8.051%
8	5.925	1508	1519	1535	rBV6	17219	39764	7.30%	0.920%
9	6.076	1550	1566	1593	rBV2	129228	273211	50.15%	6.325%
10	6.992	1839	1851	1870	rBV	39797	79317	14.56%	1.836%
11	7.320	1940	1953	1972	rBV	229709	405668	74.47%	9.391%
12	7.397	1973	1977	1991	rVB7	4125	7464	1.37%	0.173%
13	7.629	2040	2049	2071	rBV2	23171	42477	7.80%	0.983%
14	7.944	2133	2147	2151	rBV3	4740	8541	1.57%	0.198%
15	7.979	2151	2158	2175	rVB3	13486	24189	4.44%	0.560%
16	8.095	2183	2194	2227	rBV2	200212	435227	79.89%	10.075%
17	8.854	2419	2430	2458	rBV	264535	434924	79.84%	10.068%
18	9.149	2513	2522	2538	rVB4	3980	7098	1.30%	0.164%
19	10.217	2843	2854	2873	rBV	83951	132059	24.24%	3.057%
20	10.381	2894	2905	2918	rBB2	10162	16736	3.07%	0.387%
21	11.249	3161	3175	3193	rBV	224588	348550	63.98%	8.069%
22	11.532	3252	3263	3275	rBV5	4391	8180	1.50%	0.189%
23	11.622	3279	3291	3312	rBV	209498	333924	61.30%	7.730%
24	12.249	3476	3486	3497	rBV2	3626	5757	1.06%	0.133%




Sum of corrected areas: 4319837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026111.D
Acq On : 10 Jun 2022 22:29
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

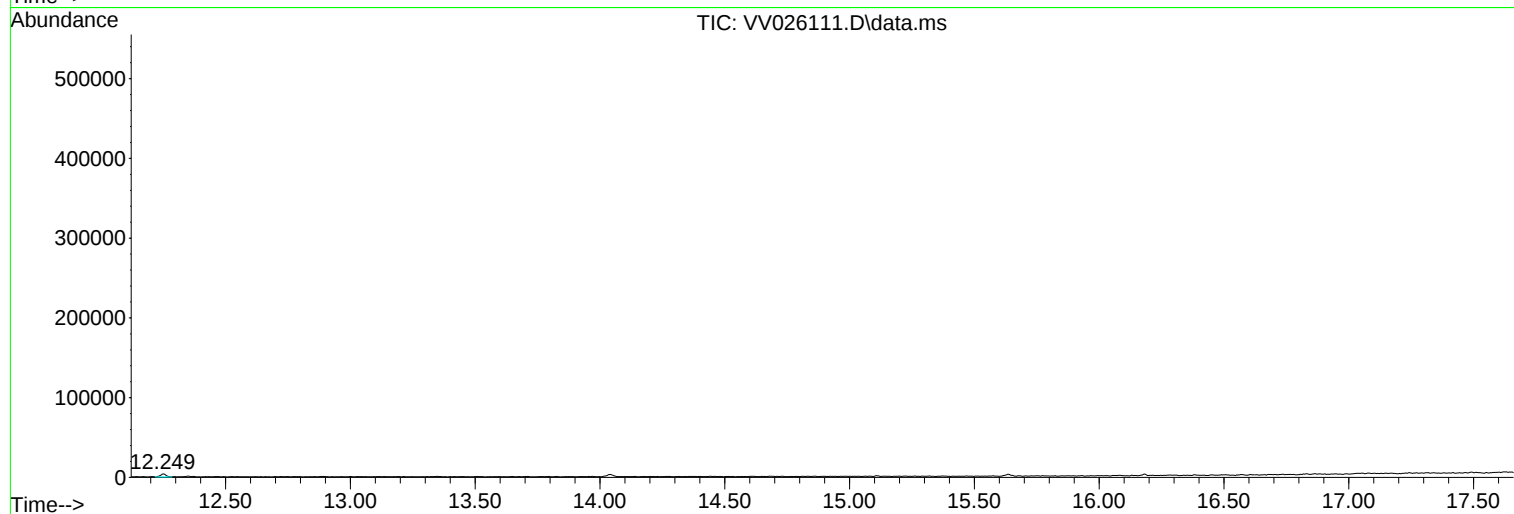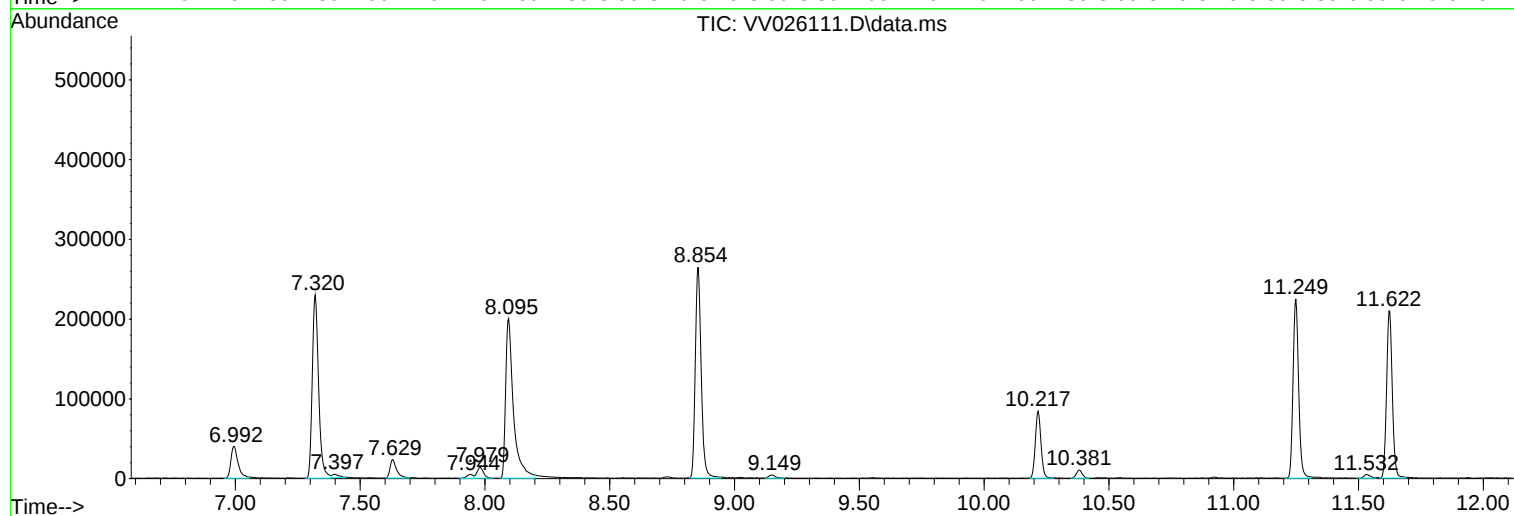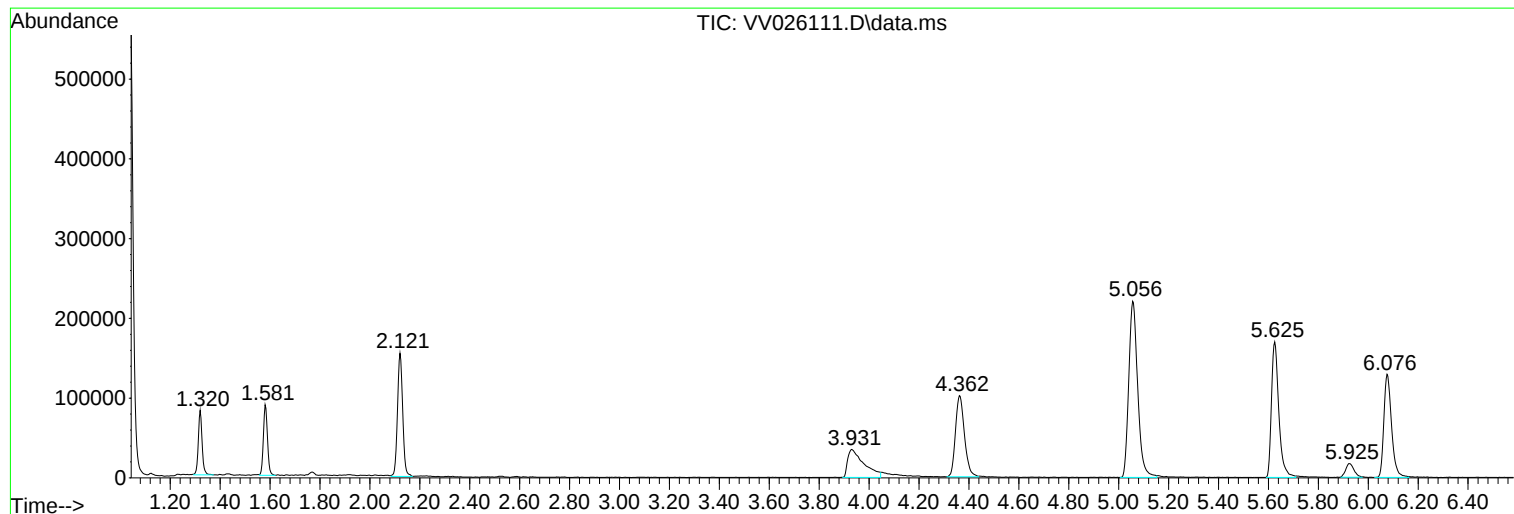

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026111.D
Acq On : 10 Jun 2022 22:29
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026111.D
Acq On : 10 Jun 2022 22:29
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc