

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026114.D
 Acq On : 10 Jun 2022 23:41
 Operator : SY/MD
 Sample : N3273-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	38	rVB2	11543	13187	2.47%	0.291%
2	1.320	78	87	98	rBV	83727	96062	17.97%	2.123%
3	1.430	115	121	129	rVB4	8077	9383	1.76%	0.207%
4	1.581	160	168	178	rBV	91398	102439	19.17%	2.264%
5	1.722	202	212	226	rBV	131019	160622	30.05%	3.550%
6	2.121	326	336	355	rVB	145975	216169	40.45%	4.777%
7	2.221	356	367	385	rVB2	25236	40587	7.59%	0.897%
8	2.526	453	462	471	rVB4	3435	6059	1.13%	0.134%
9	3.835	858	869	883	rBV6	3249	8667	1.62%	0.192%
10	3.928	883	898	926	rBV4	61665	220082	41.18%	4.864%
11	4.362	1015	1033	1059	rBV	100282	252960	47.33%	5.590%
12	5.056	1229	1249	1273	rBV3	213294	534454	100.00%	11.811%
13	5.626	1414	1426	1455	rBV	172453	359072	67.18%	7.935%
14	5.925	1507	1519	1533	rBV6	11488	26215	4.91%	0.579%
15	6.076	1553	1566	1594	rBV	129830	270621	50.64%	5.980%
16	6.992	1840	1851	1873	rBV2	38730	76695	14.35%	1.695%
17	7.320	1941	1953	1973	rBV	215983	385560	72.14%	8.520%
18	7.400	1973	1978	1989	rVB6	3496	6771	1.27%	0.150%
19	7.629	2037	2049	2064	rBV	21445	40553	7.59%	0.896%
20	7.941	2137	2146	2153	rBV2	6501	11984	2.24%	0.265%
21	7.982	2153	2159	2168	rVB5	6400	10115	1.89%	0.224%
22	8.095	2184	2194	2230	rBV2	194077	424505	79.43%	9.381%
23	8.854	2419	2430	2453	rBV	260098	438313	82.01%	9.686%
24	10.217	2843	2854	2872	rBV2	83147	132464	24.78%	2.927%
25	10.381	2893	2905	2914	rBV3	13348	19704	3.69%	0.435%
26	11.249	3164	3175	3190	rBV	228120	347469	65.01%	7.679%
27	11.622	3278	3291	3307	rBV	192394	307184	57.48%	6.788%
28	12.249	3473	3486	3495	rBV3	4490	7199	1.35%	0.159%




Sum of corrected areas: 4525095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026114.D
Acq On : 10 Jun 2022 23:41
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

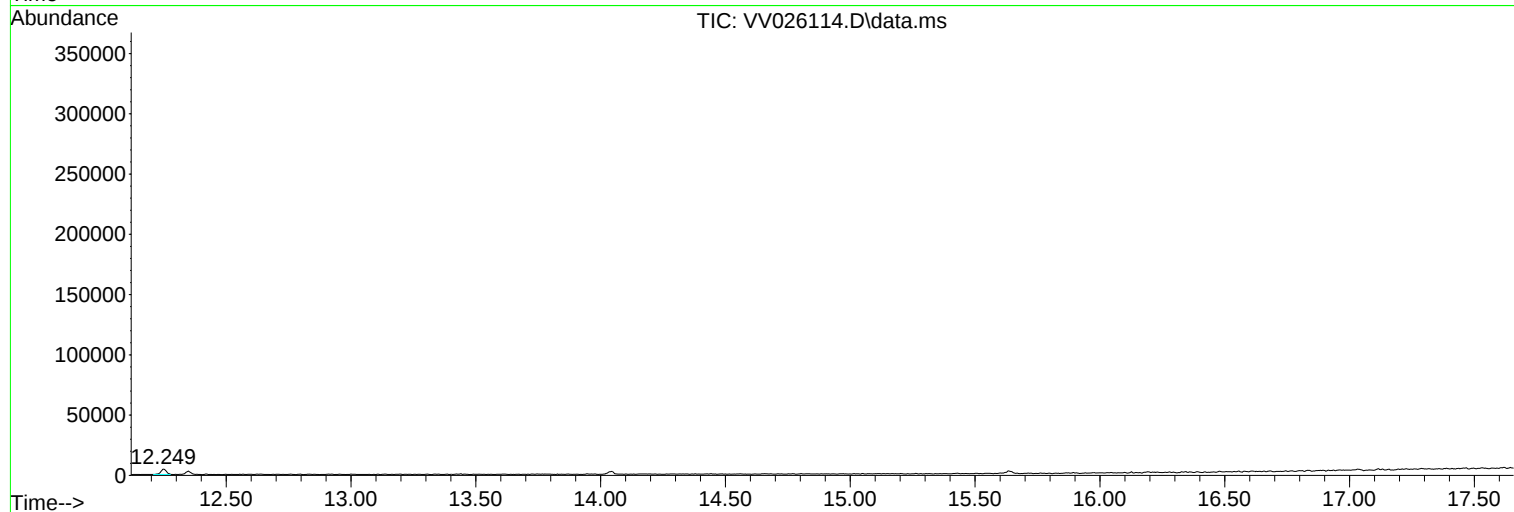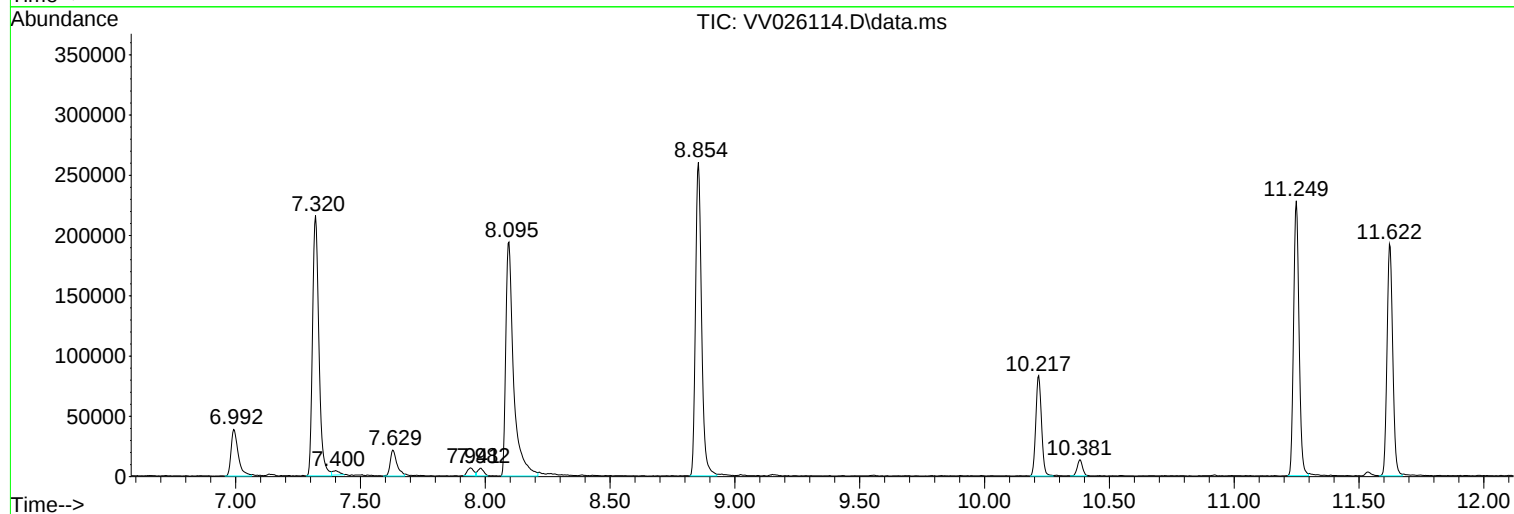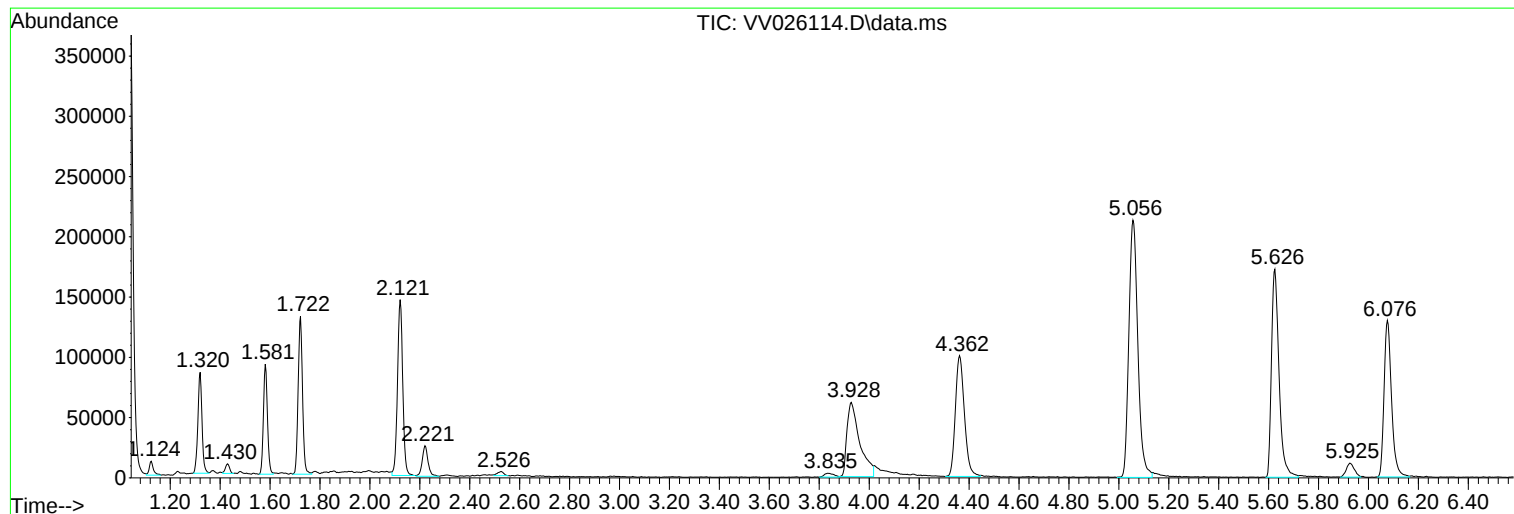

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026114.D
Acq On : 10 Jun 2022 23:41
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.722	2.24 ug/L	160622	1,4-Difluorobenzene	5.626

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Hexyne	82	C6H10	000693-02-7	7
5			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7

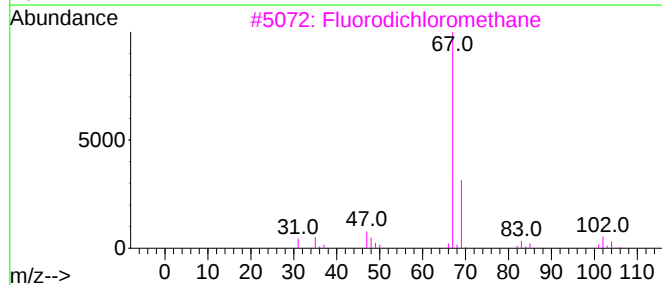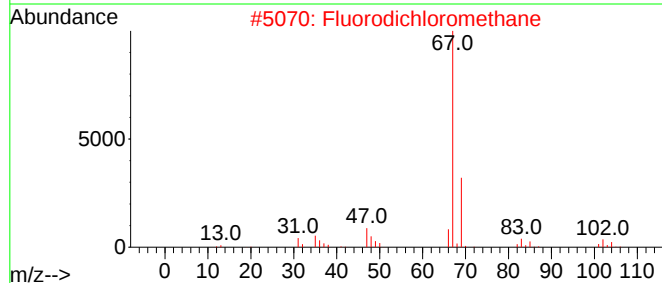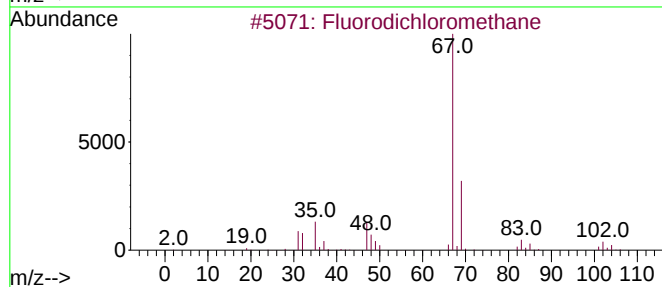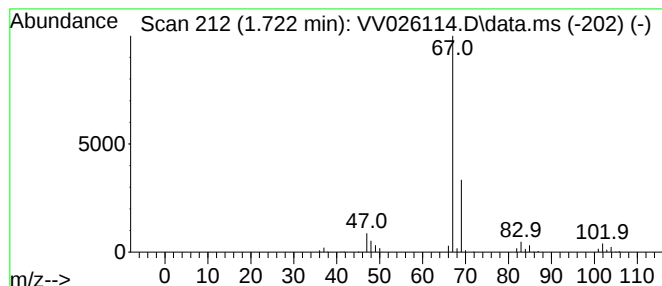

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026114.D
Acq On : 10 Jun 2022 23:41
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dimethyl sulfide Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.221	0.57 ug/L	40587	1,4-Difluorobenzene	5.626

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dimethyl sulfide	62	C2H6S	000075-18-3	91
2			Dimethyl sulfide	62	C2H6S	000075-18-3	91
3			Dimethyl sulfide	62	C2H6S	000075-18-3	91
4			Dimethyl sulfide	62	C2H6S	000075-18-3	91
5			Dimethyl sulfide	62	C2H6S	000075-18-3	91

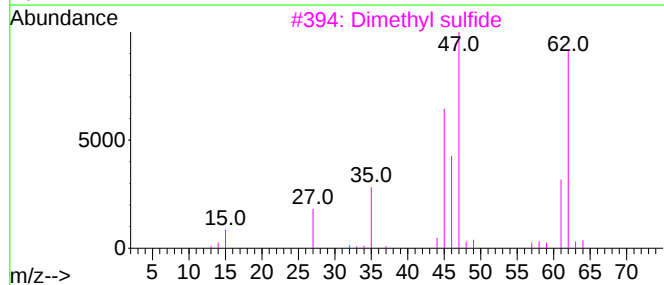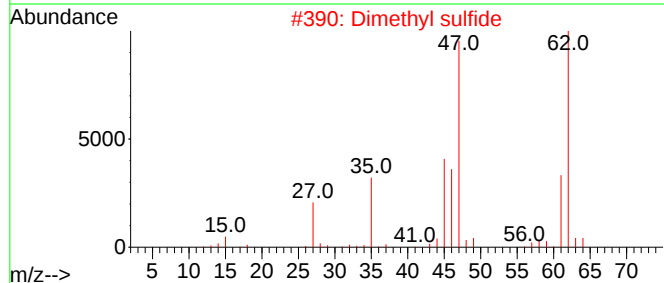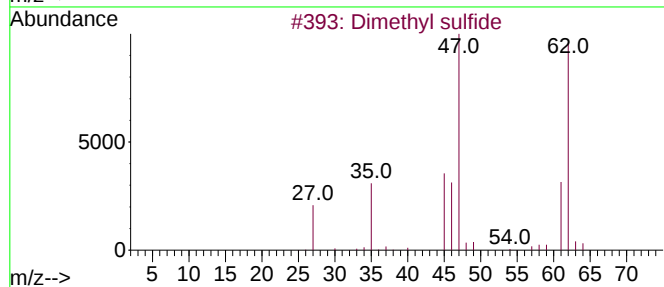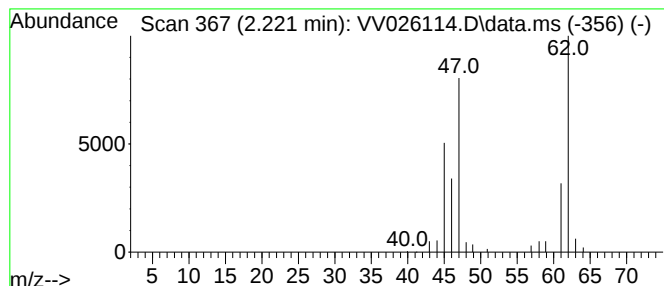

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
Data File : VV026114.D
Acq On : 10 Jun 2022 23:41
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	1.722	2.2	ug/L	160622	1	5.626	359072	5.0
Dimethyl sulfide	2.221	0.6	ug/L	40587	1	5.626	359072	5.0