
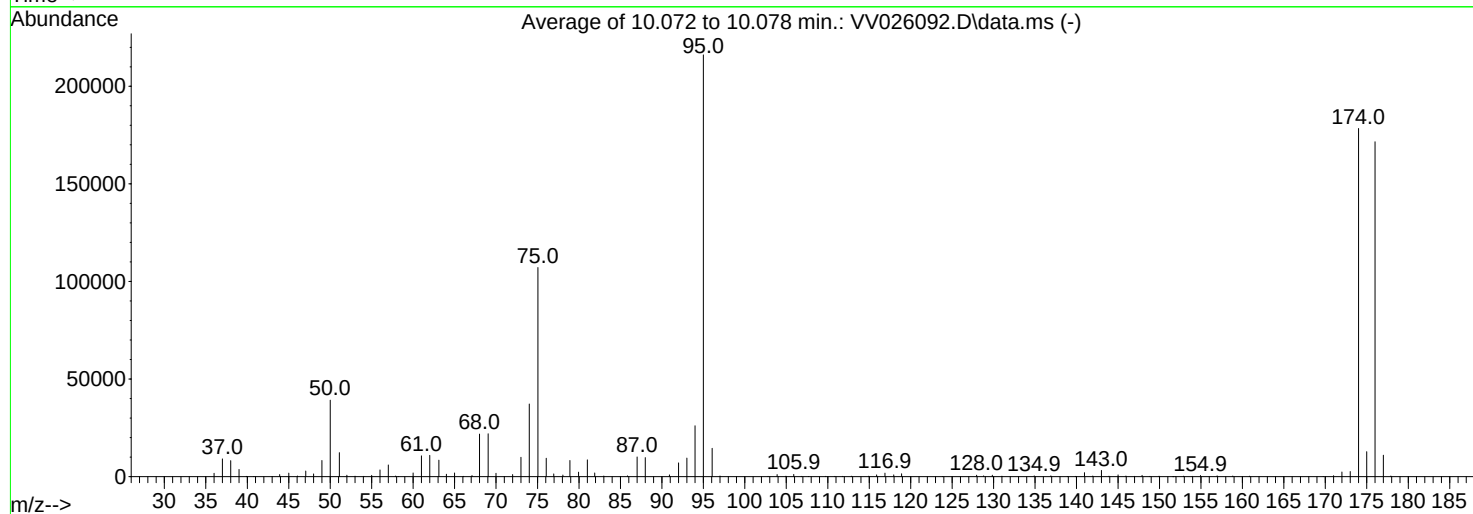


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061022\
 Data File : VV026092.D
 Acq On : 10 Jun 2022 13:30
 Operator : SY/MD
 Sample : BFB324
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB324

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 13 07:40:59 2022

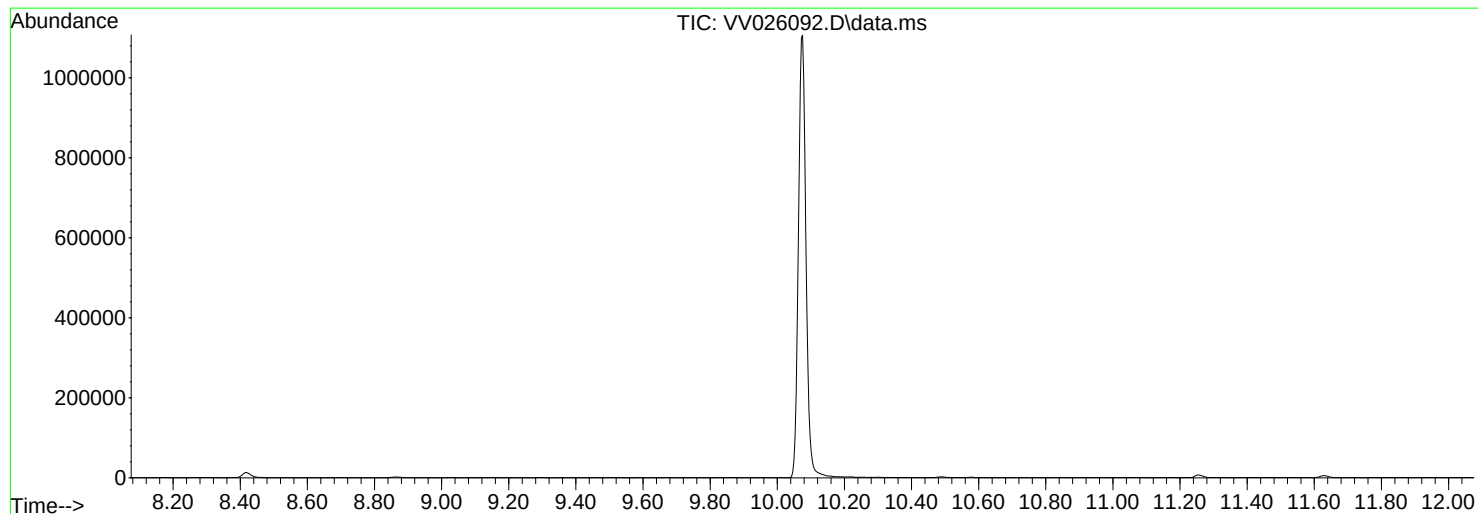

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	39197	PASS
75	95	30	80	49.6	107189	PASS
95	95	100	100	100.0	216128	PASS
96	95	5	9	6.7	14552	PASS
173	174	0.00	2	1.5	2628	PASS
174	95	50	120	82.6	178432	PASS
175	174	5	9	7.2	12817	PASS
176	174	95	105	96.2	171584	PASS
177	176	5	10	6.4	10958	PASS

Scan 2796 (10.030 min): VV026092.D\data.ms
BFB324

m/z	Abundance
39.90	198.0
43.90	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

m/z	Abundance
36.00	1807.0
37.00	9572.0
38.00	8720.0
39.00	3965.0
40.00	413.0
40.80	169.0
44.00	1483.0
45.00	1856.0
46.00	302.0
47.00	2936.0
48.00	1389.0
49.00	8952.0
50.00	41544.0
51.10	12973.0
52.00	757.0
53.00	273.0
54.10	151.0
55.00	650.0
56.00	3581.0
57.00	6185.0
57.90	378.0
60.00	1845.0
61.00	11354.0
62.00	11584.0
63.10	9223.0
64.00	1398.0
65.00	1968.0
66.00	213.0
67.10	632.0
68.00	22560.0
69.10	22432.0
70.00	1784.0
71.00	148.0
72.00	1170.0
73.00	10419.0
74.00	38088.0
75.10	111376.0
76.10	9925.0
77.00	1271.0
78.00	833.0
78.90	8805.0
80.00	2304.0
81.00	8890.0
81.90	1968.0
83.00	338.0
85.90	413.0
87.00	10454.0
88.00	9917.0
90.90	856.0
92.00	7298.0
93.00	10077.0
94.00	27224.0
95.00	222912.0
96.10	15156.0
97.00	480.0
102.80	180.0
103.90	1133.0
105.00	238.0
105.90	1146.0
106.90	212.0
107.70	110.0
109.80	135.0
110.80	208.0
111.80	122.0
112.90	220.0
114.90	218.0
115.90	976.0
116.90	1938.0
118.00	867.0
118.90	1557.0
123.90	113.0
127.90	762.0
128.80	481.0
129.90	784.0
131.00	288.0
134.90	402.0
136.90	359.0
138.90	103.0
139.90	153.0
141.00	2067.0
142.00	316.0
143.00	3427.0
143.90	277.0
145.00	1035.0
146.00	405.0
147.10	199.0
147.90	666.0
148.90	140.0
150.00	246.0
151.60	103.0
152.90	207.0
153.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

154.90	592.0
156.90	404.0
158.90	353.0
160.80	241.0
169.80	119.0
171.00	509.0
172.00	2358.0
173.00	2742.0
174.00	180736.0
175.00	13099.0
176.00	171904.0
177.00	11290.0
177.90	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

m/z	Abundance
36.00	1770.0
37.00	9392.0
38.00	8428.0
39.00	3794.0
39.90	379.0
40.80	174.0
43.00	125.0
44.00	1417.0
45.00	1863.0
46.00	291.0
47.10	2930.0
48.00	1458.0
49.00	8577.0
50.00	40464.0
51.10	12771.0
52.00	780.0
53.00	286.0
54.10	160.0
55.00	696.0
56.00	3588.0
57.00	6171.0
57.90	375.0
60.00	1997.0
61.00	10923.0
62.00	11382.0
63.10	8708.0
64.00	1273.0
65.00	1984.0
66.10	165.0
67.10	569.0
68.00	22752.0
69.10	22688.0
70.00	1794.0
72.00	1093.0
73.00	10328.0
74.00	38560.0
75.10	110560.0
76.00	9791.0
76.90	1436.0
78.10	866.0
78.90	8550.0
80.00	2317.0
81.00	8928.0
81.90	1934.0
83.00	315.0
85.80	400.0
87.00	10433.0
88.00	10212.0
90.90	955.0
92.00	7324.0
93.00	9878.0
94.00	26864.0
95.00	223232.0
96.10	15046.0
97.00	371.0
102.80	174.0
103.90	1151.0
105.00	274.0
105.90	1204.0
106.80	193.0
107.70	107.0
109.70	155.0
110.90	175.0
111.80	162.0
112.90	244.0
115.00	241.0
115.90	907.0
116.90	1911.0
117.90	954.0
118.90	1535.0
123.90	126.0
128.00	791.0
128.80	464.0
129.80	761.0
131.00	308.0
134.90	436.0
136.90	424.0
138.90	108.0
139.90	169.0
141.00	2137.0
142.00	303.0
143.00	3273.0
143.90	271.0
145.00	955.0
146.00	389.0
147.00	168.0
147.90	666.0
148.90	133.0
149.90	215.0
151.90	110.0
152.90	252.0
153.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

154.90	583.0
156.90	442.0
158.90	319.0
160.90	243.0
169.70	102.0
171.00	543.0
172.00	2436.0
173.00	2763.0
174.00	184896.0
175.00	13208.0
176.00	178176.0
177.00	11366.0
177.90	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

m/z	Abundance
36.00	1553.0
37.00	8311.0
38.00	7395.0
39.00	3325.0
39.90	380.0
43.00	156.0
43.90	1248.0
45.00	1598.0
46.10	298.0
47.10	2671.0
48.00	1349.0
49.00	7451.0
50.00	35584.0
51.10	11144.0
52.00	624.0
53.00	287.0
54.00	162.0
55.00	603.0
56.00	3106.0
57.00	5537.0
57.90	247.0
58.20	228.0
60.00	1939.0
61.00	9683.0
62.00	9846.0
63.10	7515.0
64.00	1156.0
65.00	1700.0
66.00	137.0
67.10	502.0
68.00	20224.0
69.00	20760.0
70.00	1637.0
72.00	952.0
73.00	9130.0
74.00	34912.0
75.00	99632.0
76.00	8592.0
76.90	1417.0
78.00	836.0
78.90	7537.0
79.90	2180.0
81.00	8061.0
81.90	1666.0
83.00	286.0
85.90	354.0
87.00	9264.0
88.00	9113.0
90.90	919.0
92.00	6506.0
93.00	8661.0
94.00	24256.0
95.00	202240.0
96.00	13455.0
97.00	270.0
102.80	127.0
103.90	1025.0
104.90	307.0
105.90	1105.0
106.70	169.0
109.70	133.0
110.90	160.0
111.80	160.0
112.80	235.0
115.00	257.0
115.90	714.0
116.90	1570.0
118.00	908.0
118.90	1363.0
123.80	122.0
127.90	735.0
128.80	376.0
129.80	727.0
131.00	278.0
134.90	476.0
136.90	422.0
139.90	158.0
140.90	1992.0
141.90	276.0
143.00	2814.0
143.90	223.0
145.00	801.0
145.90	332.0
146.90	165.0
147.90	568.0
148.80	115.0
149.90	194.0
151.90	128.0
152.90	255.0
154.00	178.0
155.00	511.0
157.00	376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324

158.80	286.0
160.90	254.0
171.00	479.0
172.00	2278.0
173.00	2379.0
174.00	169664.0
175.00	12143.0
176.00	164672.0
177.00	10219.0
177.90	248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB324