




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

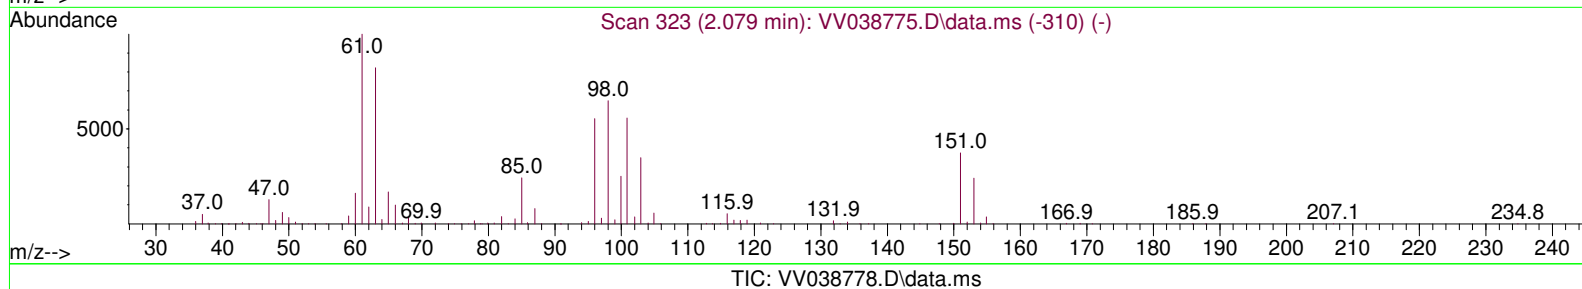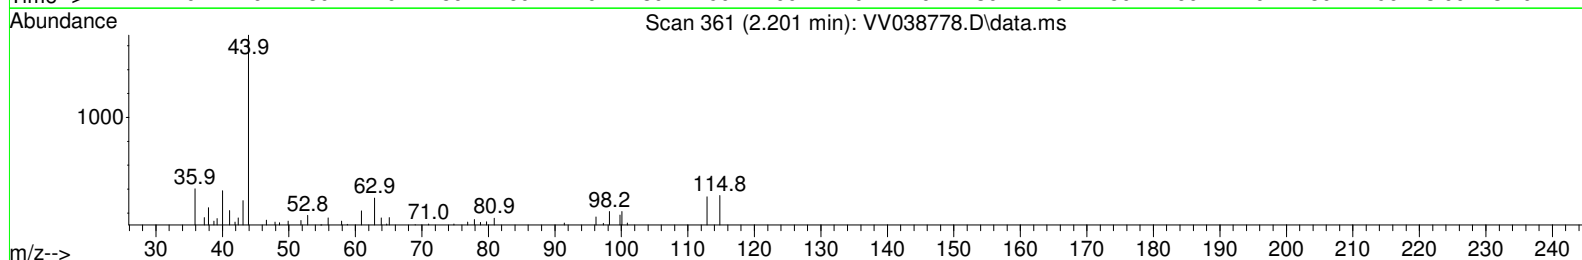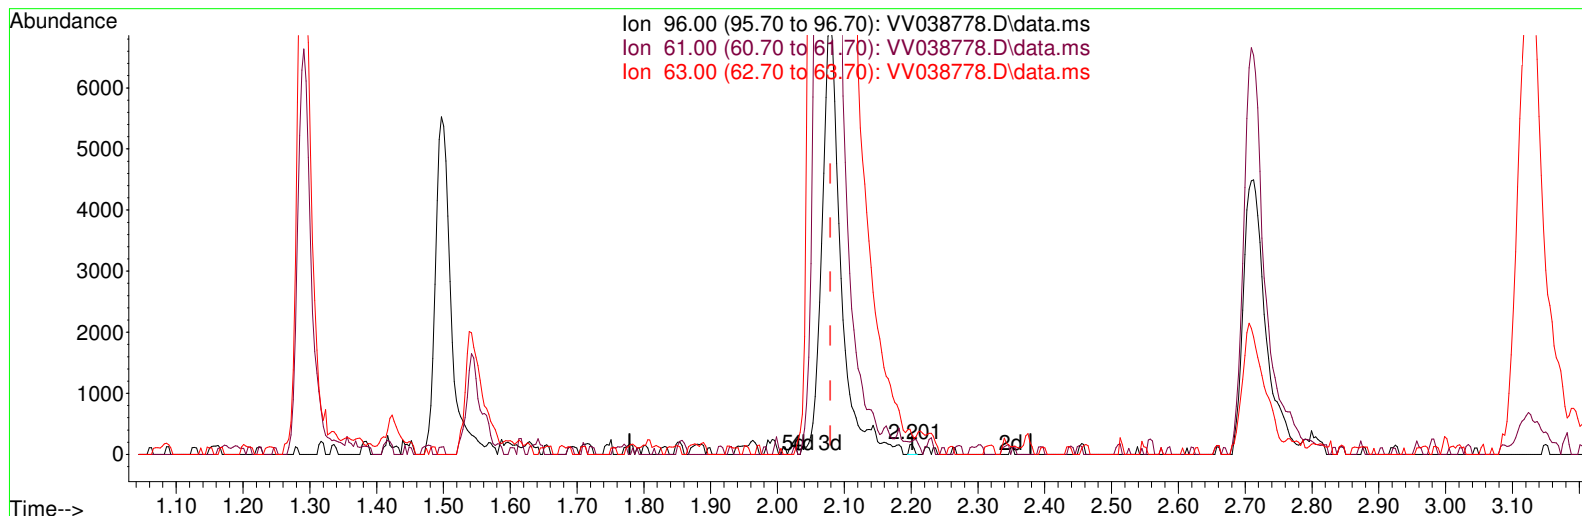

(12) 1,1-Dichloroethene (T)

2.201min (+ 0.122) 0.02 ug/L

response 81

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	172.70	130.72
63.00	158.40	196.39
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

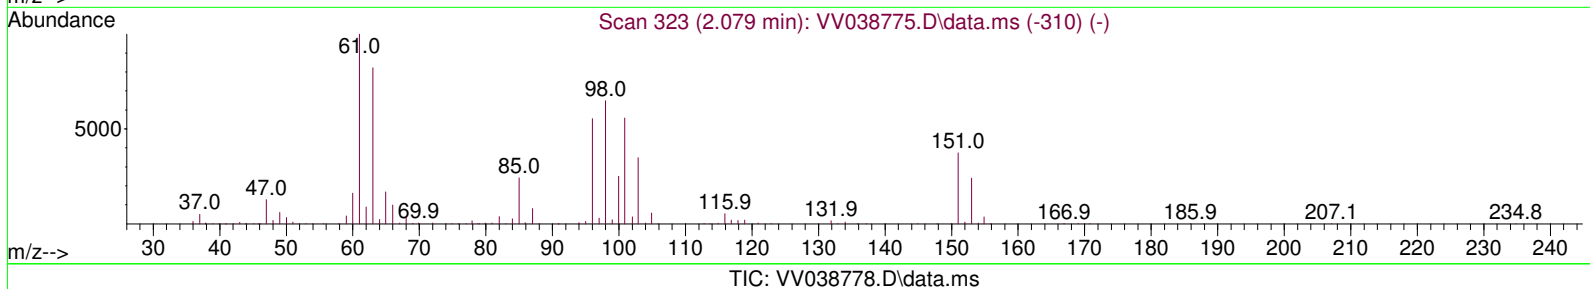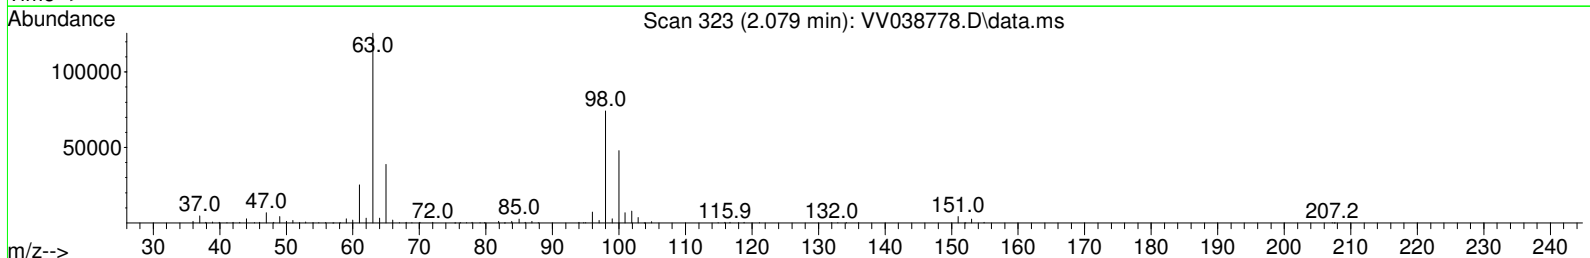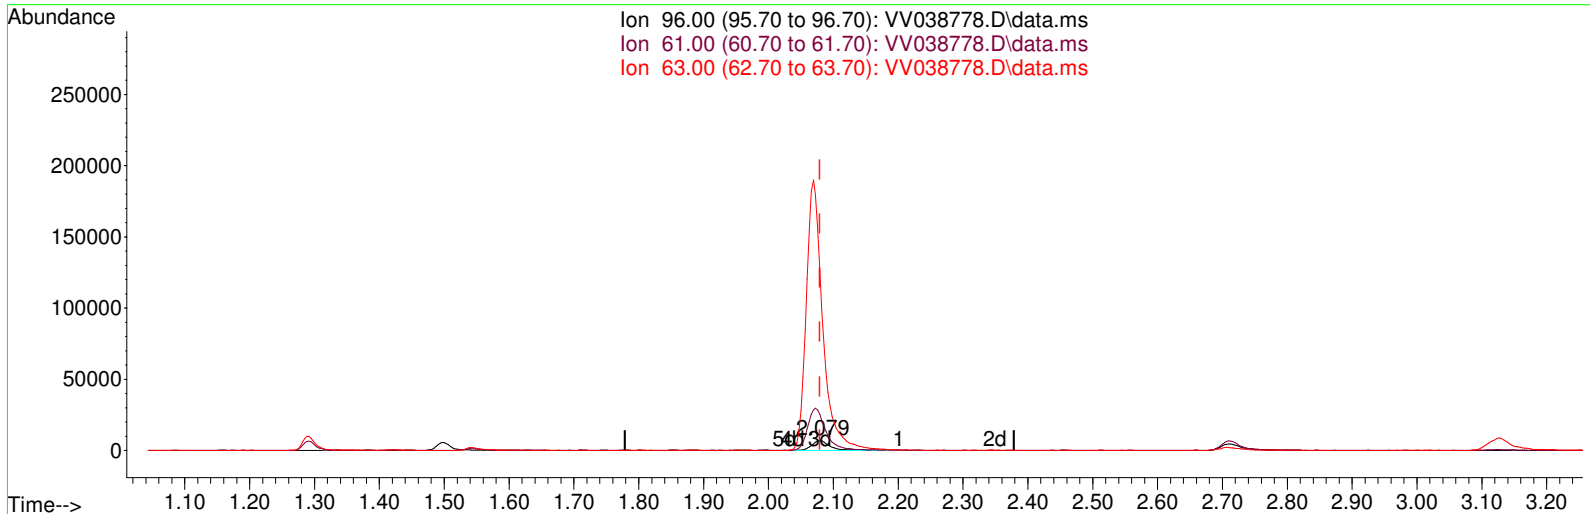

(12) 1,1-Dichloroethene (T)

2.079min (+ 0.000) 3.00 ug/L m

response 14228

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	172.70	349.60#
63.00	158.40	1747.46#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

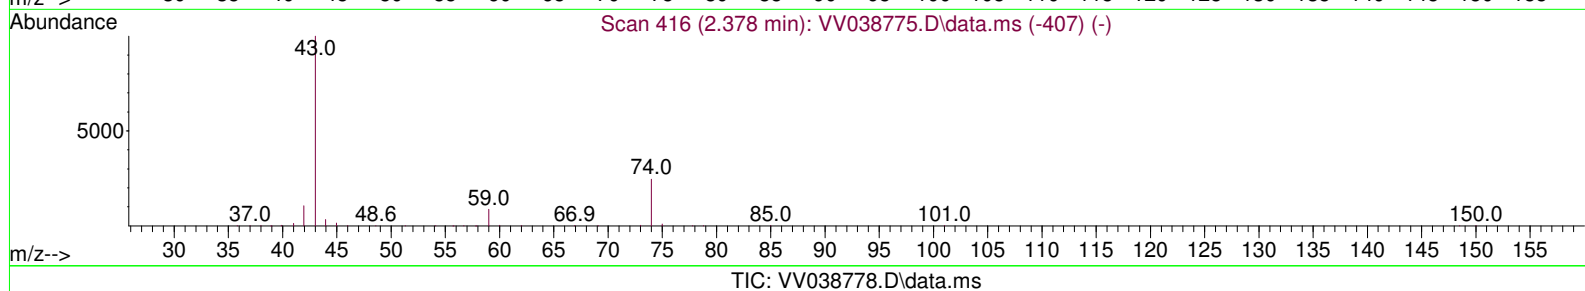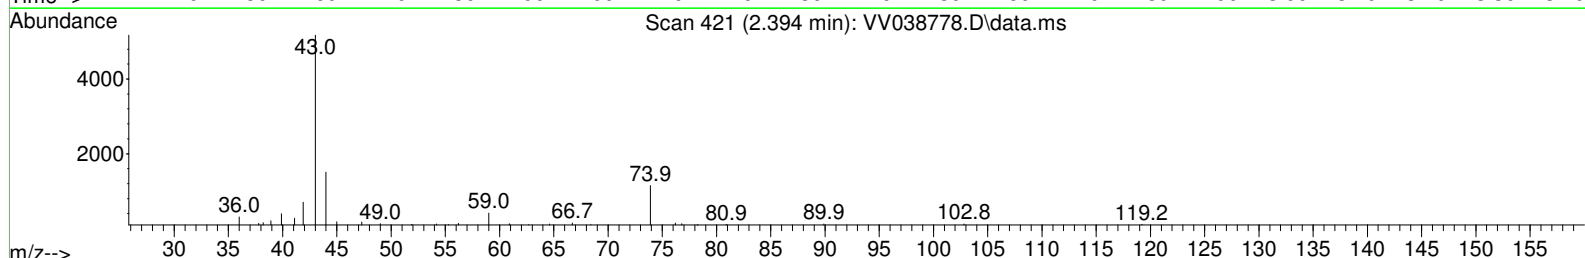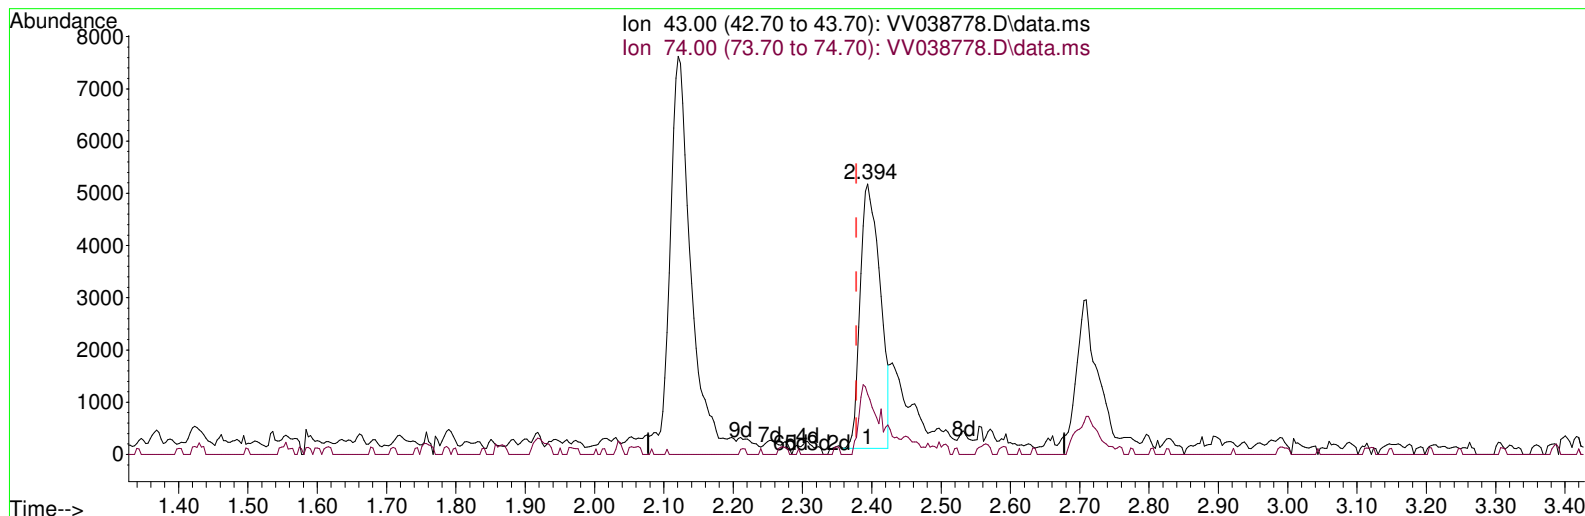

(15) Methyl Acetate (T)

2.394min (+ 0.016) 1.58 ug/L

response 10033

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	19.59#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

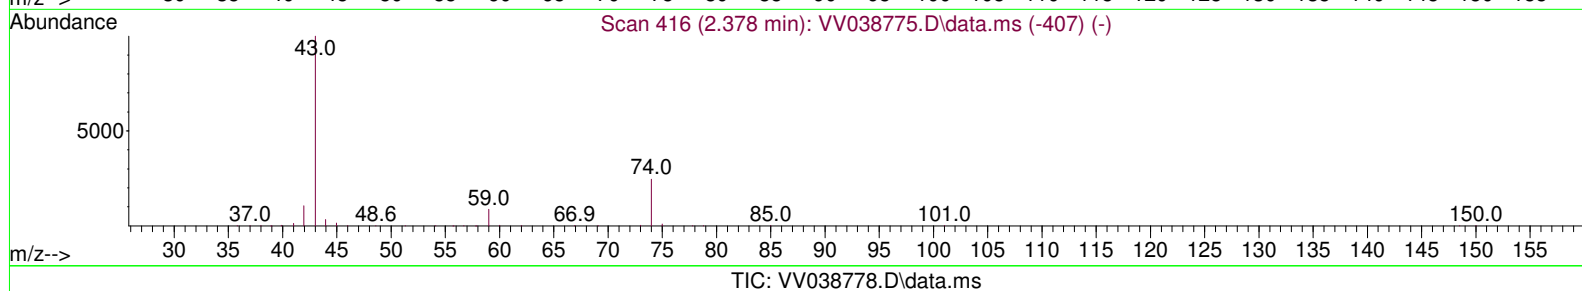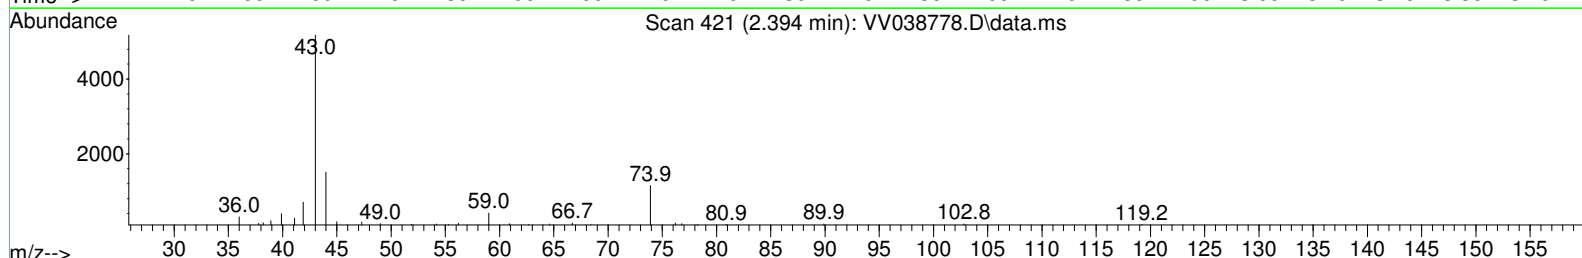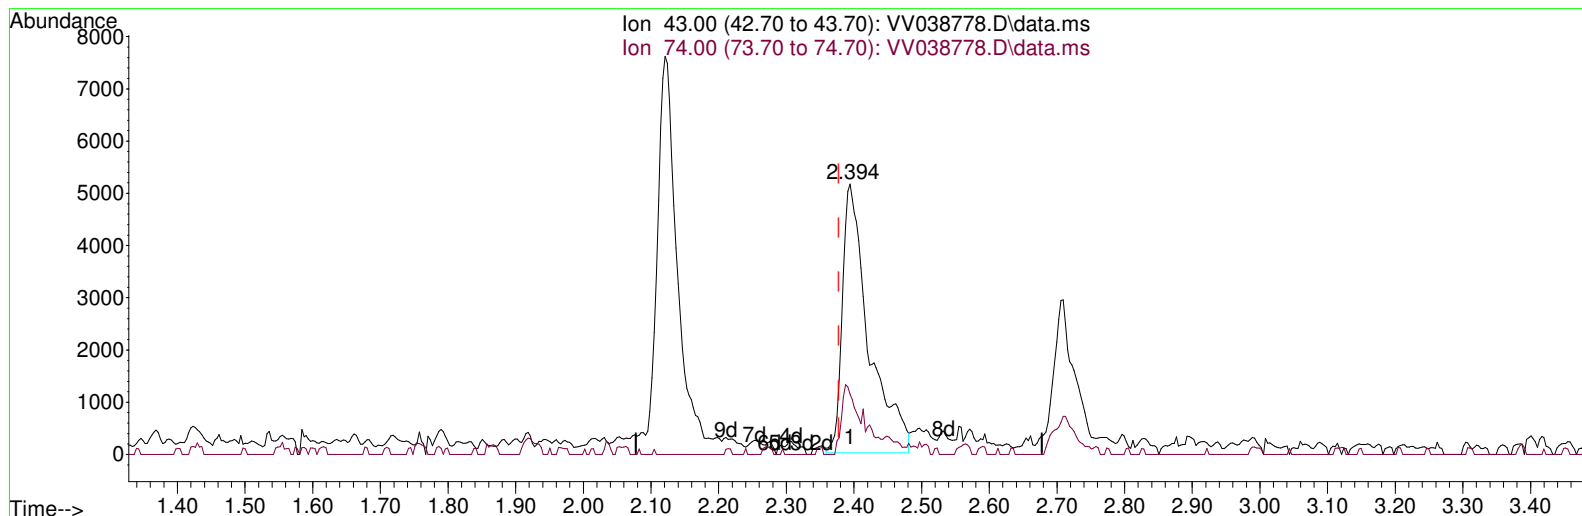

(15) Methyl Acetate (T)

2.394min (+ 0.016) 2.18 ug/L m

response 13896

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	14.14#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

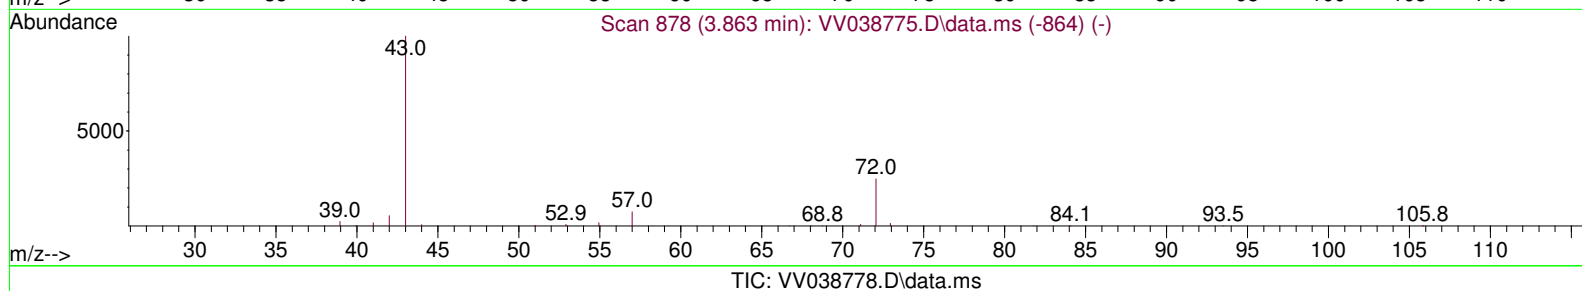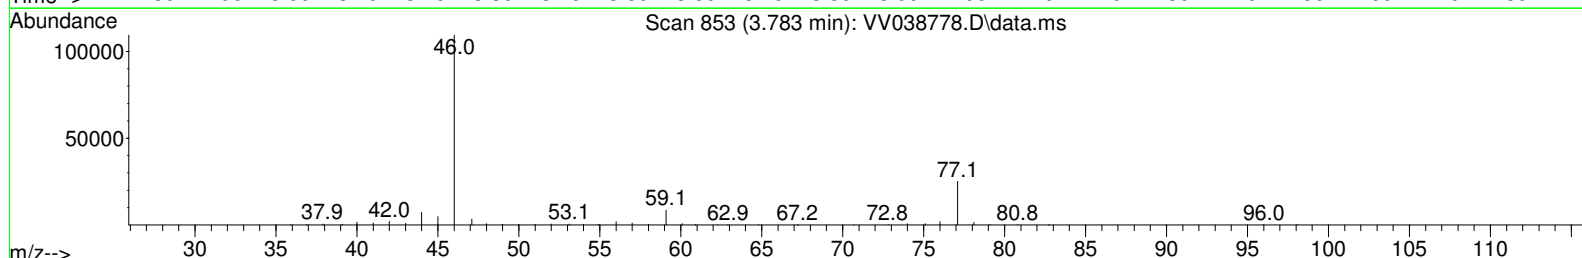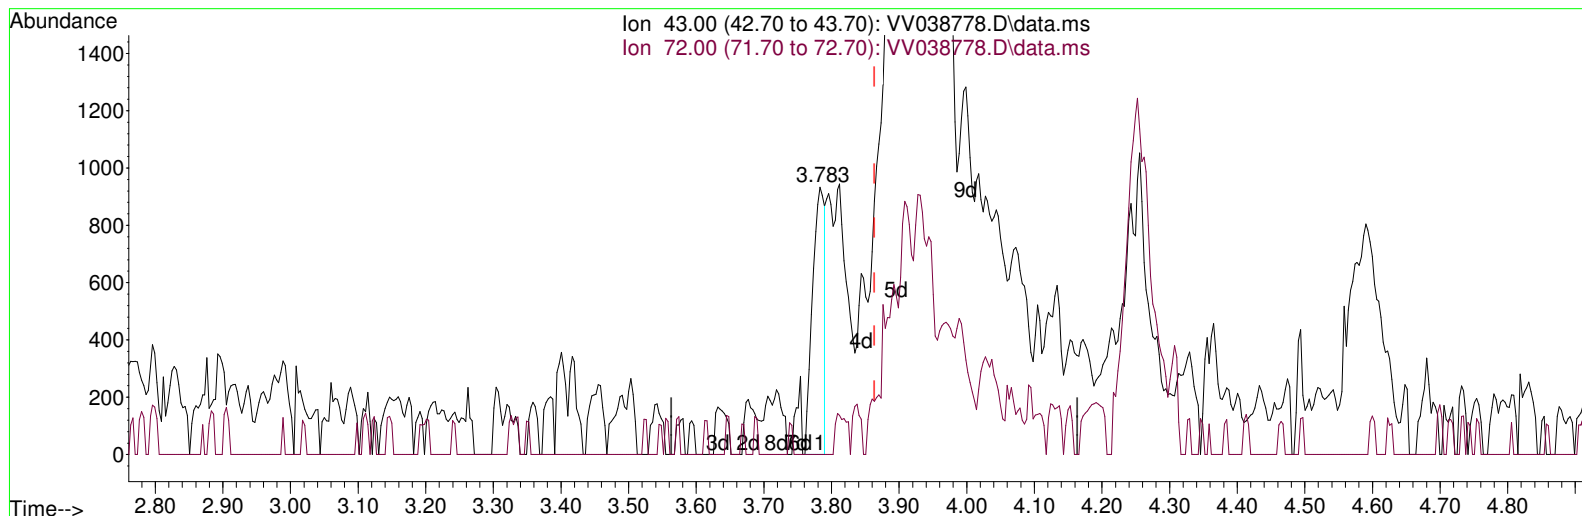

(22) 2-Butanone (T)

3.783min (-0.080) 0.30 ug/L

response 1147

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	12.55
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

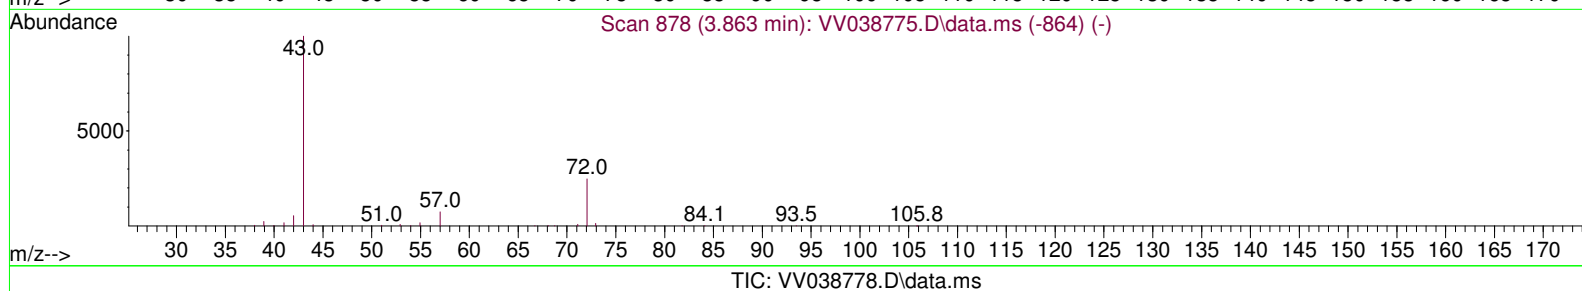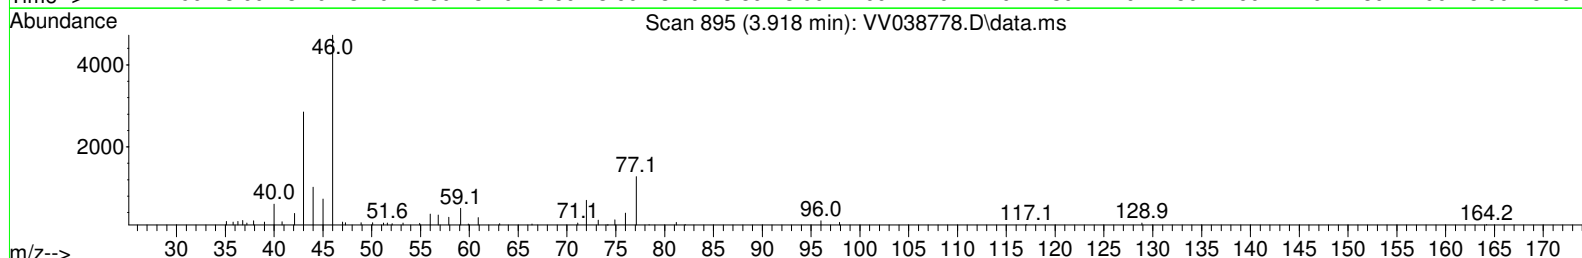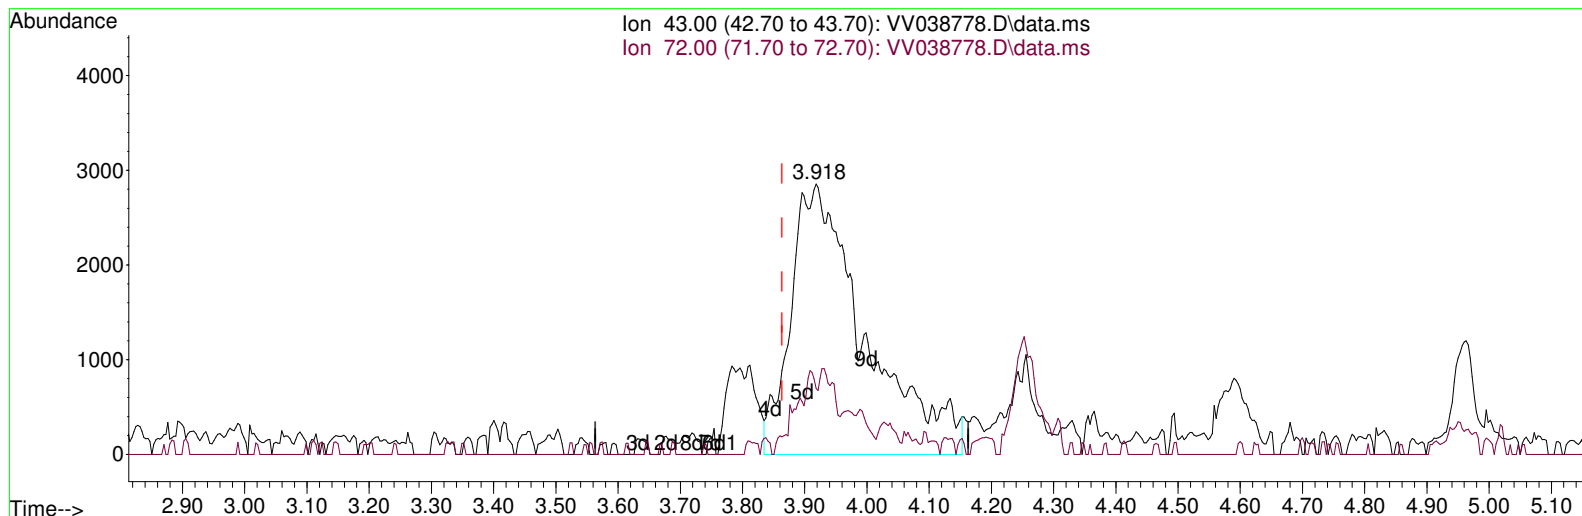

(22) 2-Butanone (T)

3.918min (+ 0.055) 6.29 ug/L m

response 23669

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	0.61#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

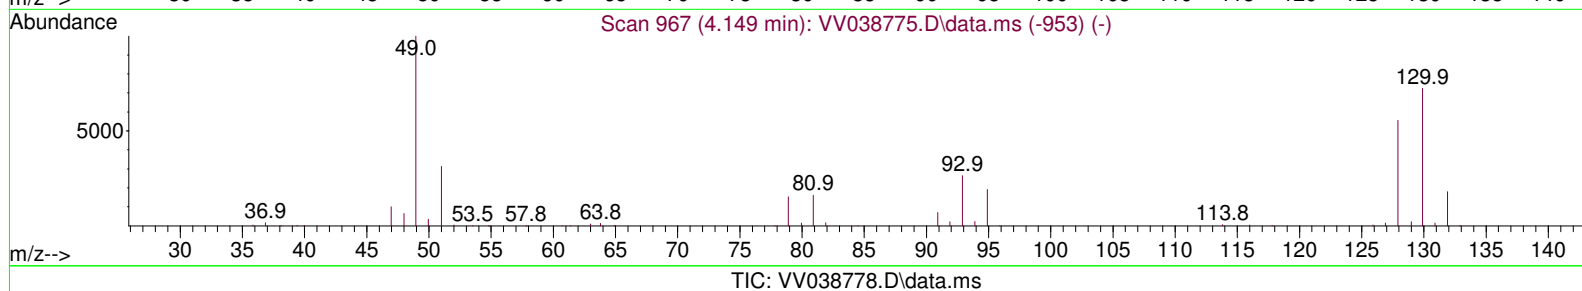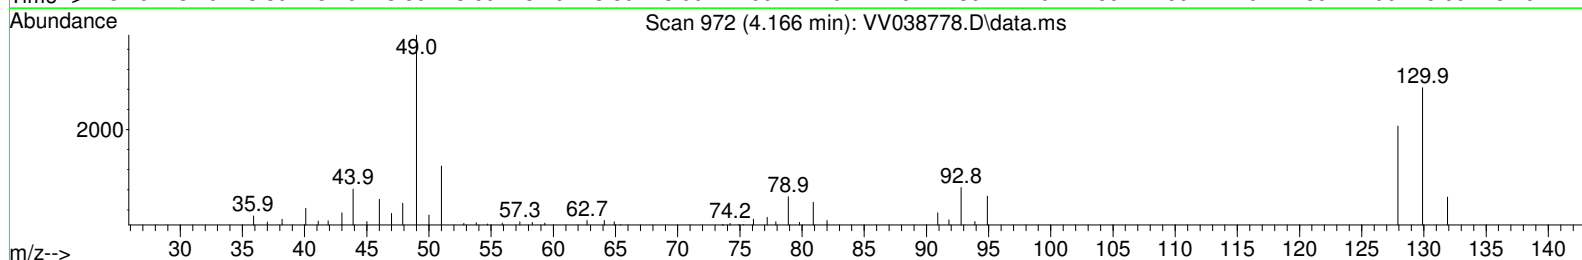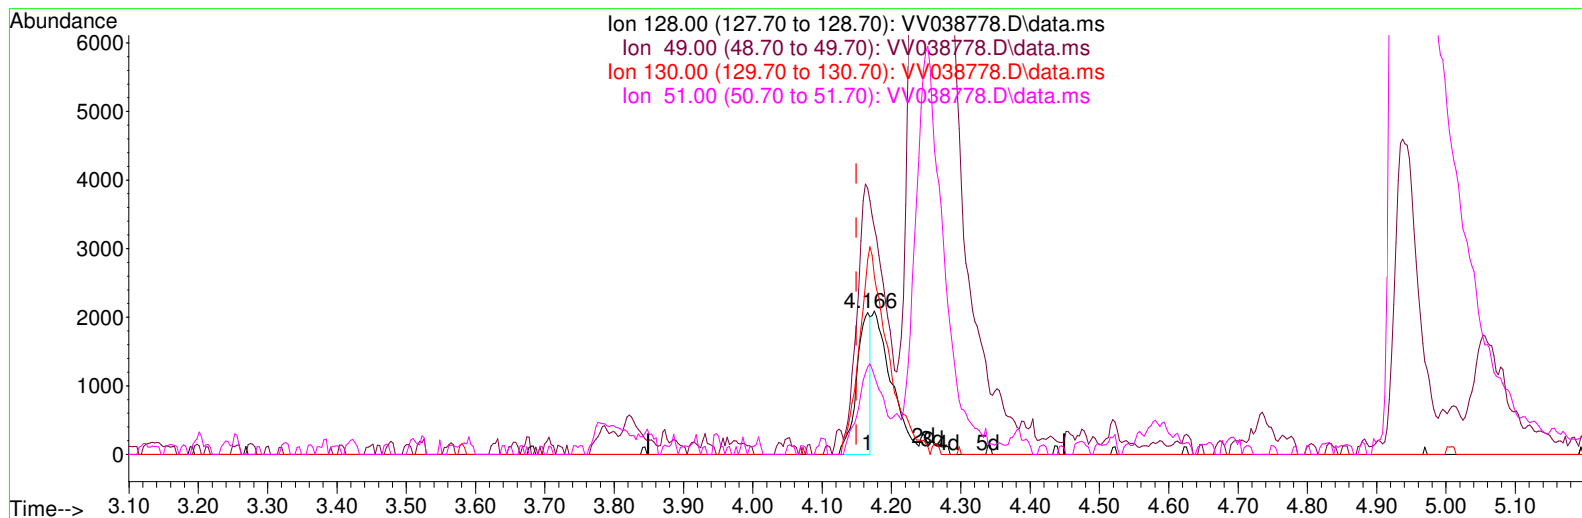

(23) Bromochloromethane (T)

4.166min (+ 0.016) 1.04 ug/L

response 2839

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	187.86
130.00	133.20	137.16
51.00	50.30	61.54#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

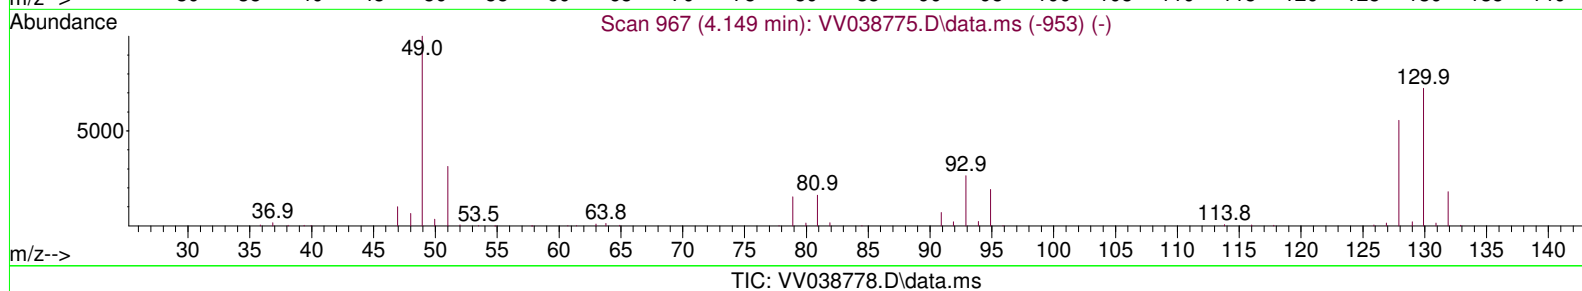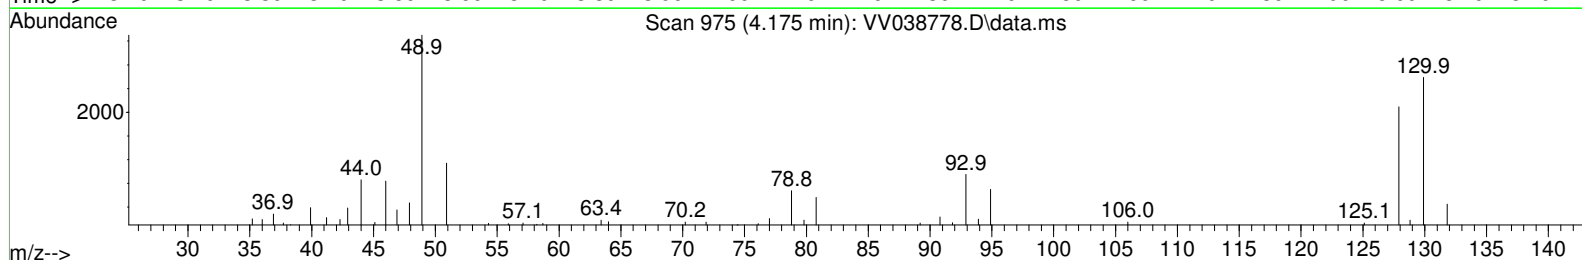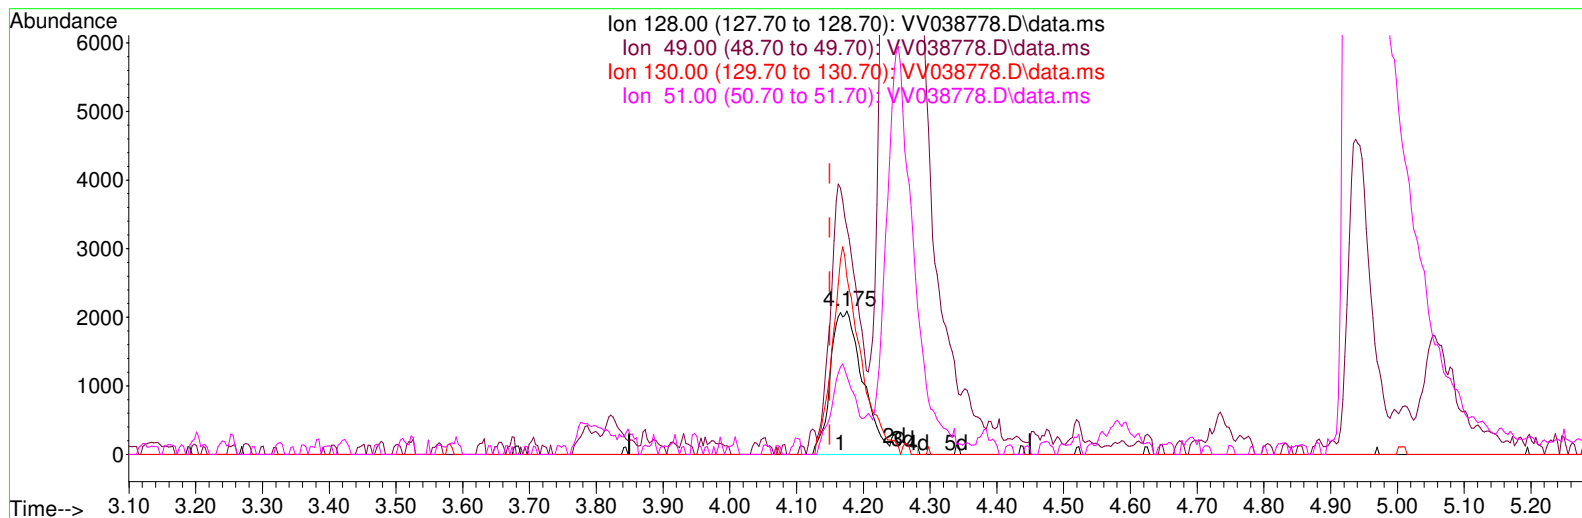

(23) Bromochloromethane (T)

4.175min (+ 0.026) 2.70 ug/L m

response 7374

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	157.84
130.00	133.20	123.71
51.00	50.30	54.59




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

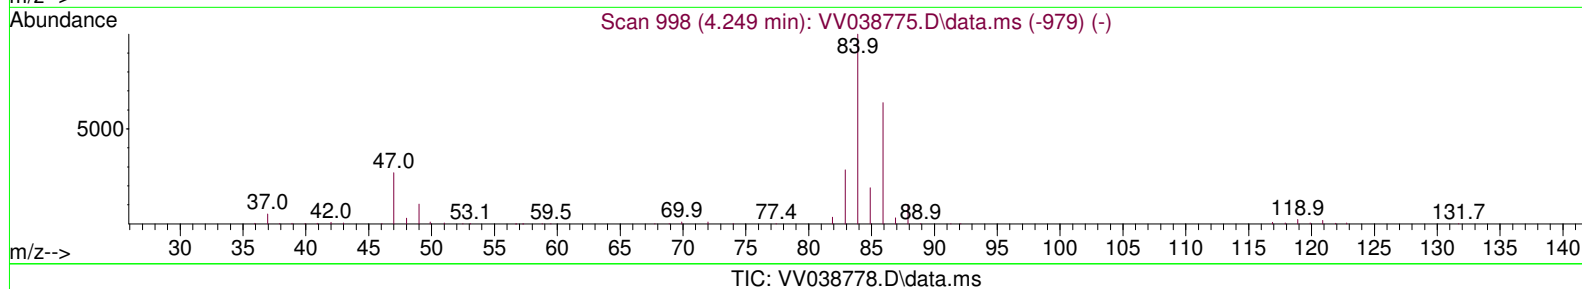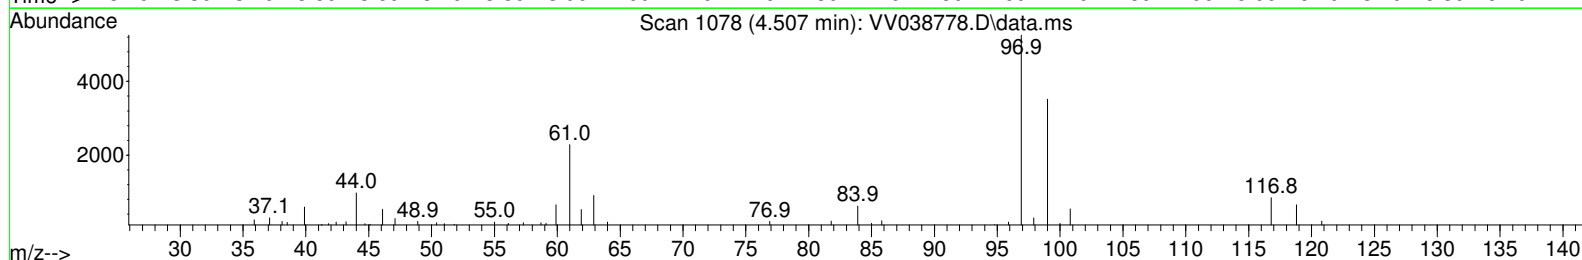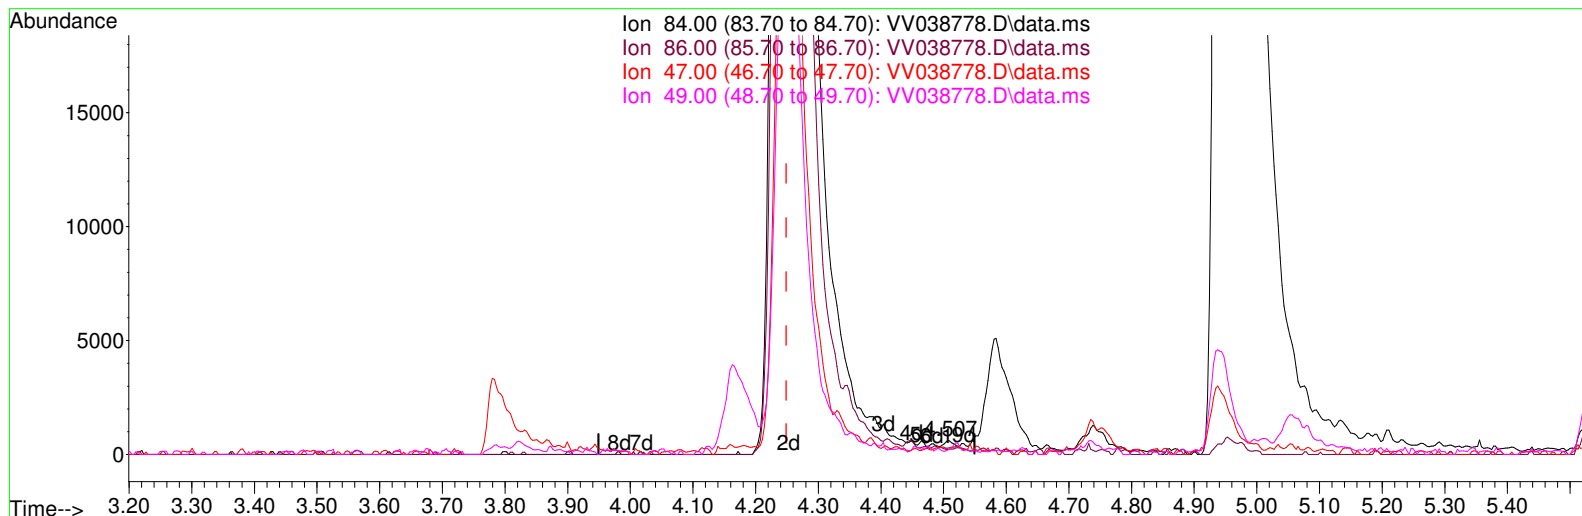

(24) Chloroform-d (S)

4.507min (+ 0.257) 0.03 ug/L

response 313

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.70	49.84
47.00	38.20	42.81
49.00	23.20	19.17




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

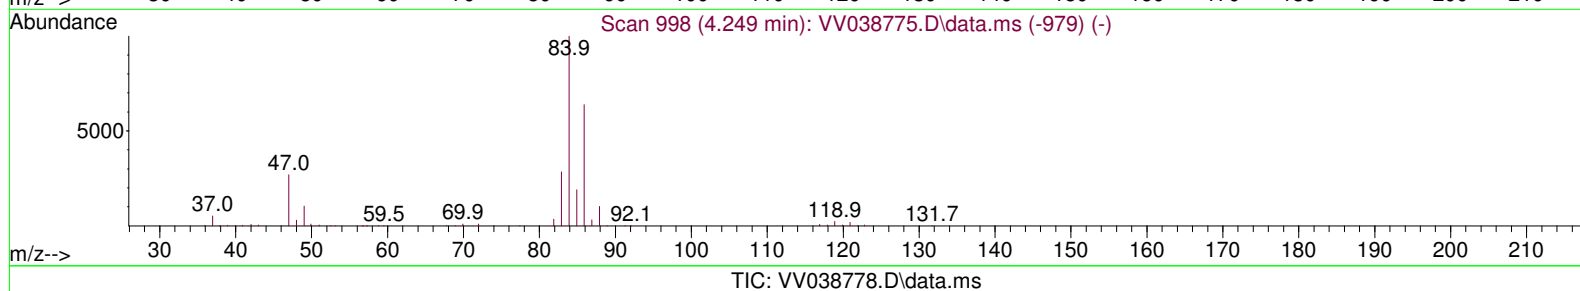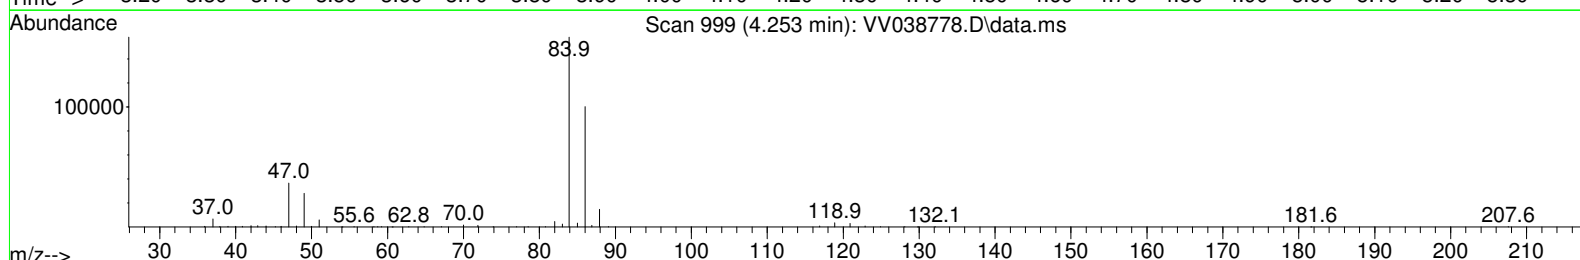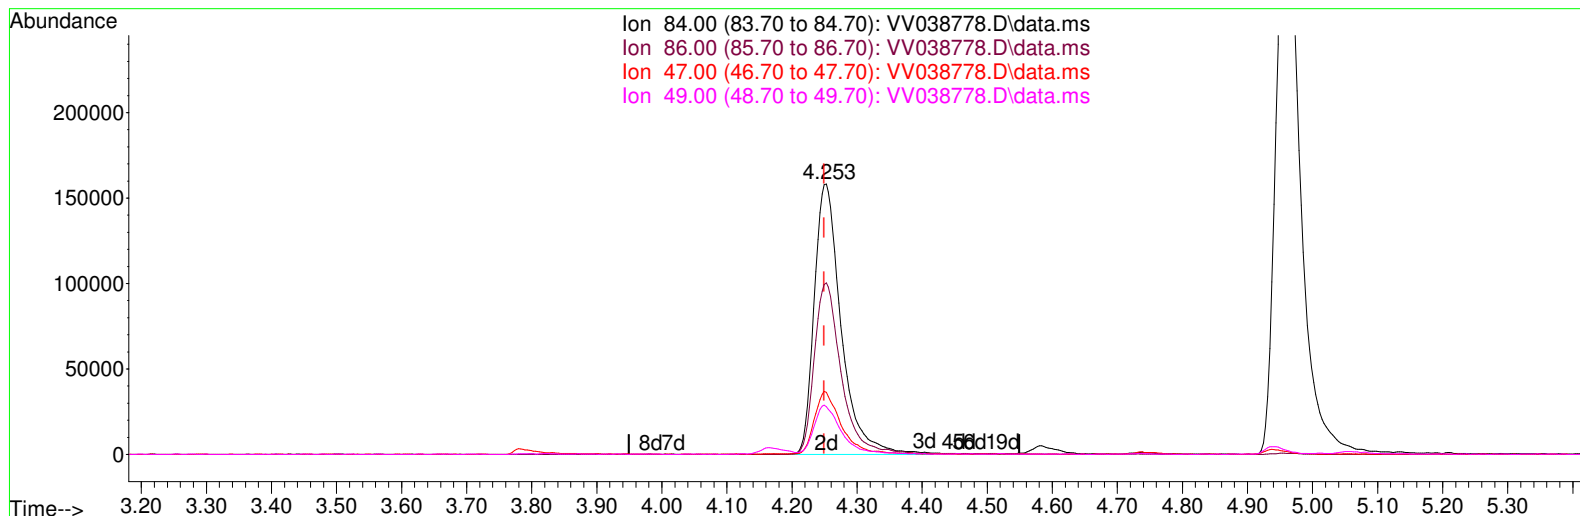

(24) Chloroform-d (S)

4.253min (+ 0.003) 47.00 ug/L m

response 456405

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.70	0.03#
47.00	38.20	0.03#
49.00	23.20	0.01#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

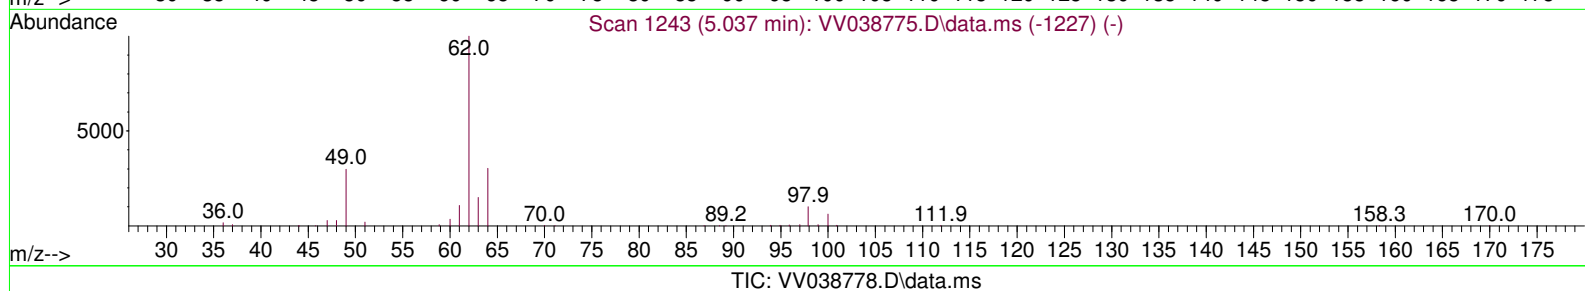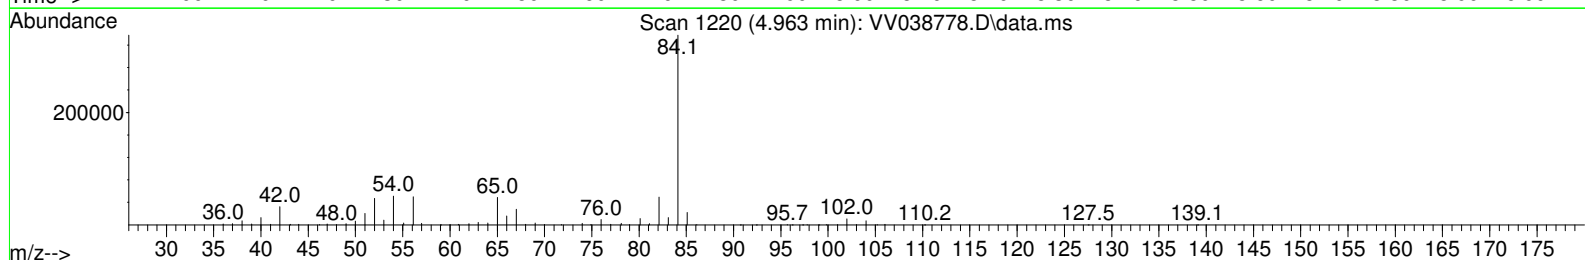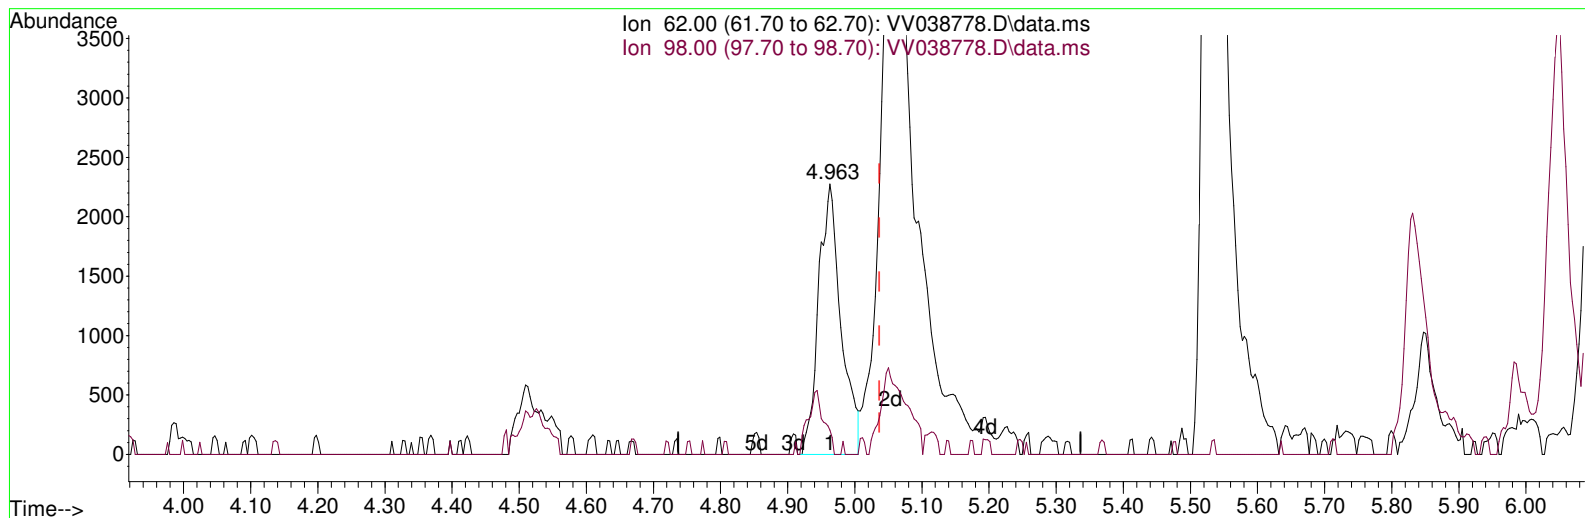

(27) 1,2-Dichloroethane (T)

4.963min (-0.074) 0.72 ug/L

response 5268

Ion	Exp%	Act%
62.00	100.00	100.00
98.00	9.40	8.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

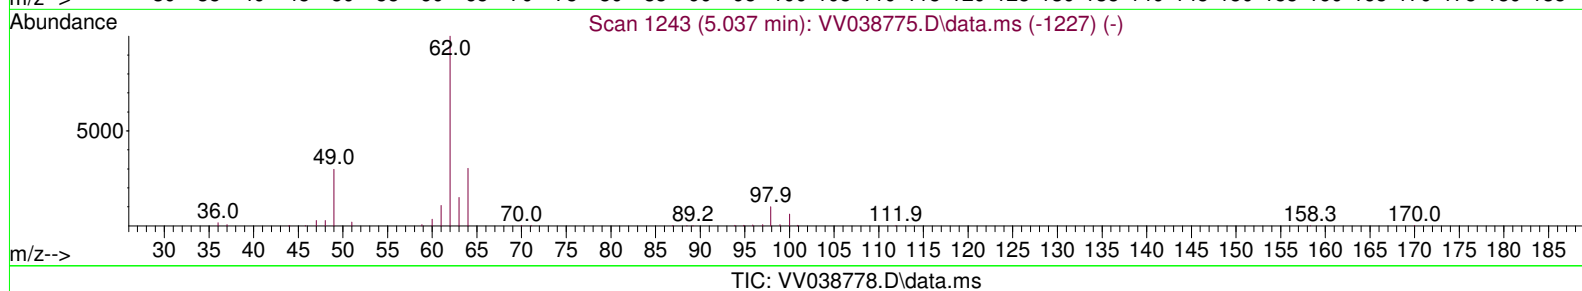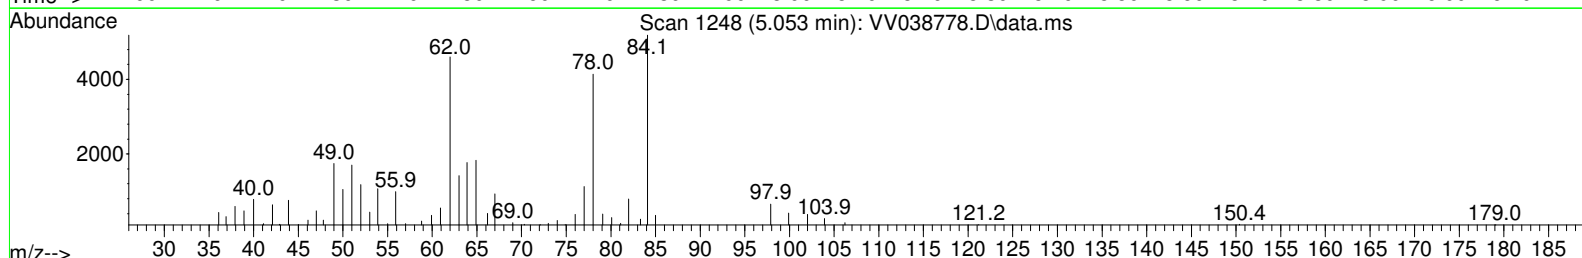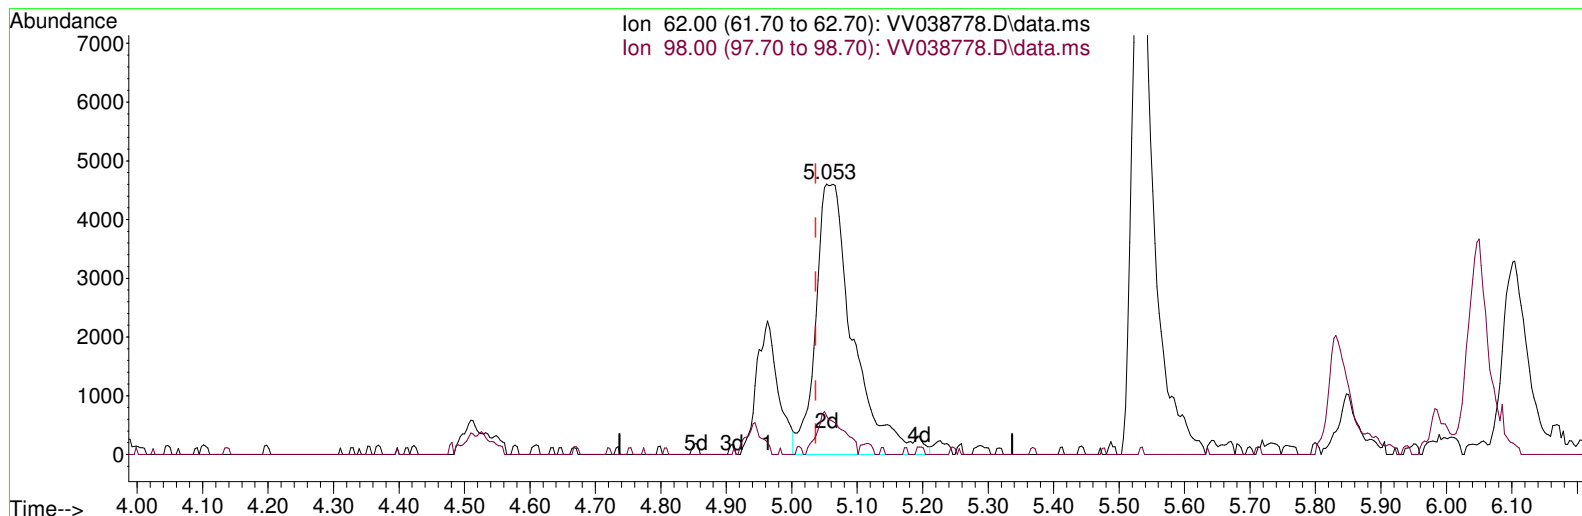

(27) 1,2-Dichloroethane (T)

5.053min (+ 0.016) 2.48 ug/L m

response 18264

Ion	Exp%	Act%
-----	------	------

62.00	100.00	100.00
-------	--------	--------

98.00	9.40	14.23#
-------	------	--------

0.00	0.00	0.00
------	------	------

0.00	0.00	0.00
------	------	------




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

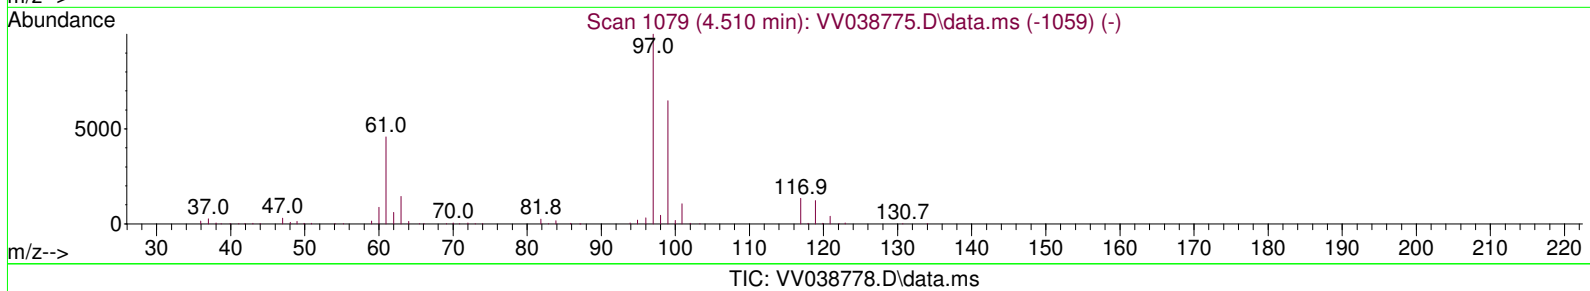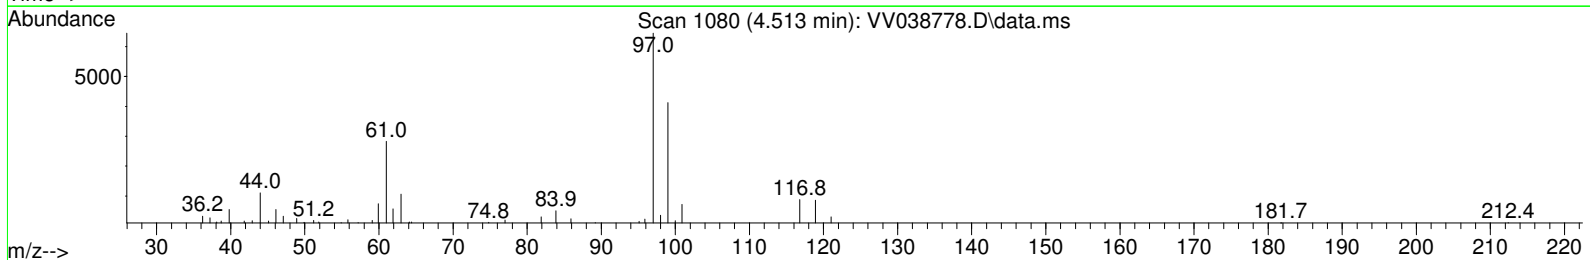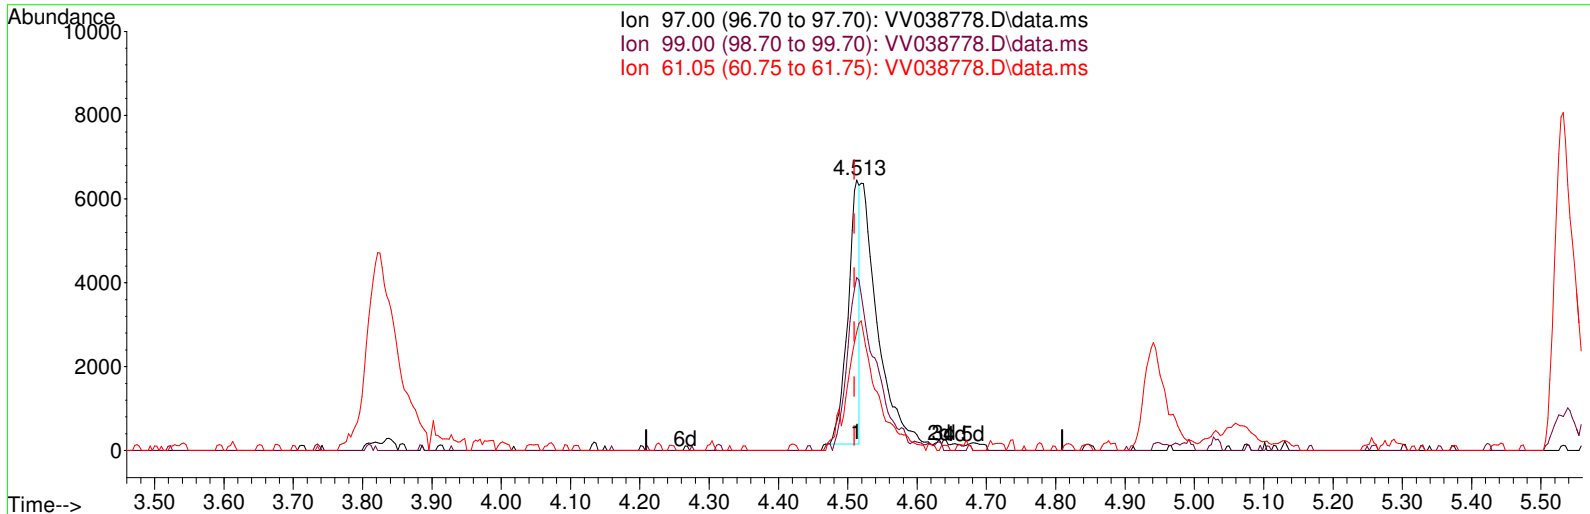

(30) 1,1,1-Trichloroethane (T)

4.513min (+ 0.003) 0.87 ug/L

response 7310

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	65.40	153.65#
61.05	42.00	114.01#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

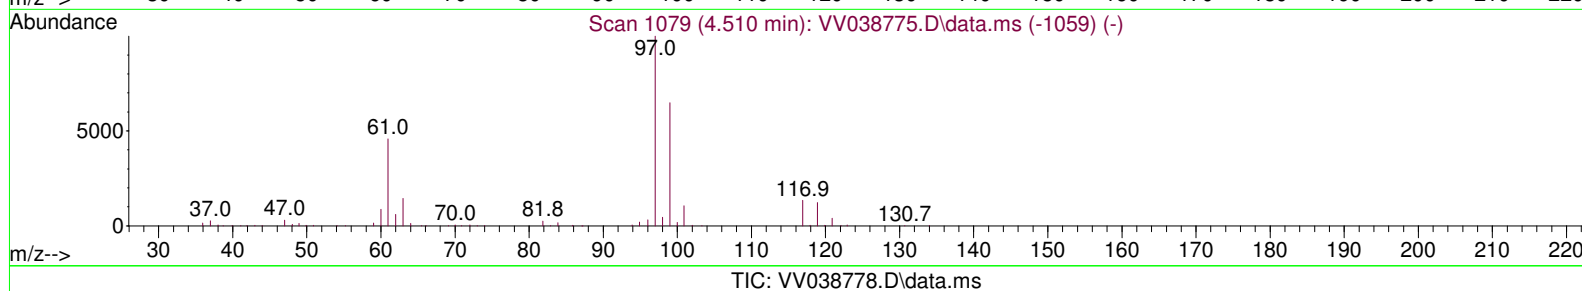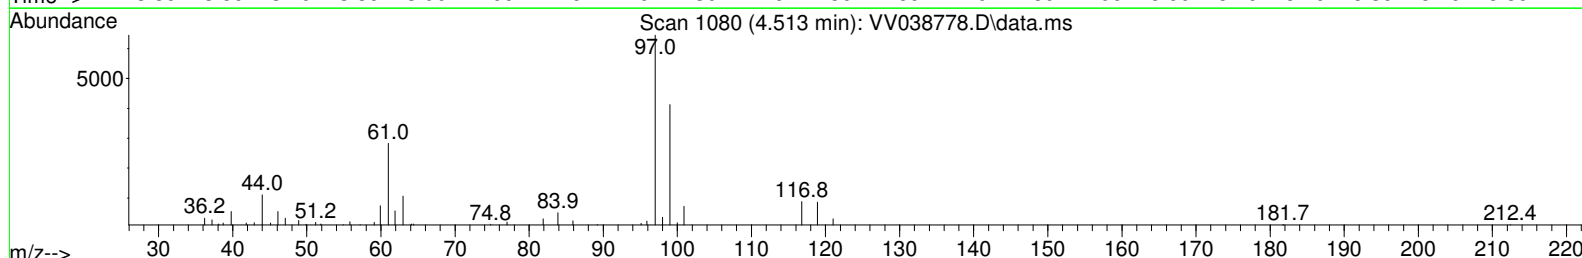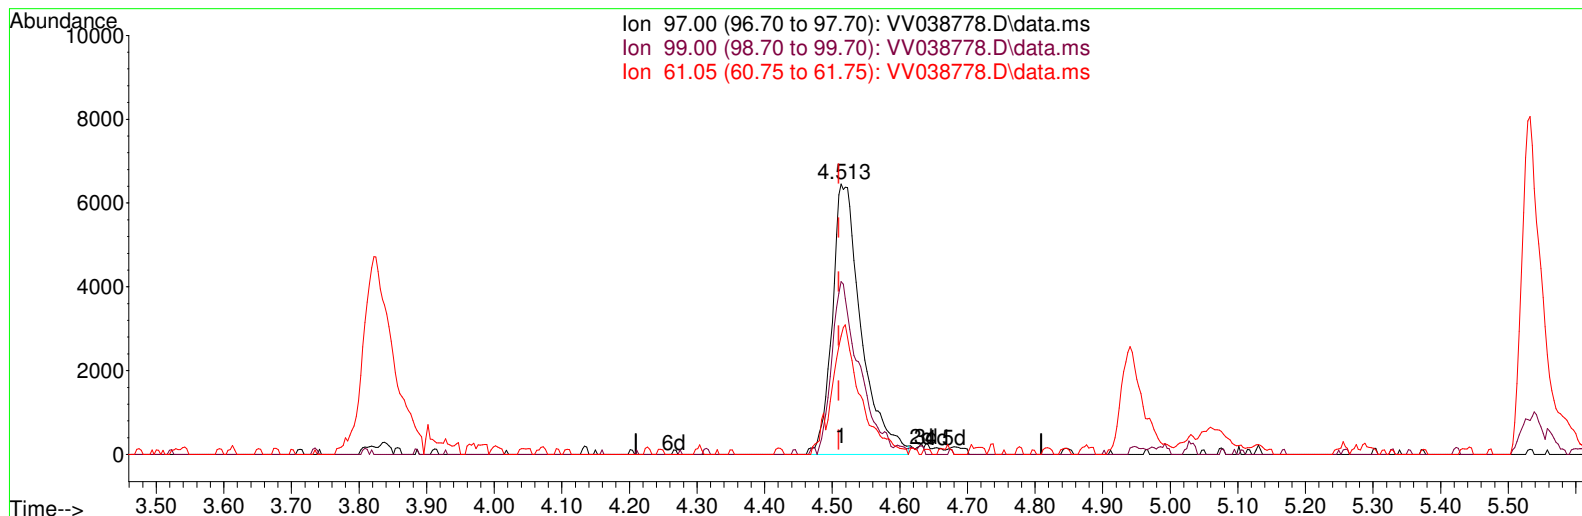

(30) 1,1,1-Trichloroethane (T)

4.513min (+ 0.003) 2.29 ug/L m

response 19243

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	65.40	58.37
61.05	42.00	43.31
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

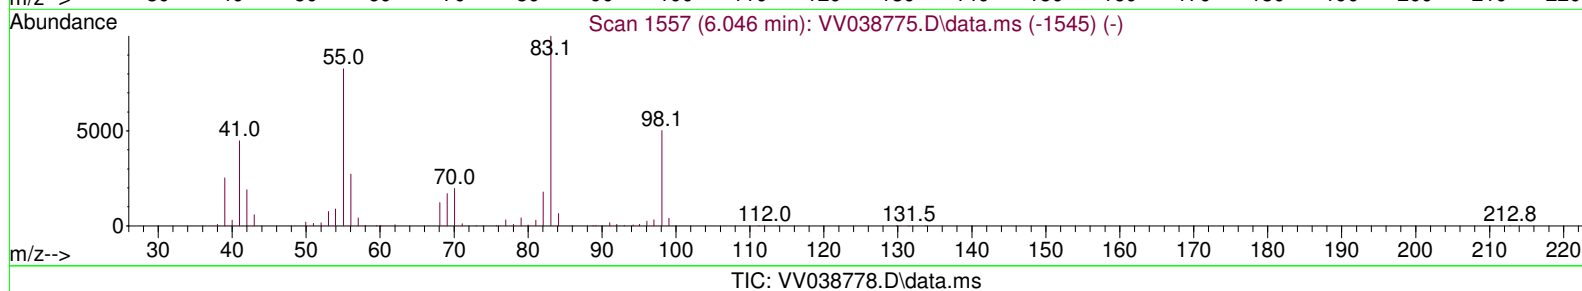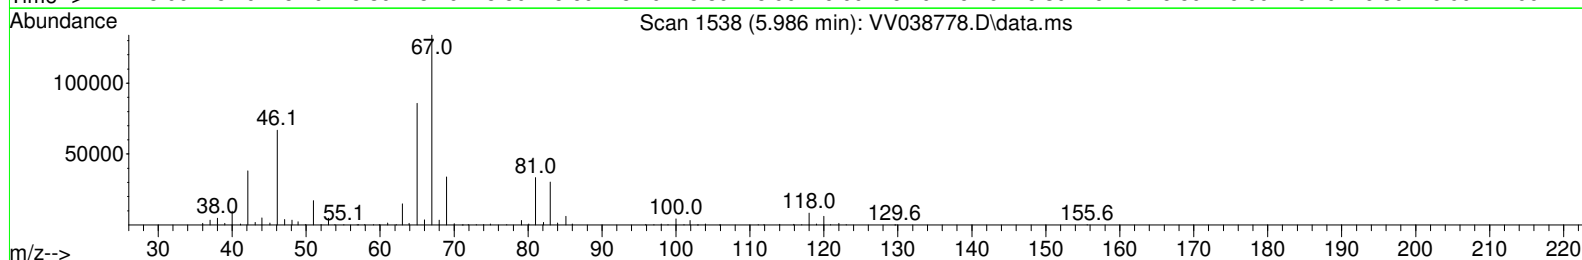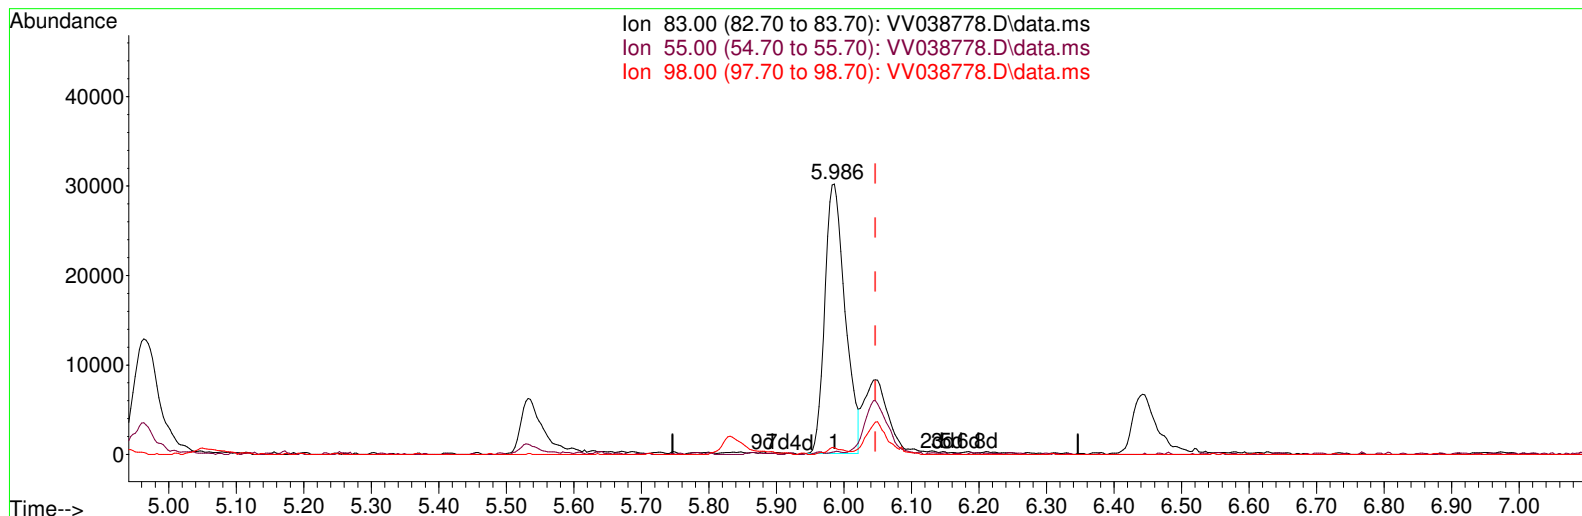

(35) Methylcyclohexane (T)

5.986min (-0.061) 7.52 ug/L

response 62843

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	73.80	0.58#
98.00	49.40	0.87#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

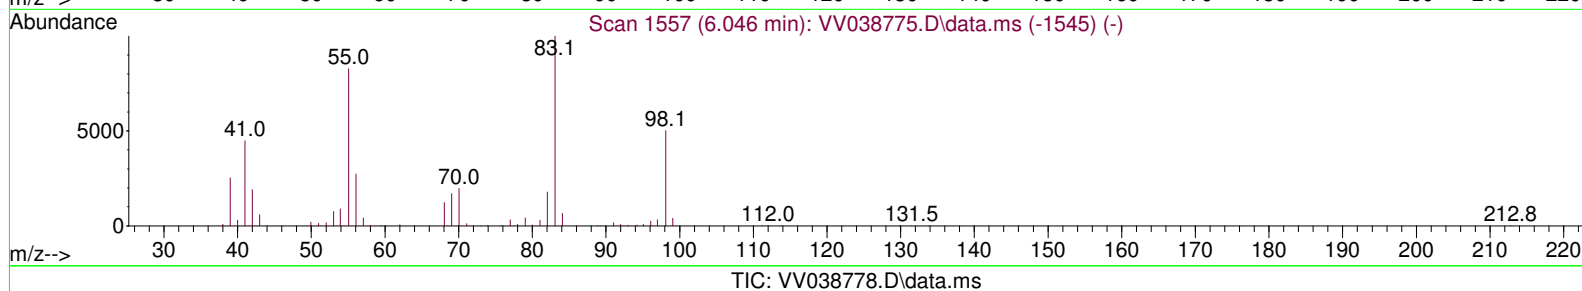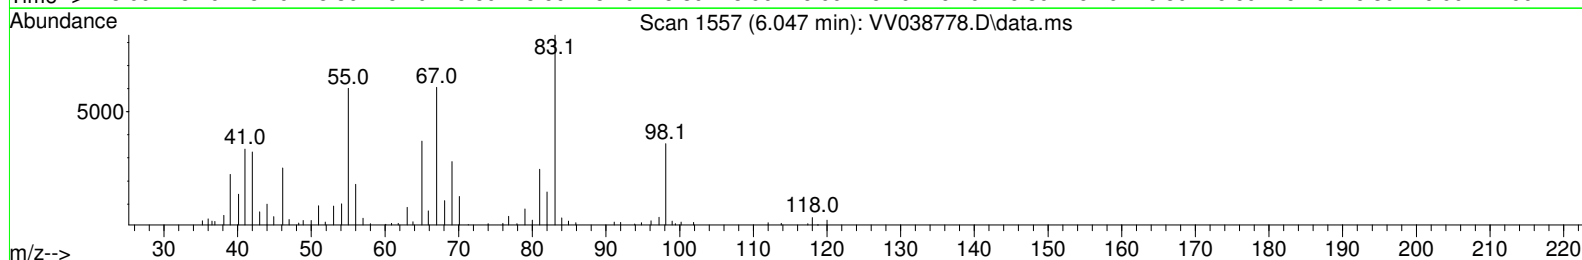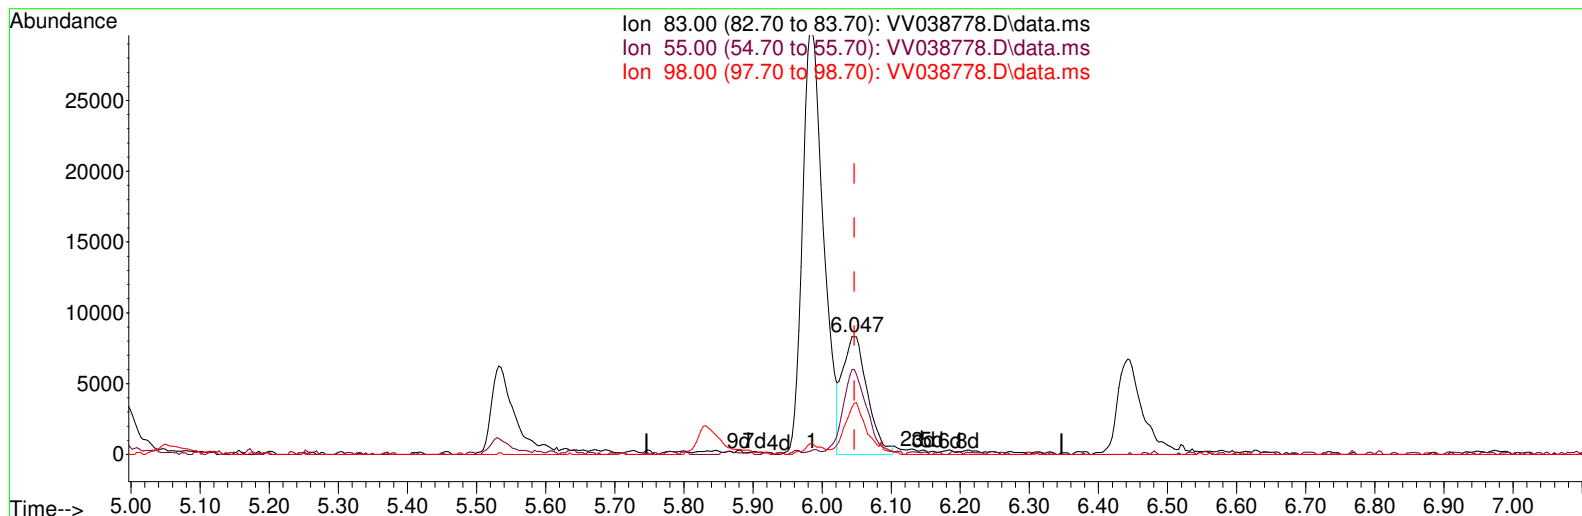

(35) Methylcyclohexane (T)

6.047min (+ 0.000) 2.52 ug/L m

response 21063

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	73.80	1.74#
98.00	49.40	2.61#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

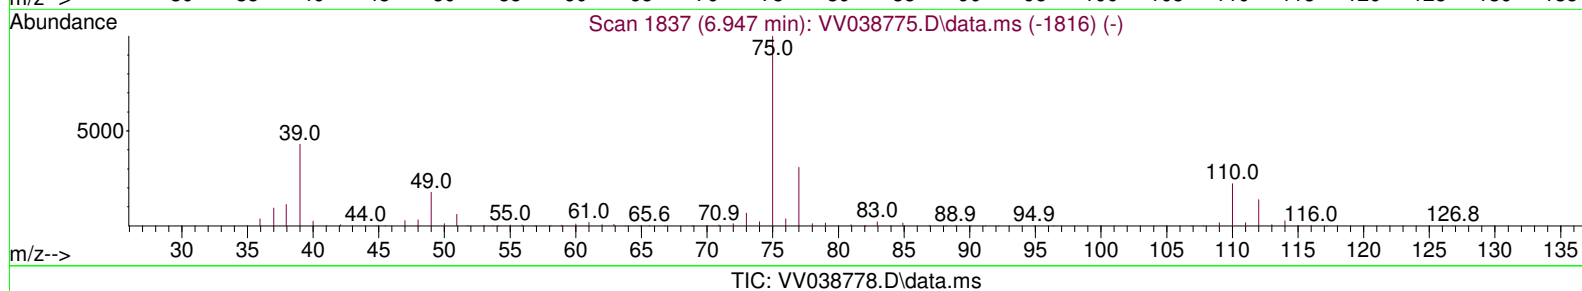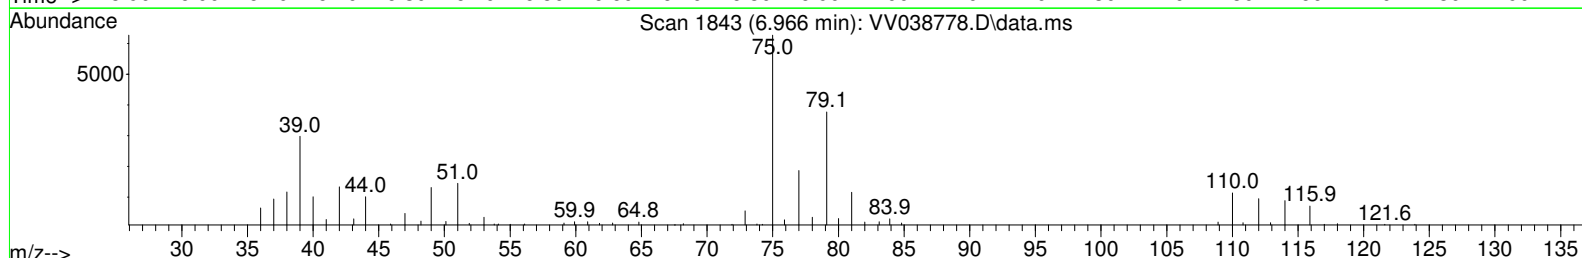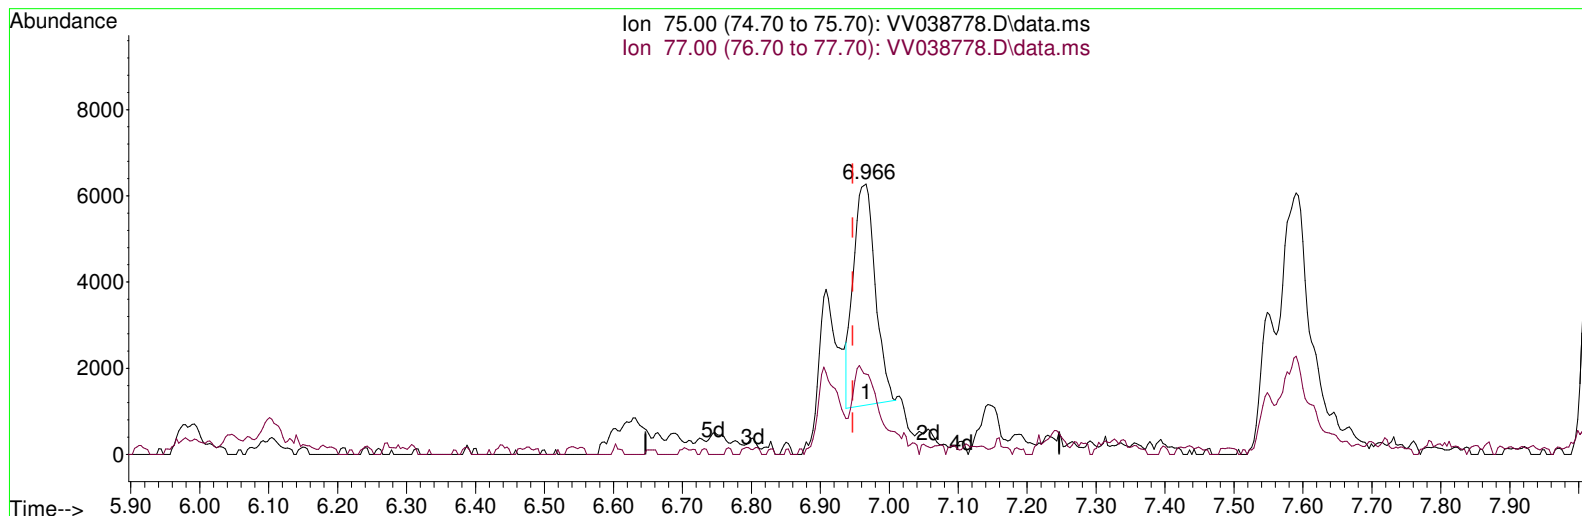

(39) cis-1,3-Dichloropropene (T)

6.966min (+ 0.019) 1.36 ug/L

response 11306

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	31.30	29.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

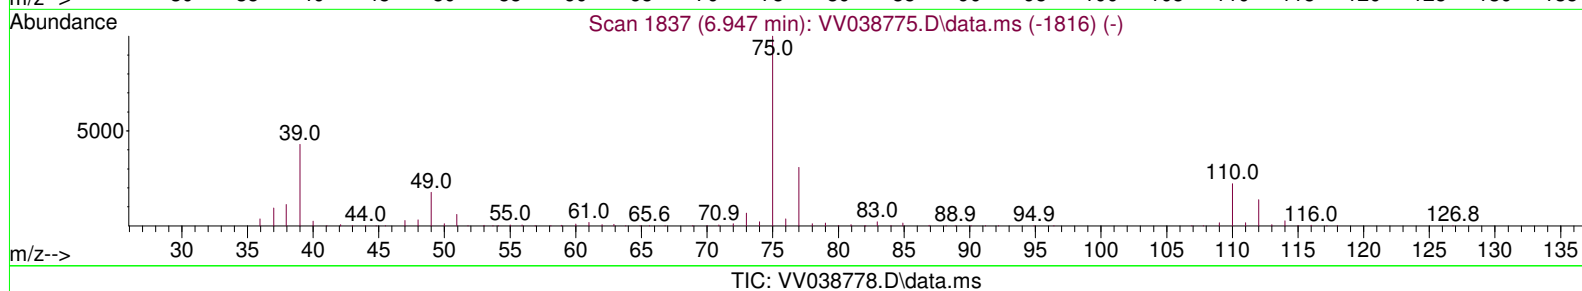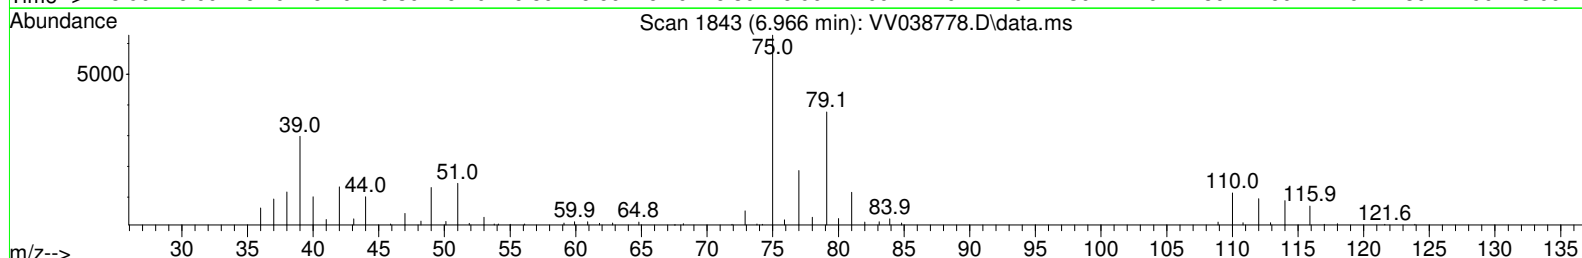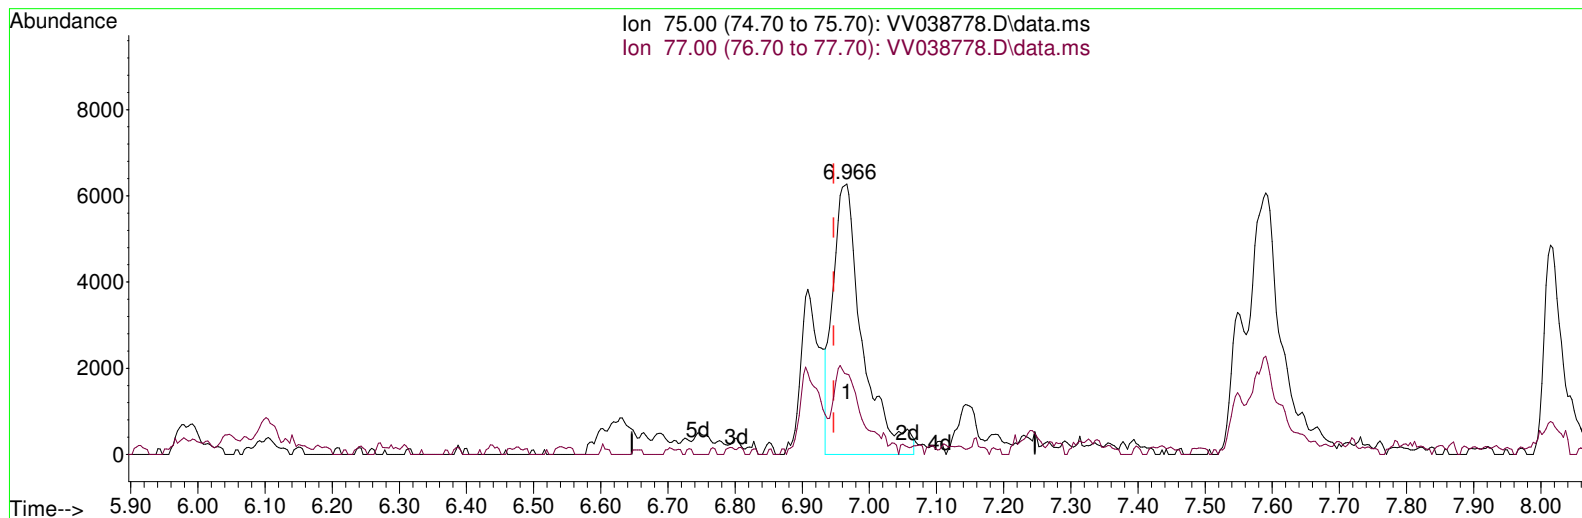

(39) cis-1,3-Dichloropropene (T)

6.966min (+ 0.019) 2.30 ug/L m

response 19136

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	31.30	29.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

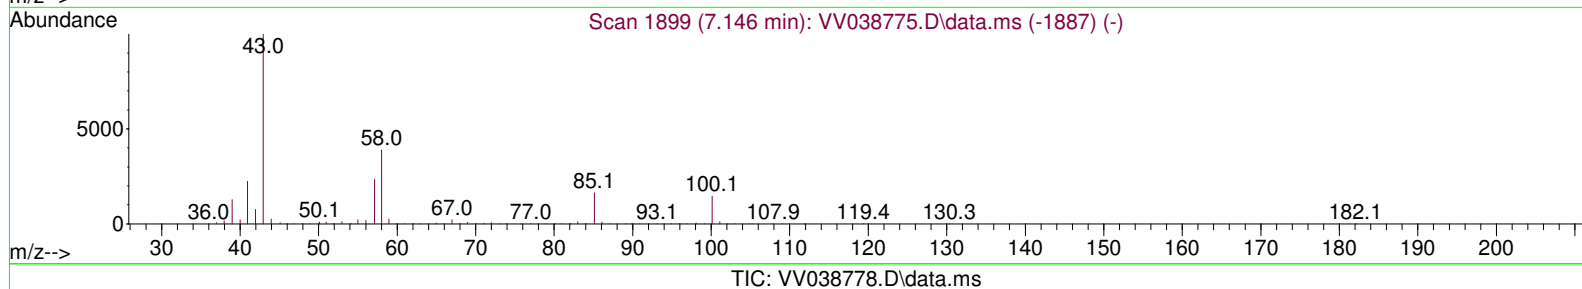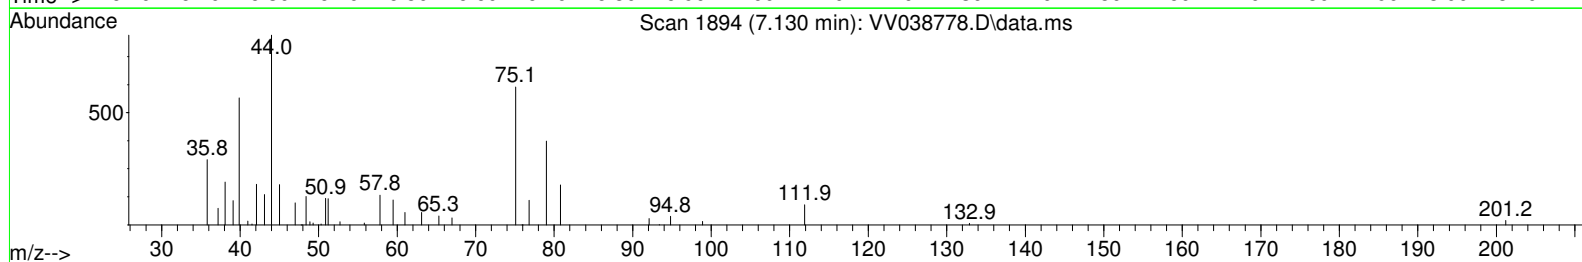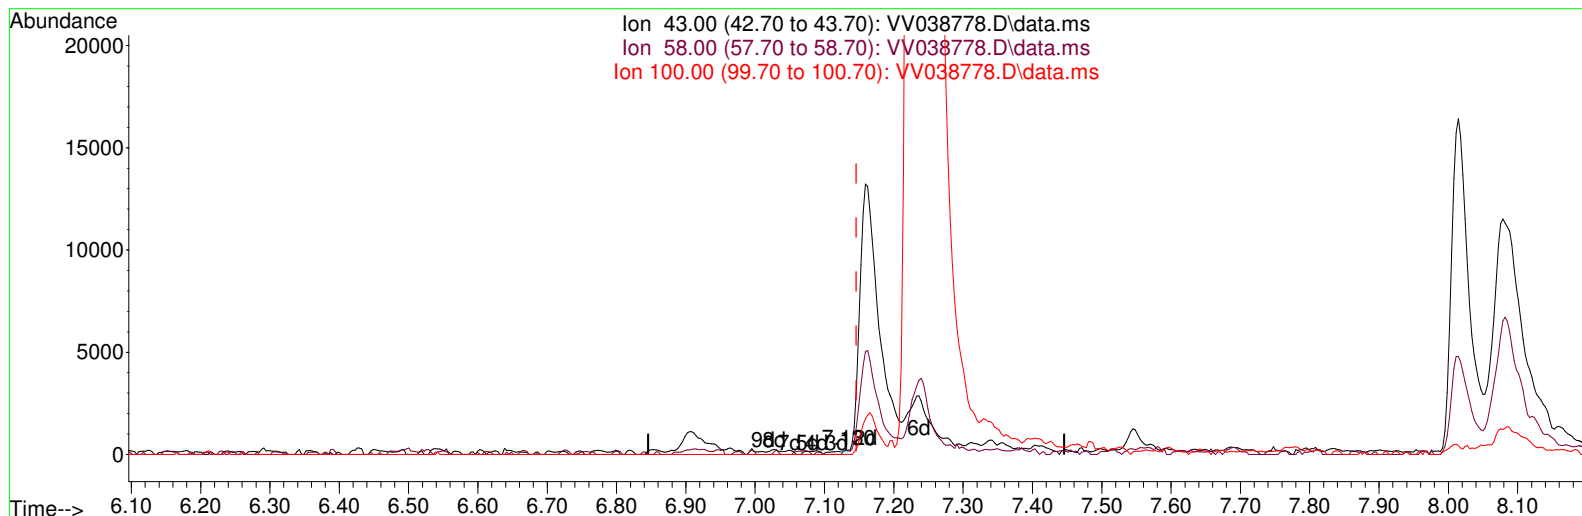

(40) 4-Methyl-2-pentanone (T)

7.130min (-0.016) 0.00 ug/L

response 38

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	40.90	365.79#
100.00	17.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

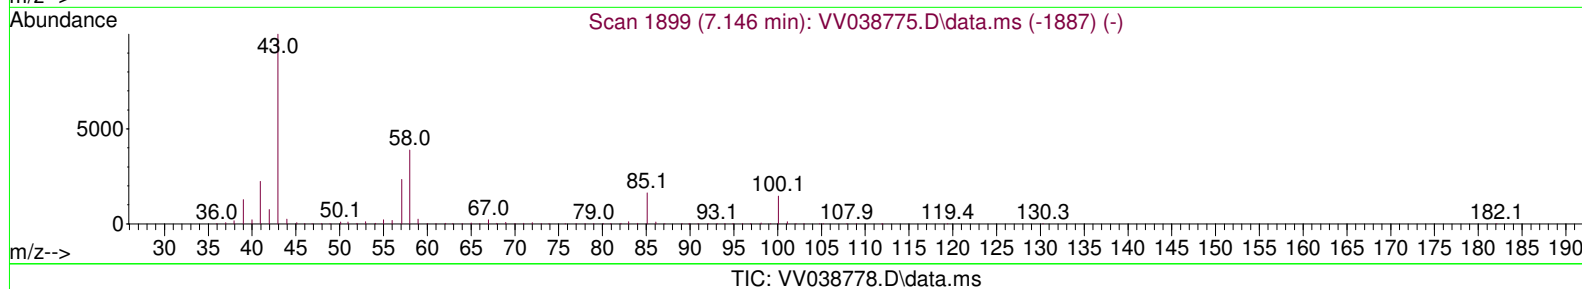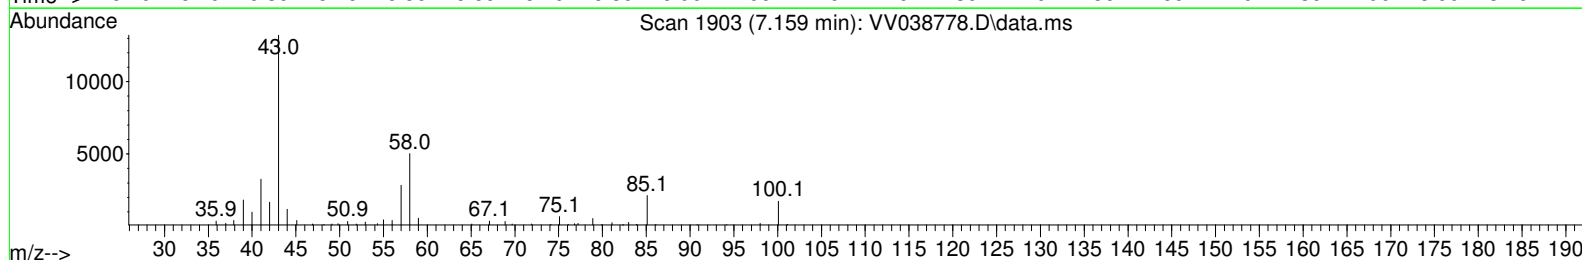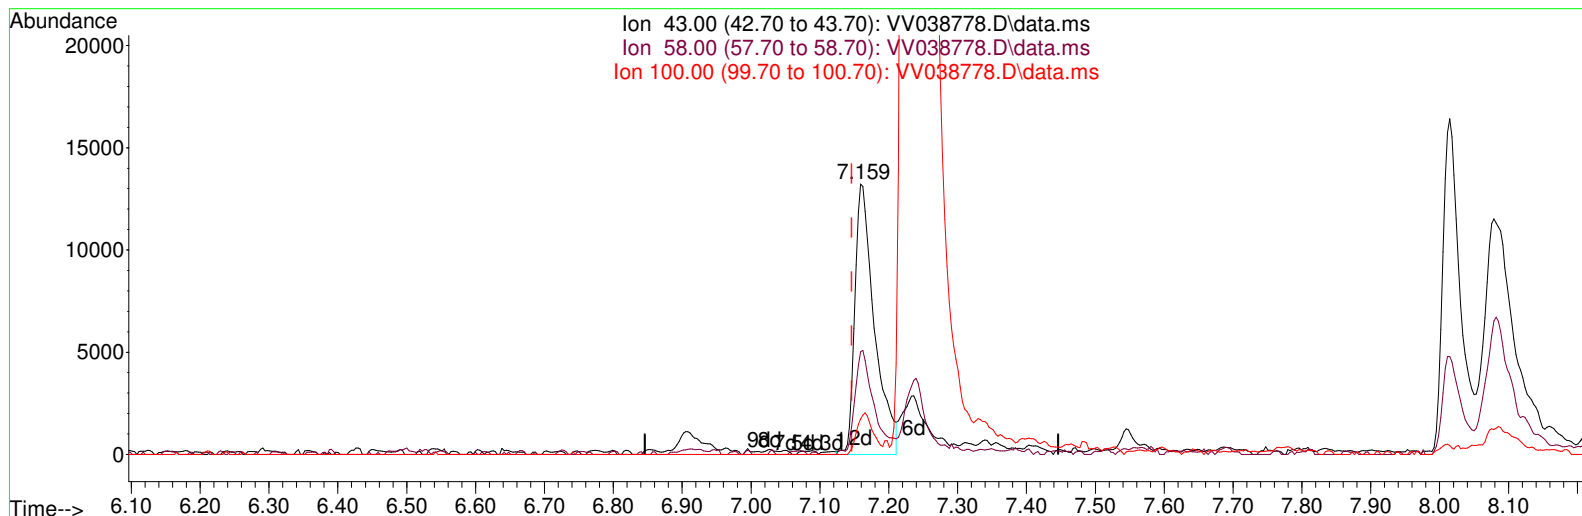

(40) 4-Methyl-2-pentanone (T)

7.159min (+ 0.013) 3.28 ug/L m

response 25988

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	40.90	0.53#
100.00	17.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

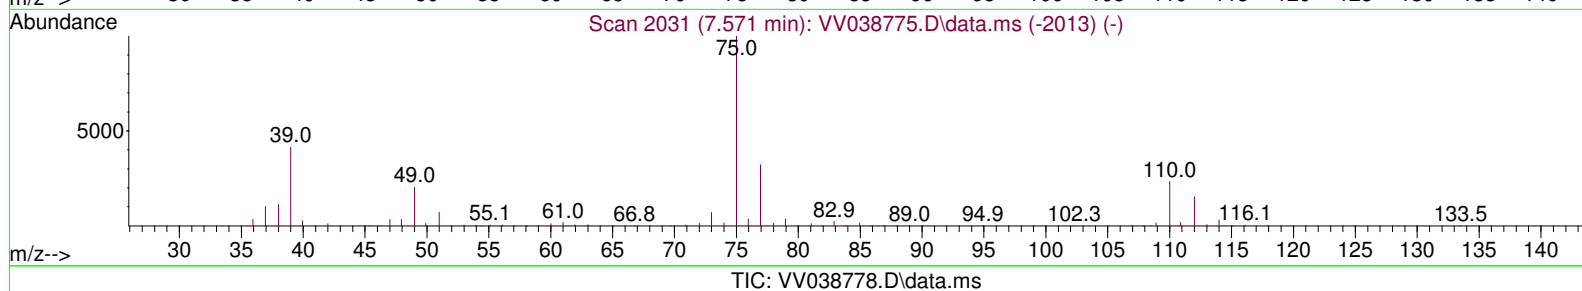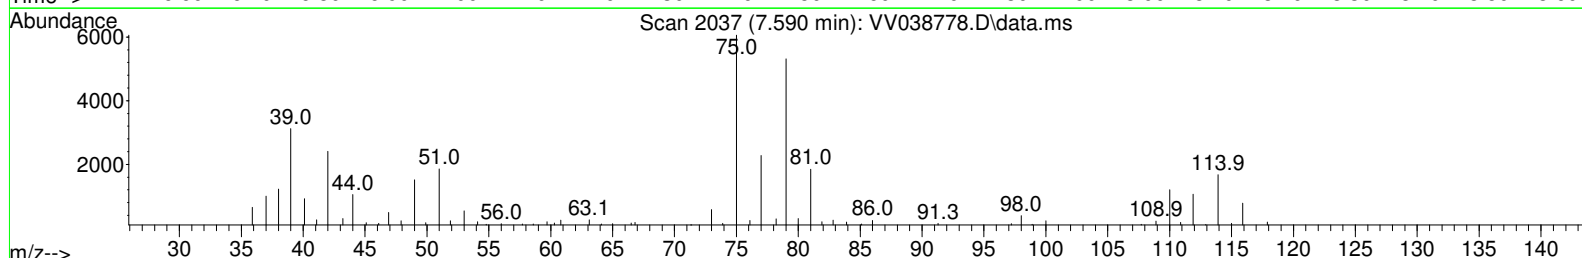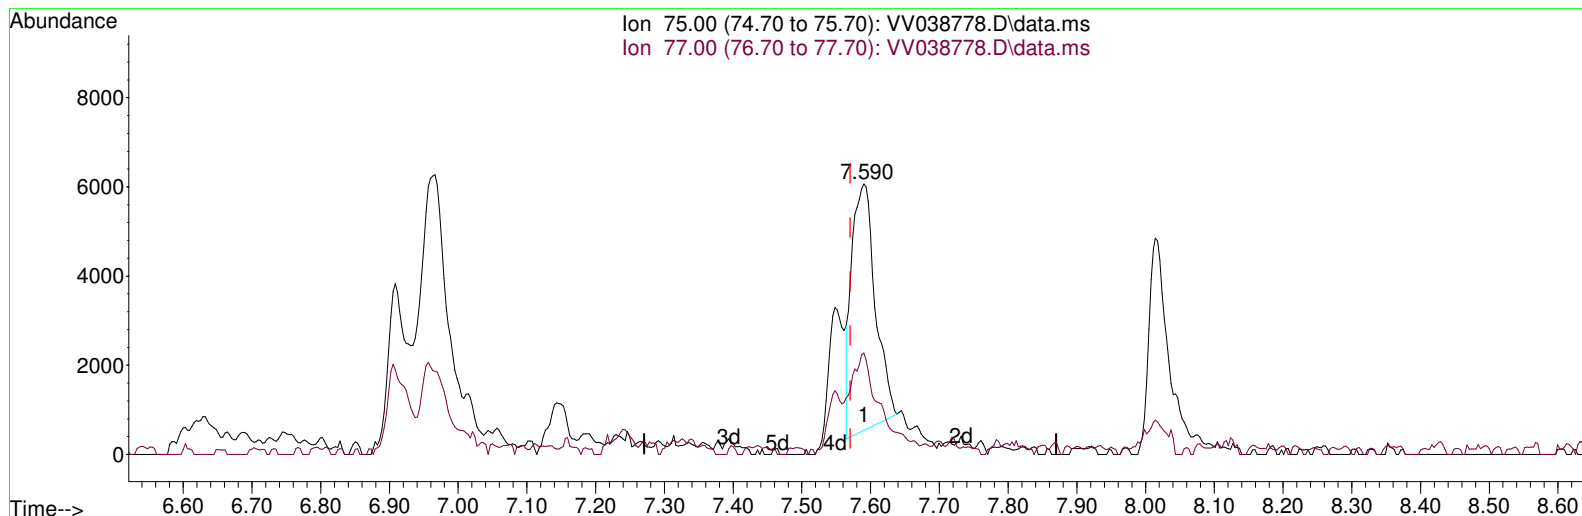

(44) trans-1,3-Dichloropropene (T)

7.590min (+ 0.019) 1.65 ug/L

response 13227

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	32.40	37.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038778.D
Acq On : 10 Jun 2025 13:26
Operator : SY/MD
Sample : Q2117-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/16/2025
Supervised By :Mahesh Dadoda 06/16/2025

Quant Time: Jun 10 14:46:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

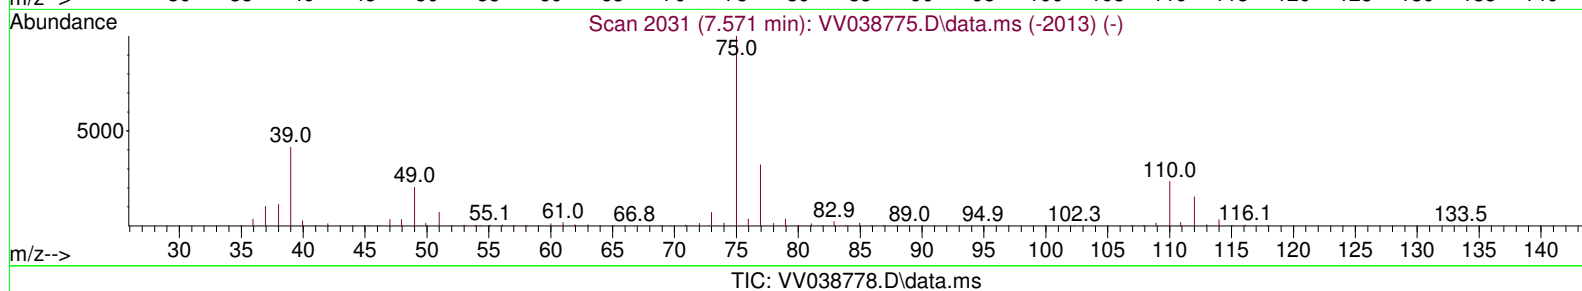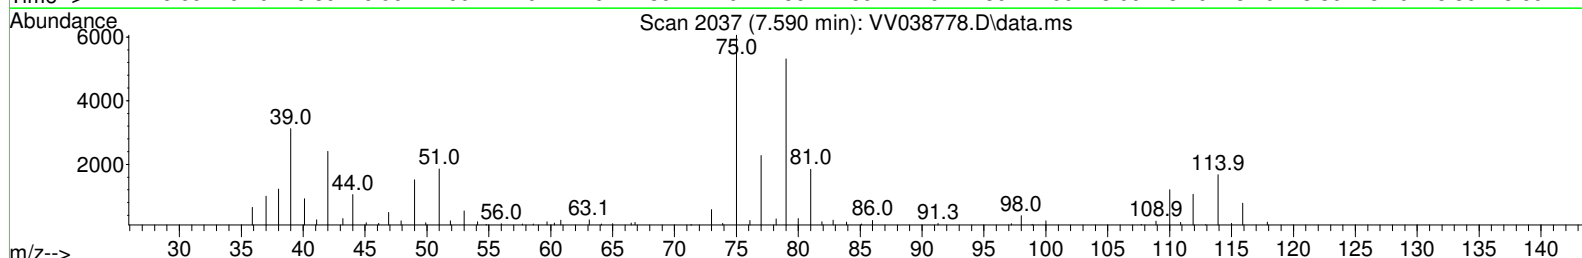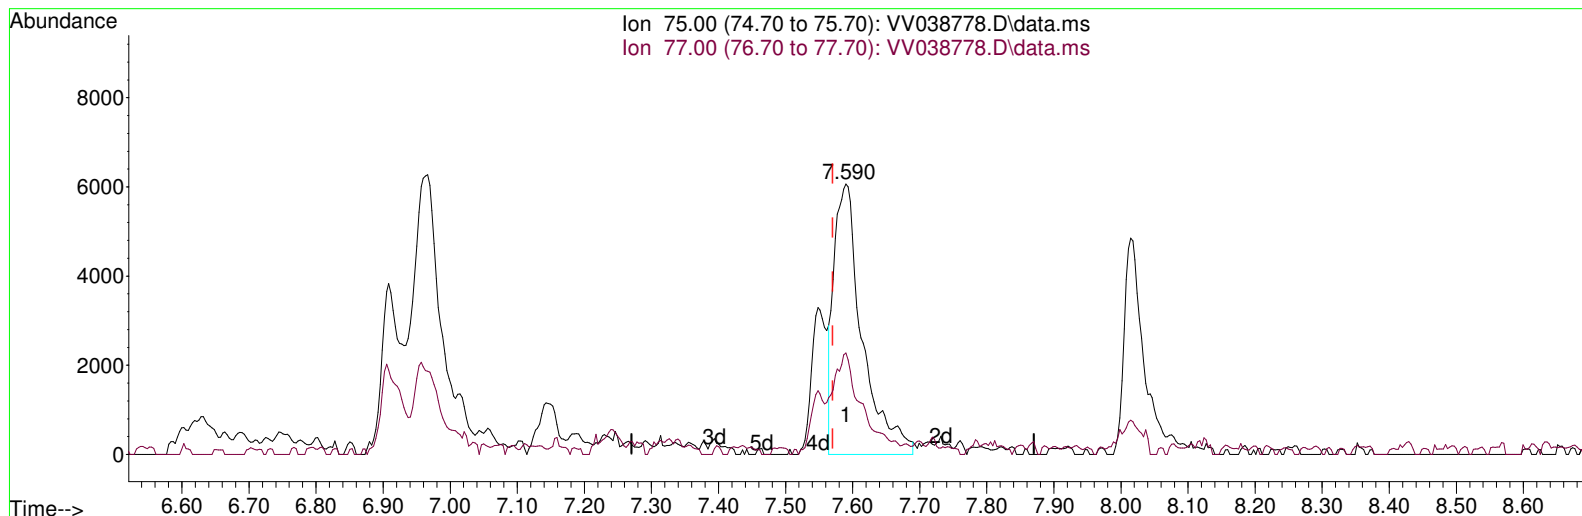

(44) trans-1,3-Dichloropropene (T)

7.590min (+ 0.019) 2.21 ug/L m

response 17763

Ion	Exp%	Act%
75.00	100.00	100.00
77.00	32.40	37.56
0.00	0.00	0.00
0.00	0.00	0.00