
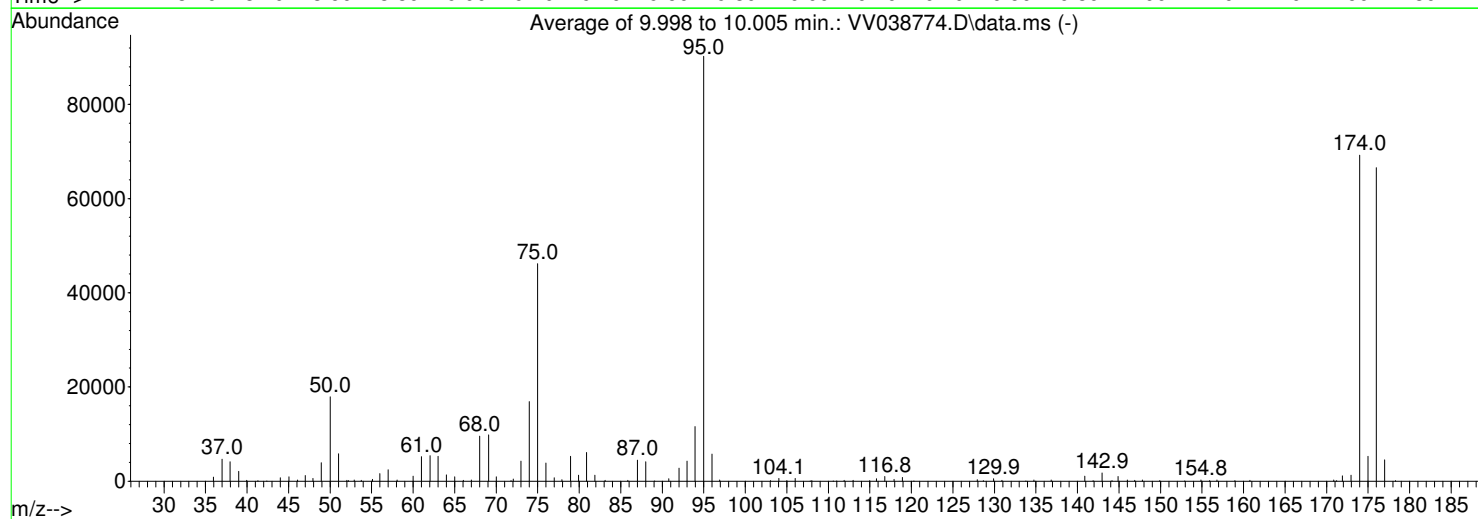


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061025\
Data File : VV038774.D
Acq On : 10 Jun 2025 11:05
Operator : SY/MD
Sample : BFB203
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB203

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Title : VOC Analysis
Last Update : Tue Jun 10 14:44:52 2025

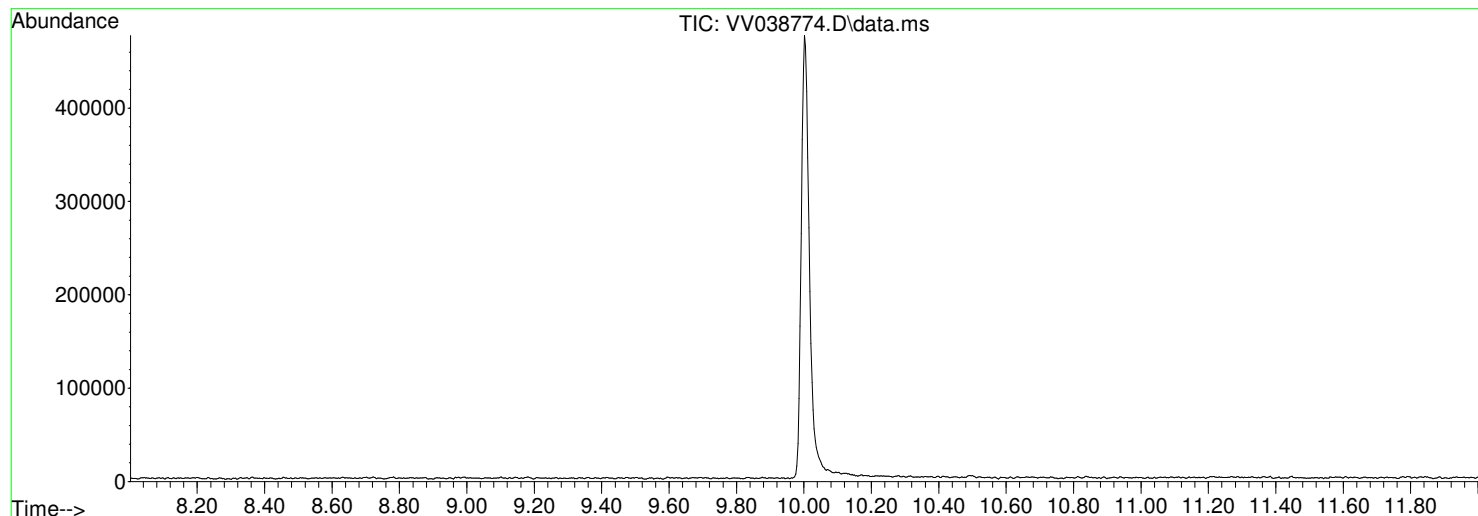

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	17885	PASS
75	95	30	80	51.2	46195	PASS
95	95	100	100	100.0	90223	PASS
96	95	5	9	6.4	5755	PASS
173	174	0.00	2	1.8	1228	PASS
174	95	50	120	76.7	69229	PASS
175	174	5	9	7.6	5286	PASS
176	174	95	105	96.2	66573	PASS
177	176	5	10	6.8	4515	PASS

m/z	Abundance
35.90	173.0
37.80	140.0
39.30	110.0
40.00	345.0
40.90	201.0
41.70	103.0
42.70	111.0
43.20	137.0
44.00	832.0
44.80	108.0
46.10	114.0
48.50	137.0
48.90	132.0
50.00	115.0
57.10	101.0
61.80	119.0
69.30	118.0
73.30	103.0
82.80	101.0
84.70	131.0
85.20	133.0
89.50	106.0
93.90	141.0
95.00	105.0
172.80	102.0
207.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	1074.0
37.00	4574.0
38.00	4325.0
39.00	2030.0
40.00	509.0
41.40	146.0
42.40	109.0
44.00	1665.0
45.10	924.0
46.10	320.0
47.00	1156.0
48.00	515.0
49.00	3839.0
50.00	17632.0
51.00	5582.0
52.00	284.0
52.80	253.0
53.80	120.0
55.10	304.0
56.00	1504.0
57.00	2288.0
58.10	198.0
60.00	1033.0
61.00	5057.0
62.10	5190.0
63.00	5099.0
64.00	1294.0
65.00	797.0
66.00	134.0
67.00	295.0
68.00	9307.0
69.10	9633.0
70.00	835.0
72.10	524.0
73.00	4207.0
74.00	16318.0
75.00	44400.0
76.00	4107.0
76.90	773.0
77.90	261.0
78.90	5152.0
79.90	1156.0
80.90	5496.0
81.90	1200.0
83.20	150.0
85.80	147.0
87.00	4252.0
88.00	3919.0
89.10	111.0
90.80	574.0
92.00	2573.0
93.00	4050.0
94.00	11709.0
95.00	86456.0
96.00	5788.0
96.90	259.0
103.00	158.0
104.00	588.0
106.00	473.0
107.80	165.0
111.00	115.0
111.90	130.0
113.00	219.0
115.00	208.0
115.80	510.0
116.80	866.0
117.90	425.0
118.90	689.0
128.00	333.0
129.90	423.0
130.90	181.0
134.80	223.0
137.00	163.0
140.90	1136.0
142.00	113.0
143.00	1694.0
144.10	161.0
144.90	876.0
146.00	213.0
146.90	150.0
147.80	177.0
149.90	104.0
152.90	127.0
154.90	300.0
156.80	207.0
160.70	145.0
170.90	222.0
171.90	1120.0
173.00	1357.0
174.00	64176.0
175.00	5190.0
176.00	62504.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

177.00

4478.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	1037.0
37.00	4668.0
38.00	4344.0
39.00	2131.0
39.90	549.0
41.30	131.0
44.00	1537.0
45.10	985.0
46.10	334.0
47.00	1234.0
47.90	564.0
49.00	4218.0
50.00	18648.0
51.00	5936.0
52.20	298.0
52.90	253.0
53.70	153.0
55.10	372.0
56.00	1578.0
57.00	2579.0
58.00	240.0
60.00	1074.0
61.00	5448.0
62.10	5518.0
63.00	5494.0
64.00	1390.0
65.00	951.0
66.00	136.0
67.00	260.0
68.00	9788.0
69.10	10340.0
70.00	946.0
71.90	443.0
72.10	459.0
73.00	4377.0
74.00	17528.0
75.00	47568.0
76.00	3842.0
77.00	699.0
77.90	285.0
79.00	5452.0
79.90	1314.0
80.90	6374.0
81.90	1327.0
83.10	208.0
85.80	192.0
87.00	4752.0
88.00	4193.0
90.80	545.0
92.00	2808.0
93.00	4434.0
94.00	12093.0
95.00	93920.0
96.00	5905.0
96.90	276.0
103.10	106.0
104.00	580.0
105.00	112.0
106.00	602.0
108.00	172.0
111.90	171.0
113.00	222.0
115.00	126.0
115.80	504.0
116.80	1022.0
117.90	391.0
118.90	805.0
128.00	337.0
128.70	129.0
129.90	558.0
130.90	180.0
133.80	103.0
134.80	210.0
136.80	245.0
140.90	1044.0
141.90	132.0
143.00	1788.0
144.20	127.0
144.90	1039.0
146.00	236.0
146.90	204.0
147.80	247.0
149.90	114.0
154.90	253.0
155.90	107.0
156.80	266.0
159.00	114.0
160.80	161.0
170.80	211.0
171.90	1198.0
173.00	1404.0
174.00	71472.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

175.00	5497.0
176.00	68784.0
177.00	4683.0
178.30	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	908.0
37.00	4687.0
38.00	4165.0
39.00	2053.0
39.90	527.0
41.20	118.0
41.90	104.0
43.00	122.0
44.00	1353.0
45.00	954.0
46.20	347.0
47.00	1180.0
47.90	629.0
49.00	4074.0
50.00	17720.0
51.00	5915.0
52.00	273.0
53.00	274.0
53.80	191.0
55.10	375.0
56.00	1630.0
57.00	2721.0
58.00	238.0
60.00	1036.0
61.00	5200.0
62.00	5420.0
63.00	5146.0
64.00	1317.0
65.00	1018.0
66.10	157.0
67.00	227.0
68.00	9568.0
69.10	9756.0
70.00	1006.0
71.80	387.0
73.00	4195.0
74.00	16912.0
75.00	46616.0
76.00	3534.0
77.10	634.0
77.90	288.0
78.90	5263.0
79.90	1415.0
80.90	6443.0
81.90	1254.0
83.00	232.0
85.90	220.0
87.00	4414.0
88.00	4183.0
90.80	463.0
92.00	2855.0
93.00	4247.0
94.00	11386.0
95.00	90608.0
96.00	5573.0
96.90	234.0
104.10	498.0
105.00	155.0
106.00	582.0
108.00	196.0
110.60	146.0
111.90	173.0
113.00	180.0
115.80	491.0
116.80	1008.0
117.90	275.0
118.90	800.0
120.30	101.0
127.90	341.0
128.60	144.0
129.90	620.0
130.90	156.0
134.70	225.0
136.80	283.0
140.90	966.0
141.80	121.0
142.90	1741.0
144.90	1056.0
146.00	209.0
146.90	192.0
147.80	259.0
149.90	114.0
154.80	266.0
155.90	138.0
156.80	269.0
158.90	135.0
160.80	134.0
170.80	258.0
171.20	240.0
171.90	1143.0
173.00	1228.0
174.00	72040.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

175.00	5170.0
176.00	68432.0
177.00	4384.0
178.30	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203