

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016858.D
 Acq On : 12 Jun 2020 03:56
 Operator : SY/MD
 Sample : L2915-17 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 12 06:01:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 12 05:55:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	357612	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	334990	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	161922	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	107302	42.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.04%
7) Chloroethane-d5	1.56	69	60026	39.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.28%
11) 1,1-Dichloroethene-d2	2.12	63	140772	33.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.44%
21) 2-Butanone-d5	3.90	46	163908	87.76	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.76%
24) Chloroform-d	4.37	84	219544	42.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.58%
26) 1,2-Dichloroethane-d4	5.05	65	160439	45.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.94%
32) Benzene-d6	5.07	84	430790	44.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.22%
36) 1,2-Dichloropropane-d6	6.09	67	131124	43.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.12%
41) Toluene-d8	7.34	98	390172	44.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.06%
43) trans-1,3-Dichloropropene-	7.64	79	63313	40.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.78%
47) 2-Hexanone-d5	8.11	63	98624	75.15	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.15%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	166908	41.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.78%
64) 1,2-Dichlorobenzene-d4	11.65	152	158801	45.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.92%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
10) 1,1,2-Trichloro-1,2,2-trif	2.12	101	1267	0.666	ug/L #	19
12) 1,1-Dichloroethene	2.12	96	1550	0.873	ug/L #	1
27) 1,2-Dichloroethane	5.12	62	14288	3.641	ug/L #	74
33) Benzene	5.12	78	1330884	134.278	ug/L	100
42) Toluene	7.41	91	78267	7.491	ug/L	99
48) 2-Hexanone	8.17	43	11149	3.937	ug/L #	66
52) Ethylbenzene	9.04	91	97346	8.411	ug/L	100
53) m,p-Xylene	9.16	106	2844	0.660	ug/L	92
54) o-xylene	9.57	106	6805	1.601	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061120\
Data File : VV016858.D
Acq On : 12 Jun 2020 03:56
Operator : SY/MD
Sample : L2915-17 250X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 12 06:01:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 12 05:55:11 2020
Response via : Initial Calibration

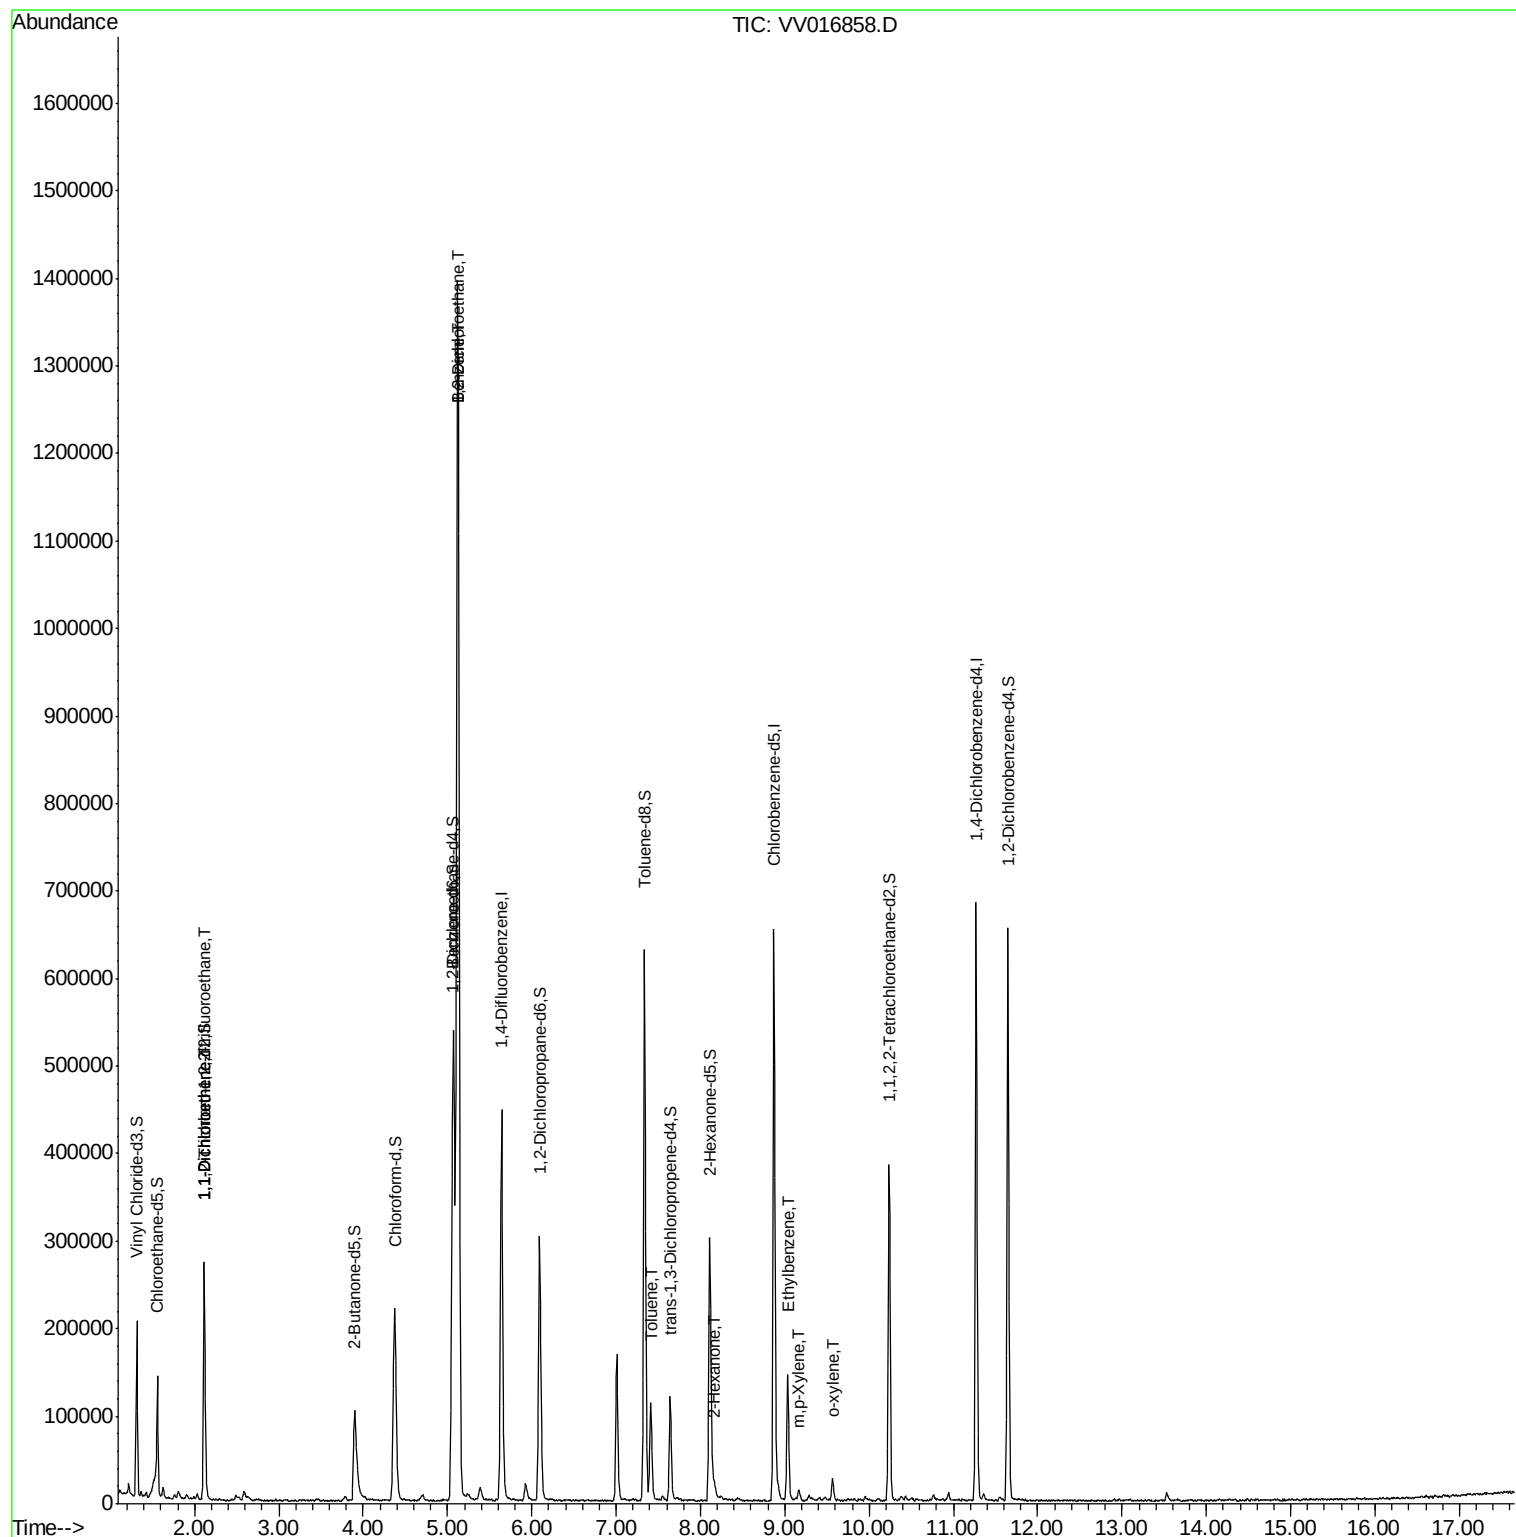

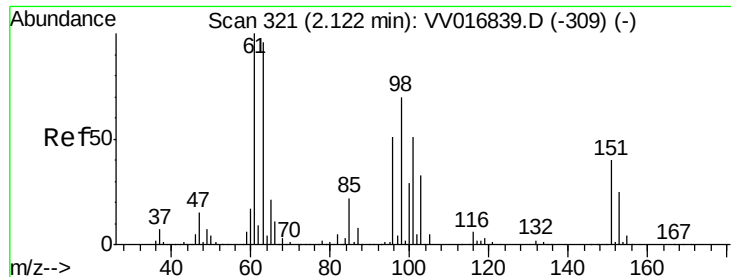

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.666 ug/L

RT: 2.12 min Scan# 319

Delta R.T. -0.01 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56

Instrument :

MSVOA_V

ClientSampleId :


Tot Ion:101 Resp: 1267

Ion Ratio Lower Upper

101 100

85 3.2 35.5 53.3#

151 0.0 63.9 95.9#

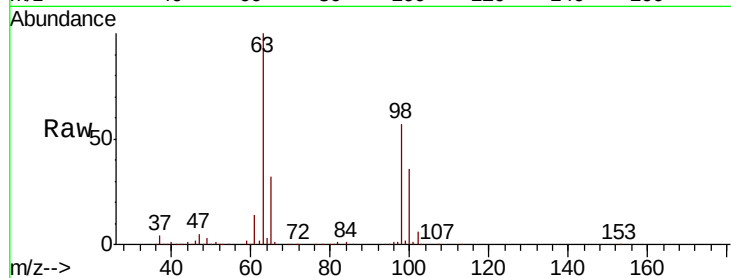



Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VV0

Ion 151.00 (150.70 to 151.70): V

2.12

Time-->

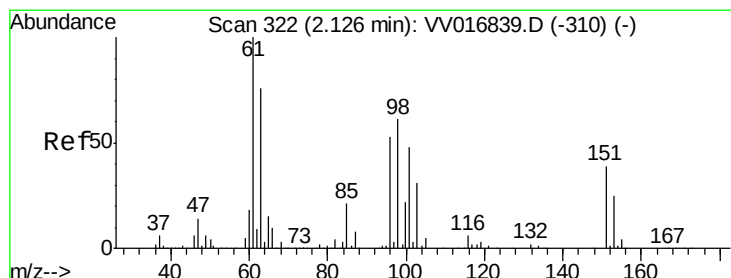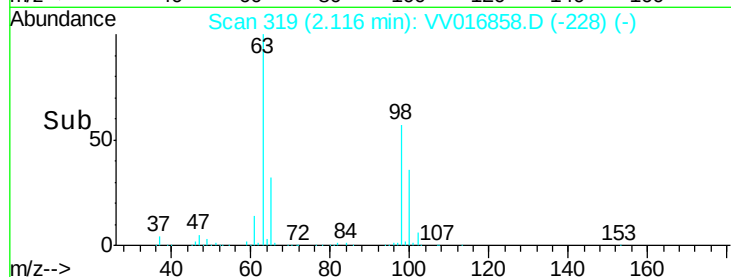

#12

1,1-Dichloroethene

Concen: 0.873 ug/L

RT: 2.12 min Scan# 319

Delta R.T. -0.01 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56


Tgt Ion: 96 Resp: 1550

Ion Ratio Lower Upper

96 100

61 1317.3 130.4 242.2#

63 9557.3 103.3 191.9#

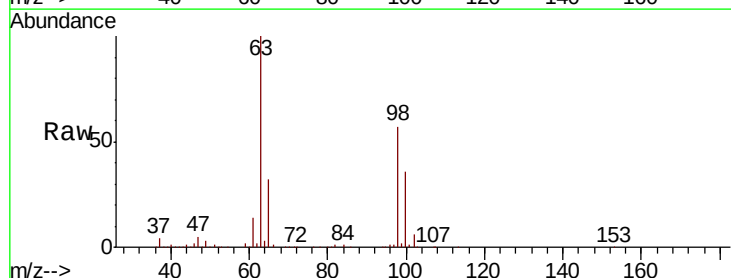


Abundance Ion 96.00 (95.70 to 96.70): VV0


Ion 61.00 (60.70 to 61.70): VV0

Ion 63.00 (62.70 to 63.70): VV0

2.12

Time-->

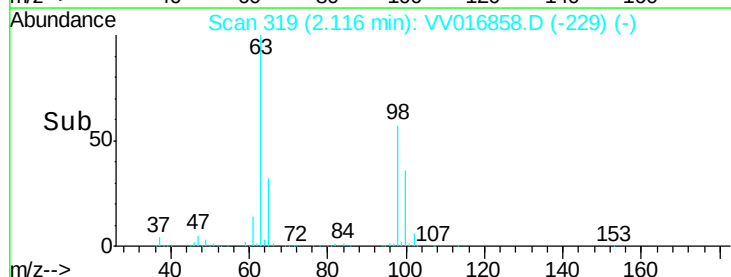

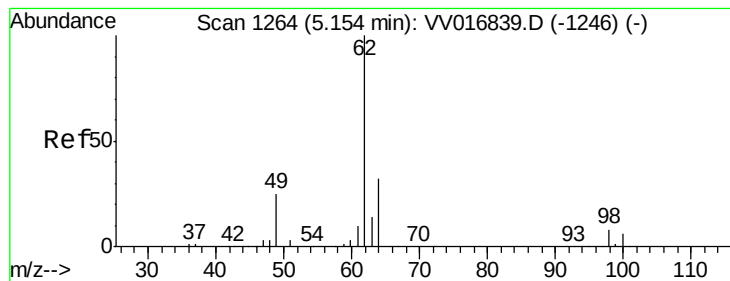

#27

1,2-Dichloroethane

Concen: 3.641 ug/L

RT: 5.12 min Scan# 1254

Delta R.T. -0.03 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56

Instrument :

MSVOA_V


ClientSampleId :

Tot Ion: 62 Resp: 14288

Ion Ratio Lower Upper




62 100

98 0.0 7.4 11.2#

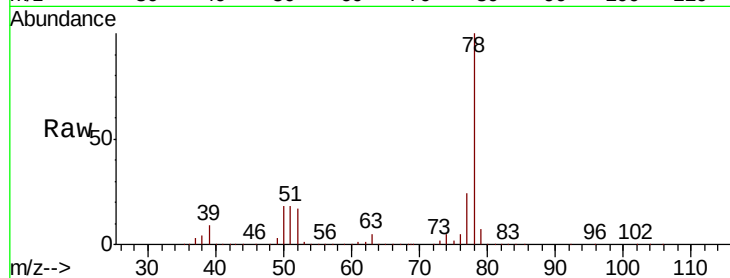

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 98.00 (97.70 to 98.70): VV0

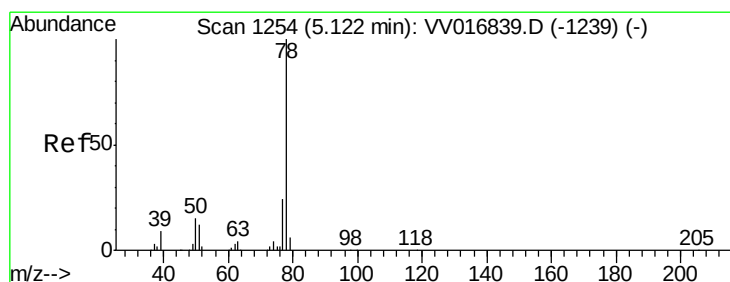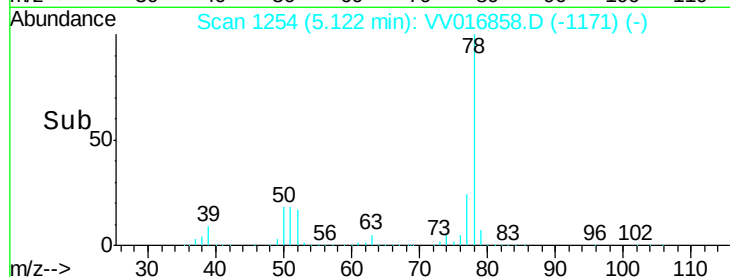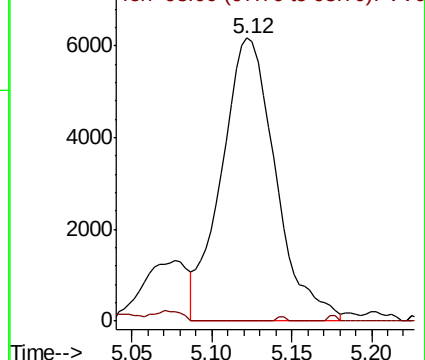

#33

Benzene

Concen: 134.278 ug/L


RT: 5.12 min Scan# 1254

Delta R.T. 0.00 min



Lab File: VV016858.D


Acq: 12 Jun 2020 03:56

Tgt Ion: 78 Resp: 1330884

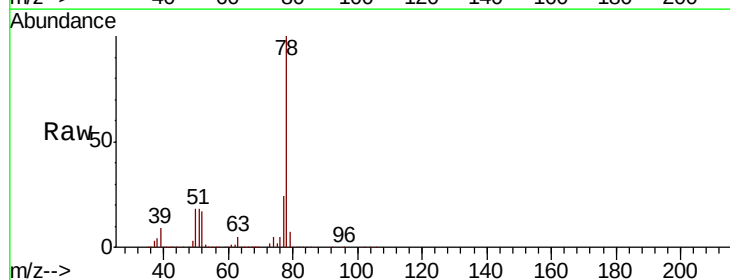

Abundance Ion 78.00 (77.70 to 78.70): VV0

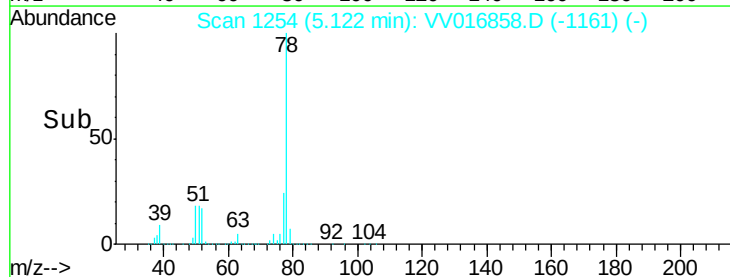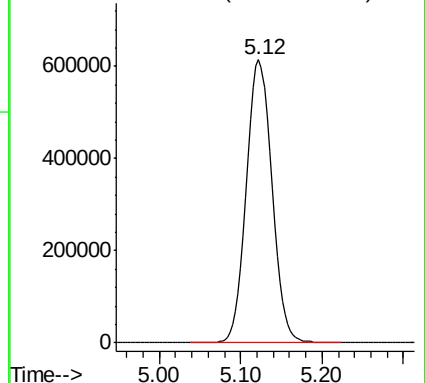

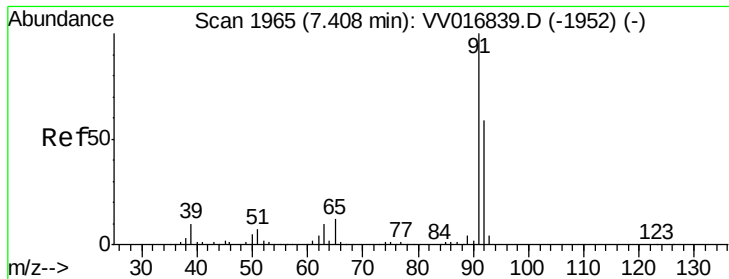

#42

Toluene

Concen: 7.491 ug/L

RT: 7.41 min Scan# 1966

Delta R.T. 0.00 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56


Instrument :
MSVOA_V
ClientSampleId :

Tot Ion: 91 Resp: 78267

Ion Ratio Lower Upper

91 100

92 56.8 40.4 75.0

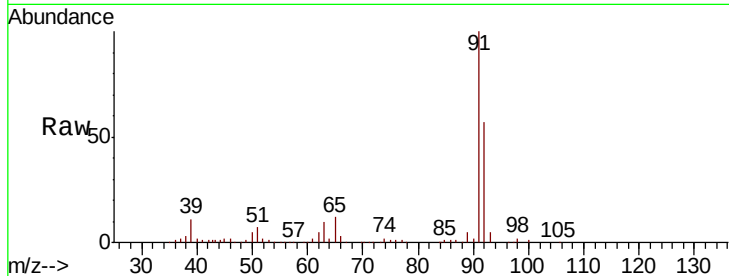

Abundance Ion 91.00 (90.70 to 91.70): VV0

Ion 92.00 (91.70 to 92.70): VV0

7.41

50000

40000

30000



20000

10000

0

Time-->

7.35 7.40 7.45 7.50

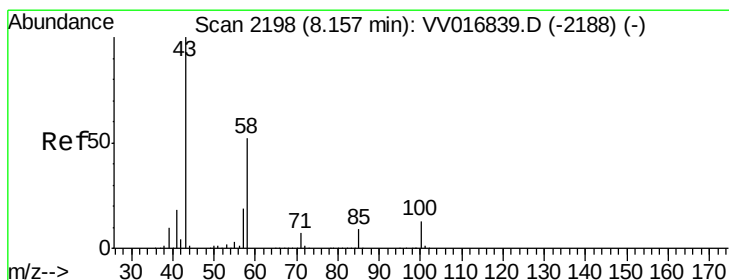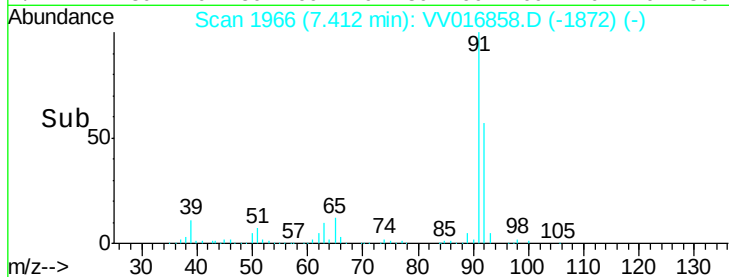

#48

2-Hexanone

Concen: 3.937 ug/L

RT: 8.17 min Scan# 2201

Delta R.T. 0.01 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56

Tgt Ion: 43 Resp: 11149


Ion Ratio Lower Upper

43 100

58 28.5 43.1 64.7#

57 3.7 15.3 22.9#

100 2.0 10.0 15.0#

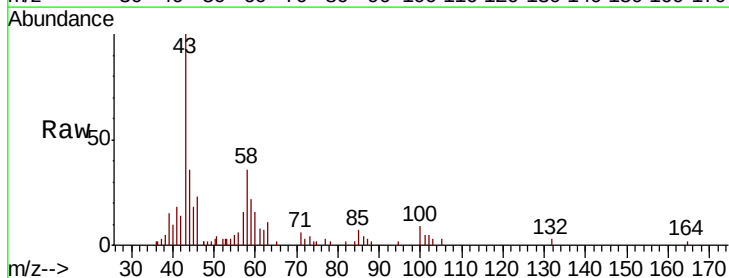

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

Ion 57.00 (56.70 to 57.70): VV0

Ion 100.00 (99.70 to 100.70): VV0

10000

8000

6000


4000


2000

0

Time-->

8.10 8.15 8.20 8.25

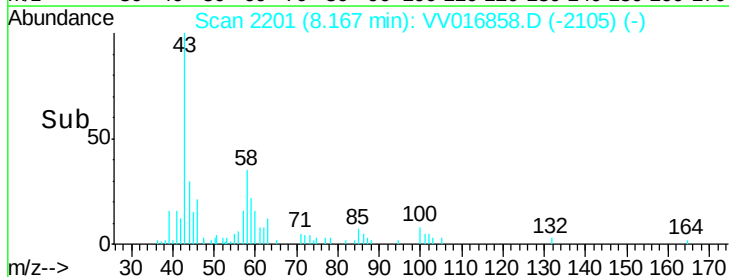

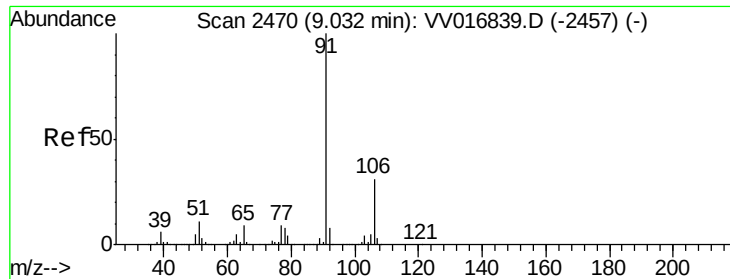

#52

Ethylbenzene

Concen: 8.411 ug/L

RT: 9.04 min Scan# 2471

Delta R.T. 0.00 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56

Instrument :

MSVOA_V





ClientSampleId :

Tot Ion: 91 Resp: 97346

Ion Ratio Lower Upper

91 100

106 30.0 21.1 39.1

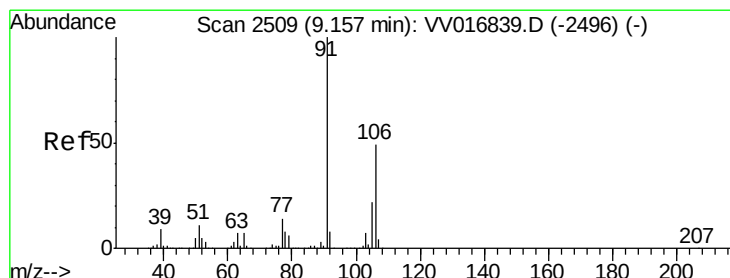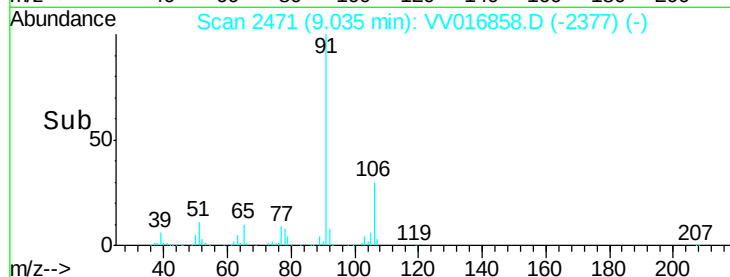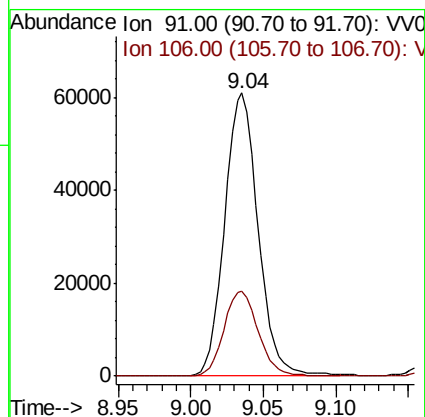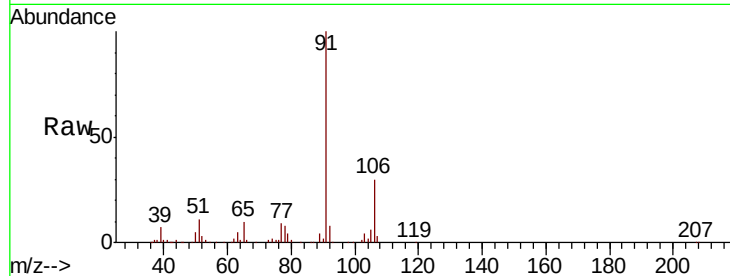

#53

m,p-Xylene

Concen: 0.660 ug/L

RT: 9.16 min Scan# 2511

Delta R.T. 0.01 min

Lab File: VV016858.D




Acq: 12 Jun 2020 03:56


Tgt Ion: 106 Resp: 2844

Ion Ratio Lower Upper

106 100

91 193.5 144.6 268.6

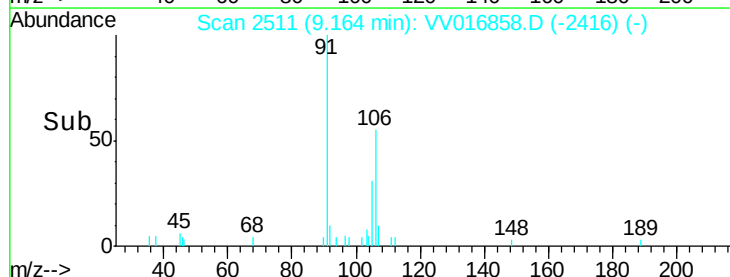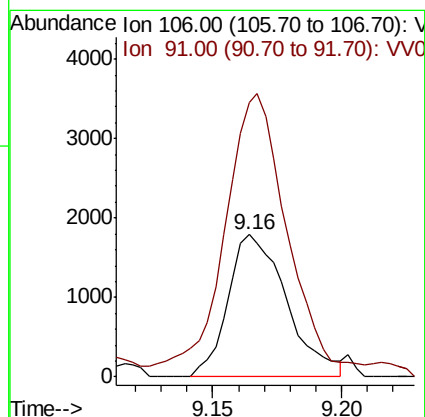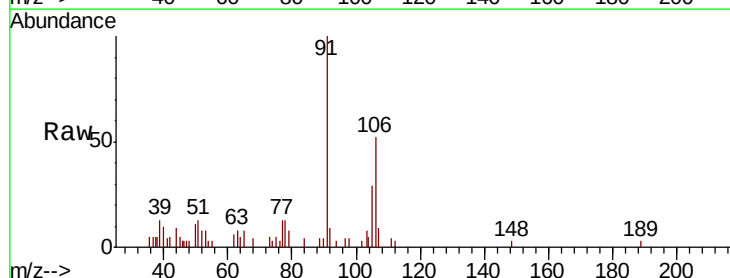

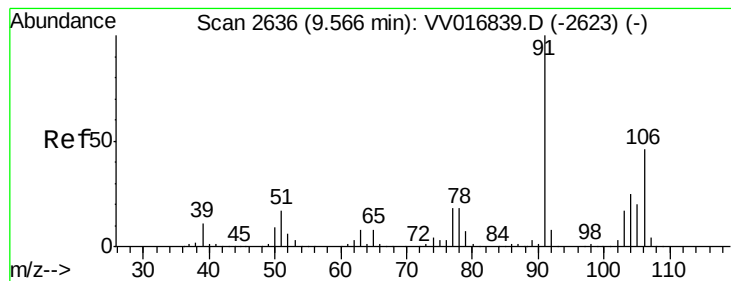

#54

o-xylene

Concen: 1.601 ug/L

RT: 9.57 min Scan# 2636

Delta R.T. 0.00 min

Lab File: VV016858.D

Acq: 12 Jun 2020 03:56

Instrument :
MSVOA_V
ClientSampleId :

Tot Ion:106 Resp: 6805

Ion Ratio Lower Upper

106 100

91 217.0 155.9 289.5

