
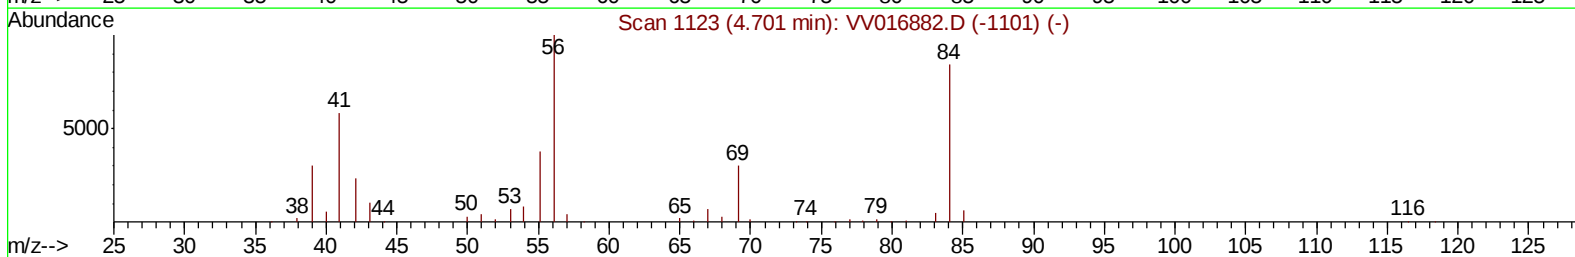
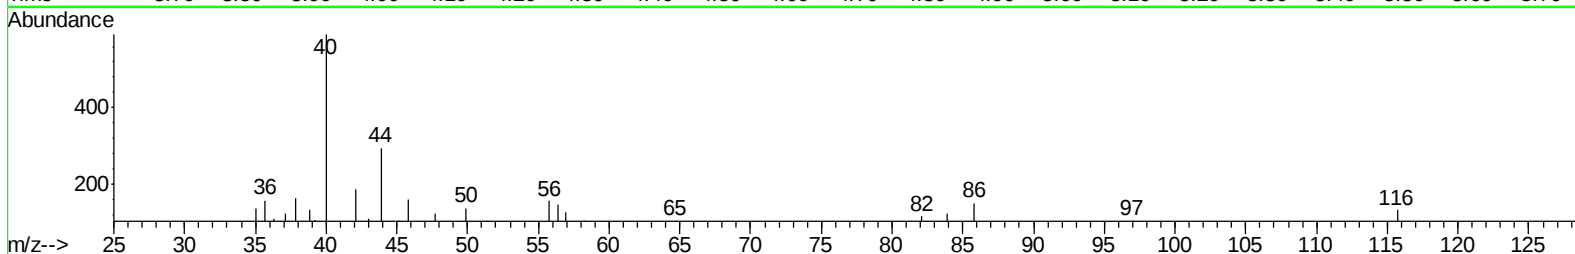


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061120\
Data File : VV016837.D
Acq On : 11 Jun 2020 19:16
Operator : SY/MD
Sample : L2914-07 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jun 12 05:36:27 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 12 01:27:40 2020
Response via : Initial Calibration

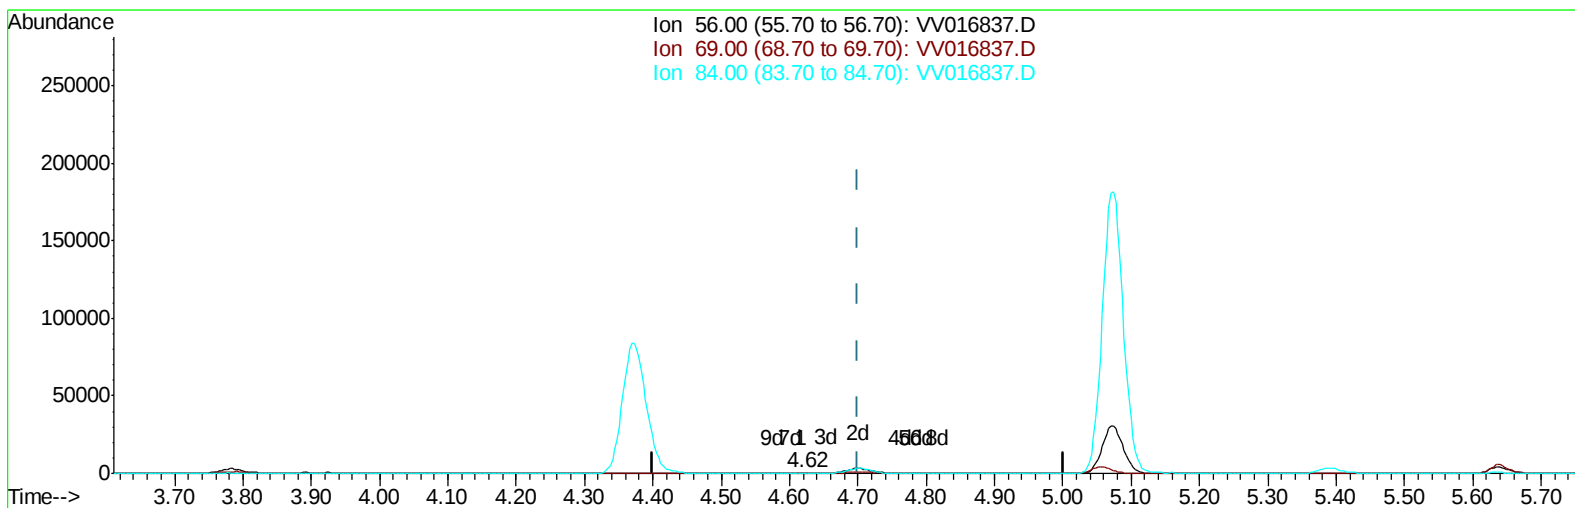

TIC: VV016837.D

(29) Cyclohexane (T)




4.617min (-0.084) 0.04ug/L

response 186

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	34.41
84.00	86.90	94.09
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061120\
 Data File : VV016837.D
 Acq On : 11 Jun 2020 19:16
 Operator : SY/MD
 Sample : L2914-07 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jun 12 05:36:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 12 01:27:40 2020
 Response via : Initial Calibration

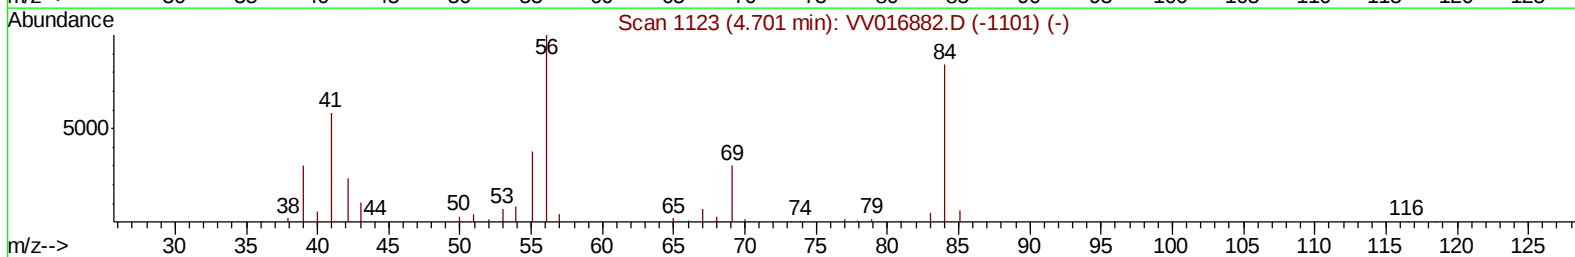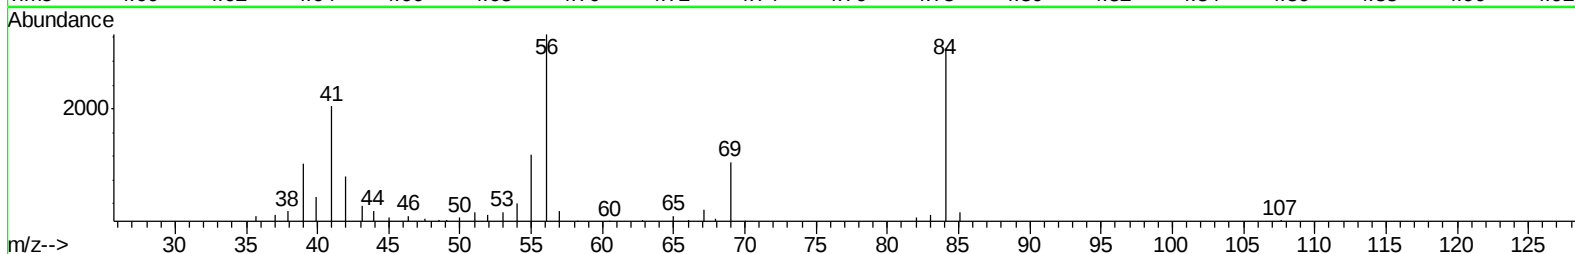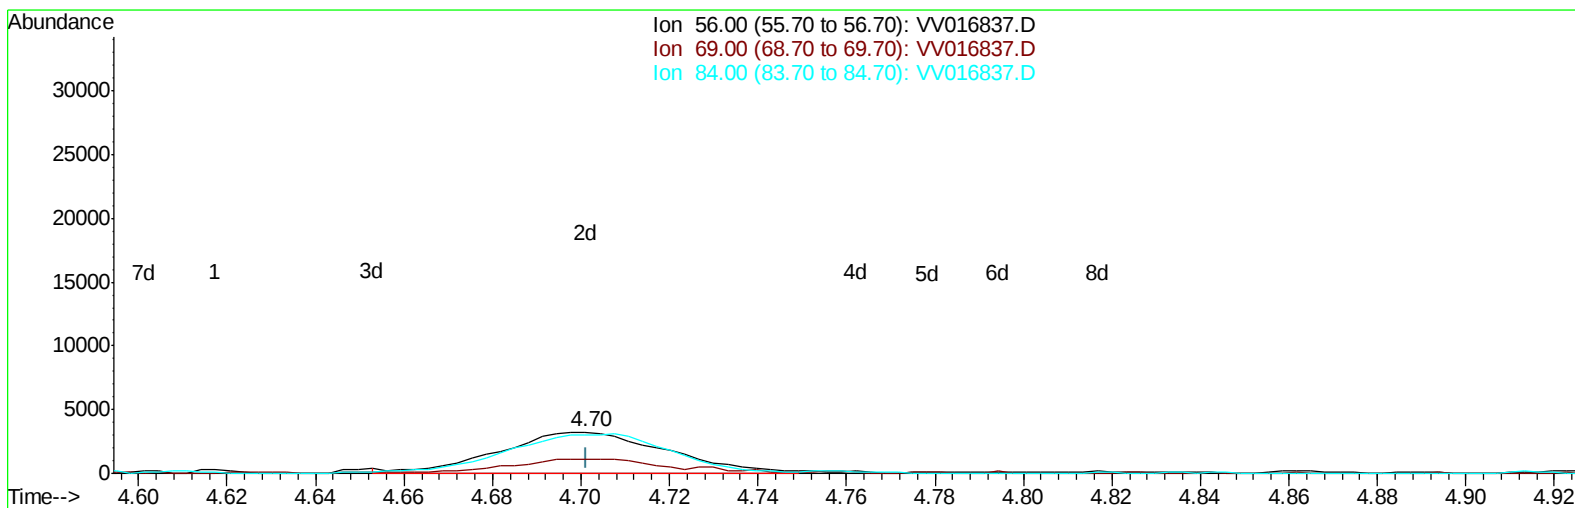

TIC: VV016837.D

(29) Cyclohexane (T)

4.701min (-0.000) 2.06ug/L m

response 8575

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	0.75#
84.00	86.90	2.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061120\
 Data File : VV016837.D
 Acq On : 11 Jun 2020 19:16
 Operator : SY/MD
 Sample : L2914-07 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jun 13 04:26:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 12 01:27:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	357078	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	334468	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	170007	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	81981	32.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	65.08%
7) Chloroethane-d5	1.55	69	60577	40.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.14%
11) 1,1-Dichloroethene-d2	2.11	63	118000	27.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	55.78%#
21) 2-Butanone-d5	3.90	46	163284	87.56	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.56%
24) Chloroform-d	4.37	84	204365	39.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.78%
26) 1,2-Dichloroethane-d4	5.05	65	150504	43.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.38%
32) Benzene-d6	5.07	84	388852	40.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.66%
36) 1,2-Dichloropropane-d6	6.09	67	121648	40.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.96%
41) Toluene-d8	7.34	98	350999	39.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.34%#
43) trans-1,3-Dichloropropene-	7.64	79	60586	38.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.42%
47) 2-Hexanone-d5	8.11	63	101454	77.43	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.43%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	172081	43.25	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.50%
64) 1,2-Dichlorobenzene-d4	11.65	152	162754	44.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.72%

Target Compounds

					Ovalue
29) Cyclohexane	4.70	56	8575m	2.063	ug/L
33) Benzene	5.12	78	1229055	124.198	ug/L
42) Toluene	7.41	91	25537	2.448	ug/L
52) Ethylbenzene	9.04	91	19307	1.671	ug/L
53) m,p-Xylene	9.16	106	17099	3.974	ug/L
54) o-xylene	9.57	106	6416	1.512	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061120\
Data File : VV016837.D
Acq On : 11 Jun 2020 19:16
Operator : SY/MD
Sample : L2914-07 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Jun 13 04:26:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 12 01:27:40 2020
Response via : Initial Calibration

