

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016814.D
 Acq On : 11 Jun 2020 10:12
 Operator : SY/MD
 Sample : L2901-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	87	rVB2	387190	411641	30.50%	3.644%
2	1.560	140	146	158	rVB	118471	141527	10.49%	1.253%
3	2.116	310	319	336	rVB	265799	390721	28.95%	3.459%
4	2.508	437	441	442	rBV5	3005	1976	0.15%	0.017%
5	2.704	499	502	505	rBV4	1584	961	0.07%	0.009%
6	2.733	505	511	515	rBV7	2130	2097	0.16%	0.019%
7	2.852	544	548	549	rBV3	1203	950	0.07%	0.008%
8	2.942	574	576	579	rBV3	1152	795	0.06%	0.007%
9	3.238	661	668	671	rBV8	1243	1240	0.09%	0.011%
10	3.412	720	722	726	rVB4	1235	779	0.06%	0.007%
11	3.434	726	729	735	rBV8	2205	2199	0.16%	0.019%
12	3.611	779	784	786	rBV5	1012	777	0.06%	0.007%
13	3.624	786	788	791	rBV4	1194	839	0.06%	0.007%
14	3.749	825	827	830	rBV3	1433	982	0.07%	0.009%
15	3.827	848	851	854	rVB4	1891	1124	0.08%	0.010%
16	3.933	857	884	908	rBV4	200110	737973	54.69%	6.533%
17	4.100	933	936	940	rBV6	1569	1395	0.10%	0.012%
18	4.370	1005	1020	1042	rBV	220719	534031	39.57%	4.728%
19	4.534	1068	1071	1072	rBV2	1747	825	0.06%	0.007%
20	4.614	1094	1096	1100	rVB4	1849	1225	0.09%	0.011%
21	4.753	1135	1139	1142	rVV6	1599	1178	0.09%	0.010%
22	4.962	1201	1204	1207	rBV5	1242	1027	0.08%	0.009%
23	5.068	1220	1237	1263	rBV2	526363	1349478	100.00%	11.947%
24	5.386	1334	1336	1340	rBV5	1246	1204	0.09%	0.011%
25	5.637	1401	1414	1432	rBV	439360	858643	63.63%	7.601%
26	5.933	1496	1506	1523	rVB7	26554	63375	4.70%	0.561%
27	6.090	1537	1555	1579	rBV	303847	621965	46.09%	5.506%
28	6.199	1586	1589	1591	rBV4	1727	1357	0.10%	0.012%
29	6.579	1704	1707	1710	rBV3	1023	903	0.07%	0.008%
30	6.650	1722	1729	1731	rBV7	1823	2008	0.15%	0.018%
31	6.682	1735	1739	1741	rVV4	1885	1377	0.10%	0.012%
32	6.701	1743	1745	1749	rVB5	2314	1616	0.12%	0.014%
33	6.724	1749	1752	1753	rBV2	1649	1010	0.07%	0.009%
34	7.006	1825	1840	1856	rBV	183674	325327	24.11%	2.880%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016814.D
 Acq On : 11 Jun 2020 10:12
 Operator : SY/MD
 Sample : L2901-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.260	1916	1919	1922	rBV4	1750	1206	0.09%	0.011%
36	7.334	1930	1942	1960	rBV	638504	1094713	81.12%	9.691%
37	7.640	2027	2037	2049	rBV	129489	219180	16.24%	1.940%
38	7.910	2119	2121	2126	rVB6	1336	858	0.06%	0.008%
39	8.106	2172	2182	2214	rBV	316537	606256	44.93%	5.367%
40	8.434	2281	2284	2288	rBV5	1083	863	0.06%	0.008%
41	8.460	2288	2292	2295	rVB6	1828	1238	0.09%	0.011%
42	8.588	2329	2332	2334	rVB4	1739	878	0.07%	0.008%
43	8.611	2336	2339	2341	rBV3	1681	1155	0.09%	0.010%
44	8.698	2363	2366	2369	rBV4	1391	959	0.07%	0.008%
45	8.871	2407	2420	2440	rBV	663931	1074304	79.61%	9.511%
46	9.116	2494	2496	2499	rBV4	1929	1402	0.10%	0.012%
47	9.154	2504	2508	2510	rBV5	2170	1855	0.14%	0.016%
48	9.373	2573	2576	2579	rVB4	1438	923	0.07%	0.008%
49	9.392	2579	2582	2584	rBV4	1988	1174	0.09%	0.010%
50	9.412	2585	2588	2591	rVV5	1388	980	0.07%	0.009%
51	9.524	2620	2623	2626	rBV3	1840	1232	0.09%	0.011%
52	9.643	2657	2660	2664	rVB5	1585	1301	0.10%	0.012%
53	9.675	2664	2670	2671	rBV5	2314	1953	0.14%	0.017%
54	9.891	2733	2737	2741	rBV5	1474	1022	0.08%	0.009%
55	9.981	2762	2765	2769	rVB4	1315	838	0.06%	0.007%
56	10.116	2801	2807	2810	rBV7	1560	1209	0.09%	0.011%
57	10.174	2823	2825	2829	rVB3	1706	808	0.06%	0.007%
58	10.238	2830	2845	2862	rBV	402780	625325	46.34%	5.536%
59	10.598	2952	2957	2963	rBV9	2086	2137	0.16%	0.019%
60	10.688	2981	2985	2990	rBV7	1621	1993	0.15%	0.018%
61	10.823	3024	3027	3028	rBV3	1534	905	0.07%	0.008%
62	10.903	3049	3052	3053	rBV3	1407	801	0.06%	0.007%
63	11.045	3090	3096	3097	rBV3	1184	790	0.06%	0.007%
64	11.183	3137	3139	3142	rBV5	1435	782	0.06%	0.007%
65	11.270	3155	3166	3183	rBV	705519	1064663	78.89%	9.425%
66	11.392	3202	3204	3209	rVB6	1611	778	0.06%	0.007%
67	11.444	3216	3220	3223	rBV4	1129	790	0.06%	0.007%
68	11.501	3235	3238	3241	rBV4	1523	1359	0.10%	0.012%
69	11.563	3253	3257	3261	rBV6	1919	1846	0.14%	0.016%
70	11.646	3272	3283	3300	rBV	698668	1079761	80.01%	9.559%
71	11.804	3329	3332	3334	rBV3	1633	929	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016814.D
 Acq On : 11 Jun 2020 10:12
 Operator : SY/MD
 Sample : L2901-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.990	3386	3390	3392	rBV3	1758	1327	0.10%	0.012%
73	12.029	3400	3402	3406	rBV5	1290	820	0.06%	0.007%
74	12.244	3466	3469	3470	rBV2	1497	848	0.06%	0.008%
75	12.370	3506	3508	3512	rVV4	1368	968	0.07%	0.009%
76	12.411	3519	3521	3527	rVB6	1386	936	0.07%	0.008%
77	12.456	3530	3535	3541	rBV8	1722	2213	0.16%	0.020%
78	12.530	3555	3558	3560	rBV3	1243	779	0.06%	0.007%
79	12.633	3588	3590	3594	rVB4	1621	879	0.07%	0.008%
80	12.720	3613	3617	3620	rBV5	1173	1091	0.08%	0.010%
81	12.755	3624	3628	3630	rBV5	1262	779	0.06%	0.007%
82	12.768	3630	3632	3637	rVB5	1719	1000	0.07%	0.009%
83	12.791	3637	3639	3641	rBV2	1740	946	0.07%	0.008%
84	12.852	3654	3658	3661	rVB5	2572	1506	0.11%	0.013%
85	12.874	3661	3665	3667	rBV5	1303	919	0.07%	0.008%
86	12.890	3667	3670	3673	rBV4	1569	1248	0.09%	0.011%
87	12.961	3690	3692	3694	rBV2	1315	864	0.06%	0.008%
88	13.096	3732	3734	3738	rBV5	1177	830	0.06%	0.007%
89	13.263	3783	3786	3787	rBV3	1475	984	0.07%	0.009%
90	13.472	3848	3851	3856	rVB5	1249	1085	0.08%	0.010%
91	13.498	3856	3859	3861	rBV3	1570	951	0.07%	0.008%
92	13.514	3861	3864	3866	rBV3	1780	1348	0.10%	0.012%
93	13.678	3911	3915	3918	rBV6	1522	1086	0.08%	0.010%
94	14.090	4041	4043	4048	rVB4	1901	997	0.07%	0.009%
95	14.260	4092	4096	4100	rVB8	1894	1544	0.11%	0.014%
96	14.279	4100	4102	4105	rBV3	1153	836	0.06%	0.007%
97	14.614	4203	4206	4209	rBV4	2024	1346	0.10%	0.012%
98	14.704	4231	4234	4240	rBV6	1162	1137	0.08%	0.010%
99	15.048	4337	4341	4346	rBV7	2182	2027	0.15%	0.018%
100	15.337	4428	4431	4433	rBV4	1637	854	0.06%	0.008%


Sum of corrected areas: 11295839

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016814.D
Acq On : 11 Jun 2020 10:12
Operator : SY/MD
Sample : L2901-09DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

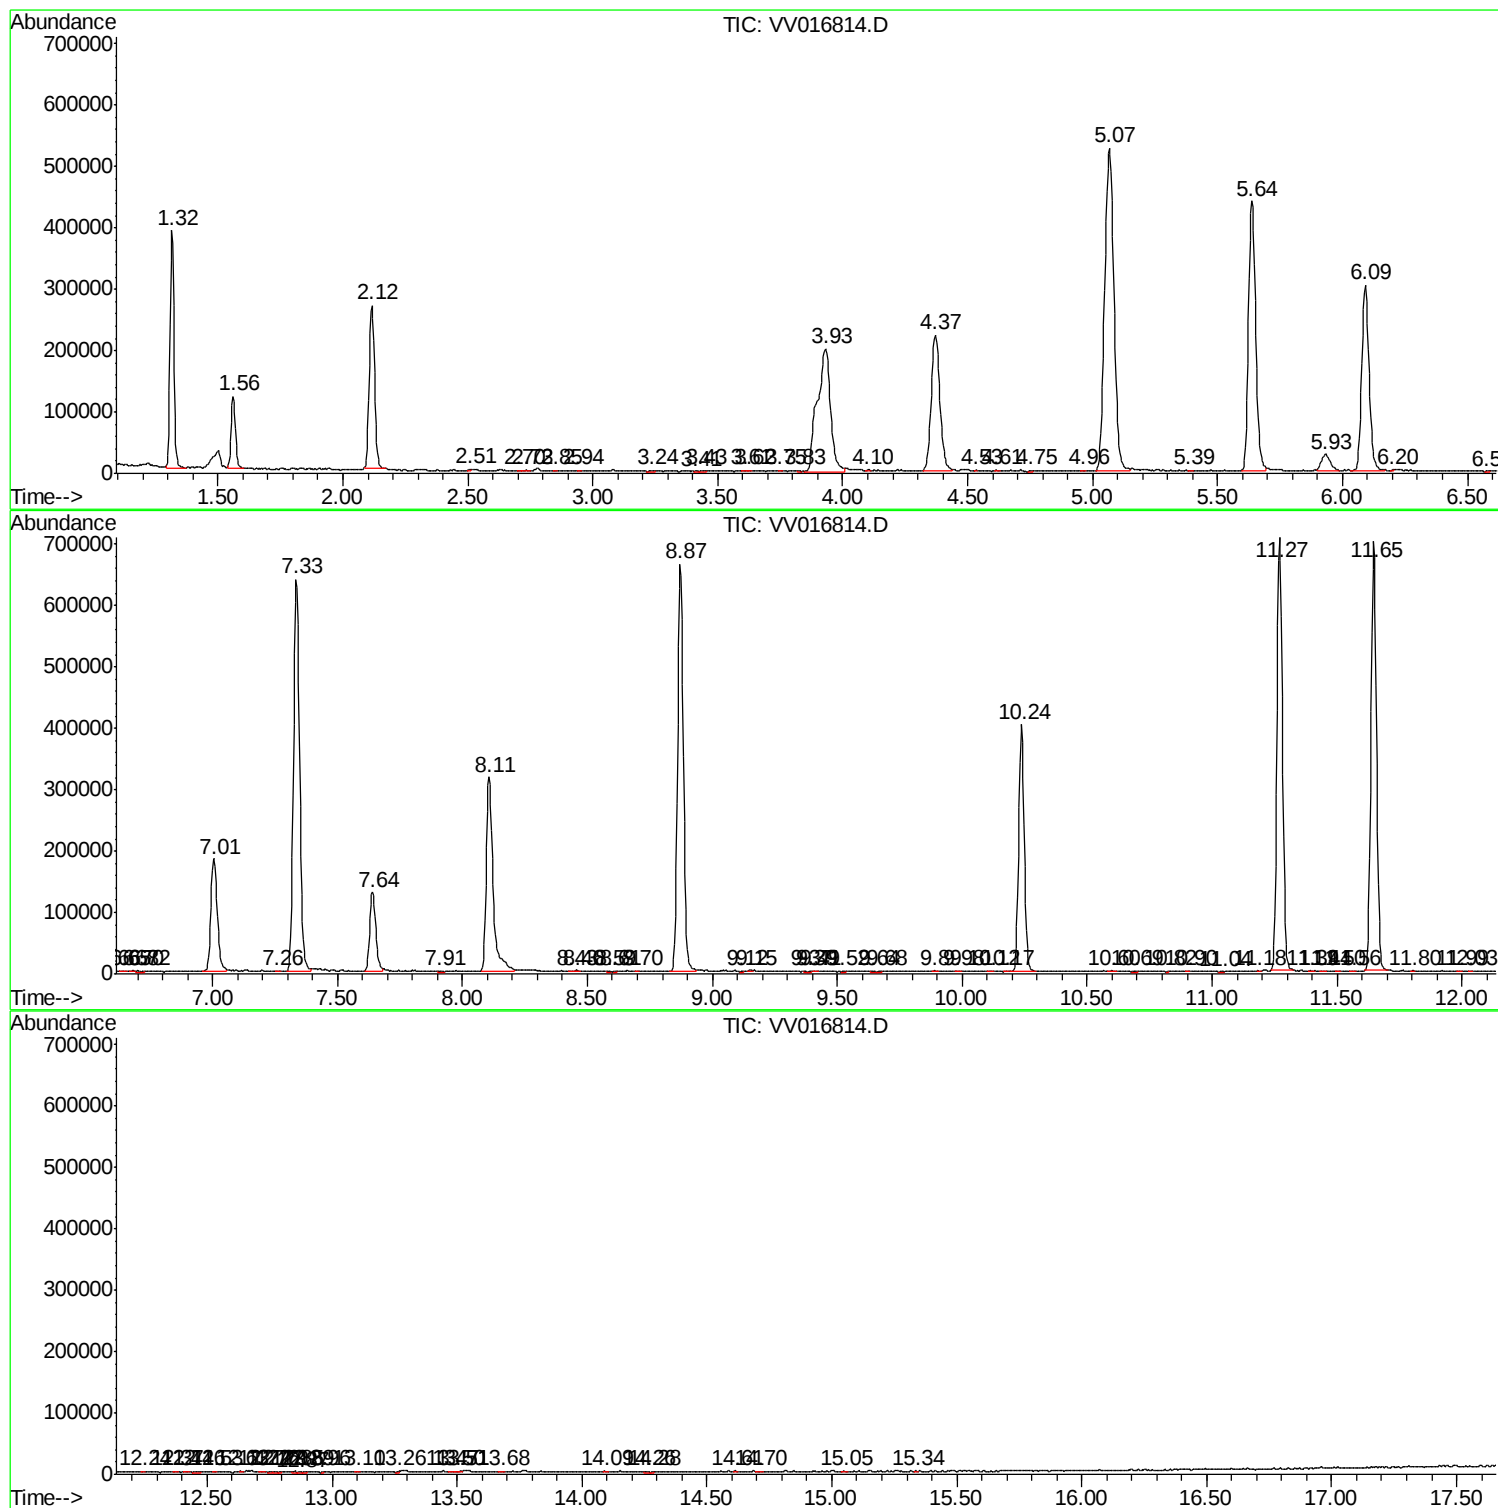

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016814.D
Acq On : 11 Jun 2020 10:12
Operator : SY/MD
Sample : L2901-09DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061120\
Data File : VV016814.D
Acq On : 11 Jun 2020 10:12
Operator : SY/MD
Sample : L2901-09DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTT4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc