

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016822.D
 Acq On : 11 Jun 2020 13:20
 Operator : SY/MD
 Sample : L2929-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	86	rVB	171001	184976	13.79%	1.781%
2	2.103	307	315	335	rVB	250651	373926	27.88%	3.601%
3	2.393	403	405	407	rBV2	1399	653	0.05%	0.006%
4	2.553	451	455	463	rBV8	1529	1891	0.14%	0.018%
5	2.627	469	478	485	rBV8	6082	12801	0.95%	0.123%
6	2.708	501	503	504	rBV2	1455	674	0.05%	0.006%
7	2.740	511	513	518	rBV4	1288	1112	0.08%	0.011%
8	2.820	536	538	540	rBV3	1190	803	0.06%	0.008%
9	2.865	545	552	554	rBV8	1710	1541	0.11%	0.015%
10	2.994	589	592	595	rVB4	1361	849	0.06%	0.008%
11	3.023	598	601	603	rBV2	1541	1139	0.08%	0.011%
12	3.052	606	610	612	rBV4	1519	783	0.06%	0.008%
13	3.074	612	617	619	rBV4	1353	967	0.07%	0.009%
14	3.187	650	652	657	rVB6	1613	1095	0.08%	0.011%
15	3.283	679	682	686	rVB5	1716	1579	0.12%	0.015%
16	3.312	686	691	695	rVB6	1588	1427	0.11%	0.014%
17	3.335	695	698	700	rBV3	1174	860	0.06%	0.008%
18	3.428	724	727	731	rBV4	1521	1540	0.11%	0.015%
19	3.557	762	767	770	rBV6	1966	2135	0.16%	0.021%
20	3.840	851	855	856	rBV4	1343	890	0.07%	0.009%
21	3.901	863	874	902	rBV	93391	281848	21.01%	2.714%
22	4.229	974	976	979	rBV3	1463	633	0.05%	0.006%
23	4.299	994	998	999	rBV3	1394	731	0.05%	0.007%
24	4.370	1006	1020	1042	rVB	220064	531974	39.66%	5.123%
25	4.537	1070	1072	1077	rBV4	1145	875	0.07%	0.008%
26	4.621	1093	1098	1100	rBV5	1859	1491	0.11%	0.014%
27	4.653	1106	1108	1112	rBV3	866	808	0.06%	0.008%
28	4.685	1112	1118	1119	rVV5	1481	1315	0.10%	0.013%
29	4.749	1133	1138	1141	rBV7	1288	1326	0.10%	0.013%
30	4.888	1179	1181	1183	rBV3	1225	706	0.05%	0.007%
31	4.978	1207	1209	1212	rVB3	1857	785	0.06%	0.008%
32	5.065	1219	1236	1260	rBV2	529264	1341197	100.00%	12.915%
33	5.354	1324	1326	1330	rVB4	2887	1600	0.12%	0.015%
34	5.476	1360	1364	1366	rBV6	1284	882	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016822.D
 Acq On : 11 Jun 2020 13:20
 Operator : SY/MD
 Sample : L2929-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.566	1388	1392	1398	rBV8	1446	1531	0.11%	0.015%
36	5.637	1401	1414	1435	rBV	374862	745196	55.56%	7.176%
37	5.881	1488	1490	1493	rBV3	1372	871	0.06%	0.008%
38	5.926	1493	1504	1512	rBV4	15399	30646	2.28%	0.295%
39	6.090	1543	1555	1577	rVB	297802	602700	44.94%	5.804%
40	6.277	1609	1613	1618	rBV7	1516	1679	0.13%	0.016%
41	6.344	1631	1634	1639	rVV6	1518	1079	0.08%	0.010%
42	6.370	1639	1642	1643	rBV4	1699	691	0.05%	0.007%
43	6.412	1652	1655	1657	rBV4	1713	923	0.07%	0.009%
44	6.425	1657	1659	1664	rBV4	1379	1159	0.09%	0.011%
45	6.502	1680	1683	1685	rBV2	1188	709	0.05%	0.007%
46	6.630	1720	1723	1724	rBV3	1488	916	0.07%	0.009%
47	6.769	1763	1766	1770	rBV4	1527	1291	0.10%	0.012%
48	6.849	1788	1791	1796	rVB7	1389	1317	0.10%	0.013%
49	7.007	1829	1840	1859	rBV	176602	314648	23.46%	3.030%
50	7.222	1906	1907	1911	rBV4	1217	795	0.06%	0.008%
51	7.335	1930	1942	1958	rBV	617489	1061182	79.12%	10.219%
52	7.640	2028	2037	2051	rBV2	124216	207041	15.44%	1.994%
53	7.753	2070	2072	2074	rBV2	1420	912	0.07%	0.009%
54	7.955	2127	2135	2148	rVV4	6544	13635	1.02%	0.131%
55	8.048	2162	2164	2166	rBV3	1577	867	0.06%	0.008%
56	8.077	2170	2173	2174	rVV4	1425	942	0.07%	0.009%
57	8.116	2174	2185	2216	rVV2	327091	692208	51.61%	6.666%
58	8.463	2289	2293	2296	rBV5	1838	1548	0.12%	0.015%
59	8.515	2306	2309	2311	rBV4	1848	1212	0.09%	0.012%
60	8.794	2394	2396	2398	rBV3	1304	627	0.05%	0.006%
61	8.807	2398	2400	2403	rVB3	1968	874	0.07%	0.008%
62	8.875	2409	2421	2440	rVV	560986	918158	68.46%	8.841%
63	9.077	2481	2484	2487	rBV4	1914	1272	0.09%	0.012%
64	9.167	2501	2512	2520	rBV8	6187	10162	0.76%	0.098%
65	9.363	2569	2573	2574	rBV5	1067	675	0.05%	0.006%
66	9.489	2608	2612	2614	rBV5	1342	682	0.05%	0.007%
67	9.566	2629	2636	2638	rBV8	2834	3163	0.24%	0.030%
68	9.688	2669	2674	2677	rBV6	1635	1656	0.12%	0.016%
69	9.804	2706	2710	2712	rBV4	1384	1215	0.09%	0.012%
70	9.881	2730	2734	2735	rBV3	1165	682	0.05%	0.007%
71	10.161	2819	2821	2825	rBV4	1082	827	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016822.D
 Acq On : 11 Jun 2020 13:20
 Operator : SY/MD
 Sample : L2929-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTZ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.241	2834	2846	2864	rBV	434990	691314	51.54%	6.657%
73	10.405	2882	2897	2909	rBV7	9360	21778	1.62%	0.210%
74	10.466	2914	2916	2920	rBV4	1633	957	0.07%	0.009%
75	10.939	3055	3063	3073	rVB4	4669	8623	0.64%	0.083%
76	11.270	3155	3166	3185	rBV	643429	993330	74.06%	9.565%
77	11.650	3272	3284	3299	rBV	726820	1142008	85.15%	10.997%
78	11.759	3315	3318	3319	rBV3	1624	823	0.06%	0.008%
79	11.961	3376	3381	3383	rBV7	1687	1382	0.10%	0.013%
80	12.190	3447	3452	3459	rBV10	1863	2675	0.20%	0.026%
81	12.248	3466	3470	3472	rBV4	1445	1261	0.09%	0.012%
82	12.367	3503	3507	3510	rBV6	2566	2520	0.19%	0.024%
83	12.669	3598	3601	3604	rBV4	2094	1510	0.11%	0.015%
84	12.707	3611	3613	3619	rBV7	1076	919	0.07%	0.009%
85	12.743	3621	3624	3626	rBV4	1620	1153	0.09%	0.011%
86	12.958	3689	3691	3694	rBV4	1470	868	0.06%	0.008%
87	13.003	3703	3705	3710	rBV5	1222	1034	0.08%	0.010%
88	13.055	3718	3721	3723	rBV4	1390	1076	0.08%	0.010%
89	13.251	3780	3782	3785	rBV4	1470	890	0.07%	0.009%
90	13.286	3788	3793	3798	rBV9	1909	2283	0.17%	0.022%
91	13.460	3845	3847	3850	rBV3	1417	921	0.07%	0.009%
92	13.527	3858	3868	3887	rBV	40368	68952	5.14%	0.664%
93	13.646	3900	3905	3907	rBV5	5765	5594	0.42%	0.054%
94	13.852	3966	3969	3972	rBV4	1802	1312	0.10%	0.013%
95	13.868	3972	3974	3977	rVB3	1904	953	0.07%	0.009%
96	14.212	4079	4081	4084	rBV3	1848	1037	0.08%	0.010%
97	14.392	4134	4137	4140	rVB3	1665	911	0.07%	0.009%
98	14.418	4140	4145	4147	rBV5	1574	1691	0.13%	0.016%
99	14.842	4268	4277	4289	rBV2	22618	42663	3.18%	0.411%
100	15.177	4379	4381	4383	rBV3	1758	884	0.07%	0.009%


Sum of corrected areas: 10384825

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016822.D
Acq On : 11 Jun 2020 13:20
Operator : SY/MD
Sample : L2929-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT21

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

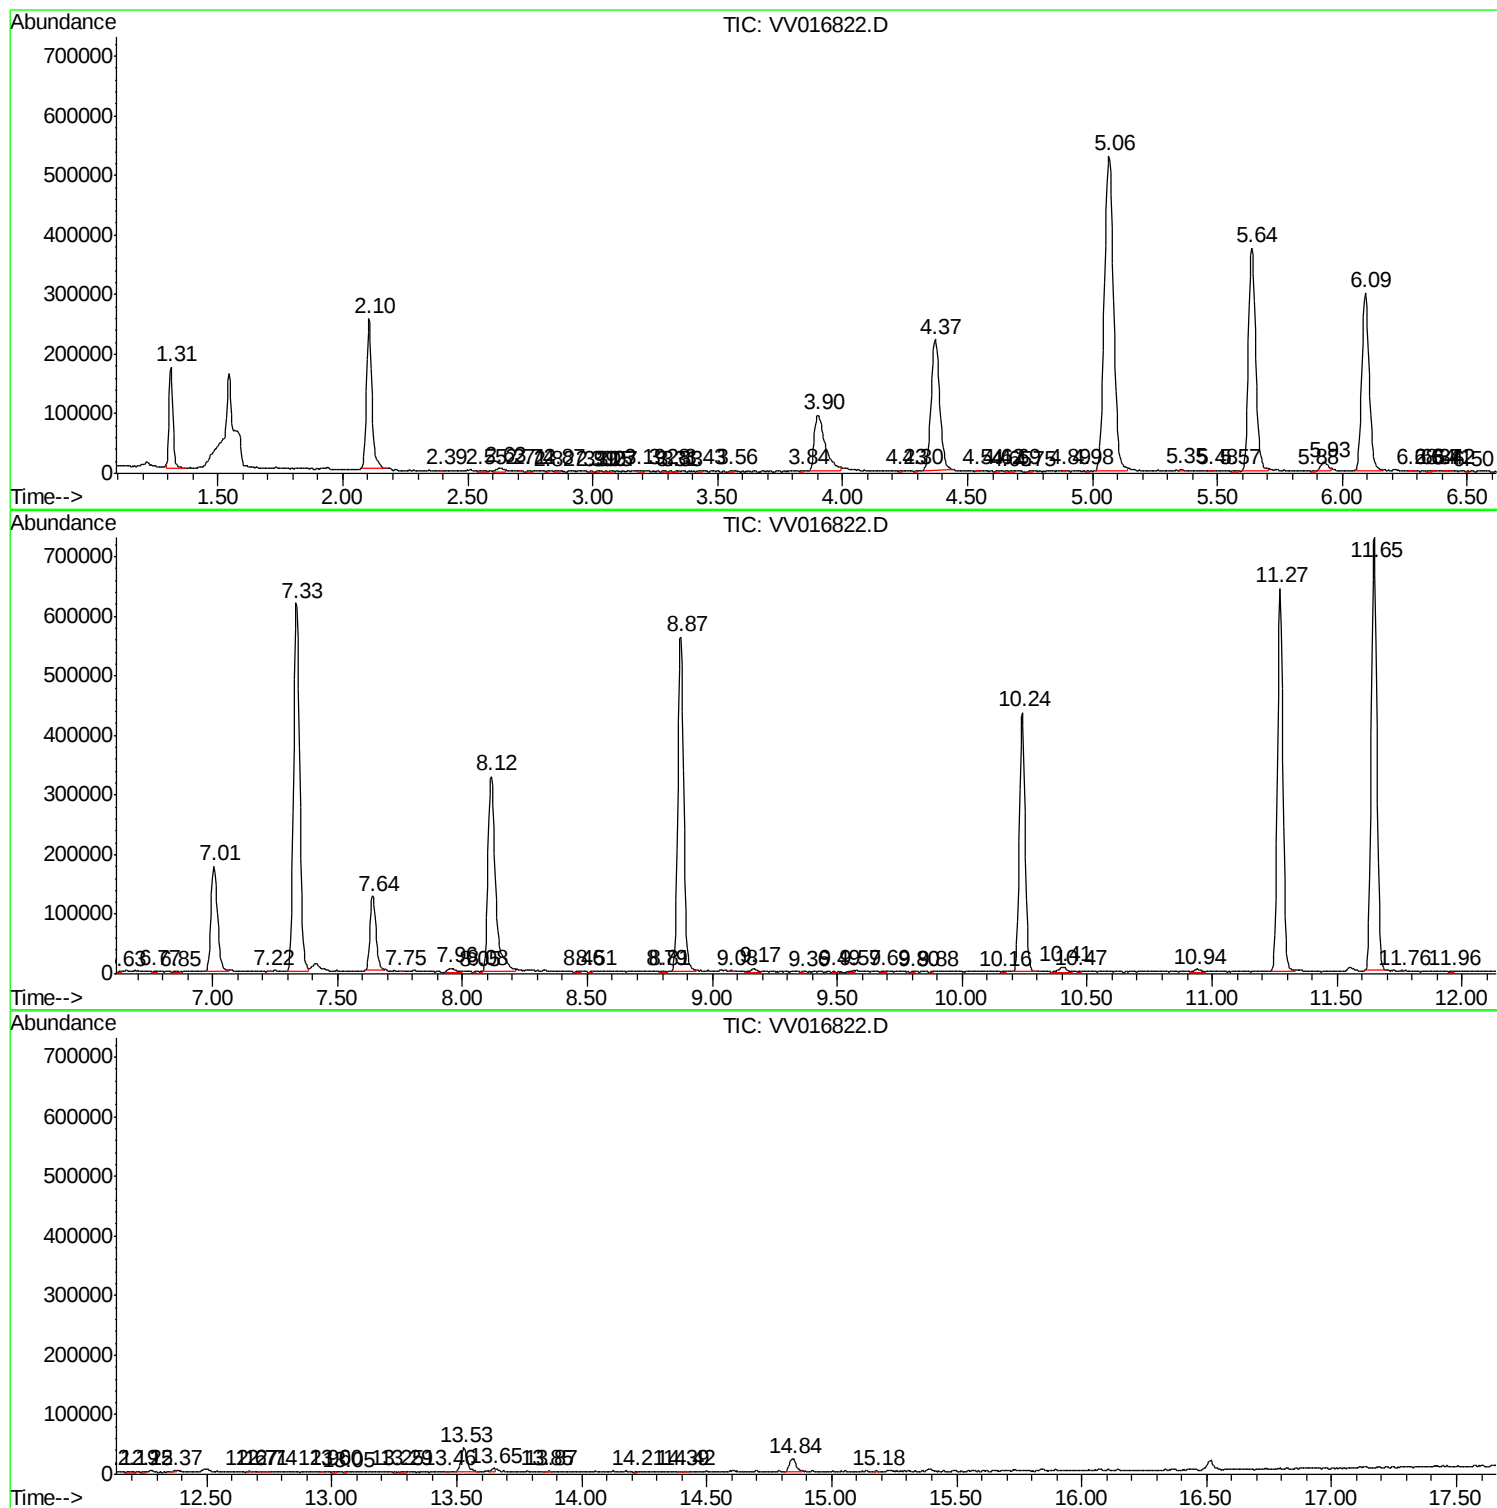

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016822.D
Acq On : 11 Jun 2020 13:20
Operator : SY/MD
Sample : L2929-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTZ1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016822.D
Acq On : 11 Jun 2020 13:20
Operator : SY/MD
Sample : L2929-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTZ1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc