

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016826.D
 Acq On : 11 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	151585	149981	11.70%	1.464%
2	1.557	138	145	156	rVB	103210	124687	9.72%	1.217%
3	2.113	309	318	332	rBV	241134	359800	28.06%	3.512%
4	2.286	365	372	374	rBV6	3751	4343	0.34%	0.042%
5	2.566	455	459	462	rBV6	1675	1196	0.09%	0.012%
6	2.704	500	502	505	rVB5	2518	1244	0.10%	0.012%
7	2.737	505	512	516	rBV8	1471	2020	0.16%	0.020%
8	2.782	524	526	531	rBV5	1350	1144	0.09%	0.011%
9	2.817	535	537	541	rBV4	1428	1194	0.09%	0.012%
10	2.862	548	551	554	rVB4	1366	925	0.07%	0.009%
11	2.885	554	558	560	rBV5	1549	1041	0.08%	0.010%
12	3.161	641	644	647	rBV5	1649	969	0.08%	0.009%
13	3.190	651	653	656	rVV4	1402	951	0.07%	0.009%
14	3.402	716	719	722	rBV4	1364	893	0.07%	0.009%
15	3.470	737	740	741	rVV3	1453	677	0.05%	0.007%
16	3.647	791	795	801	rBV8	1352	1474	0.11%	0.014%
17	3.698	808	811	815	rBV3	1609	1227	0.10%	0.012%
18	3.746	823	826	829	rBV4	1363	1023	0.08%	0.010%
19	3.830	850	852	861	rVB8	1794	1552	0.12%	0.015%
20	3.894	861	872	898	rBV	102923	273066	21.30%	2.666%
21	4.203	965	968	970	rVB4	1526	910	0.07%	0.009%
22	4.222	970	974	978	rBV6	1705	1577	0.12%	0.015%
23	4.373	1000	1021	1052	rBV	208298	522825	40.78%	5.103%
24	4.595	1087	1090	1092	rBV4	1268	1019	0.08%	0.010%
25	4.614	1092	1096	1102	rBV6	1600	1963	0.15%	0.019%
26	4.753	1136	1139	1142	rBV5	2384	1660	0.13%	0.016%
27	4.817	1156	1159	1160	rBV3	1570	691	0.05%	0.007%
28	4.923	1189	1192	1194	rBV4	1599	853	0.07%	0.008%
29	4.962	1202	1204	1206	rBV3	1868	990	0.08%	0.010%
30	4.991	1209	1213	1218	rBV7	1245	1343	0.10%	0.013%
31	5.068	1218	1237	1263	rBV2	495813	1282184	100.00%	12.516%
32	5.521	1375	1378	1385	rBV8	1403	1624	0.13%	0.016%
33	5.569	1389	1393	1394	rBV3	1491	812	0.06%	0.008%
34	5.640	1402	1415	1440	rBV	437775	865580	67.51%	8.449%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016826.D
 Acq On : 11 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.875	1482	1488	1490	rBV6	2197	1961	0.15%	0.019%
36	6.093	1542	1556	1575	rBV	281950	576481	44.96%	5.627%
37	6.290	1614	1617	1619	rBV2	1024	782	0.06%	0.008%
38	6.444	1664	1665	1669	rBV3	1329	932	0.07%	0.009%
39	6.518	1686	1688	1691	rBV3	954	708	0.06%	0.007%
40	6.627	1719	1722	1726	rBV5	1202	997	0.08%	0.010%
41	6.650	1726	1729	1732	rBV3	1819	1279	0.10%	0.012%
42	6.807	1775	1778	1782	rBV5	1499	1199	0.09%	0.012%
43	6.955	1822	1824	1826	rVB3	1694	689	0.05%	0.007%
44	7.007	1828	1840	1859	rVV	168739	300365	23.43%	2.932%
45	7.338	1930	1943	1960	rBV	581628	1012526	78.97%	9.884%
46	7.640	2029	2037	2053	rVB	117850	191944	14.97%	1.874%
47	7.923	2122	2125	2126	rBV3	1392	811	0.06%	0.008%
48	7.939	2128	2130	2132	rBV3	1871	1003	0.08%	0.010%
49	7.994	2145	2147	2151	rVV4	975	662	0.05%	0.006%
50	8.013	2151	2153	2157	rVB4	2047	944	0.07%	0.009%
51	8.042	2157	2162	2164	rBV3	1179	926	0.07%	0.009%
52	8.106	2171	2182	2214	rBV	323870	621102	48.44%	6.063%
53	8.354	2257	2259	2261	rBV3	1415	659	0.05%	0.006%
54	8.752	2380	2383	2387	rBV5	1344	1321	0.10%	0.013%
55	8.871	2409	2420	2440	rVV	665534	1068214	83.31%	10.427%
56	9.125	2497	2499	2504	rBV5	1188	1005	0.08%	0.010%
57	9.437	2594	2596	2600	rBV5	1681	804	0.06%	0.008%
58	9.479	2606	2609	2610	rBV2	1060	626	0.05%	0.006%
59	9.955	2753	2757	2758	rBV4	2078	1281	0.10%	0.013%
60	10.077	2792	2795	2796	rBV3	1492	741	0.06%	0.007%
61	10.129	2808	2811	2816	rBV7	1748	1436	0.11%	0.014%
62	10.180	2825	2827	2831	rVB5	2566	1679	0.13%	0.016%
63	10.238	2831	2845	2862	rBV	403132	632325	49.32%	6.172%
64	10.598	2955	2957	2962	rBV5	1303	834	0.07%	0.008%
65	10.730	2993	2998	3000	rVB5	1374	854	0.07%	0.008%
66	11.077	3102	3106	3111	rVB7	1060	953	0.07%	0.009%
67	11.196	3141	3143	3147	rBV4	2124	1039	0.08%	0.010%
68	11.270	3154	3166	3181	rBV	730711	1108887	86.48%	10.824%
69	11.498	3232	3237	3238	rBV4	1447	1228	0.10%	0.012%
70	11.646	3271	3283	3298	rBV	677385	1058051	82.52%	10.328%
71	11.836	3340	3342	3345	rBV2	1615	1079	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016826.D
 Acq On : 11 Jun 2020 14:55
 Operator : SY/MD
 Sample : L2929-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.875	3350	3354	3356	rBV4	1646	1203	0.09%	0.012%
73	11.920	3366	3368	3372	rBV4	1165	771	0.06%	0.008%
74	12.000	3390	3393	3397	rBV4	1634	1260	0.10%	0.012%
75	12.116	3426	3429	3431	rVB3	1291	788	0.06%	0.008%
76	12.129	3431	3433	3435	rBV3	1402	837	0.07%	0.008%
77	12.174	3445	3447	3449	rBV3	1502	660	0.05%	0.006%
78	12.241	3466	3468	3471	rBV2	1434	1004	0.08%	0.010%
79	12.350	3497	3502	3503	rBV5	1481	1145	0.09%	0.011%
80	12.392	3511	3515	3516	rBV4	1550	1034	0.08%	0.010%
81	12.595	3575	3578	3584	rVB6	1694	1529	0.12%	0.015%
82	12.739	3621	3623	3627	rVB5	1686	1031	0.08%	0.010%
83	12.913	3673	3677	3680	rBV5	1564	1419	0.11%	0.014%
84	13.051	3718	3720	3722	rVB3	1308	658	0.05%	0.006%
85	13.071	3722	3726	3727	rBV4	1220	935	0.07%	0.009%
86	13.109	3737	3738	3741	rBV3	1180	726	0.06%	0.007%
87	13.190	3759	3763	3767	rBV6	1388	1218	0.09%	0.012%
88	13.325	3803	3805	3808	rBV4	1968	1147	0.09%	0.011%
89	13.405	3827	3830	3834	rBV4	2031	1858	0.14%	0.018%
90	13.466	3845	3849	3852	rBV5	1682	1711	0.13%	0.017%
91	13.485	3853	3855	3859	rBV4	1372	947	0.07%	0.009%
92	13.669	3910	3912	3915	rBV4	1768	1006	0.08%	0.010%
93	13.858	3969	3971	3976	rBV4	884	793	0.06%	0.008%
94	14.077	4037	4039	4043	rVB4	2223	1292	0.10%	0.013%
95	14.177	4068	4070	4074	rBV4	1265	865	0.07%	0.008%
96	14.344	4118	4122	4125	rBV7	1682	1484	0.12%	0.014%
97	14.556	4185	4188	4190	rBV3	1561	1079	0.08%	0.011%
98	14.678	4224	4226	4228	rBV2	1520	788	0.06%	0.008%
99	14.833	4270	4274	4277	rBV6	2755	2856	0.22%	0.028%
100	14.984	4318	4321	4323	rBV3	958	644	0.05%	0.006%


Sum of corrected areas: 10244453

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016826.D
Acq On : 11 Jun 2020 14:55
Operator : SY/MD
Sample : L2929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

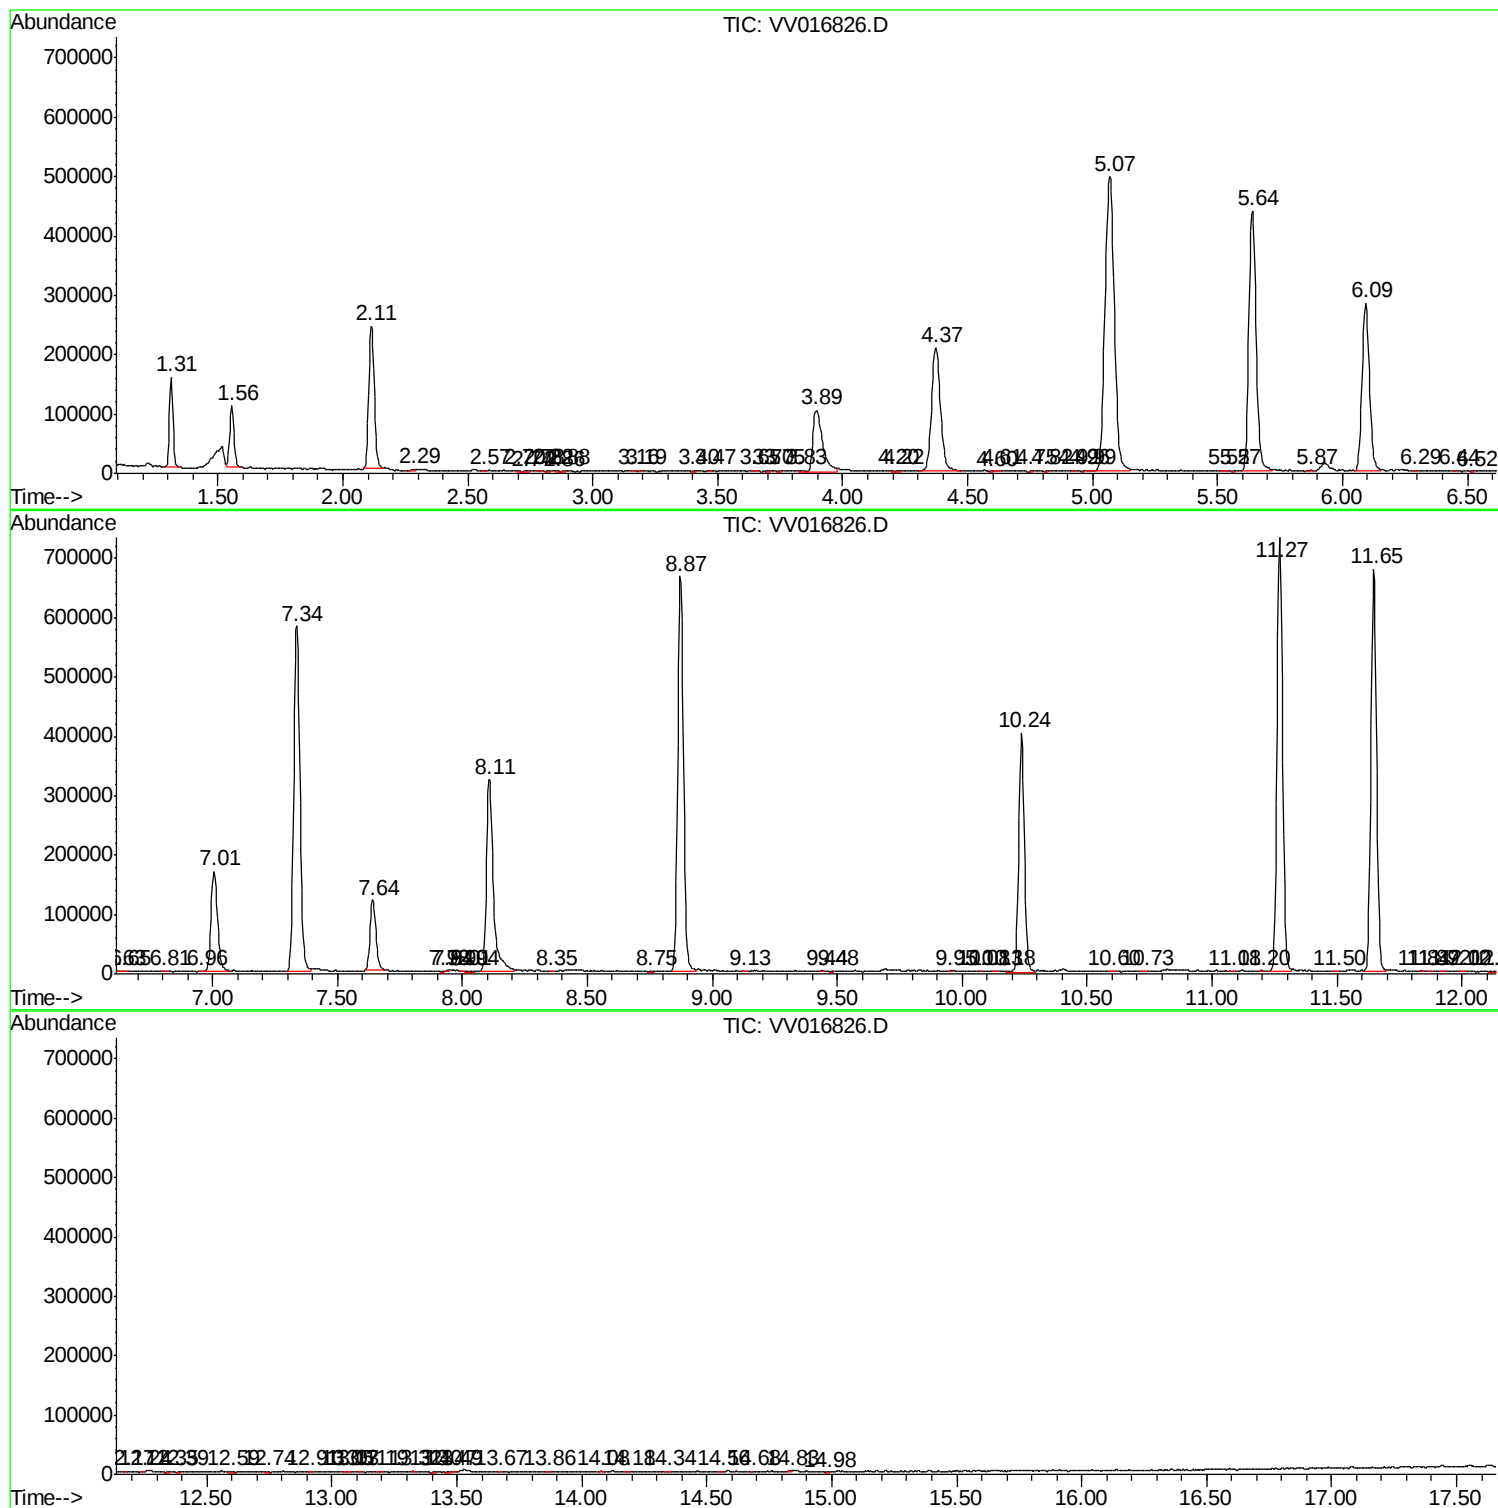

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016826.D
Acq On : 11 Jun 2020 14:55
Operator : SY/MD
Sample : L2929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016826.D
Acq On : 11 Jun 2020 14:55
Operator : SY/MD
Sample : L2929-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc