

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016827.D
 Acq On : 11 Jun 2020 15:19
 Operator : SY/MD
 Sample : L2929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	84	rVB	146850	149842	12.43%	1.523%
2	1.553	138	144	158	rVB	100976	120845	10.03%	1.228%
3	2.113	309	318	333	rBV	232428	340294	28.24%	3.458%
4	2.370	396	398	400	rBV4	1895	1009	0.08%	0.010%
5	2.589	464	466	468	rBV3	1440	615	0.05%	0.006%
6	2.946	573	577	578	rBV3	1078	731	0.06%	0.007%
7	2.987	588	590	595	rVB4	1189	881	0.07%	0.009%
8	3.090	620	622	624	rBV3	1962	1021	0.08%	0.010%
9	3.209	657	659	662	rBV4	934	469	0.04%	0.005%
10	3.229	662	665	666	rBV3	1376	630	0.05%	0.006%
11	3.241	667	669	674	rBV4	1192	870	0.07%	0.009%
12	3.383	708	713	714	rBV4	1847	1398	0.12%	0.014%
13	3.447	730	733	737	rVB5	2071	1449	0.12%	0.015%
14	3.573	770	772	774	rBV3	1449	634	0.05%	0.006%
15	3.608	779	783	786	rBV4	1734	1591	0.13%	0.016%
16	3.640	791	793	794	rBV2	914	345	0.03%	0.004%
17	3.669	800	802	804	rVB3	1159	509	0.04%	0.005%
18	3.782	835	837	841	rVB4	1110	718	0.06%	0.007%
19	3.804	841	844	846	rBV2	1574	1142	0.09%	0.012%
20	3.894	862	872	900	rBV	102150	279246	23.17%	2.838%
21	4.370	1005	1020	1041	rBV2	197347	483796	40.15%	4.917%
22	4.540	1071	1073	1078	rVB4	1080	684	0.06%	0.007%
23	4.753	1137	1139	1141	rBV4	1105	534	0.04%	0.005%
24	4.766	1141	1143	1144	rBV2	1435	675	0.06%	0.007%
25	4.811	1153	1157	1160	rBV4	1589	1155	0.10%	0.012%
26	4.836	1160	1165	1166	rBV3	1194	1099	0.09%	0.011%
27	4.926	1189	1193	1194	rBV5	1851	977	0.08%	0.010%
28	4.968	1201	1206	1211	rBV7	1599	1709	0.14%	0.017%
29	4.994	1211	1214	1220	rBV7	1741	2176	0.18%	0.022%
30	5.068	1220	1237	1259	rBV2	472752	1205100	100.00%	12.247%
31	5.322	1312	1316	1320	rBV7	1619	1796	0.15%	0.018%
32	5.447	1352	1355	1359	rBV6	1757	1179	0.10%	0.012%
33	5.492	1367	1369	1372	rBV4	2271	1132	0.09%	0.012%
34	5.547	1384	1386	1387	rBV2	1065	367	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016827.D
 Acq On : 11 Jun 2020 15:19
 Operator : SY/MD
 Sample : L2929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.637	1402	1414	1443	rBV	430130	852851	70.77%	8.667%
36	6.093	1543	1556	1576	rBV	275855	550291	45.66%	5.593%
37	6.328	1624	1629	1630	rBV4	1840	1220	0.10%	0.012%
38	6.367	1638	1641	1642	rBV3	1398	862	0.07%	0.009%
39	6.589	1707	1710	1713	rBV4	1953	1415	0.12%	0.014%
40	6.875	1796	1799	1803	rVB5	1769	1421	0.12%	0.014%
41	6.904	1806	1808	1810	rBV3	1356	928	0.08%	0.009%
42	6.942	1816	1820	1823	rBV5	1431	963	0.08%	0.010%
43	7.007	1829	1840	1864	rBV	162522	284193	23.58%	2.888%
44	7.283	1925	1926	1930	rVB2	905	434	0.04%	0.004%
45	7.338	1930	1943	1963	rBV	553422	964286	80.02%	9.800%
46	7.560	2010	2012	2016	rBV3	1828	1256	0.10%	0.013%
47	7.640	2027	2037	2060	rBV2	112601	196429	16.30%	1.996%
48	7.868	2105	2108	2110	rBV3	1999	1287	0.11%	0.013%
49	7.904	2117	2119	2123	rBV4	1812	1113	0.09%	0.011%
50	7.926	2123	2126	2128	rBV2	1821	1381	0.11%	0.014%
51	8.055	2163	2166	2168	rBV4	1017	722	0.06%	0.007%
52	8.109	2172	2183	2209	rBV	312015	597031	49.54%	6.068%
53	8.634	2342	2346	2350	rBV7	2371	1984	0.16%	0.020%
54	8.762	2384	2386	2387	rBV2	1119	442	0.04%	0.004%
55	8.785	2390	2393	2394	rBV2	1661	970	0.08%	0.010%
56	8.871	2408	2420	2437	rBV	649083	1052072	87.30%	10.692%
57	9.341	2563	2566	2567	rBV3	1181	650	0.05%	0.007%
58	9.383	2575	2579	2581	rBV3	1839	1398	0.12%	0.014%
59	9.428	2592	2593	2596	rVB4	2003	727	0.06%	0.007%
60	9.624	2650	2654	2656	rBV4	1538	871	0.07%	0.009%
61	9.881	2730	2734	2736	rBV4	1982	1689	0.14%	0.017%
62	10.109	2803	2805	2806	rBV2	1681	591	0.05%	0.006%
63	10.142	2812	2815	2816	rBV3	1273	676	0.06%	0.007%
64	10.238	2832	2845	2863	rBV	388880	603133	50.05%	6.130%
65	10.392	2889	2893	2896	rBV5	3725	3067	0.25%	0.031%
66	10.650	2969	2973	2978	rVB6	1809	1405	0.12%	0.014%
67	10.711	2989	2992	2996	rBV3	1700	1383	0.11%	0.014%
68	10.801	3018	3020	3023	rBV4	1664	997	0.08%	0.010%
69	11.209	3144	3147	3151	rBV4	1920	1616	0.13%	0.016%
70	11.270	3154	3166	3183	rBV	693490	1065353	88.40%	10.827%
71	11.476	3226	3230	3231	rBV4	1560	910	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016827.D
 Acq On : 11 Jun 2020 15:19
 Operator : SY/MD
 Sample : L2929-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3299	rBV	648820	1002501	83.19%	10.188%
73	11.878	3353	3355	3358	rBV3	1426	999	0.08%	0.010%
74	11.916	3364	3367	3368	rBV3	1345	748	0.06%	0.008%
75	12.141	3433	3437	3439	rBV5	1508	1273	0.11%	0.013%
76	12.238	3462	3467	3468	rBV4	1381	1145	0.10%	0.012%
77	12.360	3503	3505	3508	rBV3	2150	1719	0.14%	0.017%
78	12.415	3520	3522	3527	rBV4	998	817	0.07%	0.008%
79	12.460	3533	3536	3543	rVB8	1996	1785	0.15%	0.018%
80	12.492	3543	3546	3548	rBV2	1375	959	0.08%	0.010%
81	12.576	3567	3572	3575	rBV6	1928	2221	0.18%	0.023%
82	12.653	3594	3596	3598	rBV4	994	519	0.04%	0.005%
83	12.723	3615	3618	3621	rBV5	1166	1035	0.09%	0.011%
84	12.839	3652	3654	3660	rVB8	1445	945	0.08%	0.010%
85	12.871	3663	3664	3668	rVB3	1141	658	0.05%	0.007%
86	12.891	3668	3670	3677	rBV8	2004	2541	0.21%	0.026%
87	12.974	3694	3696	3699	rBV3	1632	1112	0.09%	0.011%
88	13.077	3722	3728	3730	rVV7	1324	1315	0.11%	0.013%
89	13.096	3730	3734	3738	rVB6	1849	1633	0.14%	0.017%
90	13.122	3739	3742	3743	rBV3	914	537	0.04%	0.005%
91	13.164	3751	3755	3756	rVB4	1677	1047	0.09%	0.011%
92	13.424	3832	3836	3838	rBV5	1819	1099	0.09%	0.011%
93	13.505	3855	3861	3863	rBV6	2045	2475	0.21%	0.025%
94	13.649	3904	3906	3910	rBV4	1538	1315	0.11%	0.013%
95	13.823	3959	3960	3961	rBV	1273	392	0.03%	0.004%
96	13.897	3977	3983	3984	rBV5	2045	1685	0.14%	0.017%
97	13.926	3990	3992	3994	rBV3	908	574	0.05%	0.006%
98	14.010	4016	4018	4020	rBV3	1162	370	0.03%	0.004%
99	14.537	4179	4182	4184	rBV3	1970	1231	0.10%	0.013%
100	15.492	4477	4479	4480	rBV2	1615	449	0.04%	0.005%


Sum of corrected areas: 9839734

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016827.D
Acq On : 11 Jun 2020 15:19
Operator : SY/MD
Sample : L2929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

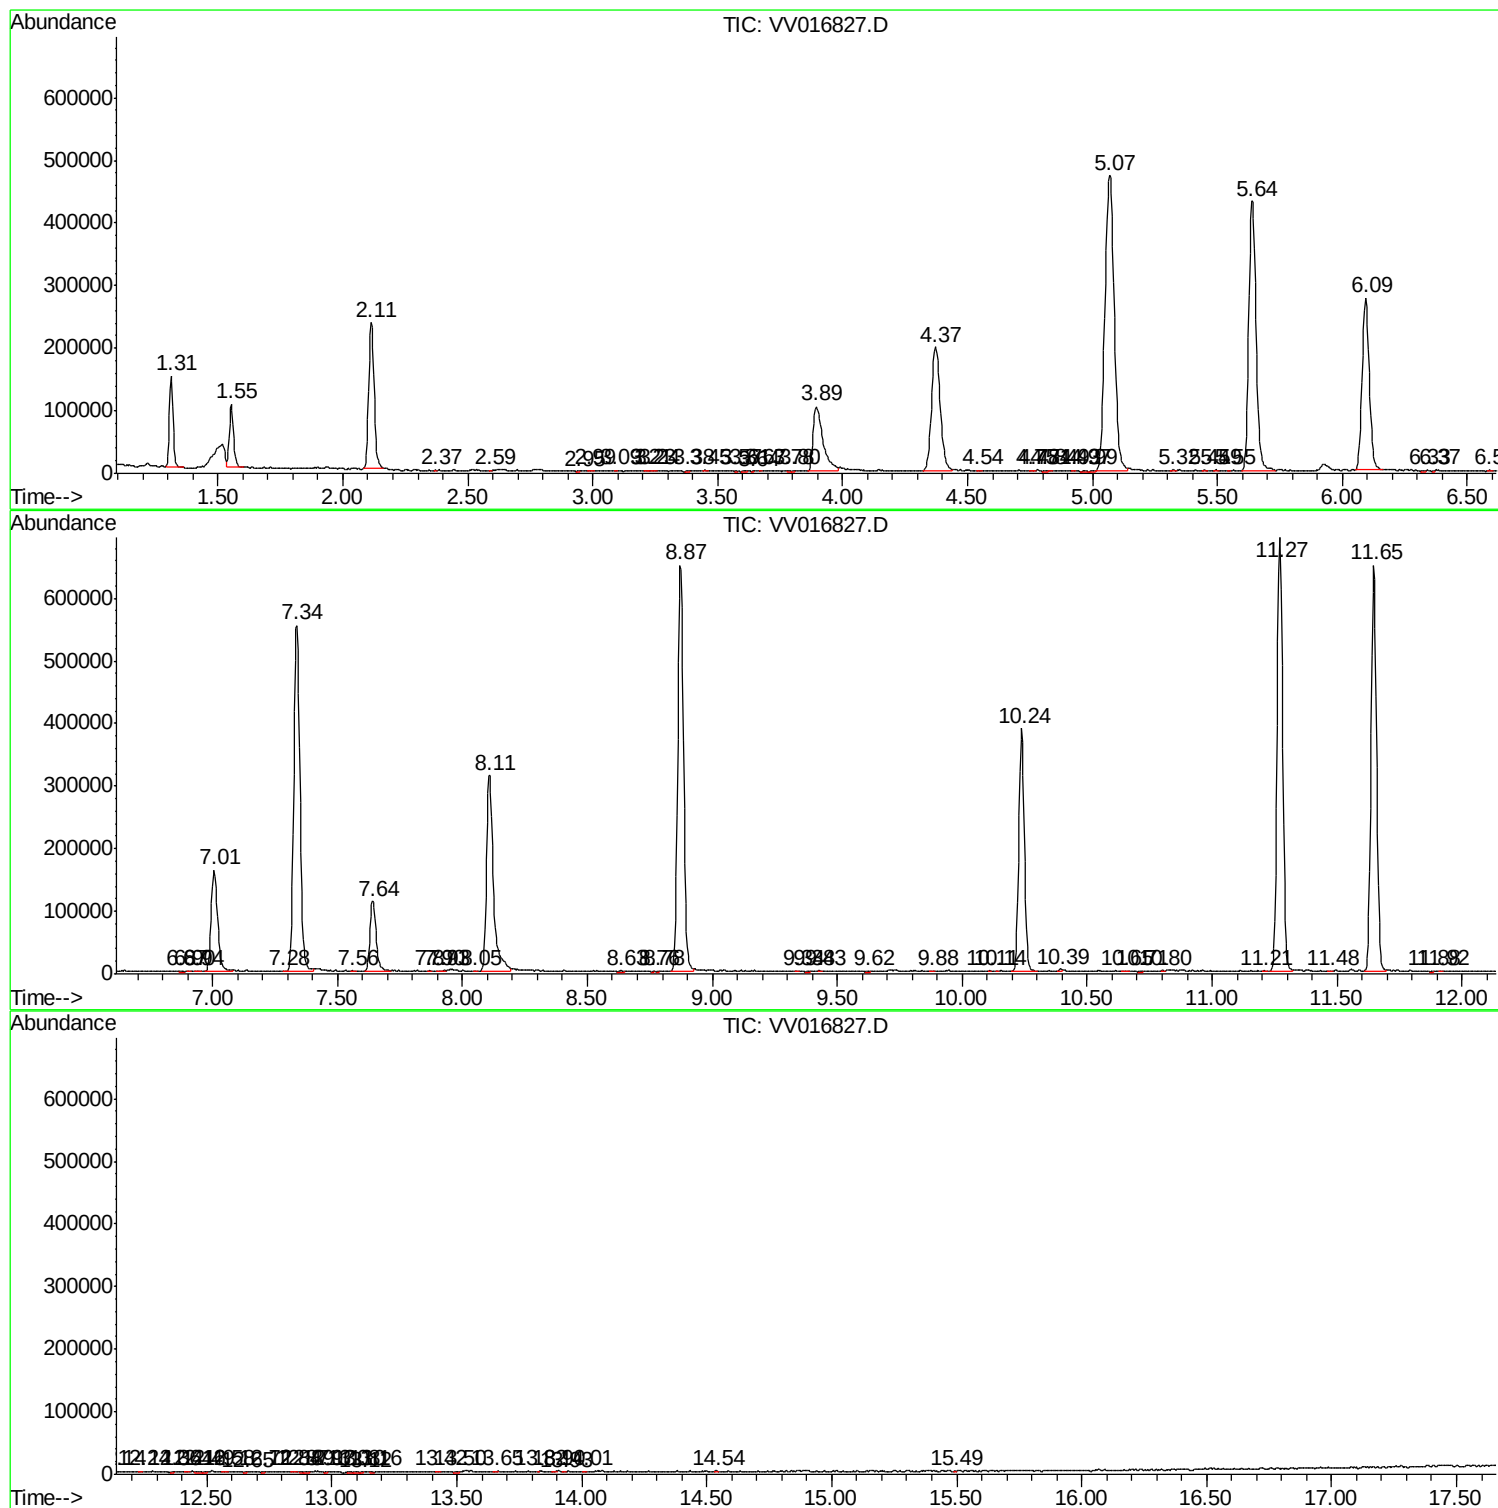

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016827.D
Acq On : 11 Jun 2020 15:19
Operator : SY/MD
Sample : L2929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016827.D
Acq On : 11 Jun 2020 15:19
Operator : SY/MD
Sample : L2929-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc