

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016831.D
 Acq On : 11 Jun 2020 16:53
 Operator : SY/MD
 Sample : L2929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	148084	149743	11.94%	1.489%
2	1.563	140	147	160	rVB	106581	128276	10.23%	1.276%
3	2.116	310	319	333	rBV	232392	339781	27.10%	3.379%
4	2.245	357	359	360	rBV2	1597	640	0.05%	0.006%
5	2.418	411	413	417	rVB3	1747	831	0.07%	0.008%
6	2.746	511	515	518	rBV5	1280	1189	0.09%	0.012%
7	2.807	531	534	539	rBV7	1536	1421	0.11%	0.014%
8	2.891	557	560	564	rBV3	1539	1361	0.11%	0.014%
9	3.097	622	624	625	rBV2	1474	657	0.05%	0.007%
10	3.174	646	648	652	rVB3	1468	1009	0.08%	0.010%
11	3.193	652	654	655	rBV2	1545	722	0.06%	0.007%
12	3.264	673	676	679	rBV5	1236	958	0.08%	0.010%
13	3.405	716	720	722	rBV5	1738	1536	0.12%	0.015%
14	3.457	733	736	739	rBV4	1124	740	0.06%	0.007%
15	3.495	745	748	754	rBV6	1499	1442	0.12%	0.014%
16	3.524	754	757	761	rVB5	1444	1026	0.08%	0.010%
17	3.740	820	824	825	rBV4	1446	878	0.07%	0.009%
18	3.811	843	846	851	rBV6	1386	791	0.06%	0.008%
19	3.894	862	872	899	rBV	104604	282046	22.49%	2.805%
20	4.373	1007	1021	1043	rVB	206794	498945	39.79%	4.962%
21	4.547	1071	1075	1084	rBV10	2972	3422	0.27%	0.034%
22	4.582	1084	1086	1087	rBV2	1327	633	0.05%	0.006%
23	4.772	1142	1145	1150	rVB6	2051	1867	0.15%	0.019%
24	4.801	1150	1154	1155	rBV2	1507	1088	0.09%	0.011%
25	4.862	1168	1173	1175	rVB5	1556	1184	0.09%	0.012%
26	4.923	1188	1192	1194	rVB5	1413	1067	0.09%	0.011%
27	4.946	1196	1199	1202	rBV5	1302	861	0.07%	0.009%
28	5.068	1221	1237	1261	rBV2	494389	1253876	100.00%	12.469%
29	5.402	1339	1341	1344	rBV3	1154	806	0.06%	0.008%
30	5.640	1402	1415	1440	rVV	441867	877400	69.98%	8.725%
31	5.794	1461	1463	1465	rBV3	1494	676	0.05%	0.007%
32	5.862	1482	1484	1486	rBV3	1615	967	0.08%	0.010%
33	5.926	1497	1504	1517	rVB3	12224	22860	1.82%	0.227%
34	6.010	1528	1530	1535	rBV6	1509	1062	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016831.D
 Acq On : 11 Jun 2020 16:53
 Operator : SY/MD
 Sample : L2929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.090	1542	1555	1574	rBV	282290	572394	45.65%	5.692%
36	6.479	1673	1676	1678	rBV3	1840	1044	0.08%	0.010%
37	6.521	1687	1689	1693	rBV4	824	630	0.05%	0.006%
38	6.637	1719	1725	1728	rBV7	2085	1877	0.15%	0.019%
39	6.823	1779	1783	1785	rBV5	1250	1017	0.08%	0.010%
40	6.881	1797	1801	1805	rBV7	1789	1518	0.12%	0.015%
41	7.007	1827	1840	1855	rBV2	159856	290632	23.18%	2.890%
42	7.293	1924	1929	1930	rBV5	1121	857	0.07%	0.009%
43	7.338	1930	1943	1960	rBV	575271	986233	78.65%	9.807%
44	7.640	2027	2037	2057	rBV	118077	200822	16.02%	1.997%
45	7.836	2095	2098	2100	rBV3	1677	1321	0.11%	0.013%
46	7.884	2109	2113	2116	rBV4	1888	1822	0.15%	0.018%
47	8.052	2163	2165	2169	rVB4	1632	959	0.08%	0.010%
48	8.106	2170	2182	2215	rBV	316935	614644	49.02%	6.112%
49	8.402	2272	2274	2276	rBV3	1381	940	0.07%	0.009%
50	8.524	2308	2312	2313	rBV4	1015	722	0.06%	0.007%
51	8.627	2342	2344	2347	rVB3	1468	707	0.06%	0.007%
52	8.871	2407	2420	2436	rBV	670419	1073896	85.65%	10.679%
53	9.174	2508	2514	2516	rBV6	2402	2637	0.21%	0.026%
54	9.354	2566	2570	2573	rVB6	2815	2230	0.18%	0.022%
55	9.389	2573	2581	2582	rBV8	1973	2057	0.16%	0.020%
56	9.457	2595	2602	2605	rBV8	1957	2553	0.20%	0.025%
57	9.579	2638	2640	2647	rVB7	1876	1534	0.12%	0.015%
58	9.650	2660	2662	2667	rVB4	1744	1274	0.10%	0.013%
59	9.759	2692	2696	2700	rBV	4248	2791	0.22%	0.028%
60	9.823	2713	2716	2717	rVV3	1365	771	0.06%	0.008%
61	9.855	2723	2726	2729	rBV5	929	646	0.05%	0.006%
62	9.923	2744	2747	2750	rBV5	1190	645	0.05%	0.006%
63	9.968	2755	2761	2764	rVB6	1796	1897	0.15%	0.019%
64	10.048	2784	2786	2789	rVB4	1323	865	0.07%	0.009%
65	10.238	2834	2845	2864	rVB	390689	607441	48.45%	6.040%
66	10.389	2889	2892	2894	rBV3	2467	1574	0.13%	0.016%
67	11.000	3079	3082	3084	rBV4	1698	1115	0.09%	0.011%
68	11.064	3100	3102	3105	rBV3	1726	808	0.06%	0.008%
69	11.129	3118	3122	3125	rVB5	1876	1376	0.11%	0.014%
70	11.270	3154	3166	3181	rBV	680847	1043254	83.20%	10.374%
71	11.553	3248	3254	3263	rBV	6328	10100	0.81%	0.100%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016831.D
 Acq On : 11 Jun 2020 16:53
 Operator : SY/MD
 Sample : L2929-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3270	3283	3299	rBV	640123	1003119	80.00%	9.975%
73	11.949	3375	3377	3384	rBV5	1096	1017	0.08%	0.010%
74	11.981	3384	3387	3388	rBV3	1619	762	0.06%	0.008%
75	12.029	3400	3402	3406	rVB5	1381	894	0.07%	0.009%
76	12.048	3406	3408	3411	rBV4	1505	873	0.07%	0.009%
77	12.064	3411	3413	3416	rBV4	1317	756	0.06%	0.008%
78	12.132	3431	3434	3435	rBV3	2853	1387	0.11%	0.014%
79	12.254	3470	3472	3475	rBV4	1778	1446	0.12%	0.014%
80	12.437	3527	3529	3533	rVB4	1132	791	0.06%	0.008%
81	12.514	3548	3553	3556	rBV7	2499	2603	0.21%	0.026%
82	12.756	3623	3628	3632	rVB7	1563	1452	0.12%	0.014%
83	13.067	3723	3725	3726	rBV2	1918	683	0.05%	0.007%
84	13.158	3750	3753	3755	rBV3	1004	665	0.05%	0.007%
85	13.238	3773	3778	3781	rBV6	1259	1175	0.09%	0.012%
86	13.357	3809	3815	3819	rBV8	1585	1683	0.13%	0.017%
87	13.595	3887	3889	3891	rBV3	1328	735	0.06%	0.007%
88	13.955	3996	4001	4004	rBV7	1368	1517	0.12%	0.015%
89	14.080	4038	4040	4044	rVB3	2680	1148	0.09%	0.011%
90	14.112	4048	4050	4056	rVV8	1688	1108	0.09%	0.011%
91	14.511	4171	4174	4175	rBV3	1182	641	0.05%	0.006%
92	14.534	4179	4181	4184	rVB4	1585	713	0.06%	0.007%
93	14.611	4203	4205	4207	rBV3	1357	693	0.06%	0.007%
94	14.675	4221	4225	4228	rBV5	2809	2255	0.18%	0.022%
95	14.916	4297	4300	4303	rBV5	2042	1407	0.11%	0.014%
96	14.939	4305	4307	4311	rVB5	1561	684	0.05%	0.007%
97	14.964	4311	4315	4318	rBV3	1328	1362	0.11%	0.014%
98	15.685	4537	4539	4544	rBV5	1958	1322	0.11%	0.013%
99	15.755	4558	4561	4567	rBV6	2063	2699	0.22%	0.027%
100	16.218	4703	4705	4708	rBV4	2331	1321	0.11%	0.013%


Sum of corrected areas: 10056275

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016831.D
Acq On : 11 Jun 2020 16:53
Operator : SY/MD
Sample : L2929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

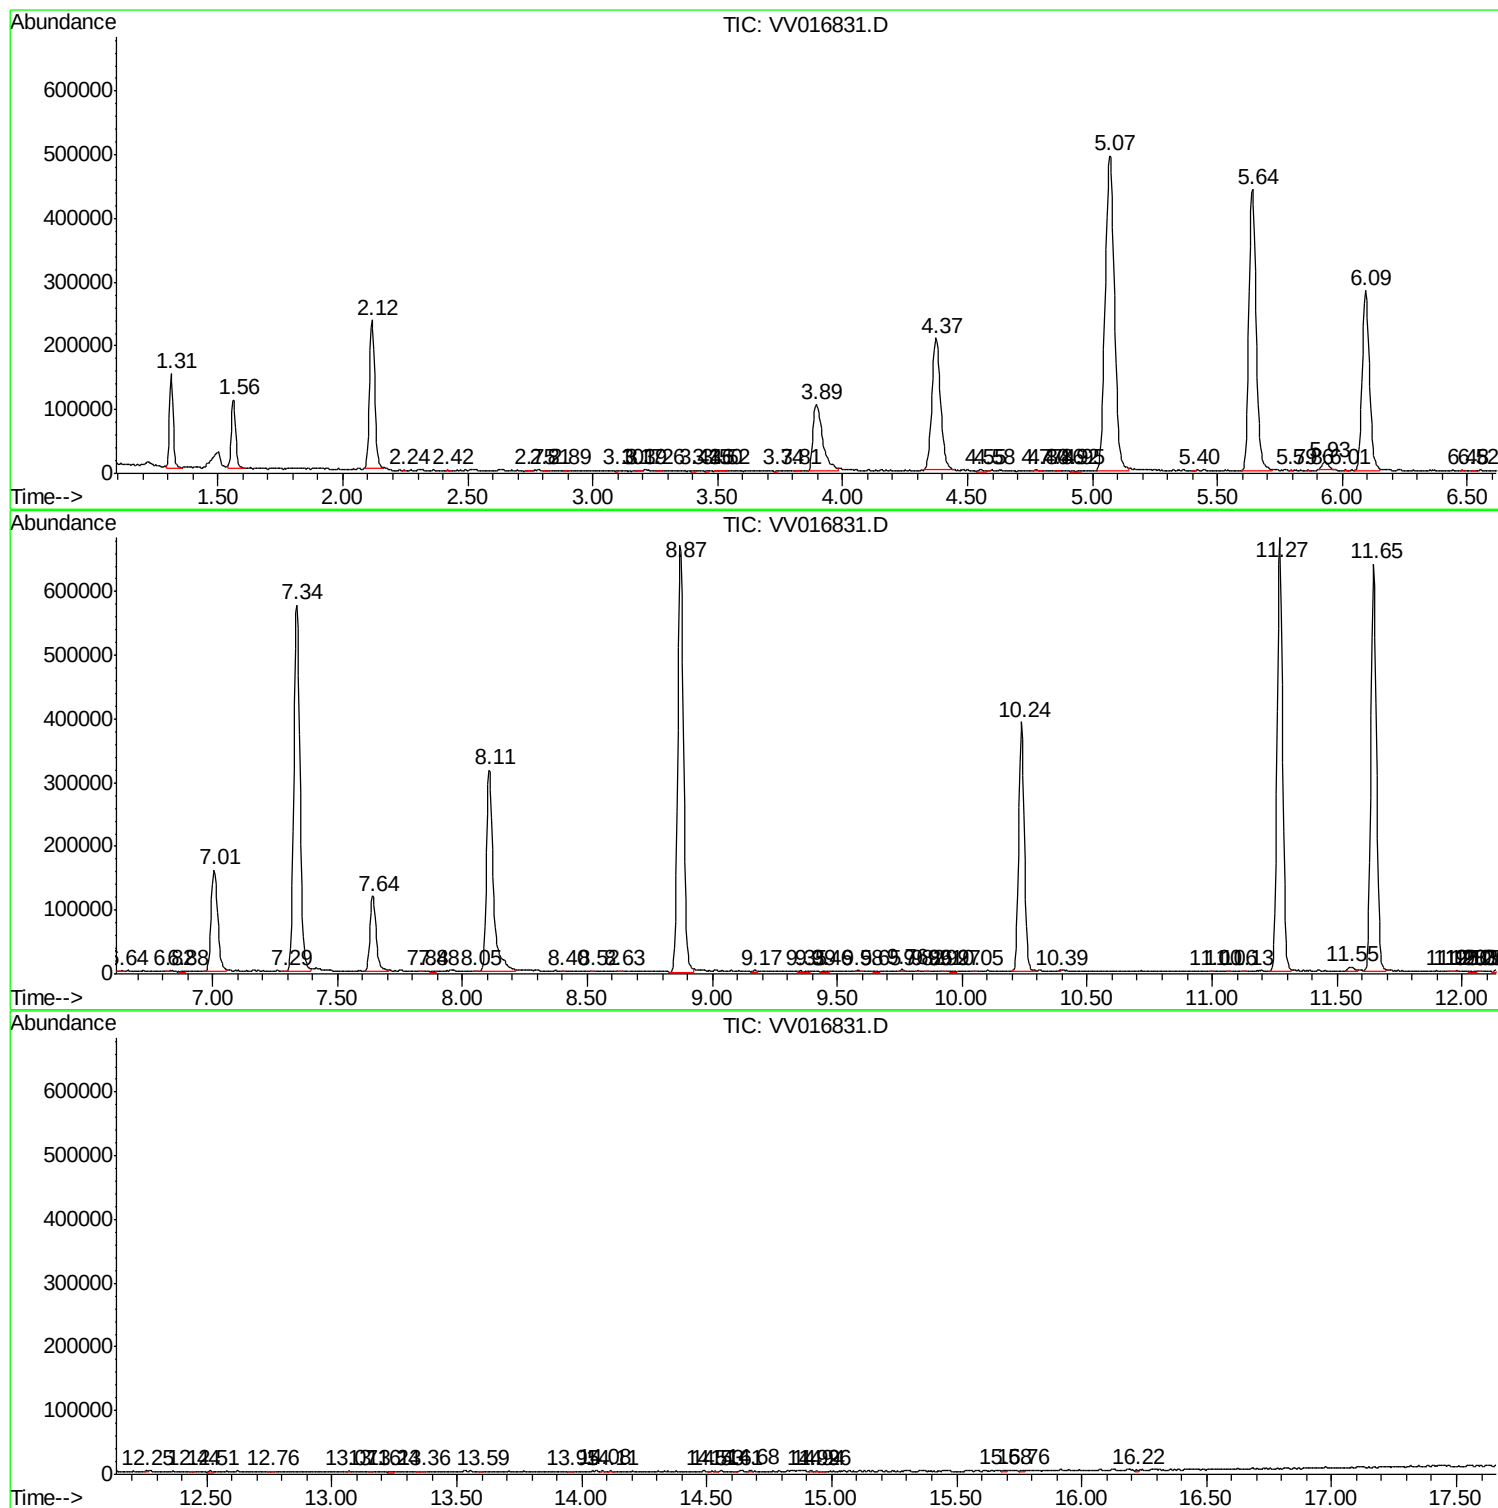

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016831.D
Acq On : 11 Jun 2020 16:53
Operator : SY/MD
Sample : L2929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016831.D
Acq On : 11 Jun 2020 16:53
Operator : SY/MD
Sample : L2929-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTX7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc