

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016834.D
 Acq On : 11 Jun 2020 18:04
 Operator : SY/MD
 Sample : L2929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	151366	147558	12.17%	1.496%
2	1.560	139	146	157	rVB	104582	125203	10.33%	1.269%
3	2.116	310	319	332	rBV	230224	334664	27.60%	3.393%
4	2.290	364	373	379	rBV3	7974	15214	1.25%	0.154%
5	2.608	470	472	475	rBV4	2107	1120	0.09%	0.011%
6	2.720	505	507	510	rVB3	1818	908	0.07%	0.009%
7	2.740	510	513	514	rBV2	1227	729	0.06%	0.007%
8	3.257	671	674	676	rBV3	1240	765	0.06%	0.008%
9	3.296	679	686	687	rBV6	1065	1100	0.09%	0.011%
10	3.476	739	742	743	rBV2	1066	679	0.06%	0.007%
11	3.618	784	786	790	rBV5	1061	679	0.06%	0.007%
12	3.672	798	803	804	rBV4	2069	1239	0.10%	0.013%
13	3.798	838	842	844	rBV4	2161	1518	0.13%	0.015%
14	3.810	844	846	848	rVV2	1665	960	0.08%	0.010%
15	3.894	862	872	900	rBV2	96890	262692	21.66%	2.664%
16	4.090	931	933	935	rBV3	1929	1108	0.09%	0.011%
17	4.216	969	972	975	rBV5	1240	760	0.06%	0.008%
18	4.373	1005	1021	1042	rBV2	198101	491480	40.53%	4.983%
19	4.618	1094	1097	1102	rVB6	2183	1322	0.11%	0.013%
20	4.701	1120	1123	1126	rBV5	2355	1390	0.11%	0.014%
21	4.749	1135	1138	1141	rVB4	1768	1008	0.08%	0.010%
22	4.775	1141	1146	1148	rBV4	1656	1231	0.10%	0.012%
23	5.068	1220	1237	1262	rBV2	470998	1212533	100.00%	12.294%
24	5.347	1321	1324	1326	rBV5	1695	1278	0.11%	0.013%
25	5.421	1345	1347	1350	rBV4	1394	920	0.08%	0.009%
26	5.457	1355	1358	1363	rBV7	2306	2112	0.17%	0.021%
27	5.495	1368	1370	1372	rBV3	1300	711	0.06%	0.007%
28	5.640	1402	1415	1438	rBV	442588	872730	71.98%	8.849%
29	5.801	1463	1465	1467	rBV3	1853	935	0.08%	0.009%
30	5.929	1495	1505	1515	rBV4	13729	29557	2.44%	0.300%
31	6.093	1543	1556	1575	rBV	280914	556850	45.92%	5.646%
32	6.498	1678	1682	1683	rBV4	2024	1504	0.12%	0.015%
33	6.563	1700	1702	1704	rBV3	1520	684	0.06%	0.007%
34	6.711	1746	1748	1750	rBV2	1522	976	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016834.D
 Acq On : 11 Jun 2020 18:04
 Operator : SY/MD
 Sample : L2929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.801	1774	1776	1778	rVB2	1766	722	0.06%	0.007%
36	6.826	1781	1784	1786	rBV4	1810	1274	0.11%	0.013%
37	6.855	1790	1793	1795	rBV3	1305	839	0.07%	0.009%
38	7.007	1827	1840	1860	rBV	157840	286934	23.66%	2.909%
39	7.251	1914	1916	1921	rVB6	1569	1063	0.09%	0.011%
40	7.277	1921	1924	1929	rBV5	1010	762	0.06%	0.008%
41	7.338	1929	1943	1962	rBV	560037	965402	79.62%	9.789%
42	7.640	2028	2037	2052	rBV	112237	184819	15.24%	1.874%
43	7.839	2096	2099	2100	rBV3	1270	707	0.06%	0.007%
44	7.997	2145	2148	2153	rBV8	1269	1404	0.12%	0.014%
45	8.106	2172	2182	2219	rVV	302297	583680	48.14%	5.918%
46	8.328	2248	2251	2254	rBV6	1341	781	0.06%	0.008%
47	8.457	2287	2291	2292	rBV4	1137	850	0.07%	0.009%
48	8.492	2299	2302	2304	rBV4	2111	1518	0.13%	0.015%
49	8.566	2322	2325	2329	rVB4	1586	1177	0.10%	0.012%
50	8.592	2329	2333	2334	rBV3	1085	739	0.06%	0.007%
51	8.640	2344	2348	2349	rBV4	1647	1121	0.09%	0.011%
52	8.682	2358	2361	2365	rBV4	1227	993	0.08%	0.010%
53	8.871	2408	2420	2440	rBV	655727	1064559	87.80%	10.794%
54	9.209	2522	2525	2526	rBV2	2141	1088	0.09%	0.011%
55	9.280	2543	2547	2548	rBV4	1846	1406	0.12%	0.014%
56	9.431	2590	2594	2596	rBV5	1809	1075	0.09%	0.011%
57	9.653	2661	2663	2666	rVB3	1905	1155	0.10%	0.012%
58	9.675	2666	2670	2673	rBV5	1449	1083	0.09%	0.011%
59	9.704	2677	2679	2681	rVB3	1738	782	0.06%	0.008%
60	9.717	2681	2683	2685	rBV2	1410	791	0.07%	0.008%
61	9.804	2708	2710	2712	rBV3	2286	1249	0.10%	0.013%
62	9.868	2728	2730	2734	rVB4	1191	681	0.06%	0.007%
63	9.887	2734	2736	2739	rBV4	1160	763	0.06%	0.008%
64	10.238	2834	2845	2859	rVV	373786	585654	48.30%	5.938%
65	10.508	2926	2929	2931	rBV4	1612	1069	0.09%	0.011%
66	10.601	2953	2958	2959	rBV4	1426	1017	0.08%	0.010%
67	10.833	3027	3030	3032	rBV3	1703	1197	0.10%	0.012%
68	10.910	3051	3054	3058	rBV5	1541	1182	0.10%	0.012%
69	10.936	3061	3062	3065	rBV3	1801	954	0.08%	0.010%
70	11.132	3120	3123	3126	rVB4	2133	1236	0.10%	0.013%
71	11.151	3126	3129	3132	rBV4	1853	1227	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016834.D
 Acq On : 11 Jun 2020 18:04
 Operator : SY/MD
 Sample : L2929-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3185	rBV	685829	1057728	87.23%	10.725%
73	11.376	3197	3199	3202	rBV3	2438	1348	0.11%	0.014%
74	11.408	3207	3209	3213	rVB5	1743	815	0.07%	0.008%
75	11.646	3271	3283	3302	rBV	630577	993663	81.95%	10.075%
76	11.891	3354	3359	3361	rBV7	2232	1521	0.13%	0.015%
77	11.955	3374	3379	3382	rBV6	2000	2041	0.17%	0.021%
78	12.026	3398	3401	3402	rBV3	1343	844	0.07%	0.009%
79	12.119	3427	3430	3434	rVB5	1221	780	0.06%	0.008%
80	12.183	3443	3450	3453	rBV9	1411	1601	0.13%	0.016%
81	12.257	3469	3473	3476	rBV4	1377	1101	0.09%	0.011%
82	12.370	3505	3508	3510	rBV3	2407	1619	0.13%	0.016%
83	12.492	3543	3546	3551	rBV6	1886	2087	0.17%	0.021%
84	12.514	3551	3553	3556	rBV3	1624	964	0.08%	0.010%
85	12.595	3572	3578	3580	rBV7	1535	1475	0.12%	0.015%
86	12.900	3670	3673	3675	rBV4	1841	1255	0.10%	0.013%
87	12.929	3680	3682	3684	rVB3	1429	677	0.06%	0.007%
88	13.006	3699	3706	3709	rBV7	1397	1877	0.15%	0.019%
89	13.148	3744	3750	3755	rBV9	1998	2485	0.20%	0.025%
90	13.289	3790	3794	3796	rBV5	1147	1025	0.08%	0.010%
91	13.527	3866	3868	3869	rBV	1550	684	0.06%	0.007%
92	13.710	3922	3925	3926	rBV3	1775	727	0.06%	0.007%
93	13.772	3938	3944	3947	rBV7	1703	2047	0.17%	0.021%
94	13.810	3953	3956	3961	rBV6	1471	1424	0.12%	0.014%
95	13.868	3971	3974	3978	rBV6	1152	1047	0.09%	0.011%
96	14.003	4013	4016	4019	rVB3	1831	1072	0.09%	0.011%
97	14.141	4057	4059	4064	rVB4	1405	783	0.06%	0.008%
98	14.164	4064	4066	4070	rBV6	1332	753	0.06%	0.008%
99	14.926	4300	4303	4305	rBV2	2491	1350	0.11%	0.014%
100	15.164	4375	4377	4381	rVB4	1666	708	0.06%	0.007%


Sum of corrected areas: 9862571

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016834.D
Acq On : 11 Jun 2020 18:04
Operator : SY/MD
Sample : L2929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

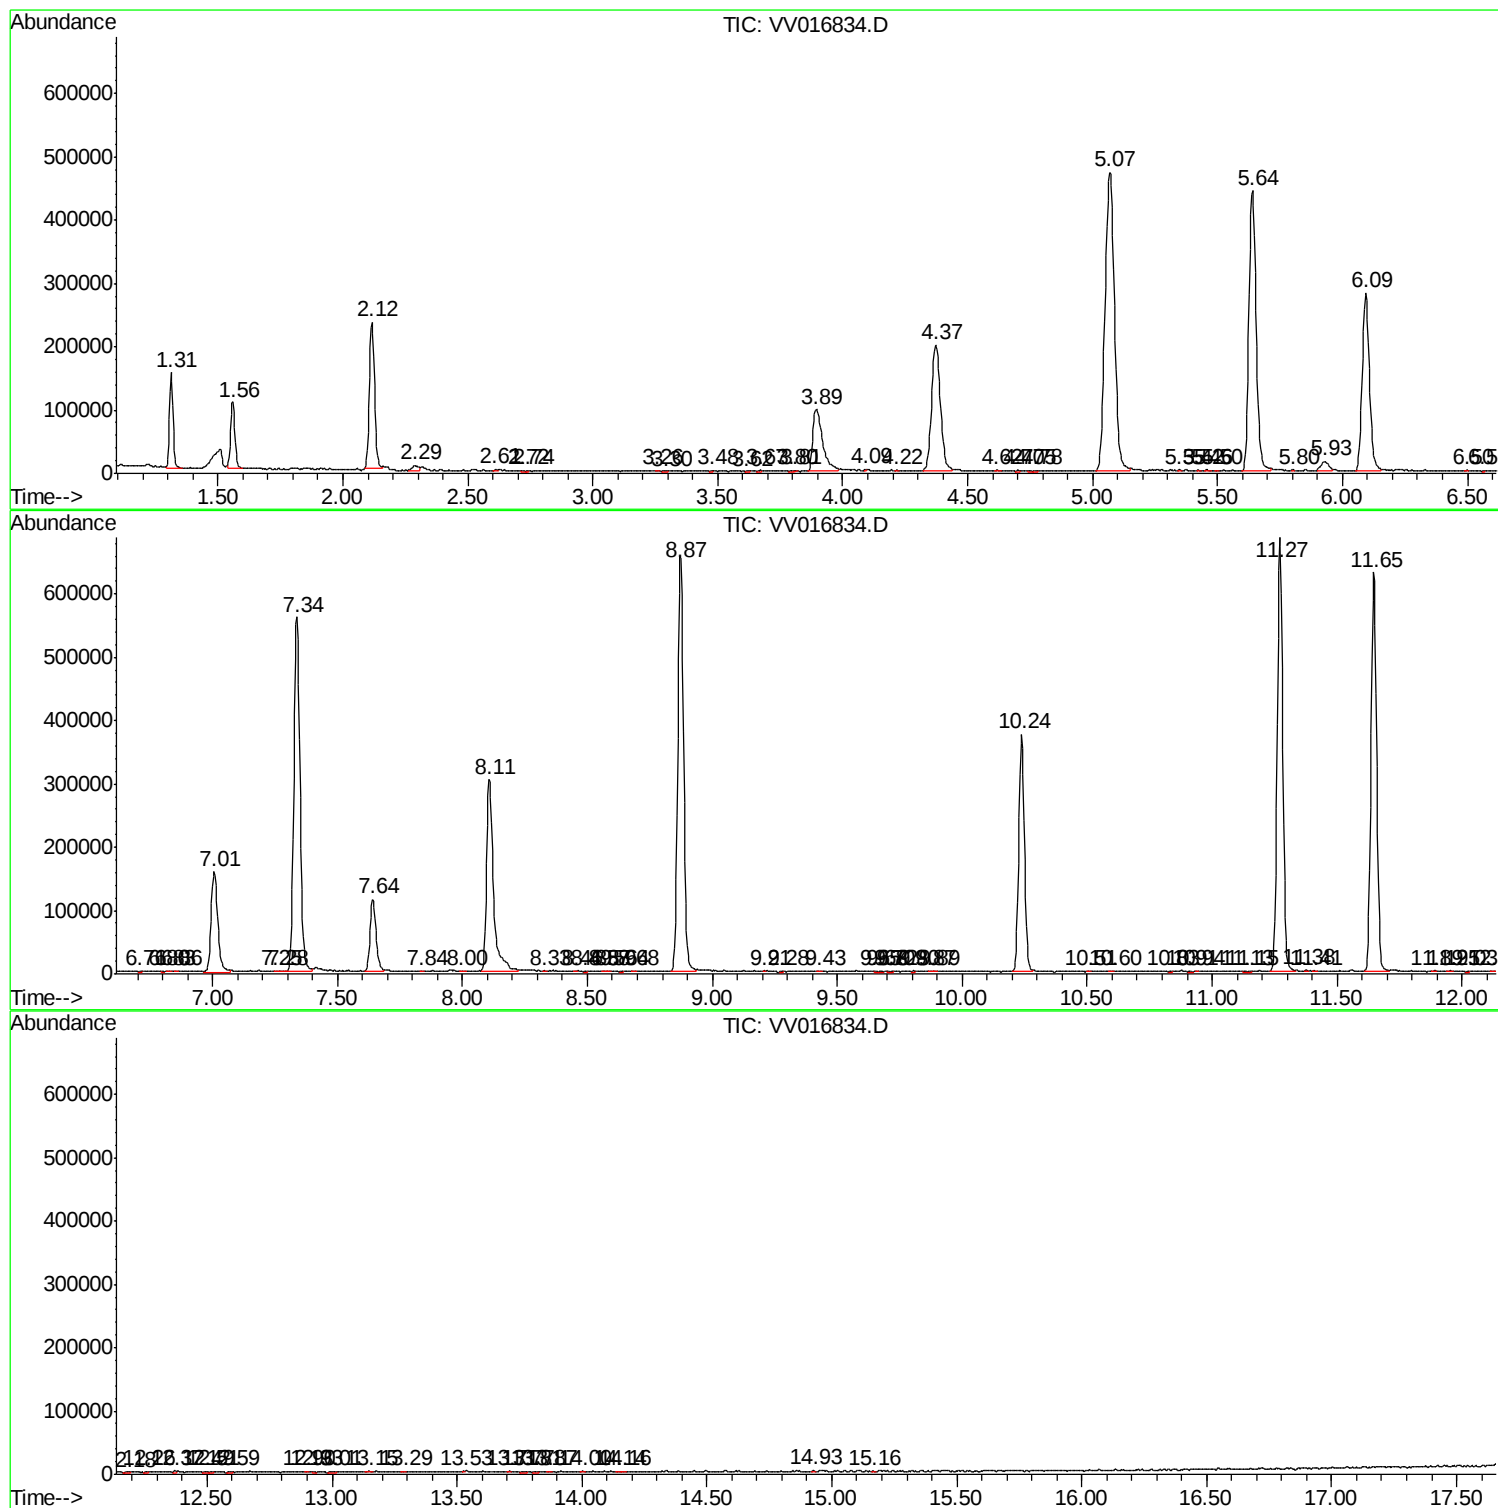

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016834.D
Acq On : 11 Jun 2020 18:04
Operator : SY/MD
Sample : L2929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016834.D
Acq On : 11 Jun 2020 18:04
Operator : SY/MD
Sample : L2929-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTW7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc