

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016835.D
 Acq On : 11 Jun 2020 18:28
 Operator : SY/MD
 Sample : L2914-05DL 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	80	rVV	188135	198478	17.08%	1.935%
2	1.364	80	85	93	rVB	25755	24166	2.08%	0.236%
3	1.422	98	103	108	rBV	21389	19571	1.68%	0.191%
4	1.553	138	144	157	rVB	103237	127484	10.97%	1.243%
5	2.113	310	318	333	rVB	224407	329638	28.37%	3.214%
6	2.425	414	415	417	rBV2	1394	660	0.06%	0.006%
7	2.862	549	551	554	rVB4	1205	528	0.05%	0.005%
8	2.881	554	557	559	rBV3	1136	789	0.07%	0.008%
9	2.914	565	567	569	rBV3	1054	409	0.04%	0.004%
10	2.949	575	578	580	rBV4	1888	1198	0.10%	0.012%
11	3.029	601	603	605	rBV2	1128	508	0.04%	0.005%
12	3.123	627	632	635	rBV6	2159	2104	0.18%	0.021%
13	3.139	635	637	640	rVV4	1858	1126	0.10%	0.011%
14	3.164	642	645	649	rVB4	1628	1373	0.12%	0.013%
15	3.225	660	664	666	rBV4	1765	1619	0.14%	0.016%
16	3.293	682	685	686	rBV3	1775	1140	0.10%	0.011%
17	3.344	697	701	703	rBV4	1862	1337	0.12%	0.013%
18	3.399	715	718	720	rBV3	1471	816	0.07%	0.008%
19	3.573	770	772	775	rBV3	1361	838	0.07%	0.008%
20	3.708	811	814	817	rBV5	2366	1461	0.13%	0.014%
21	3.894	861	872	897	rBV	102114	285010	24.53%	2.779%
22	4.373	1005	1021	1040	rBV	205744	502566	43.25%	4.900%
23	4.598	1087	1091	1092	rBV3	1365	788	0.07%	0.008%
24	4.910	1185	1188	1190	rBV4	997	580	0.05%	0.006%
25	5.068	1220	1237	1244	rBV2	479411	1161963	100.00%	11.329%
26	5.640	1402	1415	1439	rBV	421427	840978	72.38%	8.199%
27	5.801	1463	1465	1468	rVB3	1693	874	0.08%	0.009%
28	5.827	1471	1473	1477	rBV4	1201	749	0.06%	0.007%
29	5.926	1496	1504	1524	rVB5	14734	32334	2.78%	0.315%
30	6.093	1544	1556	1572	rBV	274736	548639	47.22%	5.349%
31	6.299	1617	1620	1626	rVB8	1517	1467	0.13%	0.014%
32	6.386	1645	1647	1649	rBV3	1613	949	0.08%	0.009%
33	6.486	1674	1678	1682	rVB7	1223	1032	0.09%	0.010%
34	6.534	1691	1693	1694	rBV2	1207	454	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016835.D
 Acq On : 11 Jun 2020 18:28
 Operator : SY/MD
 Sample : L2914-05DL 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.566	1698	1703	1705	rBV6	2103	2012	0.17%	0.020%
36	6.810	1776	1779	1782	rBV5	2142	1811	0.16%	0.018%
37	6.891	1802	1804	1806	rBV3	1037	518	0.04%	0.005%
38	7.007	1829	1840	1856	rBV2	161208	287727	24.76%	2.805%
39	7.286	1926	1927	1930	rVB3	2038	905	0.08%	0.009%
40	7.338	1930	1943	1957	rBV	560936	963470	82.92%	9.393%
41	7.640	2027	2037	2051	rBV	114588	193369	16.64%	1.885%
42	7.965	2136	2138	2141	rVB4	1691	746	0.06%	0.007%
43	7.984	2142	2144	2147	rVV4	1338	695	0.06%	0.007%
44	8.013	2150	2153	2155	rBV4	1715	943	0.08%	0.009%
45	8.045	2160	2163	2167	rBV6	1556	1228	0.11%	0.012%
46	8.109	2171	2183	2214	rBV2	303487	604246	52.00%	5.891%
47	8.505	2304	2306	2307	rBV	1398	602	0.05%	0.006%
48	8.666	2352	2356	2359	rBV5	1600	1133	0.10%	0.011%
49	8.740	2377	2379	2382	rBV4	712	471	0.04%	0.005%
50	8.785	2391	2393	2398	rVB6	2883	1971	0.17%	0.019%
51	8.814	2398	2402	2405	rBV7	2934	2214	0.19%	0.022%
52	8.871	2409	2420	2431	rBV	649874	1035057	89.08%	10.091%
53	9.035	2464	2471	2482	rVB	26297	41274	3.55%	0.402%
54	9.161	2502	2510	2529	rVB	68464	121380	10.45%	1.183%
55	9.248	2534	2537	2538	rBV3	1659	835	0.07%	0.008%
56	9.283	2538	2548	2555	rBV3	11014	18868	1.62%	0.184%
57	9.405	2578	2586	2596	rBV6	11325	20655	1.78%	0.201%
58	9.640	2656	2659	2661	rBV4	1382	1043	0.09%	0.010%
59	9.736	2677	2689	2702	rBV4	5965	13654	1.18%	0.133%
60	10.055	2786	2788	2789	rBV2	925	405	0.03%	0.004%
61	10.151	2816	2818	2821	rBV2	1277	898	0.08%	0.009%
62	10.193	2829	2831	2833	rBV3	1091	607	0.05%	0.006%
63	10.238	2833	2845	2860	rVV	390556	606949	52.23%	5.917%
64	10.338	2872	2876	2877	rBV3	3080	2268	0.20%	0.022%
65	10.656	2972	2975	2978	rBV5	1810	1477	0.13%	0.014%
66	10.682	2979	2983	2985	rVV5	1419	1176	0.10%	0.011%
67	10.936	3055	3062	3073	rBV	28401	44048	3.79%	0.429%
68	11.270	3154	3166	3179	rBV	696333	1064640	91.62%	10.380%
69	11.550	3244	3253	3264	rBV2	13971	25376	2.18%	0.247%
70	11.646	3273	3283	3306	rVB	665573	1025199	88.23%	9.995%
71	11.733	3308	3310	3312	rBV2	1508	895	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016835.D
 Acq On : 11 Jun 2020 18:28
 Operator : SY/MD
 Sample : L2914-05DL 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E00DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.209	3456	3458	3459	rBV2	1164	388	0.03%	0.004%
73	12.251	3469	3471	3473	rBV3	1452	793	0.07%	0.008%
74	12.293	3482	3484	3485	rBV2	1368	760	0.07%	0.007%
75	12.701	3608	3611	3612	rBV3	1741	704	0.06%	0.007%
76	12.846	3654	3656	3658	rBV3	1247	664	0.06%	0.006%
77	12.907	3666	3675	3685	rBV3	9387	15934	1.37%	0.155%
78	13.022	3707	3711	3713	rBV3	910	588	0.05%	0.006%
79	13.048	3717	3719	3720	rBV2	1201	582	0.05%	0.006%
80	13.186	3760	3762	3765	rBV4	1116	671	0.06%	0.007%
81	13.206	3765	3768	3769	rBV3	1112	731	0.06%	0.007%
82	13.325	3802	3805	3807	rBV3	1560	1028	0.09%	0.010%
83	13.463	3846	3848	3853	rVB5	2117	1474	0.13%	0.014%
84	13.527	3860	3868	3882	rVB	16899	29044	2.50%	0.283%
85	13.649	3899	3906	3913	rBV9	3616	5448	0.47%	0.053%
86	13.717	3925	3927	3929	rBV3	776	405	0.03%	0.004%
87	13.752	3936	3938	3939	rBV2	1072	356	0.03%	0.003%
88	13.836	3960	3964	3968	rBV7	1193	1234	0.11%	0.012%
89	13.929	3991	3993	3996	rBV3	864	431	0.04%	0.004%
90	14.016	4017	4020	4025	rBV5	1955	1626	0.14%	0.016%
91	14.038	4025	4027	4030	rBV4	1521	1077	0.09%	0.011%
92	14.164	4062	4066	4067	rBV3	1450	983	0.08%	0.010%
93	14.325	4114	4116	4118	rVB3	1266	558	0.05%	0.005%
94	14.344	4118	4122	4126	rBV6	1044	731	0.06%	0.007%
95	14.437	4149	4151	4153	rBV3	1130	591	0.05%	0.006%
96	14.476	4159	4163	4167	rBV6	1865	1482	0.13%	0.014%
97	14.495	4167	4169	4173	rVB4	1775	1302	0.11%	0.013%
98	14.546	4183	4185	4189	rVB4	1928	1086	0.09%	0.011%
99	14.563	4189	4190	4193	rBV3	1675	844	0.07%	0.008%
100	14.804	4261	4265	4266	rBV4	1560	990	0.09%	0.010%


Sum of corrected areas: 10256896

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061120\
Data File : VV016835.D
Acq On : 11 Jun 2020 18:28
Operator : SY/MD
Sample : L2914-05DL 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E00DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

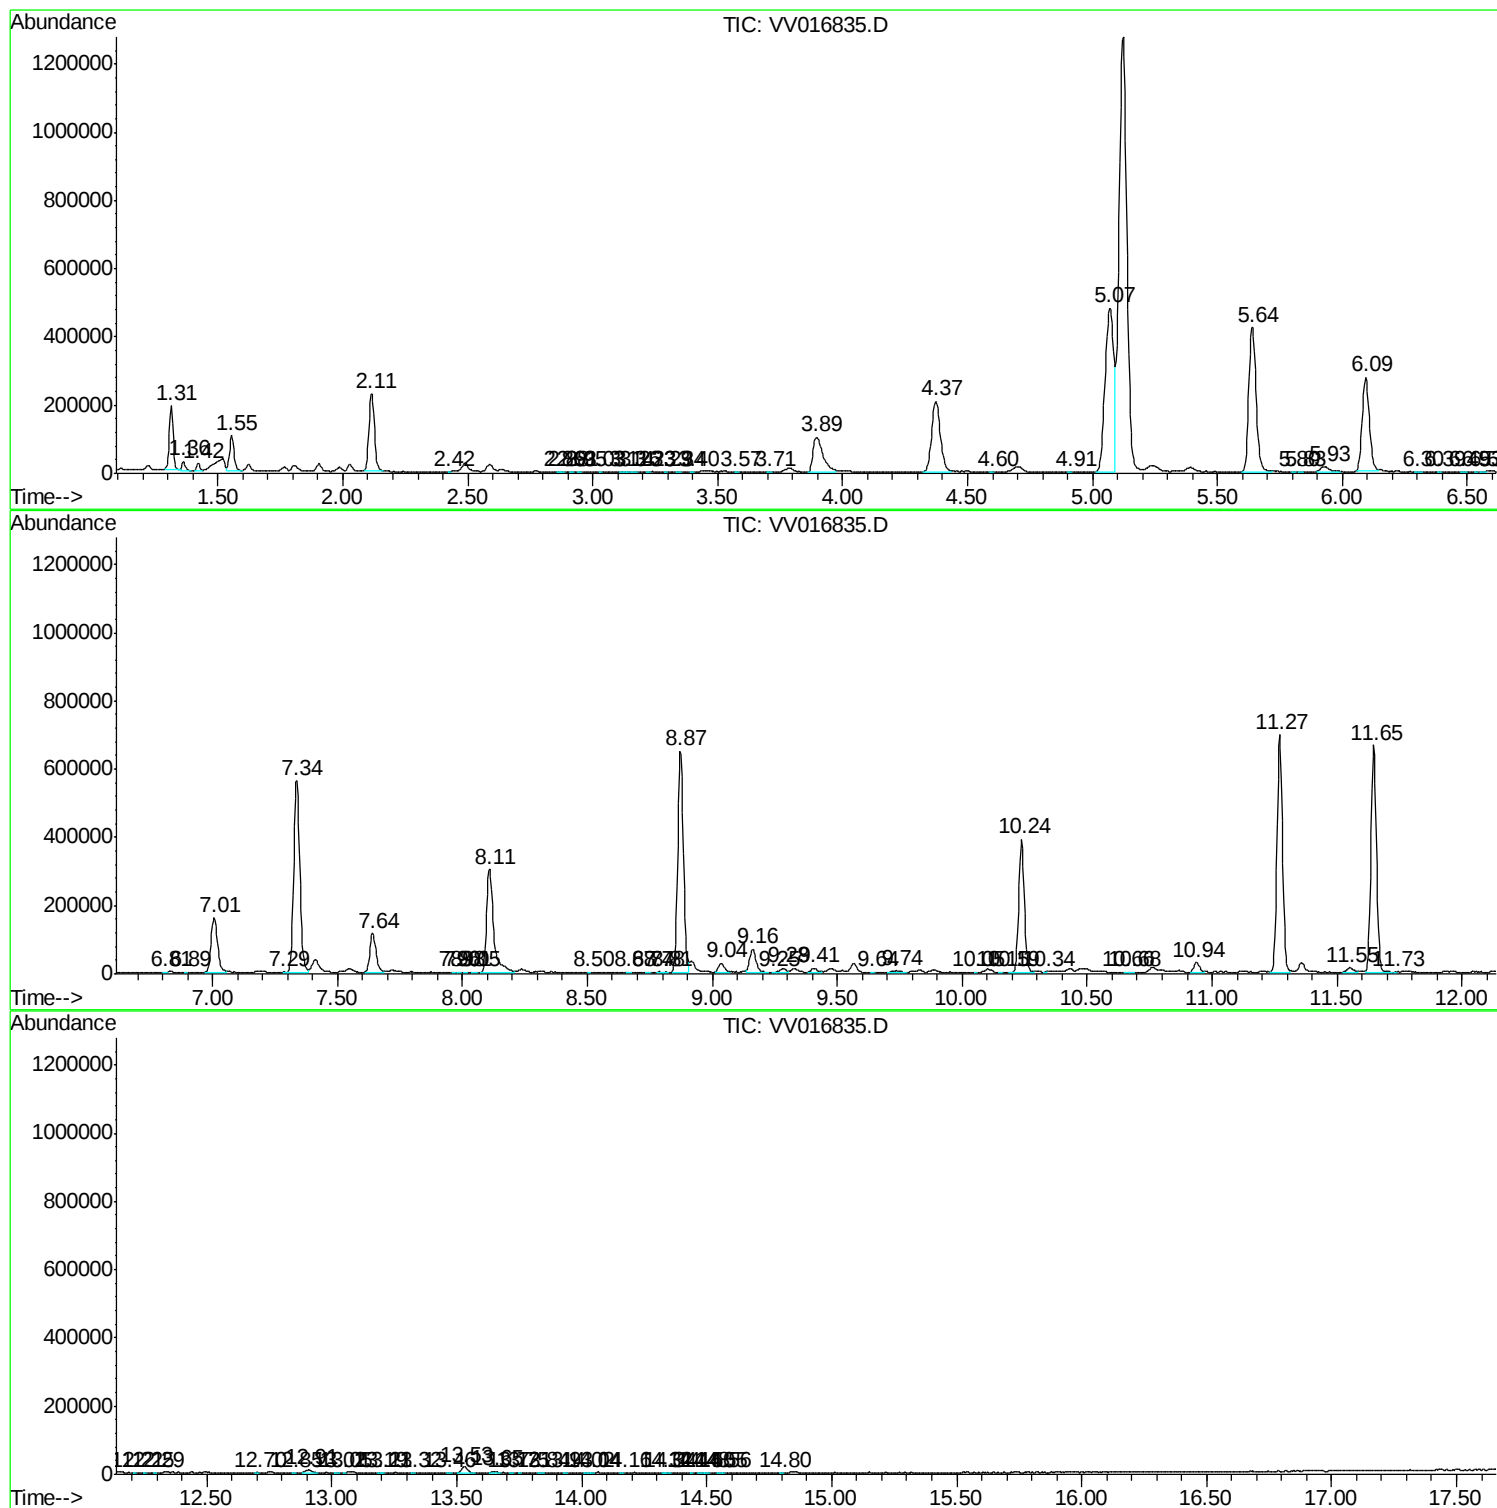

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016835.D
Acq On : 11 Jun 2020 18:28
Operator : SY/MD
Sample : L2914-05DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E00DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016835.D
Acq On : 11 Jun 2020 18:28
Operator : SY/MD
Sample : L2914-05DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E00DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc