

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016836.D
 Acq On : 11 Jun 2020 18:52
 Operator : SY/MD
 Sample : L2914-06DL 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	62	69	78	rVB	189696	198155	16.80%	1.941%
2	1.360	80	84	97	rVB	27432	29285	2.48%	0.287%
3	1.421	99	103	109	rVB	22079	18638	1.58%	0.183%
4	1.560	140	146	157	rVB	97844	119451	10.12%	1.170%
5	2.116	309	319	335	rVB	226894	338013	28.65%	3.311%
6	2.296	370	375	377	rBV5	2214	1929	0.16%	0.019%
7	2.389	401	404	405	rBV3	1650	867	0.07%	0.008%
8	2.415	411	412	414	rBV2	1128	441	0.04%	0.004%
9	2.720	504	507	508	rBV3	1190	734	0.06%	0.007%
10	2.833	539	542	545	rBV4	1333	879	0.07%	0.009%
11	2.955	578	580	584	rBV4	1637	951	0.08%	0.009%
12	3.013	596	598	600	rBV2	343	109	0.01%	0.001%
13	3.026	600	602	603	rBV2	781	399	0.03%	0.004%
14	3.116	628	630	632	rBV3	1107	570	0.05%	0.006%
15	3.135	632	636	637	rVV4	576	300	0.03%	0.003%
16	3.331	695	697	698	rBV2	1083	351	0.03%	0.003%
17	3.351	699	703	707	rVV6	1532	1499	0.13%	0.015%
18	3.441	726	731	732	rBV4	4091	3333	0.28%	0.033%
19	3.749	819	827	828	rBV6	3585	3220	0.27%	0.032%
20	3.894	860	872	896	rBV	104070	284860	24.14%	2.790%
21	4.373	1004	1021	1044	rBV	206683	505585	42.85%	4.952%
22	4.775	1145	1146	1149	rVB3	1478	398	0.03%	0.004%
23	4.884	1176	1180	1183	rBV5	1070	799	0.07%	0.008%
24	4.949	1198	1200	1202	rBV3	819	498	0.04%	0.005%
25	4.978	1207	1209	1214	rVB7	1554	880	0.07%	0.009%
26	5.068	1219	1237	1244	rBV2	491853	1179810	100.00%	11.555%
27	5.637	1401	1414	1433	rBV	445349	887929	75.26%	8.697%
28	6.093	1542	1556	1574	rBV	281184	568375	48.18%	5.567%
29	6.428	1658	1660	1665	rVB5	2186	1513	0.13%	0.015%
30	6.498	1680	1682	1686	rBV4	2045	1383	0.12%	0.014%
31	6.685	1737	1740	1741	rBV3	2125	1216	0.10%	0.012%
32	6.707	1746	1747	1750	rBV3	789	440	0.04%	0.004%
33	6.868	1793	1797	1799	rBV4	755	643	0.05%	0.006%
34	6.942	1818	1820	1821	rBV2	1324	718	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
 Data File : VV016836.D
 Acq On : 11 Jun 2020 18:52
 Operator : SY/MD
 Sample : L2914-06DL 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E01DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1828	1840	1859	rBV	163502	293331	24.86%	2.873%
36	7.338	1930	1943	1957	rBV	558400	959362	81.31%	9.396%
37	7.640	2027	2037	2051	rBV	113940	195587	16.58%	1.916%
38	7.817	2090	2092	2093	rBV2	1263	670	0.06%	0.007%
39	7.981	2140	2143	2146	rBV3	1531	1238	0.10%	0.012%
40	8.026	2155	2157	2158	rBV2	885	325	0.03%	0.003%
41	8.055	2164	2166	2170	rBV4	1626	964	0.08%	0.009%
42	8.106	2172	2182	2211	rBV	315120	606472	51.40%	5.940%
43	8.389	2267	2270	2275	rBV7	2300	2141	0.18%	0.021%
44	8.604	2334	2337	2338	rBV2	1497	902	0.08%	0.009%
45	8.649	2350	2351	2355	rBV3	1209	1026	0.09%	0.010%
46	8.698	2363	2366	2370	rBV5	1787	1286	0.11%	0.013%
47	8.739	2376	2379	2383	rBV4	1212	951	0.08%	0.009%
48	8.871	2409	2420	2431	rBV	677508	1084884	91.95%	10.626%
49	9.711	2680	2681	2683	rBV2	1440	596	0.05%	0.006%
50	10.067	2790	2792	2794	rBV3	1014	516	0.04%	0.005%
51	10.100	2795	2802	2811	rVV10	10222	17861	1.51%	0.175%
52	10.238	2834	2845	2858	rBV	391229	605103	51.29%	5.927%
53	10.762	3000	3008	3016	rBV2	14334	26757	2.27%	0.262%
54	10.939	3055	3063	3071	rBV	26620	37948	3.22%	0.372%
55	11.270	3153	3166	3182	rBV	731477	1112752	94.32%	10.899%
56	11.553	3243	3254	3266	rBV5	12200	26095	2.21%	0.256%
57	11.646	3272	3283	3299	rBV	647742	1012340	85.81%	9.915%
58	12.389	3508	3514	3516	rBV7	2166	2072	0.18%	0.020%
59	12.698	3608	3610	3614	rBV4	1160	961	0.08%	0.009%
60	12.845	3654	3656	3661	rBV4	1589	1279	0.11%	0.013%
61	12.964	3691	3693	3694	rBV2	1746	974	0.08%	0.010%
62	13.025	3710	3712	3713	rBV2	1166	592	0.05%	0.006%
63	13.077	3722	3728	3731	rBV8	3019	3942	0.33%	0.039%
64	13.128	3741	3744	3745	rBV3	2149	1088	0.09%	0.011%
65	13.225	3768	3774	3775	rBV4	2563	2198	0.19%	0.022%
66	13.431	3835	3838	3844	rBV7	1795	2012	0.17%	0.020%
67	13.498	3856	3859	3860	rBV3	1781	958	0.08%	0.009%
68	13.527	3860	3868	3886	rVB3	20726	36878	3.13%	0.361%
69	13.993	4009	4013	4014	rBV3	1451	948	0.08%	0.009%
70	14.025	4020	4023	4025	rBV3	1405	1018	0.09%	0.010%
71	14.093	4042	4044	4047	rBV2	1590	796	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061120\
Data File : VV016836.D
Acq On : 11 Jun 2020 18:52
Operator : SY/MD
Sample : L2914-06DL 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Title : VOC Analysis

72	14.189	4070	4074	4077	rVB4	2700	1670	0.14%	0.016%
73	14.212	4079	4081	4084	rBV3	1403	857	0.07%	0.008%
74	14.276	4098	4101	4103	rBV3	1902	1056	0.09%	0.010%
75	14.559	4186	4189	4192	rBV4	2192	1873	0.16%	0.018%
76	14.833	4271	4274	4275	rBV3	1859	926	0.08%	0.009%
77	15.141	4368	4370	4371	rBV2	1410	573	0.05%	0.006%
78	15.167	4376	4378	4381	rVB3	2323	1274	0.11%	0.012%
79	15.186	4381	4384	4387	rBV3	1810	1488	0.13%	0.015%
80	15.251	4400	4404	4405	rBV4	1838	1295	0.11%	0.013%


Sum of corrected areas: 10210006

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061120\
Data File : VV016836.D
Acq On : 11 Jun 2020 18:52
Operator : SY/MD
Sample : L2914-06DL 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

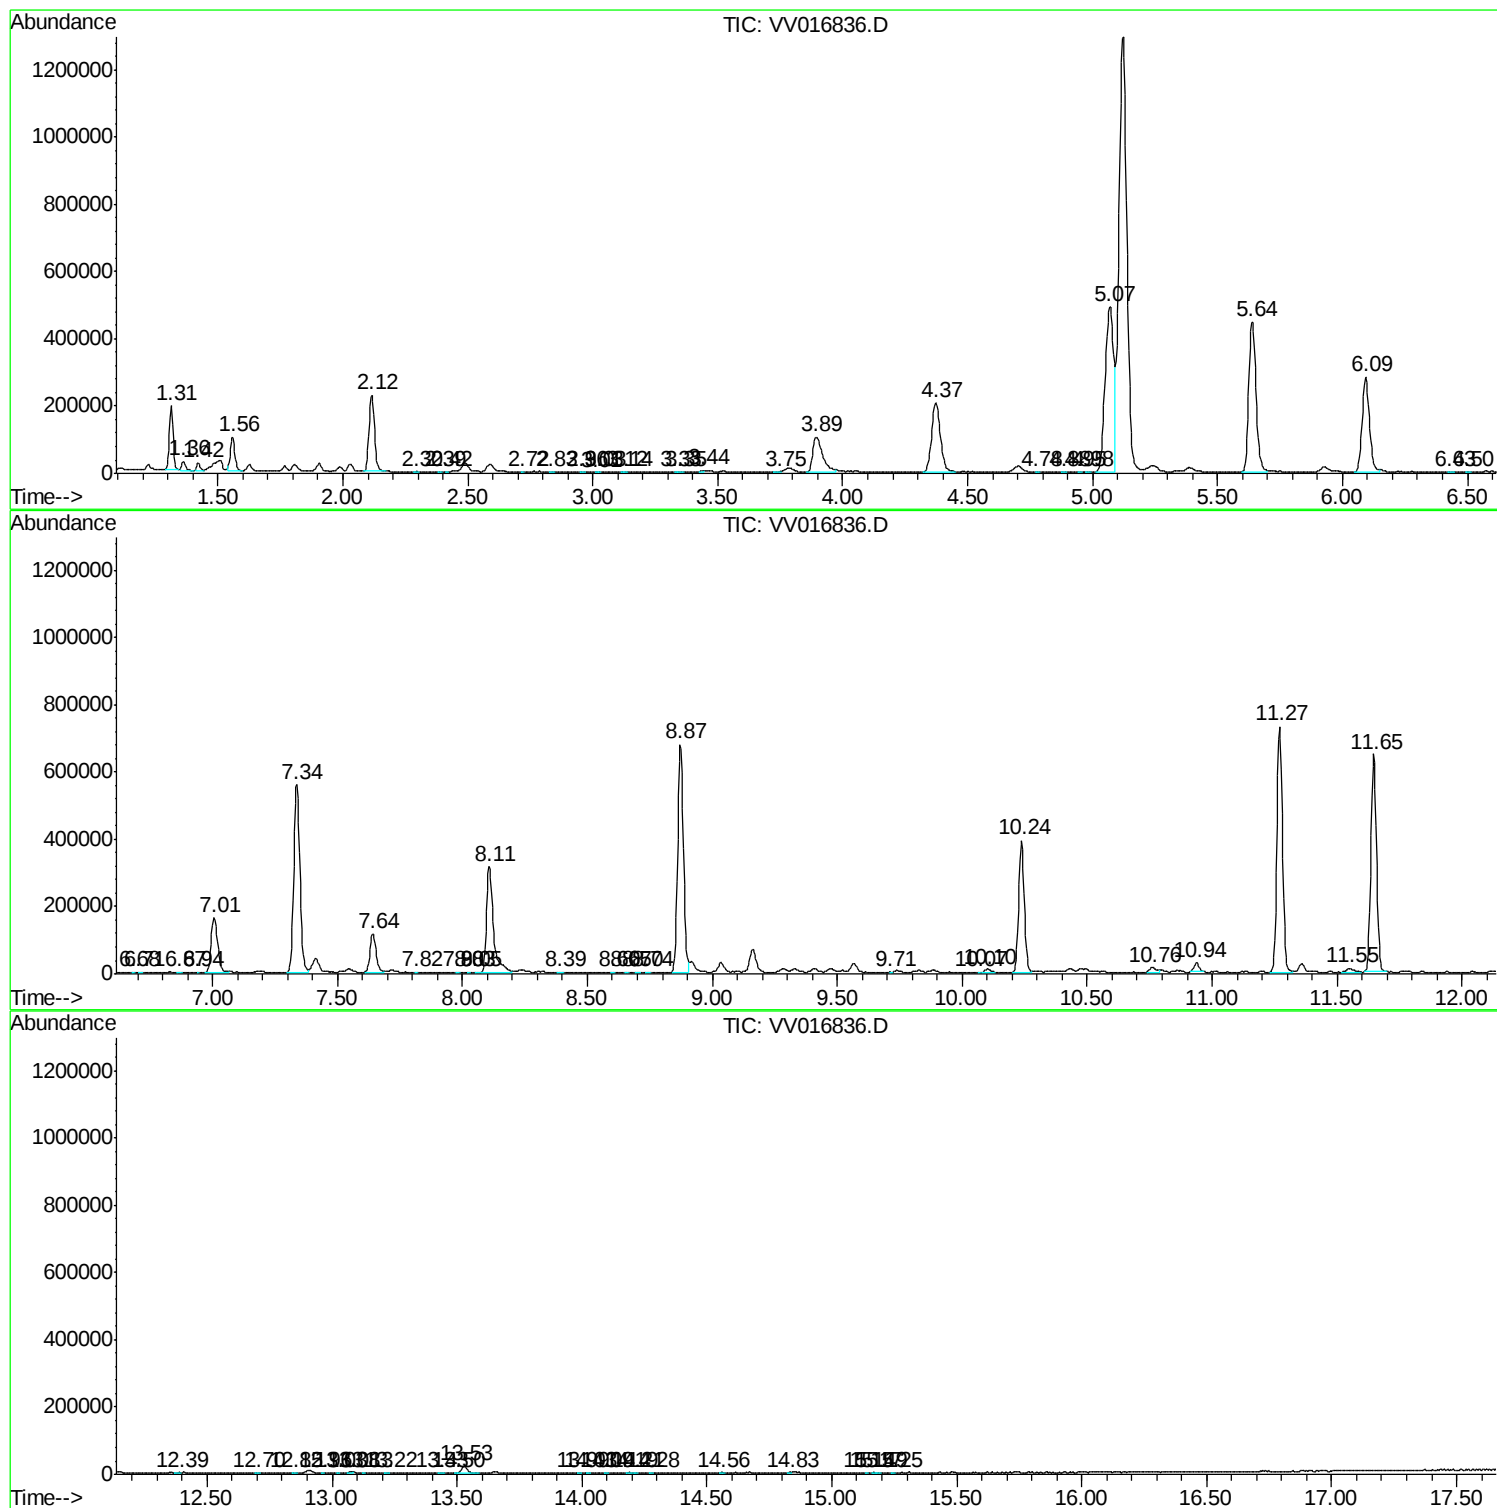

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016836.D
Acq On : 11 Jun 2020 18:52
Operator : SY/MD
Sample : L2914-06DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016836.D
Acq On : 11 Jun 2020 18:52
Operator : SY/MD
Sample : L2914-06DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E01DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
