

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016841.D
 Acq On : 11 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2915-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	175292	177653	13.19%	1.730%
2	1.560	139	146	157	rVB	120472	140172	10.41%	1.365%
3	1.978	271	276	279	rBV5	2769	2743	0.20%	0.027%
4	2.116	309	319	334	rBV	272697	400160	29.72%	3.896%
5	2.441	416	420	421	rBV4	1899	1202	0.09%	0.012%
6	2.489	432	435	436	rBV3	1528	812	0.06%	0.008%
7	2.727	506	509	511	rBV4	1343	909	0.07%	0.009%
8	2.788	526	528	531	rBV4	1378	734	0.05%	0.007%
9	2.962	577	582	584	rVV5	1359	1479	0.11%	0.014%
10	3.016	594	599	601	rBV5	1191	833	0.06%	0.008%
11	3.222	660	663	666	rBV5	904	778	0.06%	0.008%
12	3.576	768	773	776	rBV4	1510	1444	0.11%	0.014%
13	3.637	787	792	795	rBV6	1725	1561	0.12%	0.015%
14	3.695	808	810	814	rVV2	1286	893	0.07%	0.009%
15	3.714	814	816	819	rVV3	1502	974	0.07%	0.009%
16	3.894	857	872	892	rBV	99430	261546	19.42%	2.546%
17	4.167	953	957	960	rBV4	2596	2070	0.15%	0.020%
18	4.232	974	977	978	rBV3	1432	757	0.06%	0.007%
19	4.270	985	989	991	rBV4	1739	1409	0.10%	0.014%
20	4.373	1005	1021	1043	rBV	223591	559370	41.54%	5.446%
21	4.653	1104	1108	1110	rBV4	1742	1325	0.10%	0.013%
22	4.688	1114	1119	1120	rBV5	1934	1534	0.11%	0.015%
23	4.849	1166	1169	1174	rBV7	2238	2037	0.15%	0.020%
24	5.068	1218	1237	1262	rBV2	522926	1346595	100.00%	13.110%
25	5.328	1316	1318	1320	rBV4	1221	834	0.06%	0.008%
26	5.447	1348	1355	1357	rBV7	1985	2554	0.19%	0.025%
27	5.640	1402	1415	1436	rBV	425209	829200	61.58%	8.073%
28	5.926	1495	1504	1520	rBV2	26622	53341	3.96%	0.519%
29	5.994	1523	1525	1530	rBV5	1845	1795	0.13%	0.017%
30	6.093	1537	1556	1574	rBV	296122	607076	45.08%	5.910%
31	6.312	1622	1624	1626	rBV4	1594	945	0.07%	0.009%
32	6.392	1646	1649	1650	rBV3	1618	732	0.05%	0.007%
33	6.424	1658	1659	1664	rVB3	1171	766	0.06%	0.007%
34	6.444	1664	1665	1669	rBV4	1522	1032	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016841.D
 Acq On : 11 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2915-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.572	1702	1705	1707	rBV4	1363	883	0.07%	0.009%
36	6.621	1715	1720	1723	rBV6	1980	1544	0.11%	0.015%
37	6.643	1723	1727	1730	rBV4	1651	1392	0.10%	0.014%
38	6.752	1758	1761	1764	rBV5	1138	763	0.06%	0.007%
39	7.006	1828	1840	1854	rBV	172937	306479	22.76%	2.984%
40	7.241	1907	1913	1917	rBV8	2118	2085	0.15%	0.020%
41	7.338	1930	1943	1961	rBV	631235	1070650	79.51%	10.423%
42	7.640	2028	2037	2060	rVB	122848	209327	15.54%	2.038%
43	7.855	2100	2104	2107	rBV6	1584	1429	0.11%	0.014%
44	8.045	2158	2163	2164	rBV5	1618	1293	0.10%	0.013%
45	8.106	2171	2182	2214	rBV2	290576	596282	44.28%	5.805%
46	8.489	2297	2301	2303	rBV5	1787	1246	0.09%	0.012%
47	8.550	2318	2320	2322	rBV3	1631	823	0.06%	0.008%
48	8.723	2371	2374	2379	rVV6	1699	1590	0.12%	0.015%
49	8.874	2409	2421	2440	rVV	636433	1025215	76.13%	9.981%
50	9.251	2535	2538	2541	rBV5	1942	985	0.07%	0.010%
51	9.460	2601	2603	2608	rVB3	1478	1181	0.09%	0.011%
52	9.485	2608	2611	2617	rBV7	838	1141	0.08%	0.011%
53	9.566	2631	2636	2640	rBV6	2180	2372	0.18%	0.023%
54	9.640	2656	2659	2661	rBV3	1219	860	0.06%	0.008%
55	9.669	2666	2668	2674	rVB6	1962	1661	0.12%	0.016%
56	9.752	2692	2694	2696	rBV3	1687	1178	0.09%	0.011%
57	9.804	2707	2710	2711	rVV3	1543	876	0.07%	0.009%
58	10.029	2778	2780	2783	rVV5	1424	905	0.07%	0.009%
59	10.080	2794	2796	2799	rVB4	1643	845	0.06%	0.008%
60	10.100	2799	2802	2806	rBV5	1065	907	0.07%	0.009%
61	10.167	2819	2823	2825	rBV4	1375	1166	0.09%	0.011%
62	10.238	2833	2845	2861	rBV	364232	575467	42.73%	5.602%
63	10.553	2938	2943	2946	rBV5	2075	2017	0.15%	0.020%
64	10.598	2954	2957	2962	rVB6	1951	1565	0.12%	0.015%
65	10.743	3000	3002	3007	rBV6	1284	975	0.07%	0.009%
66	10.890	3043	3048	3050	rBV4	1663	1310	0.10%	0.013%
67	10.935	3059	3062	3066	rBV5	2629	2104	0.16%	0.020%
68	11.058	3097	3100	3103	rVB4	1729	948	0.07%	0.009%
69	11.080	3103	3107	3110	rVB6	1895	1617	0.12%	0.016%
70	11.157	3125	3131	3132	rBV5	1192	898	0.07%	0.009%
71	11.199	3142	3144	3150	rBV7	2010	1826	0.14%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016841.D
 Acq On : 11 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2915-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E78

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3186	rVV	638580	978352	72.65%	9.525%
73	11.514	3239	3242	3244	rBV3	1477	827	0.06%	0.008%
74	11.537	3246	3249	3252	rBV4	1574	1355	0.10%	0.013%
75	11.646	3272	3283	3298	rBV	654587	1028995	76.41%	10.018%
76	12.109	3425	3427	3433	rVB5	1214	764	0.06%	0.007%
77	12.183	3447	3450	3452	rBV4	1261	904	0.07%	0.009%
78	12.347	3498	3501	3502	rBV3	1482	793	0.06%	0.008%
79	12.675	3595	3603	3606	rBV10	3435	4738	0.35%	0.046%
80	12.813	3643	3646	3648	rBV3	1708	814	0.06%	0.008%
81	12.903	3670	3674	3677	rBV6	1383	1174	0.09%	0.011%
82	12.961	3689	3692	3693	rBV3	1752	980	0.07%	0.010%
83	13.135	3743	3746	3748	rBV3	1205	772	0.06%	0.008%
84	13.199	3762	3766	3768	rBV4	1432	1258	0.09%	0.012%
85	13.225	3771	3774	3778	rVV5	1740	1094	0.08%	0.011%
86	13.286	3788	3793	3795	rBV5	2548	2665	0.20%	0.026%
87	13.321	3802	3804	3806	rBV3	1302	740	0.05%	0.007%
88	13.350	3809	3813	3814	rBV4	1011	759	0.06%	0.007%
89	13.382	3820	3823	3826	rBV5	1049	781	0.06%	0.008%
90	13.492	3853	3857	3863	rBV8	1233	1423	0.11%	0.014%
91	13.832	3959	3963	3967	rBV7	1551	1398	0.10%	0.014%
92	13.852	3967	3969	3973	rBV3	1210	963	0.07%	0.009%
93	13.935	3991	3995	3999	rBV6	1646	1370	0.10%	0.013%
94	14.103	4044	4047	4051	rBV3	1961	1848	0.14%	0.018%
95	14.276	4097	4101	4103	rBV5	1459	1056	0.08%	0.010%
96	14.334	4117	4119	4121	rBV3	1541	721	0.05%	0.007%
97	14.476	4159	4163	4166	rBV5	1178	930	0.07%	0.009%
98	14.691	4228	4230	4232	rBV2	1205	725	0.05%	0.007%
99	14.775	4253	4256	4259	rVB4	1493	1059	0.08%	0.010%
100	14.961	4311	4314	4316	rBV2	1667	1328	0.10%	0.013%


Sum of corrected areas: 10271656

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016841.D
Acq On : 11 Jun 2020 21:12
Operator : SY/MD
Sample : L2915-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9E78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

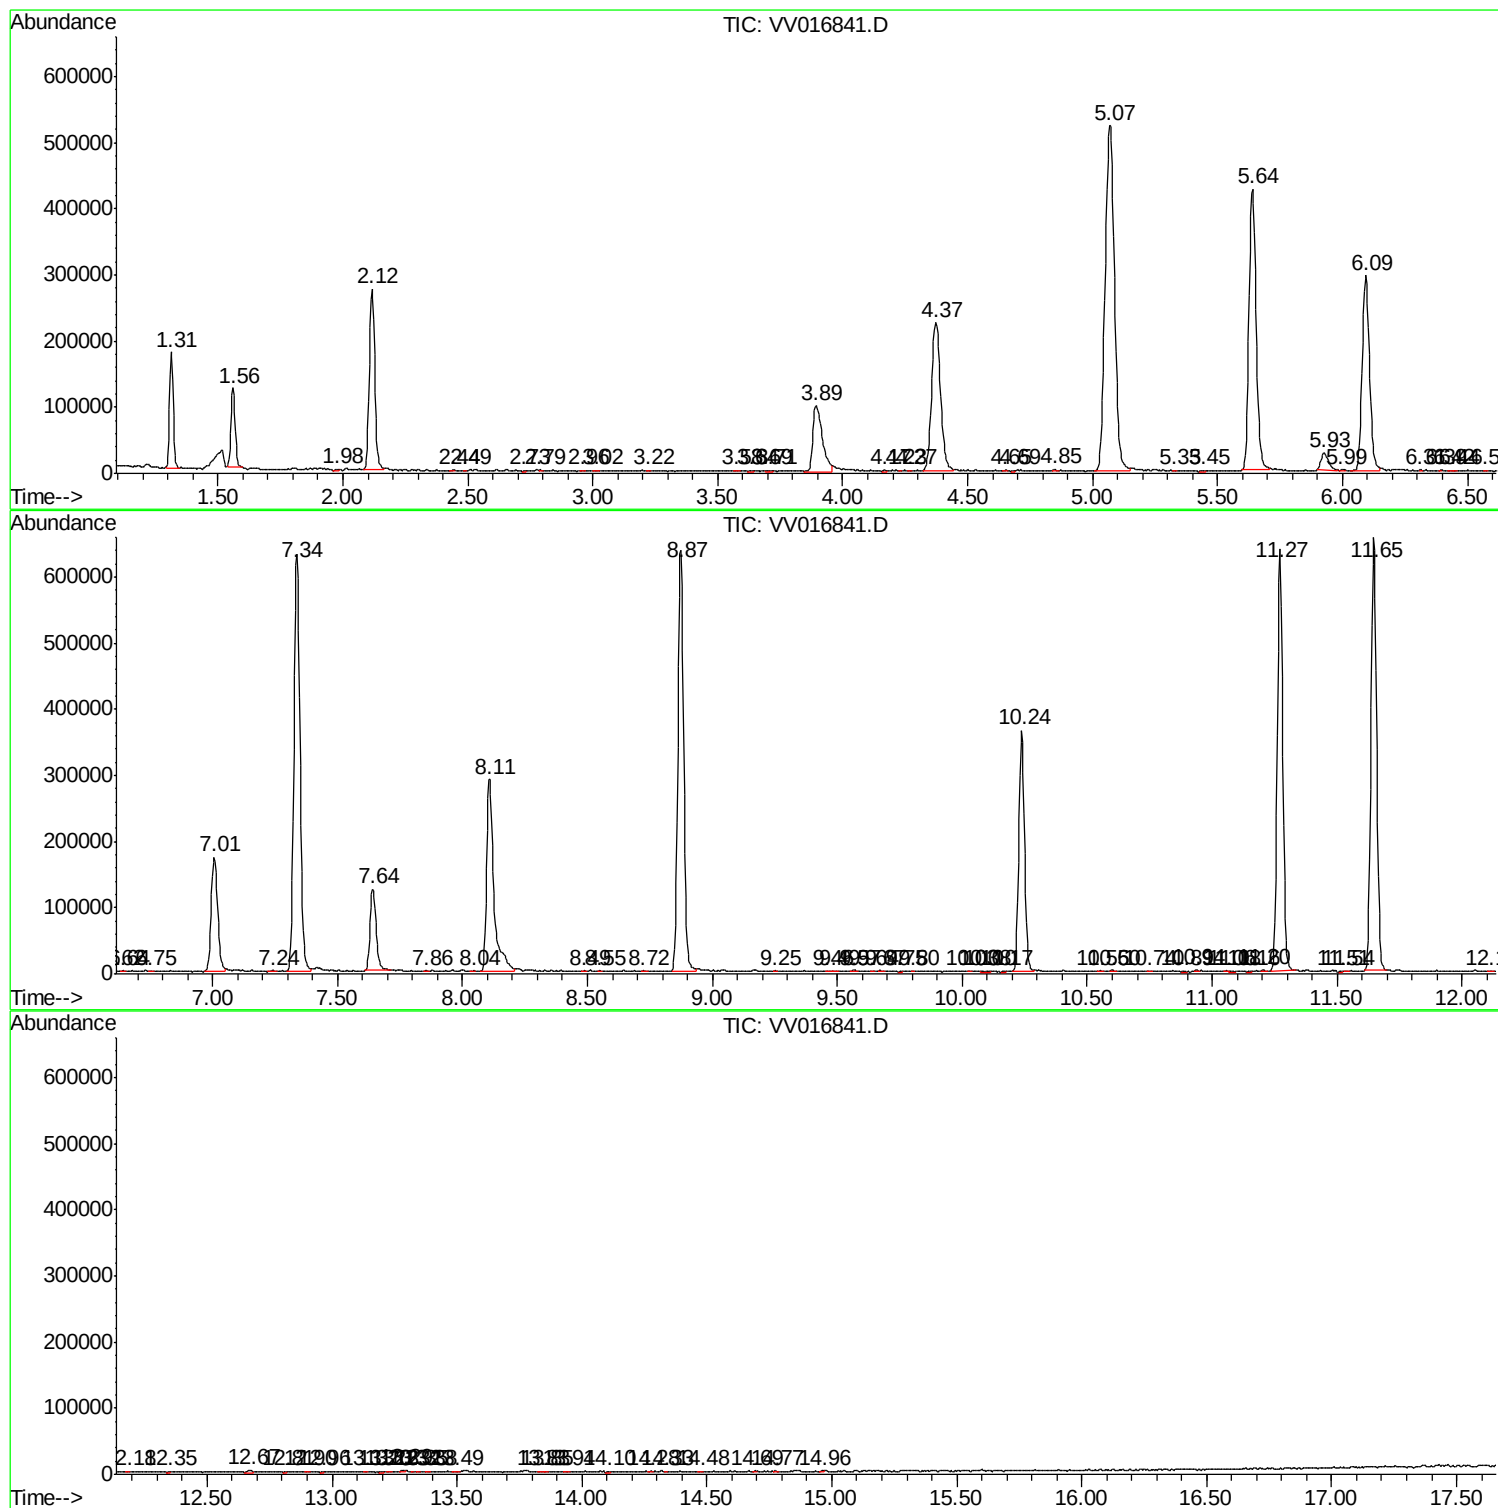

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016841.D
Acq On : 11 Jun 2020 21:12
Operator : SY/MD
Sample : L2915-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E78

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016841.D
Acq On : 11 Jun 2020 21:12
Operator : SY/MD
Sample : L2915-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E78

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc