

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016847.D
 Acq On : 11 Jun 2020 23:35
 Operator : SY/MD
 Sample : L2915-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	207254	211333	17.15%	2.014%
2	1.557	139	145	158	rVB	117400	140605	11.41%	1.340%
3	2.116	309	319	337	rVB	259696	390415	31.67%	3.720%
4	2.711	502	504	505	rBV2	919	421	0.03%	0.004%
5	2.762	518	520	522	rBV3	1885	733	0.06%	0.007%
6	3.020	597	600	603	rBV4	1314	931	0.08%	0.009%
7	3.106	620	627	629	rBV7	1471	1899	0.15%	0.018%
8	3.145	637	639	643	rVB4	1024	580	0.05%	0.006%
9	3.190	651	653	655	rBV4	1203	591	0.05%	0.006%
10	3.348	701	702	703	rBV	849	237	0.02%	0.002%
11	3.409	720	721	723	rBV2	1075	501	0.04%	0.005%
12	3.425	723	726	729	rVV4	2508	1575	0.13%	0.015%
13	3.515	750	754	758	rBV6	2019	1849	0.15%	0.018%
14	3.569	769	771	777	rVB7	2364	1947	0.16%	0.019%
15	3.602	777	781	784	rBV3	1351	1161	0.09%	0.011%
16	3.637	790	792	795	rBV4	1124	470	0.04%	0.004%
17	3.688	805	808	812	rBV6	1808	1800	0.15%	0.017%
18	3.778	829	836	838	rBV9	5205	6520	0.53%	0.062%
19	3.843	854	856	858	rBV3	1284	609	0.05%	0.006%
20	3.897	862	873	901	rVV2	100675	274396	22.26%	2.615%
21	4.373	1007	1021	1044	rVB	211194	511113	41.47%	4.870%
22	4.592	1087	1089	1093	rVB4	1852	947	0.08%	0.009%
23	4.611	1093	1095	1097	rBV3	923	453	0.04%	0.004%
24	4.840	1162	1166	1169	rBV6	1361	962	0.08%	0.009%
25	4.875	1175	1177	1180	rBV4	1468	1018	0.08%	0.010%
26	4.907	1185	1187	1189	rBV3	1675	920	0.07%	0.009%
27	4.955	1199	1202	1204	rBV4	1074	676	0.05%	0.006%
28	4.987	1210	1212	1214	rBV3	924	450	0.04%	0.004%
29	5.068	1221	1237	1244	rBV2	519867	1232612	100.00%	11.745%
30	5.640	1402	1415	1439	rBV	416096	835465	67.78%	7.961%
31	6.093	1542	1556	1576	rBV	290689	593295	48.13%	5.653%
32	6.338	1630	1632	1636	rBV4	1634	1278	0.10%	0.012%
33	6.389	1645	1648	1651	rVB5	1992	1084	0.09%	0.010%
34	6.415	1654	1656	1658	rBV2	1370	633	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016847.D
 Acq On : 11 Jun 2020 23:35
 Operator : SY/MD
 Sample : L2915-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.634	1722	1724	1725	rBV2	1154	375	0.03%	0.004%
36	6.659	1730	1732	1735	rVV3	1276	552	0.04%	0.005%
37	6.907	1806	1809	1813	rBV4	1067	762	0.06%	0.007%
38	6.955	1822	1824	1827	rVB3	1889	1137	0.09%	0.011%
39	7.007	1827	1840	1855	rBV	165157	300665	24.39%	2.865%
40	7.338	1931	1943	1956	rBV	608876	1032343	83.75%	9.837%
41	7.640	2028	2037	2053	rBV	116664	196598	15.95%	1.873%
42	7.897	2115	2117	2122	rVB5	1820	1122	0.09%	0.011%
43	7.974	2138	2141	2144	rBV5	2054	1547	0.13%	0.015%
44	8.106	2172	2182	2209	rBV	308710	589073	47.79%	5.613%
45	8.569	2324	2326	2332	rBV6	2085	1849	0.15%	0.018%
46	8.788	2392	2394	2396	rBV2	1105	320	0.03%	0.003%
47	8.798	2396	2397	2400	rVB3	976	409	0.03%	0.004%
48	8.871	2408	2420	2443	rBV	630115	1044250	84.72%	9.951%
49	9.032	2461	2470	2486	rVB	177719	279623	22.69%	2.665%
50	9.566	2628	2636	2656	rVB	33990	60907	4.94%	0.580%
51	9.916	2743	2745	2746	rBV	999	366	0.03%	0.003%
52	9.952	2750	2756	2762	rBV8	4971	7802	0.63%	0.074%
53	10.068	2786	2792	2796	rVB10	1776	2284	0.19%	0.022%
54	10.097	2796	2801	2802	rBV4	3022	2545	0.21%	0.024%
55	10.238	2833	2845	2860	rBV	381463	599334	48.62%	5.711%
56	10.309	2864	2867	2871	rBV6	1803	1238	0.10%	0.012%
57	10.531	2932	2936	2939	rBV6	1723	1344	0.11%	0.013%
58	10.842	3028	3033	3035	rBV4	1384	1527	0.12%	0.015%
59	10.936	3055	3062	3071	rBV4	7367	12058	0.98%	0.115%
60	11.061	3099	3101	3104	rBV4	1240	832	0.07%	0.008%
61	11.170	3133	3135	3136	rBV2	692	248	0.02%	0.002%
62	11.206	3144	3146	3147	rBV2	922	265	0.02%	0.003%
63	11.270	3155	3166	3183	rBV	687238	1035574	84.01%	9.868%
64	11.437	3216	3218	3220	rBB2	564	123	0.01%	0.001%
65	11.450	3220	3222	3225	rBV4	2066	1717	0.14%	0.016%
66	11.592	3263	3266	3267	rBV4	1404	800	0.06%	0.008%
67	11.646	3271	3283	3298	rVV	678125	1049128	85.11%	9.997%
68	11.932	3368	3372	3374	rBV4	1208	729	0.06%	0.007%
69	12.029	3401	3402	3404	rBV2	1131	362	0.03%	0.003%
70	12.058	3408	3411	3420	rBV10	1870	2315	0.19%	0.022%
71	12.293	3481	3484	3486	rBV4	1332	837	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016847.D
 Acq On : 11 Jun 2020 23:35
 Operator : SY/MD
 Sample : L2915-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E06DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.354	3499	3503	3506	rBV4	2181	1773	0.14%	0.017%
73	12.434	3524	3528	3532	rBV7	1178	1042	0.08%	0.010%
74	12.489	3541	3545	3555	rVB10	3068	4003	0.32%	0.038%
75	12.527	3555	3557	3560	rBV3	1431	1058	0.09%	0.010%
76	12.547	3560	3563	3565	rBV3	1148	831	0.07%	0.008%
77	12.630	3586	3589	3590	rBV3	1657	700	0.06%	0.007%
78	12.662	3596	3599	3601	rBV2	1595	1202	0.10%	0.011%
79	12.855	3653	3659	3664	rBV8	2509	2816	0.23%	0.027%
80	13.019	3709	3710	3712	rBV2	969	466	0.04%	0.004%
81	13.029	3712	3713	3716	rVV2	1156	566	0.05%	0.005%
82	13.058	3720	3722	3724	rBV3	1320	824	0.07%	0.008%
83	13.209	3766	3769	3770	rBV3	1652	913	0.07%	0.009%
84	13.276	3787	3790	3791	rBV3	1230	594	0.05%	0.006%
85	13.347	3810	3812	3813	rBV2	1349	562	0.05%	0.005%
86	13.530	3859	3869	3880	rBV	9300	18250	1.48%	0.174%
87	13.701	3920	3922	3925	rBV5	1394	793	0.06%	0.008%
88	13.891	3979	3981	3983	rBV3	725	549	0.04%	0.005%
89	13.965	4000	4004	4008	rBV6	1166	1211	0.10%	0.012%
90	14.013	4016	4019	4020	rBV2	1650	917	0.07%	0.009%
91	14.344	4119	4122	4125	rBV3	1028	693	0.06%	0.007%
92	14.386	4133	4135	4139	rVB4	1279	842	0.07%	0.008%
93	14.411	4141	4143	4144	rBV3	1406	595	0.05%	0.006%
94	15.180	4380	4382	4386	rVB5	1609	743	0.06%	0.007%


Sum of corrected areas: 10494382

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016847.D
Acq On : 11 Jun 2020 23:35
Operator : SY/MD
Sample : L2915-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E06DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

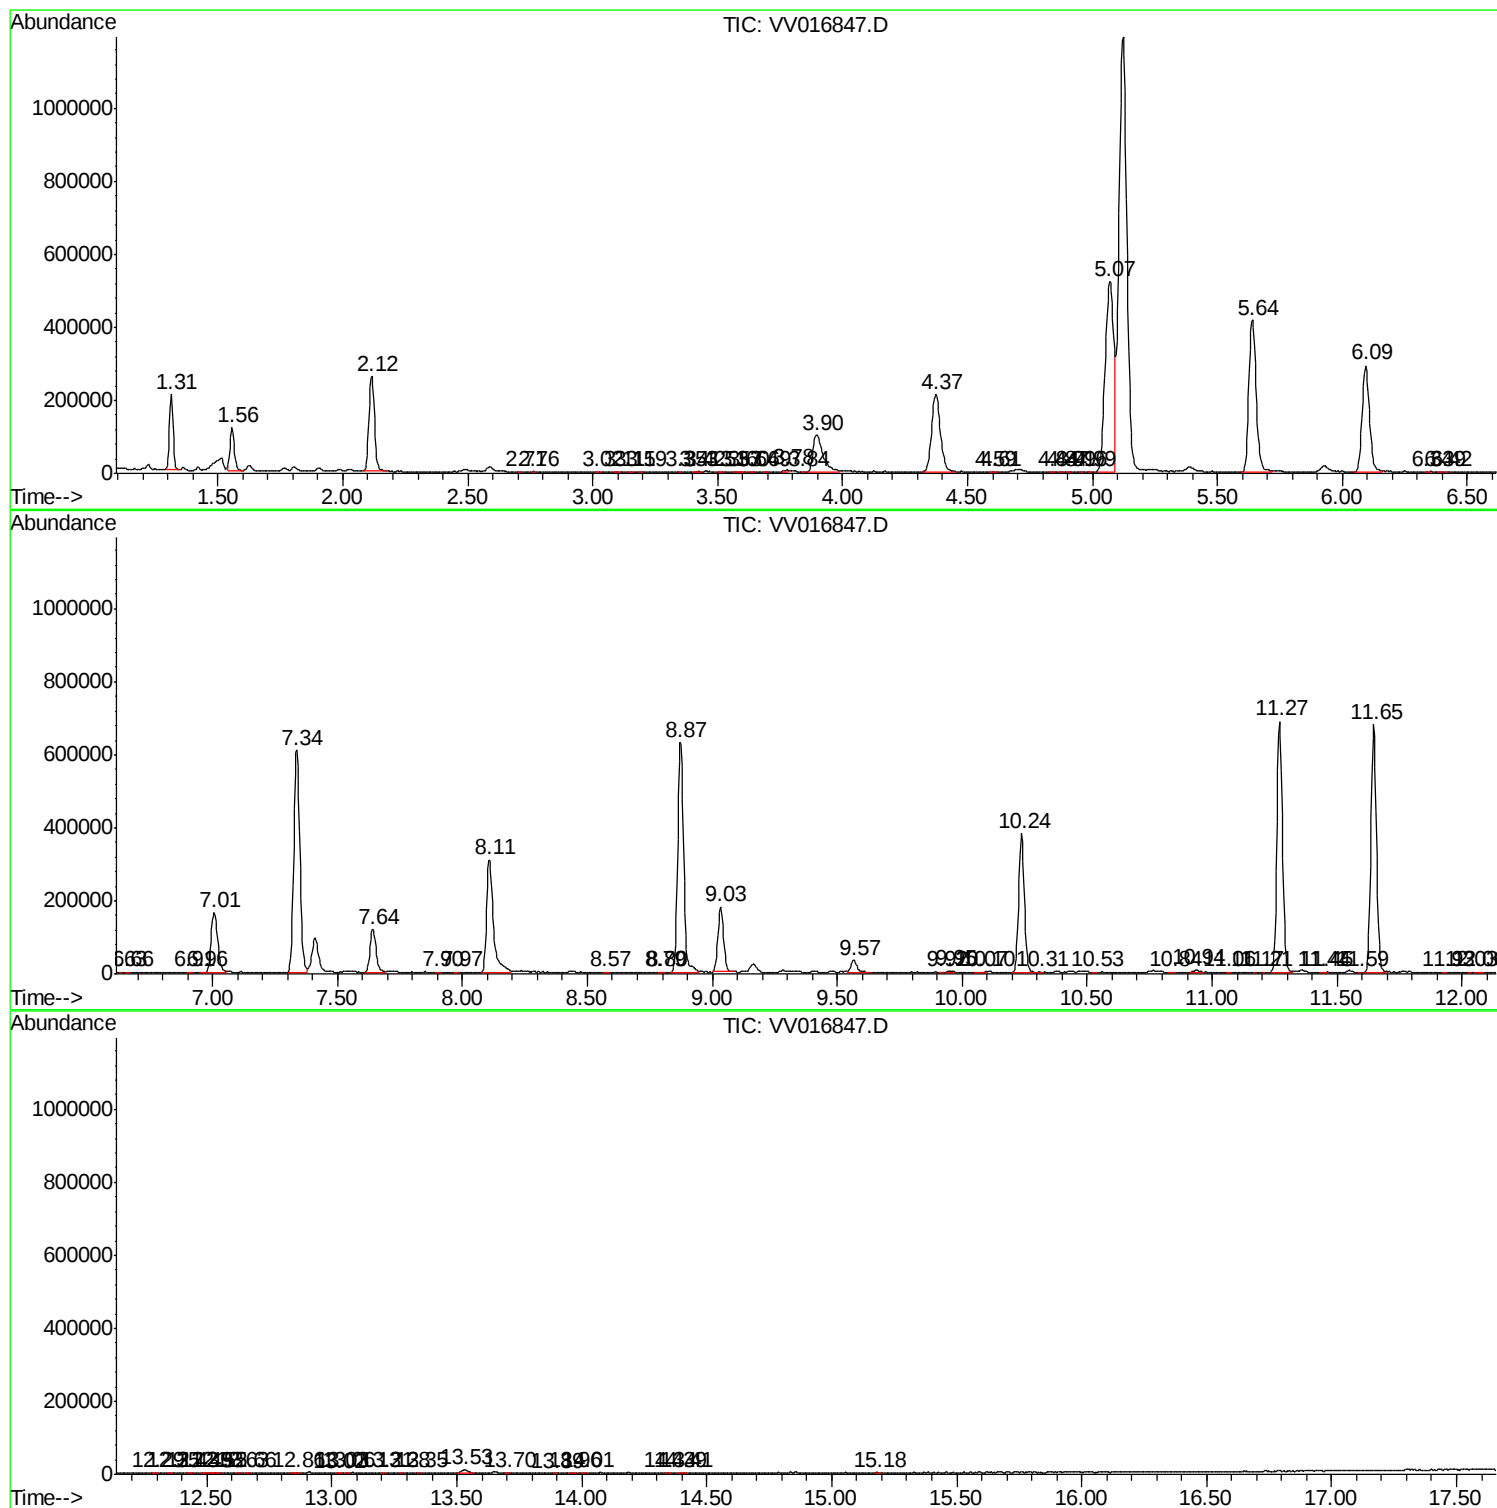

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016847.D
Acq On : 11 Jun 2020 23:35
Operator : SY/MD
Sample : L2915-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E06DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016847.D
Acq On : 11 Jun 2020 23:35
Operator : SY/MD
Sample : L2915-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E06DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc