

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016851.D
 Acq On : 12 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2915-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E20DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	221050	232163	16.92%	2.082%
2	1.560	142	146	157	rVB	138427	154536	11.26%	1.386%
3	2.116	309	319	336	rVB	280799	416076	30.33%	3.732%
4	2.428	411	416	419	rBV7	2431	2324	0.17%	0.021%
5	2.447	419	422	423	rBV3	1493	793	0.06%	0.007%
6	2.868	551	553	556	rVB3	1855	963	0.07%	0.009%
7	2.891	556	560	562	rBV5	1419	854	0.06%	0.008%
8	2.991	590	591	596	rBV4	1423	1123	0.08%	0.010%
9	3.065	612	614	617	rVB4	2183	1482	0.11%	0.013%
10	3.110	625	628	630	rBV4	1696	1058	0.08%	0.009%
11	3.270	674	678	679	rBV3	1705	1003	0.07%	0.009%
12	3.444	729	732	735	rBV4	3432	3355	0.24%	0.030%
13	3.560	765	768	770	rBV4	2438	1478	0.11%	0.013%
14	3.611	777	784	789	rBV9	1574	2073	0.15%	0.019%
15	3.695	805	810	812	rBV4	1738	1349	0.10%	0.012%
16	3.746	823	826	829	rBV5	1597	1160	0.08%	0.010%
17	3.782	829	837	841	rBV8	5257	8396	0.61%	0.075%
18	3.901	861	874	904	rVV	103918	298241	21.74%	2.675%
19	4.065	922	925	929	rBV5	2092	1587	0.12%	0.014%
20	4.373	1005	1021	1045	rVV	224936	551020	40.16%	4.942%
21	4.589	1085	1088	1090	rBV3	1808	1194	0.09%	0.011%
22	4.859	1169	1172	1175	rBV4	1587	1278	0.09%	0.011%
23	4.987	1207	1212	1216	rVB7	1009	961	0.07%	0.009%
24	5.071	1218	1238	1245	rBV2	556127	1371906	100.00%	12.305%
25	5.505	1370	1373	1379	rBV8	1715	1438	0.10%	0.013%
26	5.640	1402	1415	1436	rVV	458266	900937	65.67%	8.081%
27	5.926	1494	1504	1518	rBV4	18671	39810	2.90%	0.357%
28	6.045	1537	1541	1542	rBV4	1546	1101	0.08%	0.010%
29	6.093	1542	1556	1573	rVV	312235	628522	45.81%	5.637%
30	6.267	1606	1610	1614	rBV6	1689	1576	0.11%	0.014%
31	6.286	1614	1616	1622	rVB7	2067	1742	0.13%	0.016%
32	6.515	1684	1687	1688	rBV2	1280	807	0.06%	0.007%
33	6.569	1701	1704	1706	rBV4	1717	1169	0.09%	0.010%
34	6.782	1765	1770	1772	rBV5	1608	1225	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016851.D
 Acq On : 12 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2915-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E20DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.913	1809	1811	1814	rBV4	1453	930	0.07%	0.008%
36	6.962	1820	1826	1827	rBV6	1998	1359	0.10%	0.012%
37	7.007	1830	1840	1858	rVV	176654	307668	22.43%	2.760%
38	7.338	1930	1943	1956	rBV	650595	1110366	80.94%	9.959%
39	7.640	2029	2037	2054	rVB	123837	204358	14.90%	1.833%
40	7.855	2102	2104	2107	rBV4	2687	1700	0.12%	0.015%
41	7.949	2130	2133	2137	rBV4	1351	1333	0.10%	0.012%
42	8.109	2172	2183	2218	rBV	303893	619128	45.13%	5.553%
43	8.511	2304	2308	2310	rBV5	1338	998	0.07%	0.009%
44	8.556	2318	2322	2325	rVB4	1214	1113	0.08%	0.010%
45	8.617	2335	2341	2343	rBV7	1809	1452	0.11%	0.013%
46	8.653	2349	2352	2356	rBV6	1266	1089	0.08%	0.010%
47	8.675	2356	2359	2363	rVV5	1943	1448	0.11%	0.013%
48	8.756	2378	2384	2387	rBV6	1482	1798	0.13%	0.016%
49	8.875	2409	2421	2433	rBV	678270	1095442	79.85%	9.825%
50	9.035	2461	2471	2485	rBV	160713	252951	18.44%	2.269%
51	9.383	2576	2579	2581	rBV3	1909	1450	0.11%	0.013%
52	9.473	2598	2607	2617	rBV3	5719	12245	0.89%	0.110%
53	9.566	2629	2636	2648	rVB	45081	72702	5.30%	0.652%
54	9.675	2666	2670	2673	rBV5	1418	929	0.07%	0.008%
55	9.952	2749	2756	2763	rBV6	5251	7759	0.57%	0.070%
56	10.051	2785	2787	2791	rVB4	1935	947	0.07%	0.008%
57	10.077	2791	2795	2798	rBV5	1141	1233	0.09%	0.011%
58	10.103	2798	2803	2804	rBV4	2920	2202	0.16%	0.020%
59	10.238	2833	2845	2860	rVV	393834	613915	44.75%	5.506%
60	10.334	2873	2875	2877	rBV3	1557	835	0.06%	0.007%
61	10.688	2983	2985	2988	rVV2	1266	802	0.06%	0.007%
62	10.759	2998	3007	3014	rBV7	7178	11799	0.86%	0.106%
63	10.939	3056	3063	3070	rBV4	7970	11553	0.84%	0.104%
64	11.048	3094	3097	3099	rBV4	1682	1023	0.07%	0.009%
65	11.080	3103	3107	3111	rBV6	1567	1250	0.09%	0.011%
66	11.270	3154	3166	3181	rBV	690451	1054478	76.86%	9.458%
67	11.511	3237	3241	3242	rBV4	1183	794	0.06%	0.007%
68	11.646	3271	3283	3301	rBV	673786	1054137	76.84%	9.455%
69	11.903	3359	3363	3365	rBV5	1592	1423	0.10%	0.013%
70	12.119	3428	3430	3434	rBV4	1490	1123	0.08%	0.010%
71	12.167	3443	3445	3448	rBV3	1297	1030	0.08%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016851.D
 Acq On : 12 Jun 2020 01:10
 Operator : SY/MD
 Sample : L2915-12DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E20DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.215	3458	3460	3465	rVB4	1207	817	0.06%	0.007%
73	12.244	3466	3469	3472	rBV5	1304	959	0.07%	0.009%
74	12.402	3513	3518	3521	rBV6	1226	1004	0.07%	0.009%
75	12.621	3582	3586	3590	rVB6	1241	929	0.07%	0.008%
76	12.649	3590	3595	3597	rBV4	1660	1274	0.09%	0.011%
77	12.672	3599	3602	3604	rBV3	1335	1029	0.08%	0.009%
78	12.711	3609	3614	3616	rBV4	1499	1367	0.10%	0.012%
79	12.784	3635	3637	3641	rBV4	1411	986	0.07%	0.009%
80	12.839	3649	3654	3656	rBV6	1758	1228	0.09%	0.011%
81	13.032	3711	3714	3719	rVV7	1630	1507	0.11%	0.014%
82	13.129	3742	3744	3747	rBV4	1432	1102	0.08%	0.010%
83	13.334	3804	3808	3809	rBV4	1060	864	0.06%	0.008%
84	13.411	3827	3832	3833	rBV6	1792	1271	0.09%	0.011%
85	13.485	3852	3855	3860	rBV7	1342	1248	0.09%	0.011%
86	13.530	3860	3869	3880	rVV3	10834	19363	1.41%	0.174%
87	13.608	3890	3893	3895	rBV4	1335	788	0.06%	0.007%
88	13.640	3895	3903	3904	rBV6	2785	3083	0.22%	0.028%
89	13.894	3979	3982	3986	rBV6	1963	1725	0.13%	0.015%
90	13.955	3998	4001	4005	rVB4	1887	958	0.07%	0.009%
91	14.235	4085	4088	4091	rBV5	1497	990	0.07%	0.009%
92	14.395	4135	4138	4142	rBV3	1585	1476	0.11%	0.013%
93	14.479	4159	4164	4170	rBV8	2979	3174	0.23%	0.028%
94	14.540	4181	4183	4186	rVV3	1736	862	0.06%	0.008%
95	14.572	4190	4193	4196	rVB4	2197	1389	0.10%	0.012%
96	14.665	4219	4222	4223	rBV3	2090	1126	0.08%	0.010%
97	14.845	4274	4278	4282	rBV7	2143	2230	0.16%	0.020%
98	14.974	4316	4318	4321	rBV5	1382	856	0.06%	0.008%
99	15.006	4323	4328	4331	rBV6	2629	2562	0.19%	0.023%
100	15.424	4455	4458	4461	rBV5	2192	1474	0.11%	0.013%


Sum of corrected areas: 11149103

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016851.D
Acq On : 12 Jun 2020 01:10
Operator : SY/MD
Sample : L2915-12DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E20DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

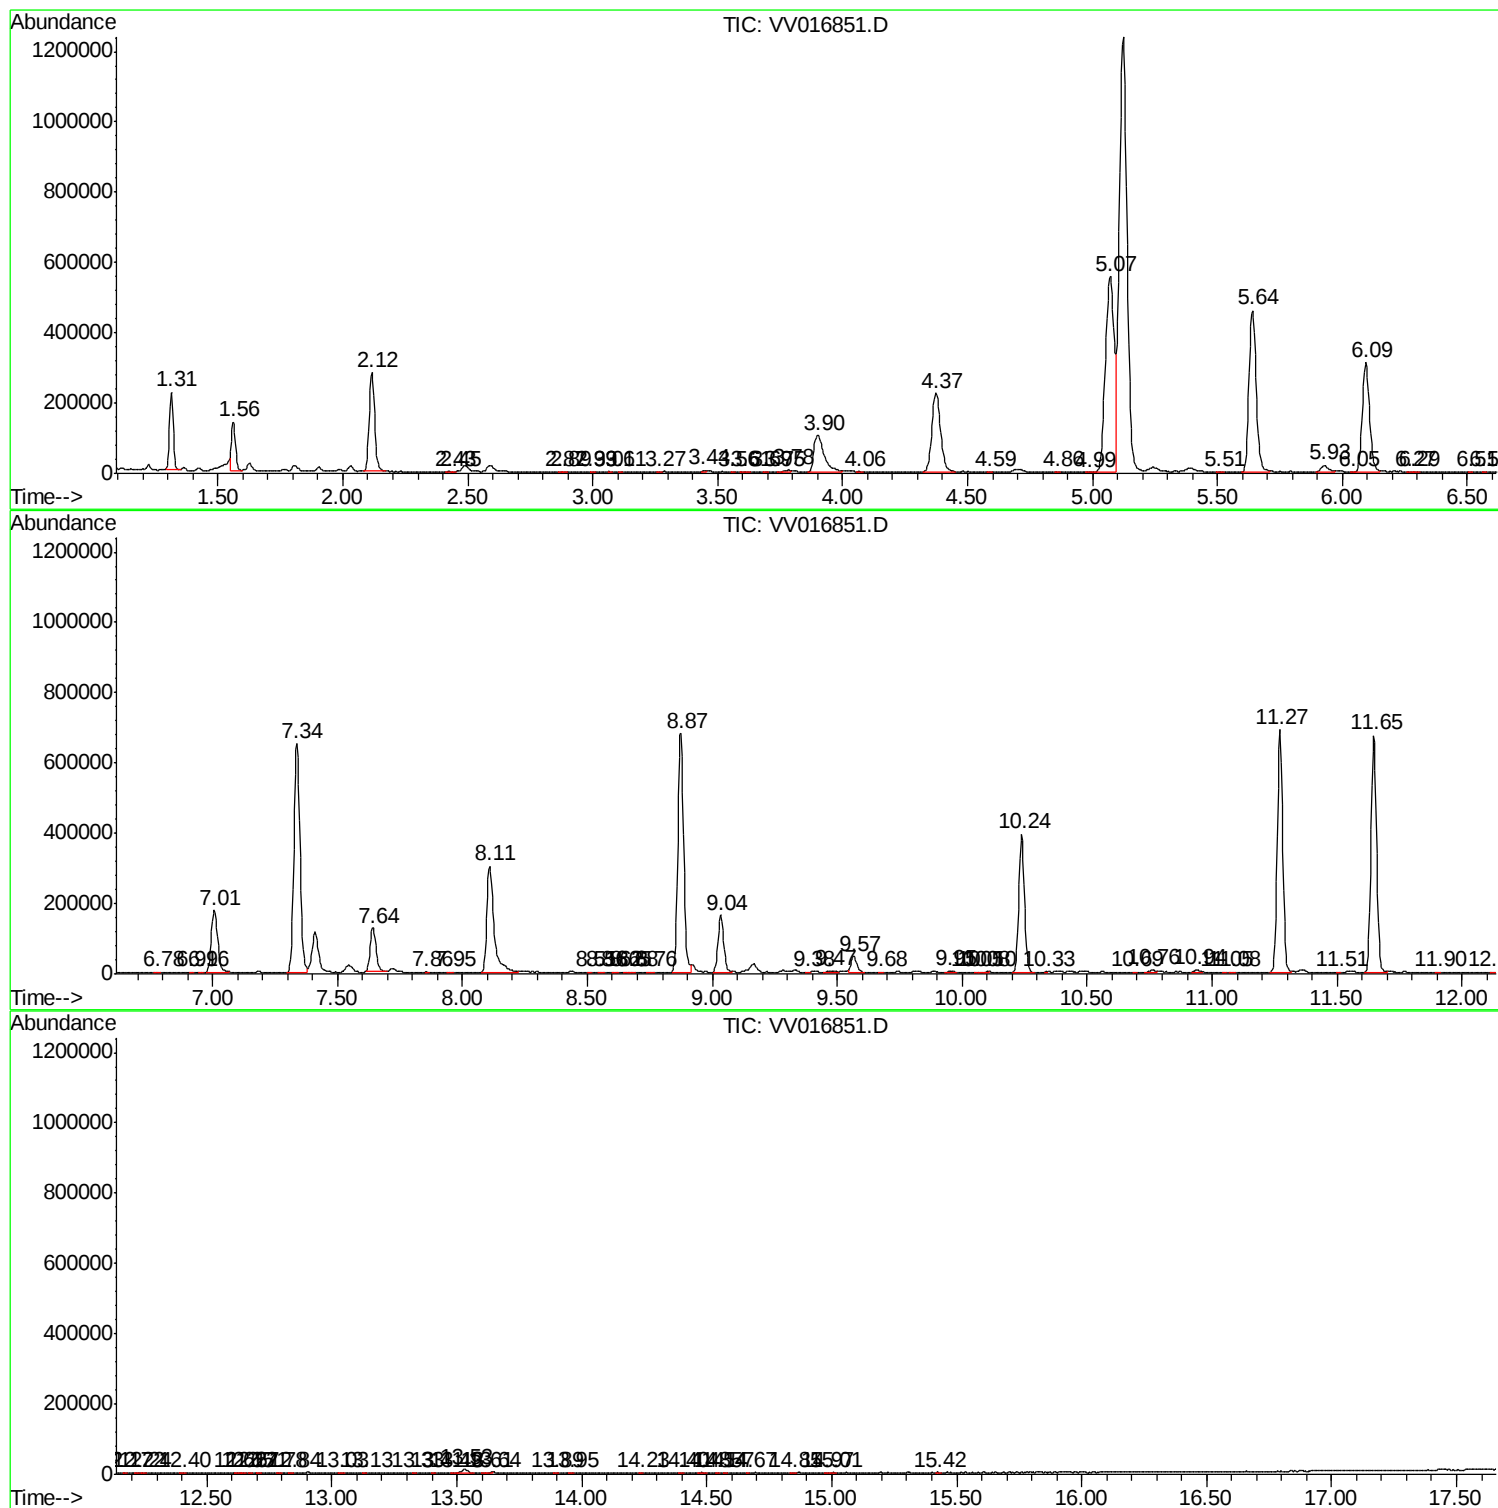

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016851.D
Acq On : 12 Jun 2020 01:10
Operator : SY/MD
Sample : L2915-12DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E20DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016851.D
Acq On : 12 Jun 2020 01:10
Operator : SY/MD
Sample : L2915-12DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E20DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc