

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016853.D
 Acq On : 12 Jun 2020 01:58
 Operator : SY/MD
 Sample : L2915-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E22DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	209613	214804	16.34%	1.901%
2	1.560	141	146	159	rVB	122374	144473	10.99%	1.278%
3	2.116	310	319	335	rVB	271547	397925	30.27%	3.521%
4	2.418	411	413	414	rBV2	1931	707	0.05%	0.006%
5	2.691	496	498	503	rBV5	1733	1308	0.10%	0.012%
6	2.862	548	551	553	rBV4	1253	727	0.06%	0.006%
7	3.032	601	604	607	rBV5	1553	1121	0.09%	0.010%
8	3.145	637	639	641	rVB3	1671	652	0.05%	0.006%
9	3.164	641	645	646	rBV3	947	648	0.05%	0.006%
10	3.245	667	670	674	rVB5	2466	1679	0.13%	0.015%
11	3.273	677	679	681	rBV3	1291	831	0.06%	0.007%
12	3.415	716	723	725	rBV7	2179	2170	0.17%	0.019%
13	3.521	754	756	759	rBV4	1820	979	0.07%	0.009%
14	3.627	785	789	793	rBV7	1074	880	0.07%	0.008%
15	3.695	806	810	814	rVB6	1451	1373	0.10%	0.012%
16	3.714	814	816	822	rVB6	1563	1109	0.08%	0.010%
17	3.749	822	827	829	rBV5	2779	2598	0.20%	0.023%
18	3.852	857	859	862	rBV4	1554	1071	0.08%	0.009%
19	3.897	862	873	900	rBV	103416	293834	22.35%	2.600%
20	4.322	1001	1005	1006	rBV3	1921	1216	0.09%	0.011%
21	4.373	1006	1021	1040	rVV	216744	528193	40.17%	4.673%
22	4.540	1070	1073	1076	rBV4	1219	1015	0.08%	0.009%
23	4.781	1143	1148	1150	rBV5	1588	1059	0.08%	0.009%
24	4.826	1157	1162	1167	rBV7	1990	2258	0.17%	0.020%
25	4.884	1176	1180	1184	rBV5	1404	1422	0.11%	0.013%
26	5.003	1215	1217	1220	rBV3	1497	1014	0.08%	0.009%
27	5.071	1220	1238	1245	rBV2	537907	1314762	100.00%	11.633%
28	5.537	1381	1383	1386	rBV4	1380	925	0.07%	0.008%
29	5.640	1402	1415	1436	rBV	445561	884420	67.27%	7.825%
30	6.093	1543	1556	1574	rVV	302225	603517	45.90%	5.340%
31	6.322	1624	1627	1629	rBV3	1571	1041	0.08%	0.009%
32	6.434	1660	1662	1667	rVB5	2907	2018	0.15%	0.018%
33	6.486	1676	1678	1684	rBV6	2484	1796	0.14%	0.016%
34	6.514	1684	1687	1688	rBV3	1652	922	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016853.D
 Acq On : 12 Jun 2020 01:58
 Operator : SY/MD
 Sample : L2915-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E22DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.566	1700	1703	1706	rBV5	1495	934	0.07%	0.008%
36	6.656	1728	1731	1732	rBV3	1663	767	0.06%	0.007%
37	6.730	1750	1754	1759	rBV7	1593	1694	0.13%	0.015%
38	6.756	1759	1762	1764	rVB3	1189	727	0.06%	0.006%
39	6.797	1773	1775	1777	rBV2	1314	742	0.06%	0.007%
40	6.929	1812	1816	1819	rBV6	2378	1669	0.13%	0.015%
41	6.945	1819	1821	1824	rBV3	1228	747	0.06%	0.007%
42	7.006	1830	1840	1858	rBV	167497	295214	22.45%	2.612%
43	7.338	1931	1943	1956	rBV	617732	1069859	81.37%	9.466%
44	7.408	1956	1965	1980	rVB	268093	459161	34.92%	4.062%
45	7.601	2021	2025	2027	rBV4	2087	1478	0.11%	0.013%
46	7.643	2028	2038	2054	rVV2	119657	200542	15.25%	1.774%
47	7.939	2127	2130	2133	rVB4	1663	1330	0.10%	0.012%
48	7.955	2133	2135	2137	rBV3	1403	805	0.06%	0.007%
49	8.109	2171	2183	2215	rBV	311375	616490	46.89%	5.454%
50	8.556	2319	2322	2325	rBV4	1552	1120	0.09%	0.010%
51	8.614	2337	2340	2342	rBV3	1205	959	0.07%	0.008%
52	8.717	2370	2372	2378	rVB7	1673	1247	0.09%	0.011%
53	8.752	2381	2383	2384	rBV2	1544	651	0.05%	0.006%
54	8.807	2398	2400	2403	rVB2	1339	667	0.05%	0.006%
55	8.875	2409	2421	2434	rBV	655538	1064539	80.97%	9.419%
56	9.035	2461	2471	2485	rBV	173865	275040	20.92%	2.433%
57	9.161	2494	2510	2524	rVB2	31791	67668	5.15%	0.599%
58	9.257	2538	2540	2542	rBV2	1712	726	0.06%	0.006%
59	9.566	2629	2636	2651	rVB	33739	56362	4.29%	0.499%
60	9.688	2672	2674	2677	rVB3	1338	681	0.05%	0.006%
61	9.791	2702	2706	2708	rBV5	1403	1135	0.09%	0.010%
62	9.881	2730	2734	2735	rBV3	2505	1781	0.14%	0.016%
63	9.945	2751	2754	2756	rBV4	3217	2386	0.18%	0.021%
64	10.238	2833	2845	2861	rBV	390201	605291	46.04%	5.355%
65	10.363	2882	2884	2886	rBV3	2034	1152	0.09%	0.010%
66	10.656	2972	2975	2979	rVB3	1166	650	0.05%	0.006%
67	10.710	2990	2992	2995	rBV4	1254	869	0.07%	0.008%
68	11.045	3091	3096	3100	rBV7	1167	1507	0.11%	0.013%
69	11.180	3135	3138	3139	rBV3	1511	839	0.06%	0.007%
70	11.270	3153	3166	3184	rBV	687863	1051561	79.98%	9.304%
71	11.553	3246	3254	3260	rBV10	5725	7476	0.57%	0.066%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016853.D
 Acq On : 12 Jun 2020 01:58
 Operator : SY/MD
 Sample : L2915-14DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E22DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3299	rBV	672948	1042782	79.31%	9.226%
73	11.842	3340	3344	3346	rBV5	1303	991	0.08%	0.009%
74	11.900	3359	3362	3366	rBV5	1186	949	0.07%	0.008%
75	12.099	3422	3424	3426	rVB3	2289	936	0.07%	0.008%
76	12.122	3426	3431	3434	rBV6	2048	2121	0.16%	0.019%
77	12.190	3448	3452	3454	rBV4	1424	1140	0.09%	0.010%
78	12.344	3498	3500	3503	rVB3	1755	643	0.05%	0.006%
79	12.460	3532	3536	3537	rBV3	1459	957	0.07%	0.008%
80	12.553	3562	3565	3566	rBV4	1221	693	0.05%	0.006%
81	12.894	3668	3671	3672	rBV3	2481	1246	0.09%	0.011%
82	12.968	3691	3694	3698	rBV5	1415	931	0.07%	0.008%
83	13.045	3715	3718	3721	rBV4	1470	999	0.08%	0.009%
84	13.228	3771	3775	3777	rBV5	1117	972	0.07%	0.009%
85	13.321	3800	3804	3806	rBV4	1427	1086	0.08%	0.010%
86	13.447	3838	3843	3846	rBV6	2188	2127	0.16%	0.019%
87	13.530	3861	3869	3879	rVB	12678	19130	1.46%	0.169%
88	13.636	3900	3902	3904	rBV4	2142	1312	0.10%	0.012%
89	13.833	3959	3963	3964	rBV4	1669	1114	0.08%	0.010%
90	14.000	4012	4015	4017	rBV3	1525	779	0.06%	0.007%
91	14.148	4059	4061	4066	rBV4	1324	1044	0.08%	0.009%
92	14.270	4097	4099	4102	rBV4	1138	793	0.06%	0.007%
93	14.389	4130	4136	4137	rBV6	1115	954	0.07%	0.008%
94	14.424	4145	4147	4151	rBV4	1493	1336	0.10%	0.012%
95	14.636	4211	4213	4215	rBV3	1141	674	0.05%	0.006%
96	14.678	4223	4226	4229	rBV3	1960	1226	0.09%	0.011%
97	15.363	4437	4439	4442	rBV3	1541	995	0.08%	0.009%
98	15.604	4512	4514	4517	rBV4	2179	1195	0.09%	0.011%
99	15.868	4593	4596	4597	rBV2	1787	1131	0.09%	0.010%
100	15.955	4621	4623	4626	rBV3	2005	1237	0.09%	0.011%


Sum of corrected areas: 11302426

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016853.D
Acq On : 12 Jun 2020 01:58
Operator : SY/MD
Sample : L2915-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E22DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

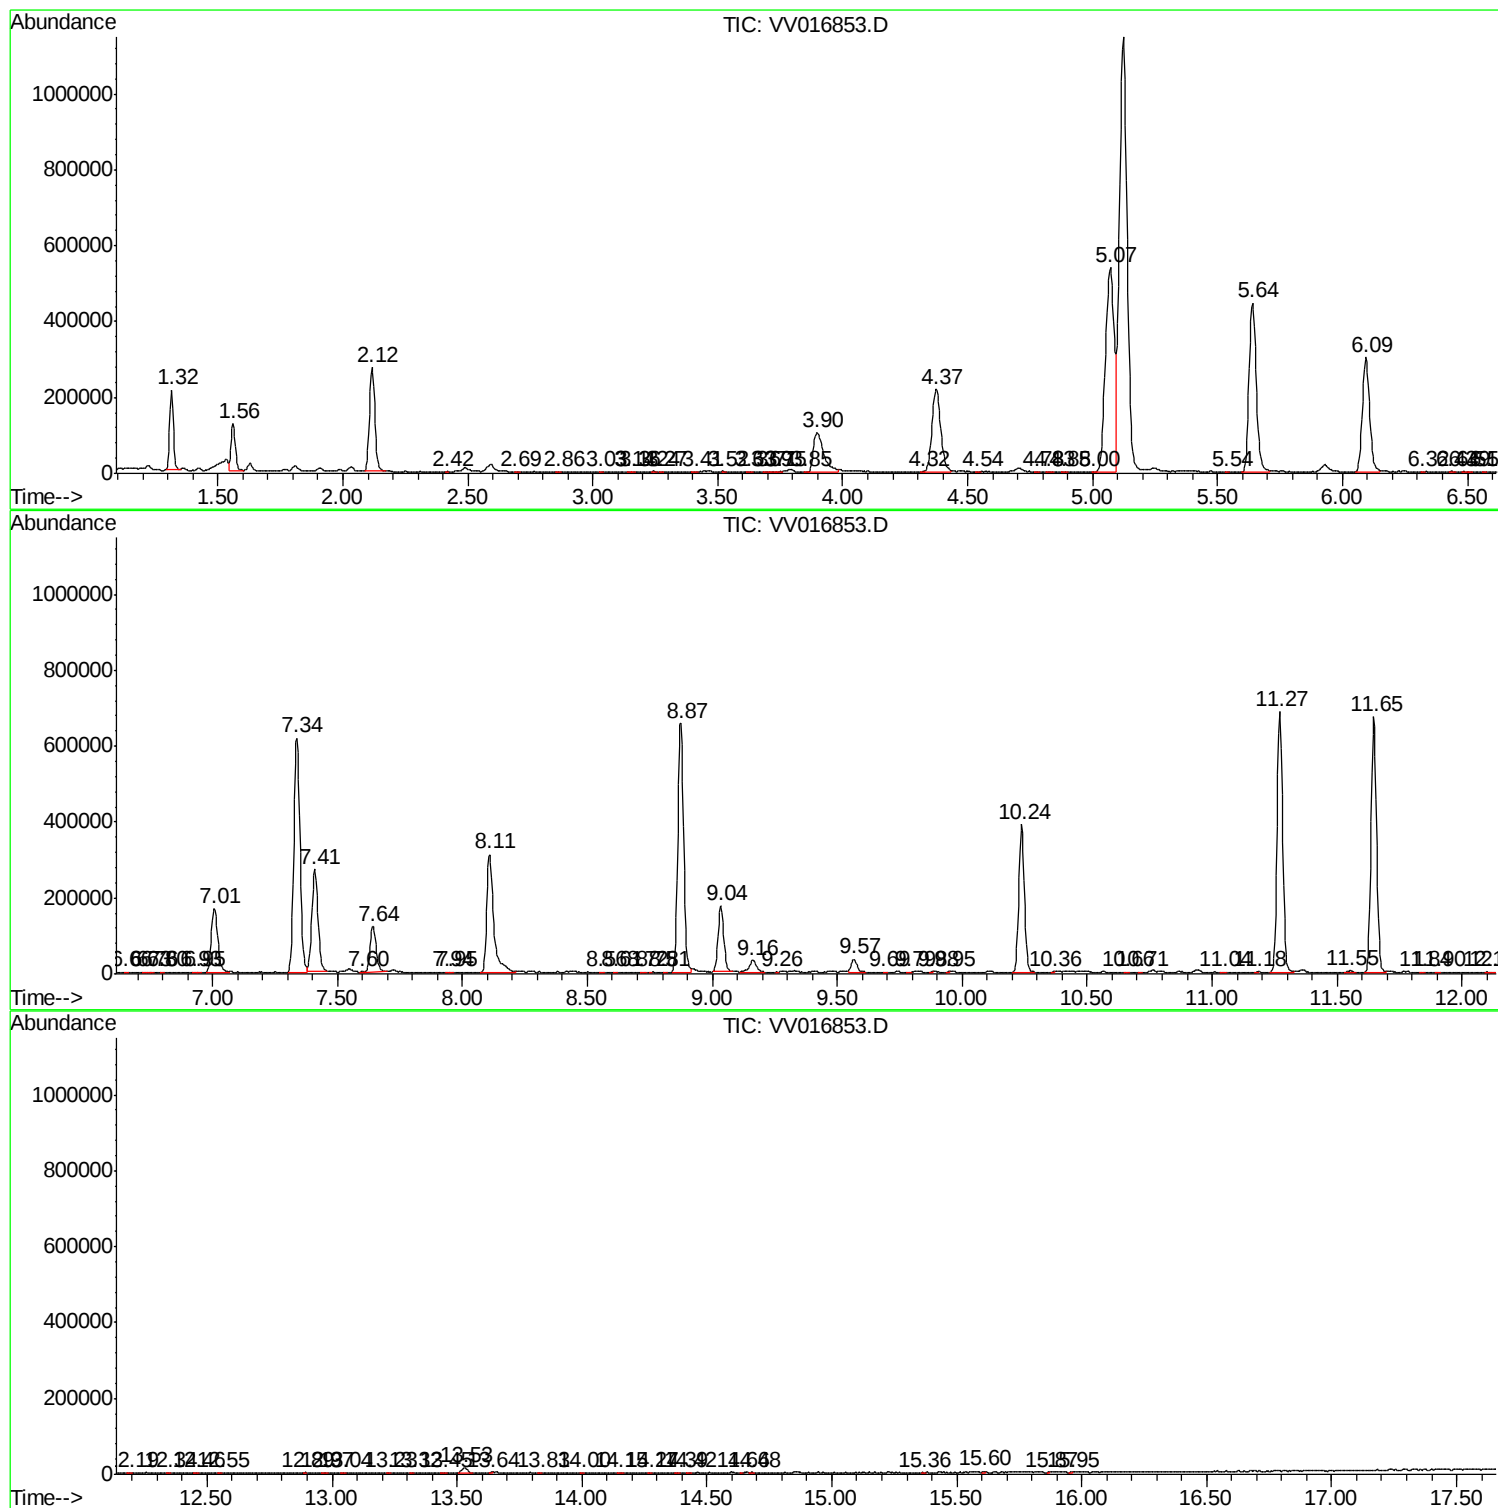

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016853.D
Acq On : 12 Jun 2020 01:58
Operator : SY/MD
Sample : L2915-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E22DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016853.D
Acq On : 12 Jun 2020 01:58
Operator : SY/MD
Sample : L2915-14DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E22DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc