

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016854.D
 Acq On : 12 Jun 2020 02:21
 Operator : SY/MD
 Sample : L2915-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	207884	211894	16.84%	1.863%
2	1.553	138	144	154	rVB	110772	133200	10.59%	1.171%
3	2.113	309	318	332	rBV	263767	393857	31.31%	3.462%
4	2.428	414	416	418	rBV3	1749	820	0.07%	0.007%
5	2.769	517	522	528	rVB9	2070	2579	0.20%	0.023%
6	2.942	574	576	579	rBV4	1560	925	0.07%	0.008%
7	3.010	595	597	599	rBV3	1271	754	0.06%	0.007%
8	3.280	679	681	684	rBV3	1489	843	0.07%	0.007%
9	3.441	727	731	732	rBV3	2375	1617	0.13%	0.014%
10	3.534	755	760	765	rBV8	2392	2642	0.21%	0.023%
11	3.573	770	772	775	rBV4	1040	770	0.06%	0.007%
12	3.605	780	782	789	rVV8	1949	1733	0.14%	0.015%
13	3.650	793	796	800	rBV6	1525	959	0.08%	0.008%
14	3.897	862	873	903	rVV	103296	292920	23.28%	2.575%
15	4.248	979	982	986	rBV5	1640	1236	0.10%	0.011%
16	4.373	1007	1021	1045	rVB	217030	525575	41.77%	4.620%
17	4.785	1147	1149	1153	rVV5	1086	723	0.06%	0.006%
18	4.933	1190	1195	1197	rBV6	1423	892	0.07%	0.008%
19	5.071	1221	1238	1244	rBV2	524898	1258128	100.00%	11.060%
20	5.640	1402	1415	1433	rVV	435813	861686	68.49%	7.575%
21	5.839	1474	1477	1479	rBV3	2362	1249	0.10%	0.011%
22	5.926	1495	1504	1517	rBV4	17889	34604	2.75%	0.304%
23	6.093	1542	1556	1575	rBV	295696	599497	47.65%	5.270%
24	6.373	1641	1643	1647	rVB5	1836	1086	0.09%	0.010%
25	6.457	1666	1669	1671	rBV3	1349	869	0.07%	0.008%
26	7.007	1827	1840	1857	rBV	170229	304176	24.18%	2.674%
27	7.138	1877	1881	1882	rBV3	1305	787	0.06%	0.007%
28	7.177	1891	1893	1896	rBV4	1880	975	0.08%	0.009%
29	7.293	1926	1929	1930	rBV4	1581	855	0.07%	0.008%
30	7.338	1930	1943	1955	rVV	622269	1064322	84.60%	9.356%
31	7.408	1956	1965	1982	rVB	298805	502650	39.95%	4.419%
32	7.640	2028	2037	2052	rBV	124345	200071	15.90%	1.759%
33	7.836	2091	2098	2102	rBV9	2156	2331	0.19%	0.020%
34	7.868	2105	2108	2109	rBV2	1150	735	0.06%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016854.D
 Acq On : 12 Jun 2020 02:21
 Operator : SY/MD
 Sample : L2915-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.878	2109	2111	2117	rVB7	1254	841	0.07%	0.007%
36	7.965	2132	2138	2141	rBV7	1436	1224	0.10%	0.011%
37	8.003	2148	2150	2152	rBV3	1387	843	0.07%	0.007%
38	8.109	2171	2183	2215	rVV	315323	621567	49.40%	5.464%
39	8.617	2337	2341	2343	rBV4	1435	1191	0.09%	0.010%
40	8.659	2352	2354	2359	rVB6	1699	1369	0.11%	0.012%
41	8.701	2364	2367	2370	rBV5	1878	1251	0.10%	0.011%
42	8.746	2377	2381	2383	rBV4	1153	802	0.06%	0.007%
43	8.810	2398	2401	2406	rBV7	1464	1314	0.10%	0.012%
44	8.871	2409	2420	2434	rBV	661378	1058266	84.11%	9.303%
45	9.035	2460	2471	2486	rVB	184097	290905	23.12%	2.557%
46	9.331	2556	2563	2570	rBV	3743	6574	0.52%	0.058%
47	9.460	2601	2603	2605	rBV3	2118	1323	0.11%	0.012%
48	9.505	2615	2617	2618	rBV3	1819	894	0.07%	0.008%
49	9.566	2629	2636	2652	rVB	38142	62528	4.97%	0.550%
50	9.801	2703	2709	2713	rBV10	2499	2866	0.23%	0.025%
51	9.955	2753	2757	2767	rVB10	4611	6459	0.51%	0.057%
52	9.997	2767	2770	2773	rBV4	1420	1250	0.10%	0.011%
53	10.161	2815	2821	2823	rBV6	1036	1018	0.08%	0.009%
54	10.238	2833	2845	2864	rBV	396431	610588	48.53%	5.368%
55	10.379	2881	2889	2891	rBV6	4571	6120	0.49%	0.054%
56	10.669	2976	2979	2982	rBV4	1446	927	0.07%	0.008%
57	10.759	2997	3007	3014	rBV4	6755	12949	1.03%	0.114%
58	10.936	3052	3062	3074	rBV4	8171	15287	1.22%	0.134%
59	11.029	3085	3091	3094	rVV8	1118	1197	0.10%	0.011%
60	11.180	3134	3138	3140	rBV4	1822	1583	0.13%	0.014%
61	11.270	3154	3166	3182	rBV	712146	1078440	85.72%	9.480%
62	11.553	3247	3254	3259	rBV7	5416	7645	0.61%	0.067%
63	11.646	3271	3283	3300	rBV	695621	1095915	87.11%	9.634%
64	11.833	3337	3341	3342	rBV3	1737	1201	0.10%	0.011%
65	11.891	3356	3359	3363	rVV4	1291	1067	0.08%	0.009%
66	11.919	3365	3368	3371	rBV5	1290	766	0.06%	0.007%
67	11.955	3376	3379	3381	rBV4	2430	1600	0.13%	0.014%
68	12.045	3401	3407	3408	rBV6	2637	2378	0.19%	0.021%
69	12.080	3416	3418	3420	rVB3	1743	736	0.06%	0.006%
70	12.103	3422	3425	3430	rVB6	2057	1824	0.14%	0.016%
71	12.167	3442	3445	3448	rBV4	1832	1583	0.13%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016854.D
 Acq On : 12 Jun 2020 02:21
 Operator : SY/MD
 Sample : L2915-15DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E23DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.231	3461	3465	3468	rBV4	1746	1121	0.09%	0.010%
73	12.270	3474	3477	3479	rBV4	1463	956	0.08%	0.008%
74	12.334	3493	3497	3498	rBV4	1097	721	0.06%	0.006%
75	12.389	3511	3514	3519	rVB5	1728	1260	0.10%	0.011%
76	12.624	3584	3587	3592	rBV6	1235	1021	0.08%	0.009%
77	12.694	3605	3609	3613	rBV5	1404	1319	0.10%	0.012%
78	12.733	3618	3621	3624	rBV4	1795	1271	0.10%	0.011%
79	12.804	3639	3643	3647	rBV7	1300	1290	0.10%	0.011%
80	12.900	3667	3673	3676	rBV7	2725	3084	0.25%	0.027%
81	13.026	3708	3712	3717	rVB8	1909	1669	0.13%	0.015%
82	13.055	3717	3721	3723	rBV4	1706	1310	0.10%	0.012%
83	13.141	3745	3748	3753	rBV7	1889	1648	0.13%	0.014%
84	13.215	3767	3771	3773	rBV4	1095	808	0.06%	0.007%
85	13.263	3783	3786	3788	rBV3	1647	903	0.07%	0.008%
86	13.386	3822	3824	3831	rVB6	1769	1497	0.12%	0.013%
87	13.466	3844	3849	3852	rBV6	2091	1632	0.13%	0.014%
88	13.527	3859	3868	3880	rBV3	15866	27126	2.16%	0.238%
89	13.649	3903	3906	3912	rVB8	2631	2519	0.20%	0.022%
90	13.746	3934	3936	3939	rBV4	1181	869	0.07%	0.008%
91	13.797	3950	3952	3956	rVB3	1491	1050	0.08%	0.009%
92	13.855	3966	3970	3974	rBV6	2102	1574	0.13%	0.014%
93	13.890	3977	3981	3984	rBV4	2074	1276	0.10%	0.011%
94	14.270	4096	4099	4102	rBV5	1035	783	0.06%	0.007%
95	14.434	4148	4150	4152	rBV3	1601	912	0.07%	0.008%
96	14.662	4217	4221	4223	rBV5	2059	1635	0.13%	0.014%
97	14.804	4263	4265	4267	rVB3	1761	749	0.06%	0.007%
98	15.048	4339	4341	4344	rBV4	1597	834	0.07%	0.007%
99	15.257	4403	4406	4409	rBV4	2038	1407	0.11%	0.012%
100	15.350	4433	4435	4438	rBV4	2095	1014	0.08%	0.009%


Sum of corrected areas: 11375509

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016854.D
Acq On : 12 Jun 2020 02:21
Operator : SY/MD
Sample : L2915-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

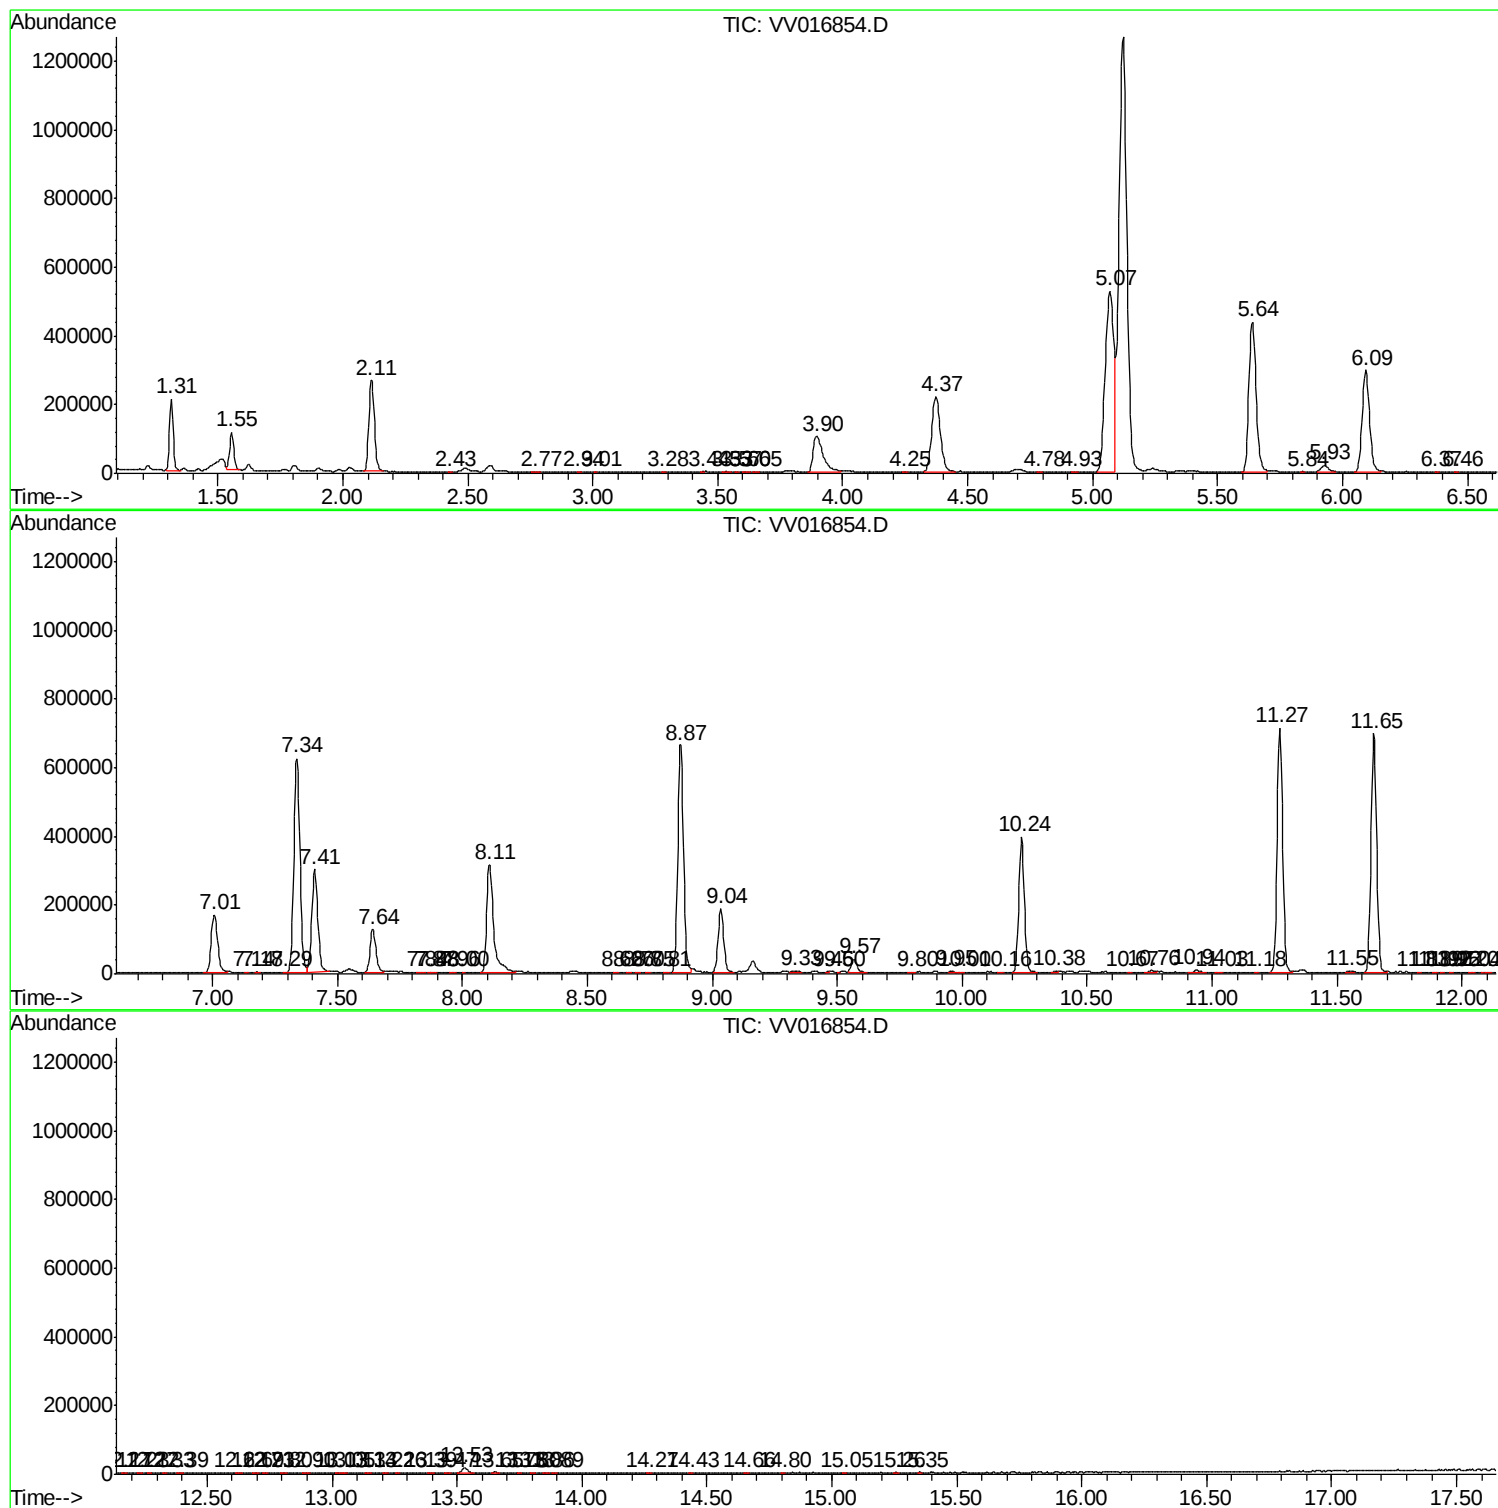

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016854.D
Acq On : 12 Jun 2020 02:21
Operator : SY/MD
Sample : L2915-15DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061120\
Data File : VV016854.D
Acq On : 12 Jun 2020 02:21
Operator : SY/MD
Sample : L2915-15DL 200X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9E23DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc