

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016857.D
 Acq On : 12 Jun 2020 03:32
 Operator : SY/MD
 Sample : L2915-16DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	201769	208079	15.54%	1.895%
2	2.116	309	319	335	rBV	268868	401288	29.97%	3.654%
3	2.714	501	505	509	rBV5	969	861	0.06%	0.008%
4	2.846	543	546	550	rBV6	1444	1531	0.11%	0.014%
5	2.884	555	558	562	rBV4	1559	1117	0.08%	0.010%
6	2.949	576	578	581	rBV3	1523	1084	0.08%	0.010%
7	3.196	650	655	656	rBV4	1507	1008	0.08%	0.009%
8	3.232	662	666	672	rBV8	2045	1750	0.13%	0.016%
9	3.257	672	674	676	rBV4	1646	1000	0.07%	0.009%
10	3.380	709	712	715	rVB5	1217	879	0.07%	0.008%
11	3.566	767	770	772	rBV4	1208	1004	0.07%	0.009%
12	3.598	777	780	784	rBV4	1310	1016	0.08%	0.009%
13	3.698	809	811	813	rVB3	1394	729	0.05%	0.007%
14	3.720	813	818	819	rBV5	1473	1199	0.09%	0.011%
15	3.759	825	830	832	rBV5	2542	2436	0.18%	0.022%
16	3.897	863	873	910	rBV	105572	296241	22.12%	2.698%
17	4.109	935	939	940	rBV5	1550	999	0.07%	0.009%
18	4.196	959	966	972	rBV10	1642	2526	0.19%	0.023%
19	4.373	1006	1021	1046	rVB2	222715	540867	40.39%	4.925%
20	4.823	1157	1161	1162	rBV3	1824	1133	0.08%	0.010%
21	4.897	1180	1184	1187	rBV4	1637	1353	0.10%	0.012%
22	4.939	1195	1197	1199	rVB3	1777	811	0.06%	0.007%
23	5.010	1216	1219	1221	rBV4	1960	1332	0.10%	0.012%
24	5.071	1221	1238	1245	rBV3	543187	1338951	100.00%	12.192%
25	5.486	1364	1367	1370	rBV5	1528	1339	0.10%	0.012%
26	5.502	1370	1372	1374	rBV2	1923	1127	0.08%	0.010%
27	5.582	1394	1397	1400	rBV5	2068	1389	0.10%	0.013%
28	5.640	1402	1415	1438	rVV	448022	890744	66.53%	8.111%
29	6.093	1541	1556	1576	rBV	305106	619906	46.30%	5.645%
30	6.351	1634	1636	1639	rBV4	1677	977	0.07%	0.009%
31	6.630	1720	1723	1725	rBV3	1621	1158	0.09%	0.011%
32	6.685	1738	1740	1744	rVB5	1713	1060	0.08%	0.010%
33	6.820	1779	1782	1785	rBV4	1077	983	0.07%	0.009%
34	6.939	1817	1819	1822	rBV4	1370	809	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016857.D
 Acq On : 12 Jun 2020 03:32
 Operator : SY/MD
 Sample : L2915-16DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1830	1840	1858	rVV	167892	298810	22.32%	2.721%
36	7.235	1907	1911	1913	rBV4	1186	920	0.07%	0.008%
37	7.267	1919	1921	1924	rVB4	1881	1046	0.08%	0.010%
38	7.338	1931	1943	1956	rBV	635929	1086181	81.12%	9.891%
39	7.408	1957	1965	1983	rVB	198894	349601	26.11%	3.183%
40	7.640	2028	2037	2050	rBV	122424	200876	15.00%	1.829%
41	7.894	2112	2116	2117	rBV3	1145	671	0.05%	0.006%
42	7.971	2133	2140	2142	rBV8	1657	1979	0.15%	0.018%
43	7.984	2142	2144	2148	rBV4	1207	1151	0.09%	0.010%
44	8.058	2164	2167	2168	rBV3	1505	718	0.05%	0.007%
45	8.109	2172	2183	2210	rBV	306965	605099	45.19%	5.510%
46	8.875	2407	2421	2444	rBV	681489	1090568	81.45%	9.931%
47	9.035	2460	2471	2482	rBV	126944	199580	14.91%	1.817%
48	9.402	2578	2585	2594	rBV	4273	6749	0.50%	0.061%
49	9.566	2630	2636	2653	rVB2	26716	45469	3.40%	0.414%
50	9.739	2685	2690	2692	rBV5	1838	1494	0.11%	0.014%
51	9.804	2704	2710	2712	rBV6	1746	2116	0.16%	0.019%
52	9.936	2747	2751	2753	rBV5	1101	823	0.06%	0.007%
53	10.083	2793	2797	2799	rBV3	1410	1170	0.09%	0.011%
54	10.100	2799	2802	2803	rBV3	1724	989	0.07%	0.009%
55	10.180	2825	2827	2830	rBV4	1641	690	0.05%	0.006%
56	10.238	2834	2845	2859	rVV	383977	606935	45.33%	5.527%
57	10.559	2943	2945	2952	rVB8	2853	2580	0.19%	0.023%
58	10.649	2971	2973	2975	rBV3	1536	795	0.06%	0.007%
59	10.665	2975	2978	2981	rVB5	1406	884	0.07%	0.008%
60	10.710	2989	2992	2993	rBV3	1302	728	0.05%	0.007%
61	10.810	3020	3023	3024	rBV2	1326	697	0.05%	0.006%
62	10.939	3058	3063	3068	rBV5	5106	5581	0.42%	0.051%
63	10.981	3073	3076	3081	rBV6	1122	803	0.06%	0.007%
64	11.138	3122	3125	3127	rVB4	1914	1010	0.08%	0.009%
65	11.190	3139	3141	3147	rVB7	1441	1364	0.10%	0.012%
66	11.270	3155	3166	3184	rVV	683184	1040053	77.68%	9.471%
67	11.482	3228	3232	3235	rBV6	1775	1474	0.11%	0.013%
68	11.524	3242	3245	3247	rBV4	1400	934	0.07%	0.009%
69	11.537	3247	3249	3250	rBV2	1786	756	0.06%	0.007%
70	11.646	3272	3283	3297	rBV	673089	1044704	78.02%	9.513%
71	11.932	3370	3372	3374	rVB3	1495	699	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016857.D
 Acq On : 12 Jun 2020 03:32
 Operator : SY/MD
 Sample : L2915-16DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.029	3399	3402	3405	rBV4	1440	741	0.06%	0.007%
73	12.048	3405	3408	3410	rBV4	1420	803	0.06%	0.007%
74	12.141	3431	3437	3440	rVB5	2511	2100	0.16%	0.019%
75	12.212	3455	3459	3462	rBV5	1744	1540	0.12%	0.014%
76	12.235	3462	3466	3468	rBV5	1376	1004	0.07%	0.009%
77	12.299	3481	3486	3489	rVV6	1784	1349	0.10%	0.012%
78	12.395	3513	3516	3517	rBV3	1497	774	0.06%	0.007%
79	12.408	3517	3520	3523	rVV5	1216	995	0.07%	0.009%
80	12.585	3570	3575	3577	rBV5	1607	1339	0.10%	0.012%
81	12.598	3577	3579	3582	rBV3	1047	753	0.06%	0.007%
82	12.704	3609	3612	3616	rBV4	1032	1004	0.07%	0.009%
83	12.746	3622	3625	3627	rBV3	1137	731	0.05%	0.007%
84	12.804	3641	3643	3646	rBV5	1266	801	0.06%	0.007%
85	12.903	3670	3674	3677	rVV6	2060	1741	0.13%	0.016%
86	13.038	3714	3716	3719	rBV4	1560	884	0.07%	0.008%
87	13.357	3813	3815	3818	rBV2	1240	733	0.05%	0.007%
88	13.453	3841	3845	3847	rBV5	1740	1202	0.09%	0.011%
89	13.527	3860	3868	3878	rVV2	8201	15455	1.15%	0.141%
90	13.691	3916	3919	3921	rBV5	1321	806	0.06%	0.007%
91	14.006	4011	4017	4020	rBV6	2069	2292	0.17%	0.021%
92	14.067	4033	4036	4039	rVV4	2119	1528	0.11%	0.014%
93	14.083	4039	4041	4043	rVV3	1849	735	0.05%	0.007%
94	14.115	4050	4051	4055	rBV4	1166	833	0.06%	0.008%
95	14.382	4132	4134	4137	rBV3	1572	965	0.07%	0.009%
96	14.485	4163	4166	4167	rBV3	1766	888	0.07%	0.008%
97	14.820	4266	4270	4271	rBV3	1223	805	0.06%	0.007%
98	15.009	4324	4329	4331	rBV5	1996	1382	0.10%	0.013%
99	15.386	4442	4446	4448	rBV5	1292	922	0.07%	0.008%
100	15.656	4527	4530	4533	rBV4	1871	1489	0.11%	0.014%


Sum of corrected areas: 10981977

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016857.D
Acq On : 12 Jun 2020 03:32
Operator : SY/MD
Sample : L2915-16DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E24DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

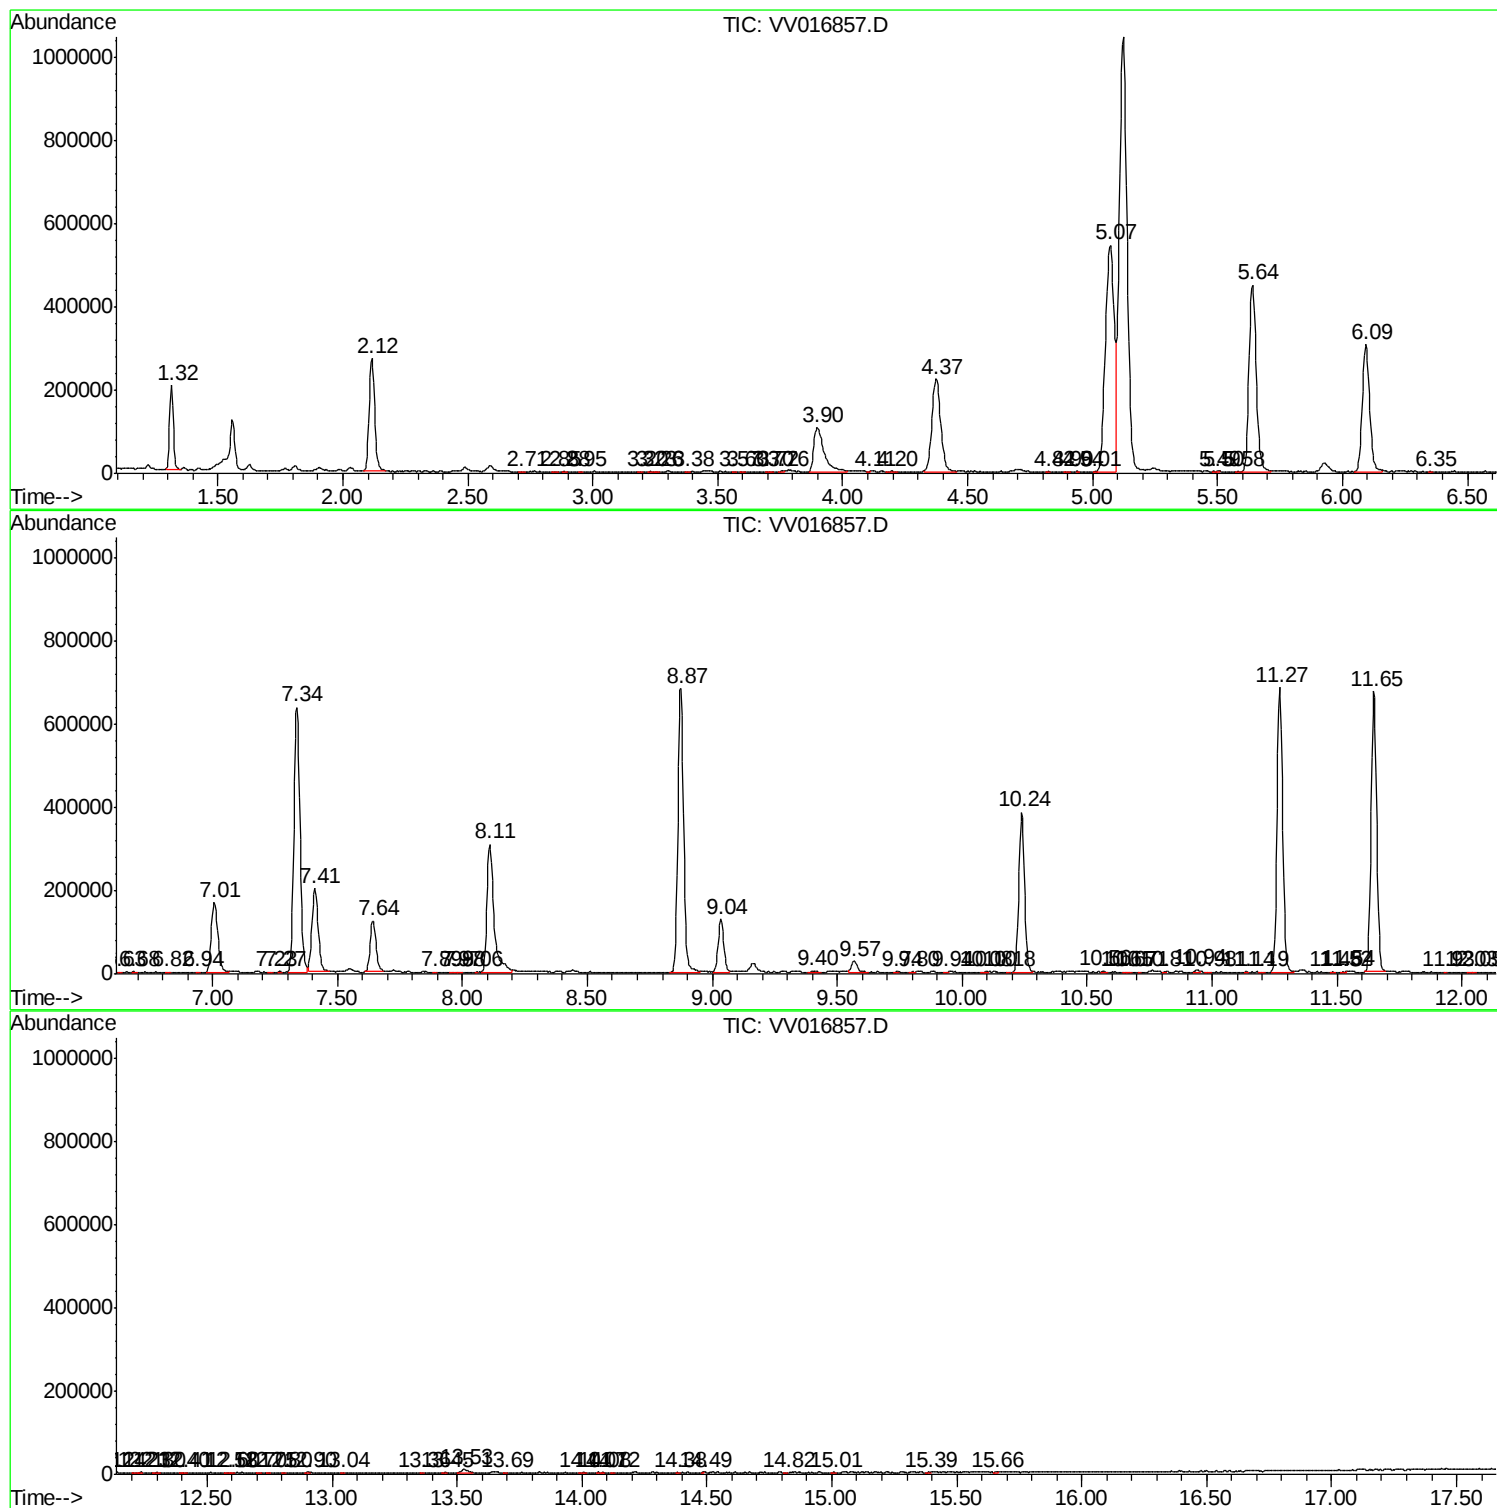

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016857.D
Acq On : 12 Jun 2020 03:32
Operator : SY/MD
Sample : L2915-16DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E24DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016857.D
Acq On : 12 Jun 2020 03:32
Operator : SY/MD
Sample : L2915-16DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E24DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc