

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016859.D
 Acq On : 12 Jun 2020 04:20
 Operator : SY/MD
 Sample : L2915-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E08DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	79	rVB	189464	198747	14.86%	1.860%
2	1.563	143	147	158	rVB	116067	127939	9.56%	1.197%
3	2.116	309	319	336	rBV	277829	415631	31.07%	3.889%
4	2.225	351	353	357	rVB4	1667	794	0.06%	0.007%
5	2.277	366	369	371	rBV3	1259	787	0.06%	0.007%
6	2.438	416	419	422	rBV5	2258	2037	0.15%	0.019%
7	2.586	458	465	475	rBV8	5325	9520	0.71%	0.089%
8	2.740	510	513	515	rBV3	1243	705	0.05%	0.007%
9	2.820	533	538	541	rBV7	1090	1066	0.08%	0.010%
10	3.029	601	603	606	rBV3	2085	1422	0.11%	0.013%
11	3.084	618	620	623	rBV4	1335	958	0.07%	0.009%
12	3.110	626	628	631	rVB3	1335	795	0.06%	0.007%
13	3.225	661	664	665	rBV3	1029	618	0.05%	0.006%
14	3.499	747	749	751	rBV3	1721	963	0.07%	0.009%
15	3.547	758	764	766	rBV6	1959	1944	0.15%	0.018%
16	3.621	785	787	790	rVB3	1915	1167	0.09%	0.011%
17	3.640	790	793	795	rBV3	1700	1088	0.08%	0.010%
18	3.682	804	806	809	rBV4	1022	734	0.05%	0.007%
19	3.695	809	810	816	rVB6	1521	914	0.07%	0.009%
20	3.724	816	819	822	rVB4	1874	1130	0.08%	0.011%
21	3.897	863	873	905	rVV	105565	304465	22.76%	2.849%
22	4.315	1001	1003	1005	rBV3	1421	843	0.06%	0.008%
23	4.373	1007	1021	1049	rVB	226745	548977	41.04%	5.137%
24	4.608	1092	1094	1097	rVB3	1345	650	0.05%	0.006%
25	4.627	1097	1100	1103	rBV5	1477	1196	0.09%	0.011%
26	4.862	1169	1173	1175	rBV4	1491	1147	0.09%	0.011%
27	4.923	1190	1192	1197	rVB6	1214	710	0.05%	0.007%
28	4.962	1199	1204	1206	rBV5	1375	1147	0.09%	0.011%
29	4.991	1210	1213	1214	rBV2	1682	984	0.07%	0.009%
30	5.071	1218	1238	1245	rBV2	549413	1337680	100.00%	12.517%
31	5.486	1364	1367	1369	rBV3	1629	1161	0.09%	0.011%
32	5.640	1402	1415	1436	rBV	442910	877557	65.60%	8.212%
33	5.926	1490	1504	1518	rBV6	22018	46753	3.50%	0.437%
34	6.032	1534	1537	1539	rBV4	1200	841	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016859.D
 Acq On : 12 Jun 2020 04:20
 Operator : SY/MD
 Sample : L2915-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E08DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.093	1544	1556	1579	rVB	309701	625725	46.78%	5.855%
36	6.383	1644	1646	1648	rBV3	1592	674	0.05%	0.006%
37	6.428	1656	1660	1667	rVB8	1841	1797	0.13%	0.017%
38	6.486	1674	1678	1681	rBV6	780	678	0.05%	0.006%
39	6.592	1709	1711	1713	rBV2	1873	1028	0.08%	0.010%
40	6.650	1726	1729	1731	rBV4	1241	1026	0.08%	0.010%
41	6.753	1759	1761	1765	rVB5	1255	827	0.06%	0.008%
42	6.920	1811	1813	1816	rBV4	1581	1180	0.09%	0.011%
43	6.952	1820	1823	1825	rBV4	1455	835	0.06%	0.008%
44	7.007	1830	1840	1862	rVV	170940	305641	22.85%	2.860%
45	7.338	1931	1943	1958	rBV	643502	1100103	82.24%	10.294%
46	7.592	2020	2022	2028	rBV6	1433	923	0.07%	0.009%
47	7.643	2028	2038	2050	rBV	123889	209117	15.63%	1.957%
48	7.859	2102	2105	2108	rBV6	1708	1131	0.08%	0.011%
49	7.888	2110	2114	2118	rVV7	1852	1893	0.14%	0.018%
50	7.917	2121	2123	2126	rVB3	1312	815	0.06%	0.008%
51	7.936	2126	2129	2134	rBV8	1190	1193	0.09%	0.011%
52	7.958	2134	2136	2140	rVB4	1386	733	0.05%	0.007%
53	8.109	2169	2183	2212	rBV	304722	609910	45.59%	5.707%
54	8.441	2281	2286	2294	rVV10	3069	5062	0.38%	0.047%
55	8.486	2298	2300	2304	rBV4	2013	1437	0.11%	0.013%
56	8.733	2373	2377	2380	rBV5	2089	1580	0.12%	0.015%
57	8.756	2382	2384	2388	rVV3	1063	667	0.05%	0.006%
58	8.875	2407	2421	2441	rBV	659067	1080782	80.80%	10.113%
59	9.035	2462	2471	2486	rVB	92628	146285	10.94%	1.369%
60	9.254	2537	2539	2542	rBV3	1566	1063	0.08%	0.010%
61	9.566	2629	2636	2647	rVB	21618	34342	2.57%	0.321%
62	10.058	2785	2789	2790	rBV4	1870	1346	0.10%	0.013%
63	10.068	2790	2792	2797	rVB5	1668	1119	0.08%	0.010%
64	10.109	2797	2805	2809	rBV9	2036	3114	0.23%	0.029%
65	10.238	2834	2845	2859	rBV	382991	594099	44.41%	5.559%
66	10.466	2913	2916	2918	rBV5	2491	1765	0.13%	0.017%
67	10.746	3000	3003	3004	rBV3	1252	736	0.06%	0.007%
68	10.759	3004	3007	3013	rVV6	2847	3283	0.25%	0.031%
69	10.852	3034	3036	3039	rBV4	1394	893	0.07%	0.008%
70	11.013	3084	3086	3091	rBV5	744	599	0.04%	0.006%
71	11.158	3127	3131	3133	rBV4	1657	1444	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016859.D
 Acq On : 12 Jun 2020 04:20
 Operator : SY/MD
 Sample : L2915-04DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E08DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3186	rBV	651268	1000149	74.77%	9.359%
73	11.508	3236	3240	3241	rBV3	1124	716	0.05%	0.007%
74	11.646	3271	3283	3300	rBV	668710	1020993	76.33%	9.554%
75	11.875	3349	3354	3355	rBV4	1259	1132	0.08%	0.011%
76	11.884	3355	3357	3360	rVB3	1221	749	0.06%	0.007%
77	12.022	3396	3400	3402	rBV3	1416	1238	0.09%	0.012%
78	12.106	3423	3426	3428	rBV4	1451	1109	0.08%	0.010%
79	12.154	3440	3441	3446	rVB4	1024	874	0.07%	0.008%
80	12.241	3465	3468	3470	rBV4	1815	1125	0.08%	0.011%
81	12.315	3489	3491	3494	rBV2	1810	1026	0.08%	0.010%
82	12.334	3494	3497	3498	rBV3	1329	841	0.06%	0.008%
83	12.530	3554	3558	3563	rBV7	1759	1114	0.08%	0.010%
84	12.595	3574	3578	3581	rBV3	2021	1903	0.14%	0.018%
85	12.804	3640	3643	3644	rBV3	1305	758	0.06%	0.007%
86	13.032	3709	3714	3716	rBV6	1622	1182	0.09%	0.011%
87	13.045	3716	3718	3722	rVB4	1632	933	0.07%	0.009%
88	13.186	3760	3762	3764	rBV3	1621	862	0.06%	0.008%
89	13.286	3791	3793	3797	rVB4	1247	685	0.05%	0.006%
90	13.305	3797	3799	3801	rBV2	1844	929	0.07%	0.009%
91	13.360	3814	3816	3817	rBV2	1354	613	0.05%	0.006%
92	13.887	3977	3980	3981	rBV3	1101	691	0.05%	0.006%
93	14.051	4029	4031	4035	rBV4	1607	1468	0.11%	0.014%
94	14.347	4121	4123	4125	rBV3	1452	750	0.06%	0.007%
95	14.437	4149	4151	4155	rVB5	1756	1180	0.09%	0.011%
96	14.460	4155	4158	4163	rBV6	1703	1384	0.10%	0.013%
97	14.656	4217	4219	4221	rBV2	1768	695	0.05%	0.007%
98	15.206	4388	4390	4393	rBV4	1706	930	0.07%	0.009%
99	15.366	4436	4440	4442	rBV4	2006	1775	0.13%	0.017%
100	15.427	4456	4459	4461	rBV4	1970	1063	0.08%	0.010%


Sum of corrected areas: 10686782

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016859.D
Acq On : 12 Jun 2020 04:20
Operator : SY/MD
Sample : L2915-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E08DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

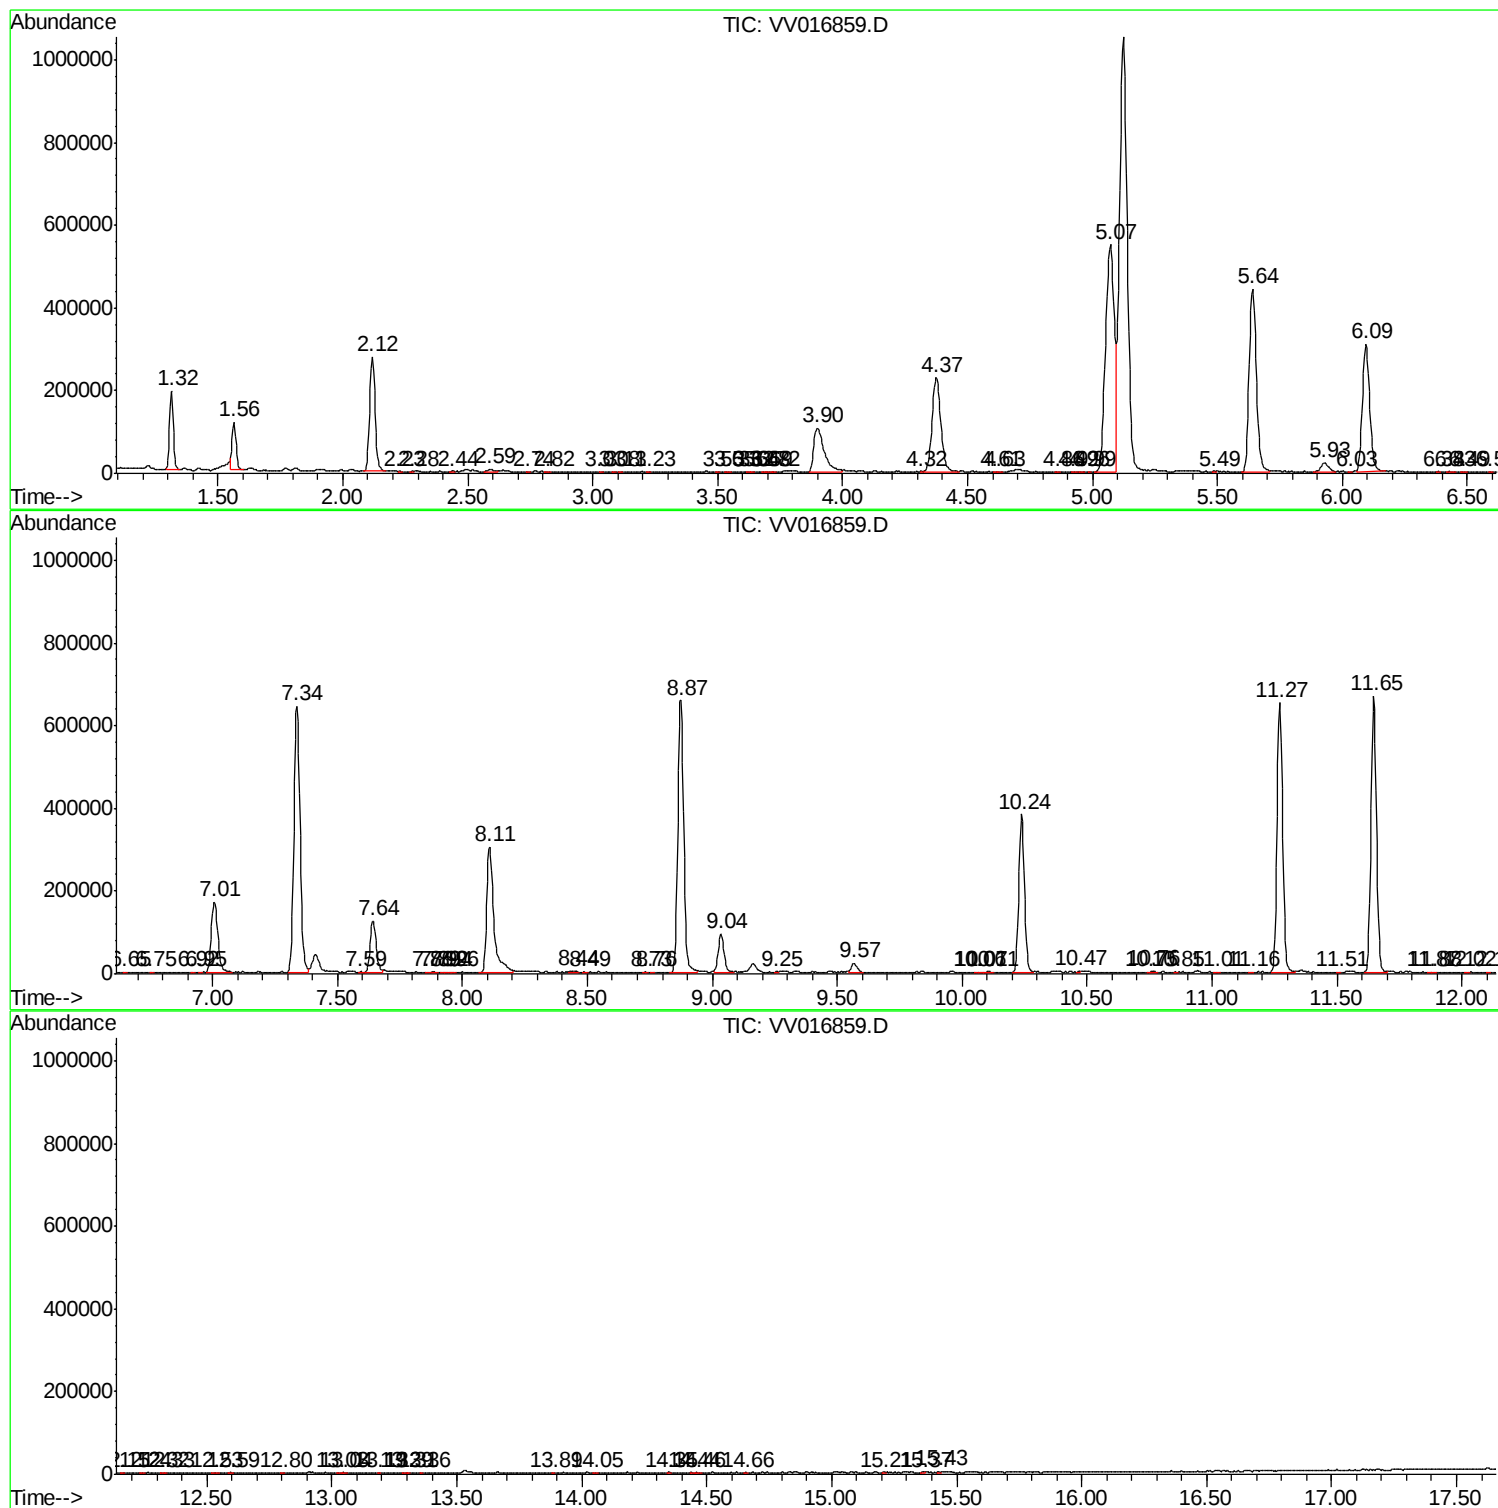

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016859.D
Acq On : 12 Jun 2020 04:20
Operator : SY/MD
Sample : L2915-04DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E08DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061120\
Data File : VV016859.D
Acq On : 12 Jun 2020 04:20
Operator : SY/MD
Sample : L2915-04DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9E08DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
