

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016862.D
 Acq On : 12 Jun 2020 05:31
 Operator : SY/MD
 Sample : L2915-07DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E11DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	80	rVB	185902	197180	14.99%	1.889%
2	1.560	142	146	158	rVB	123071	137901	10.48%	1.321%
3	2.116	309	319	335	rBV	271304	399295	30.35%	3.825%
4	2.380	399	401	402	rBV2	1704	753	0.06%	0.007%
5	2.437	418	419	422	rBV3	1220	733	0.06%	0.007%
6	2.450	422	423	426	rVV2	1492	621	0.05%	0.006%
7	2.753	513	517	518	rBV3	1435	1056	0.08%	0.010%
8	2.817	534	537	539	rBV3	1686	1159	0.09%	0.011%
9	2.881	555	557	559	rBV3	1597	804	0.06%	0.008%
10	2.929	570	572	576	rBV3	1817	1027	0.08%	0.010%
11	2.952	576	579	582	rBV2	1776	1341	0.10%	0.013%
12	3.026	598	602	606	rBV6	1110	1087	0.08%	0.010%
13	3.103	623	626	633	rBV8	1634	1511	0.11%	0.014%
14	3.138	633	637	638	rBV5	1113	822	0.06%	0.008%
15	3.299	685	687	690	rVB3	1375	751	0.06%	0.007%
16	3.325	693	695	698	rVV4	1525	926	0.07%	0.009%
17	3.363	702	707	710	rVV7	1162	880	0.07%	0.008%
18	3.405	716	720	724	rBV6	1642	1283	0.10%	0.012%
19	3.576	771	773	779	rBV6	1357	1008	0.08%	0.010%
20	3.634	787	791	793	rBV5	1426	925	0.07%	0.009%
21	3.727	816	820	821	rBV4	1381	990	0.08%	0.009%
22	3.778	826	836	837	rBV8	3612	4021	0.31%	0.039%
23	3.897	863	873	908	rBV	104547	296641	22.54%	2.842%
24	4.190	961	964	968	rBV4	1513	1005	0.08%	0.010%
25	4.212	968	971	975	rBV6	2046	1747	0.13%	0.017%
26	4.373	1006	1021	1041	rBV	221614	534206	40.60%	5.118%
27	4.515	1060	1065	1067	rBV6	1601	1621	0.12%	0.016%
28	4.733	1131	1133	1137	rVB4	1552	665	0.05%	0.006%
29	4.817	1156	1159	1162	rBV6	815	674	0.05%	0.006%
30	4.881	1176	1179	1183	rBV6	1479	1100	0.08%	0.011%
31	4.923	1186	1192	1194	rBV6	1850	1645	0.13%	0.016%
32	5.071	1221	1238	1245	rBV3	534073	1315816	100.00%	12.606%
33	5.640	1398	1415	1441	rBV	443298	883437	67.14%	8.464%
34	6.093	1544	1556	1579	rVB	306964	609785	46.34%	5.842%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016862.D
 Acq On : 12 Jun 2020 05:31
 Operator : SY/MD
 Sample : L2915-07DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E11DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.498	1680	1682	1684	rVB3	1970	689	0.05%	0.007%
36	6.566	1700	1703	1704	rBV2	1242	707	0.05%	0.007%
37	6.891	1798	1804	1805	rBV6	1632	1583	0.12%	0.015%
38	7.006	1830	1840	1857	rBV	165722	289512	22.00%	2.774%
39	7.096	1865	1868	1871	rBV5	1924	1382	0.11%	0.013%
40	7.338	1931	1943	1957	rBV	636041	1077724	81.91%	10.325%
41	7.640	2027	2037	2056	rBV	117660	202900	15.42%	1.944%
42	8.109	2169	2183	2212	rBV	294829	595416	45.25%	5.704%
43	8.498	2301	2304	2308	rBV6	2117	1591	0.12%	0.015%
44	8.604	2335	2337	2340	rBV4	1872	1374	0.10%	0.013%
45	8.871	2409	2420	2443	rVV	641032	1052354	79.98%	10.082%
46	9.035	2462	2471	2483	rVB	83262	130125	9.89%	1.247%
47	9.222	2527	2529	2533	rVB4	1287	799	0.06%	0.008%
48	9.331	2557	2563	2566	rBV8	2991	3074	0.23%	0.029%
49	9.405	2581	2586	2588	rBV6	2062	2261	0.17%	0.022%
50	9.469	2604	2606	2608	rBV3	1834	960	0.07%	0.009%
51	9.665	2664	2667	2671	rBV6	2045	1610	0.12%	0.015%
52	9.685	2671	2673	2676	rBV3	1168	658	0.05%	0.006%
53	9.884	2729	2735	2739	rBV7	2711	3043	0.23%	0.029%
54	10.013	2771	2775	2779	rBV6	1401	1100	0.08%	0.011%
55	10.061	2786	2790	2793	rVB4	2083	1434	0.11%	0.014%
56	10.074	2793	2794	2797	rBV3	1287	857	0.07%	0.008%
57	10.109	2797	2805	2809	rVB3	2662	3212	0.24%	0.031%
58	10.238	2834	2845	2862	rBV	376393	584774	44.44%	5.602%
59	10.469	2912	2917	2918	rBV4	1966	1648	0.13%	0.016%
60	10.495	2923	2925	2927	rBV3	2074	1129	0.09%	0.011%
61	10.530	2934	2936	2939	rVB3	1309	716	0.05%	0.007%
62	10.727	2995	2997	2999	rBV3	1540	814	0.06%	0.008%
63	10.823	3025	3027	3029	rVB2	1508	654	0.05%	0.006%
64	10.862	3037	3039	3042	rBV4	1257	757	0.06%	0.007%
65	10.974	3071	3074	3076	rVB3	1570	923	0.07%	0.009%
66	11.022	3085	3089	3094	rVB7	1632	1795	0.14%	0.017%
67	11.173	3133	3136	3139	rBV5	1542	1245	0.09%	0.012%
68	11.270	3154	3166	3182	rBV	650096	1002396	76.18%	9.603%
69	11.646	3270	3283	3298	rBV	668350	1021709	77.65%	9.788%
70	11.842	3342	3344	3350	rVB6	1375	954	0.07%	0.009%
71	11.980	3383	3387	3391	rBV6	1042	997	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016862.D
 Acq On : 12 Jun 2020 05:31
 Operator : SY/MD
 Sample : L2915-07DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E11DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.122	3428	3431	3435	rBV5	1559	1489	0.11%	0.014%
73	12.234	3462	3466	3469	rBV4	2241	1434	0.11%	0.014%
74	12.312	3487	3490	3494	rBV6	1535	1402	0.11%	0.013%
75	12.366	3503	3507	3511	rBV5	1398	1445	0.11%	0.014%
76	12.476	3537	3541	3542	rVV3	878	723	0.05%	0.007%
77	12.537	3558	3560	3562	rBV3	1451	624	0.05%	0.006%
78	12.550	3562	3564	3566	rVV3	1703	885	0.07%	0.008%
79	12.678	3602	3604	3608	rVB5	1251	843	0.06%	0.008%
80	12.720	3615	3617	3621	rVB4	1604	1050	0.08%	0.010%
81	12.739	3621	3623	3626	rBV4	1213	807	0.06%	0.008%
82	12.752	3626	3627	3631	rVB3	1413	702	0.05%	0.007%
83	12.775	3631	3634	3636	rBV3	1767	1202	0.09%	0.012%
84	13.067	3722	3725	3728	rBV3	1818	975	0.07%	0.009%
85	13.141	3745	3748	3750	rBV3	1002	795	0.06%	0.008%
86	13.202	3763	3767	3769	rVB5	2012	1535	0.12%	0.015%
87	13.222	3769	3773	3774	rBV3	1170	712	0.05%	0.007%
88	13.279	3788	3791	3793	rBV3	1817	1173	0.09%	0.011%
89	13.533	3861	3870	3875	rBV5	5810	9281	0.71%	0.089%
90	13.630	3896	3900	3901	rBV3	1474	1202	0.09%	0.012%
91	13.733	3927	3932	3935	rBV6	1837	1594	0.12%	0.015%
92	13.955	3999	4001	4005	rVB5	2213	1412	0.11%	0.014%
93	14.029	4022	4024	4027	rBV3	1500	895	0.07%	0.009%
94	14.115	4048	4051	4053	rBV4	1170	835	0.06%	0.008%
95	14.302	4107	4109	4114	rBV6	1095	745	0.06%	0.007%
96	14.405	4138	4141	4143	rBV3	1868	1217	0.09%	0.012%
97	14.559	4186	4189	4192	rBV4	1513	1289	0.10%	0.012%
98	14.906	4295	4297	4299	rBV3	1457	696	0.05%	0.007%
99	14.955	4310	4312	4314	rVB2	1837	718	0.05%	0.007%
100	15.389	4444	4447	4450	rBV5	1436	1178	0.09%	0.011%


Sum of corrected areas: 10438150

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016862.D
Acq On : 12 Jun 2020 05:31
Operator : SY/MD
Sample : L2915-07DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9E11DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

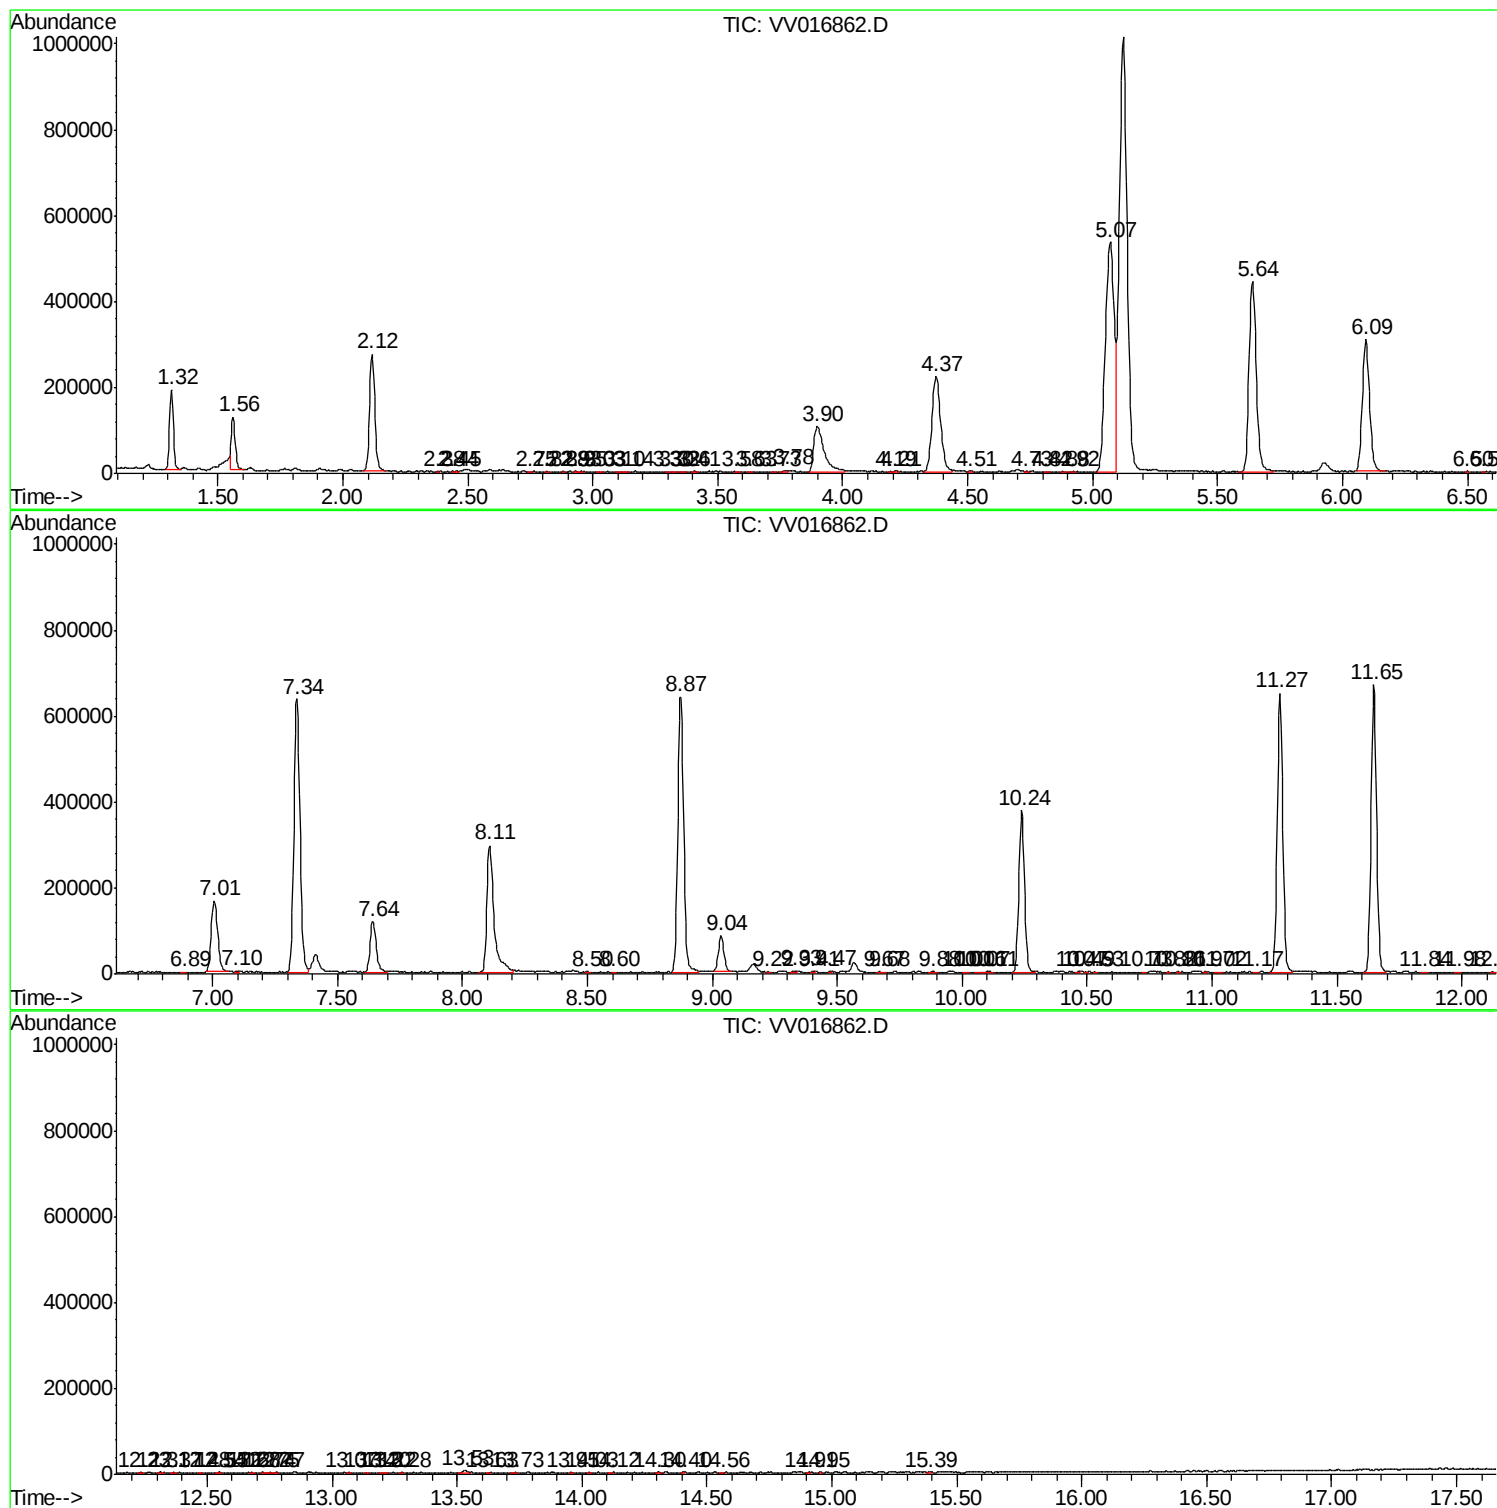

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016862.D
Acq On : 12 Jun 2020 05:31
Operator : SY/MD
Sample : L2915-07DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E11DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061120\
Data File : VV016862.D
Acq On : 12 Jun 2020 05:31
Operator : SY/MD
Sample : L2915-07DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9E11DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
