

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016864.D
 Acq On : 12 Jun 2020 06:43
 Operator : SY/MD
 Sample : VV0611WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	83	rVB	149304	159571	12.12%	1.568%
2	1.563	143	147	157	rVB	113564	121569	9.24%	1.194%
3	2.116	309	319	344	rVB	255634	387717	29.46%	3.809%
4	2.347	389	391	395	rVB4	1773	1178	0.09%	0.012%
5	2.380	399	401	403	rBV3	1290	840	0.06%	0.008%
6	2.460	422	426	427	rBV3	1355	761	0.06%	0.007%
7	2.515	439	443	444	rBV3	1622	1166	0.09%	0.011%
8	2.630	473	479	485	rBV9	2578	3311	0.25%	0.033%
9	2.945	573	577	582	rBV8	1080	1131	0.09%	0.011%
10	2.974	582	586	589	rVV5	1473	1298	0.10%	0.013%
11	3.084	617	620	621	rBV3	1637	990	0.08%	0.010%
12	3.328	694	696	700	rBV4	2064	894	0.07%	0.009%
13	3.383	711	713	717	rBV5	1482	885	0.07%	0.009%
14	3.437	723	730	731	rBV6	1286	1231	0.09%	0.012%
15	3.479	740	743	744	rBV2	1035	723	0.05%	0.007%
16	3.524	756	757	762	rBV4	1018	897	0.07%	0.009%
17	3.547	762	764	769	rVV6	1076	905	0.07%	0.009%
18	3.595	776	779	781	rBV3	1156	735	0.06%	0.007%
19	3.695	807	810	813	rBV4	1255	811	0.06%	0.008%
20	3.746	823	826	829	rVB4	1198	812	0.06%	0.008%
21	3.814	845	847	850	rVB4	1669	1003	0.08%	0.010%
22	3.836	850	854	856	rBV4	1681	1352	0.10%	0.013%
23	3.900	863	874	904	rBV	103678	288137	21.89%	2.831%
24	4.116	939	941	943	rBV2	1595	850	0.06%	0.008%
25	4.154	952	953	957	rBV3	1685	1352	0.10%	0.013%
26	4.373	1004	1021	1046	rBV	220625	540050	41.03%	5.306%
27	4.585	1085	1087	1092	rBV4	1874	1424	0.11%	0.014%
28	4.971	1205	1207	1209	rVB3	2122	829	0.06%	0.008%
29	4.990	1209	1213	1216	rBV6	1677	1278	0.10%	0.013%
30	5.071	1221	1238	1259	rVV2	514312	1316148	100.00%	12.932%
31	5.498	1367	1371	1374	rVB5	1692	1260	0.10%	0.012%
32	5.527	1374	1380	1384	rBV7	1879	2346	0.18%	0.023%
33	5.576	1391	1395	1397	rBV3	1479	1287	0.10%	0.013%
34	5.640	1402	1415	1434	rBV	443510	879129	66.80%	8.638%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016864.D
 Acq On : 12 Jun 2020 06:43
 Operator : SY/MD
 Sample : VV0611WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.842	1474	1478	1481	rBV5	1910	1779	0.14%	0.017%
36	5.926	1494	1504	1518	rBV3	24263	50622	3.85%	0.497%
37	6.093	1544	1556	1580	rVB	298084	599941	45.58%	5.895%
38	6.286	1613	1616	1617	rBV3	1850	779	0.06%	0.008%
39	6.463	1669	1671	1675	rVB4	1332	725	0.06%	0.007%
40	6.511	1684	1686	1691	rVB5	1796	1280	0.10%	0.013%
41	6.653	1728	1730	1733	rVB4	1945	866	0.07%	0.009%
42	6.701	1743	1745	1747	rBV3	1359	752	0.06%	0.007%
43	6.736	1752	1756	1758	rVV5	1352	1042	0.08%	0.010%
44	6.836	1784	1787	1789	rBV4	1374	933	0.07%	0.009%
45	7.006	1829	1840	1857	rBV	161368	284126	21.59%	2.792%
46	7.338	1931	1943	1960	rBV	610398	1040101	79.03%	10.219%
47	7.643	2026	2038	2058	rBV	114661	199649	15.17%	1.962%
48	7.714	2058	2060	2063	rBV3	1909	1135	0.09%	0.011%
49	7.871	2107	2109	2114	rBV6	1263	1078	0.08%	0.011%
50	8.071	2165	2171	2172	rBV4	1759	1638	0.12%	0.016%
51	8.109	2173	2183	2215	rVV	302033	600523	45.63%	5.900%
52	8.620	2340	2342	2346	rVB5	1369	768	0.06%	0.008%
53	8.646	2346	2350	2353	rVB5	1370	963	0.07%	0.009%
54	8.874	2409	2421	2436	rBV	662323	1062458	80.72%	10.439%
55	9.000	2458	2460	2463	rBV3	1508	1001	0.08%	0.010%
56	9.264	2540	2542	2546	rBV5	1651	1316	0.10%	0.013%
57	9.341	2561	2566	2567	rVV5	1170	914	0.07%	0.009%
58	9.444	2594	2598	2601	rVB4	1792	1231	0.09%	0.012%
59	9.463	2601	2604	2607	rBV4	1822	1320	0.10%	0.013%
60	9.659	2662	2665	2672	rBV8	1435	1626	0.12%	0.016%
61	10.238	2834	2845	2858	rBV	375561	581659	44.19%	5.715%
62	10.514	2928	2931	2935	rVB6	2200	1407	0.11%	0.014%
63	10.575	2947	2950	2954	rVB6	2183	1490	0.11%	0.015%
64	10.675	2980	2981	2985	rVB4	1674	885	0.07%	0.009%
65	11.270	3156	3166	3185	rVB	644054	981426	74.57%	9.643%
66	11.524	3242	3245	3247	rBV4	1659	1182	0.09%	0.012%
67	11.646	3270	3283	3303	rBV	624692	988101	75.08%	9.708%
68	11.935	3371	3373	3376	rBV3	1300	921	0.07%	0.009%
69	12.093	3420	3422	3427	rBV4	1516	1447	0.11%	0.014%
70	12.135	3433	3435	3439	rVB4	1766	998	0.08%	0.010%
71	12.199	3453	3455	3458	rBV4	1665	1021	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016864.D
 Acq On : 12 Jun 2020 06:43
 Operator : SY/MD
 Sample : VV0611WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.280	3475	3480	3481	rBV5	956	917	0.07%	0.009%
73	12.665	3597	3600	3602	rBV4	2144	1533	0.12%	0.015%
74	12.755	3626	3628	3633	rBV4	1090	1091	0.08%	0.011%
75	12.833	3649	3652	3655	rVB6	1426	885	0.07%	0.009%
76	12.865	3655	3662	3666	rBV9	1793	2129	0.16%	0.021%
77	13.164	3750	3755	3757	rBV5	1575	1186	0.09%	0.012%
78	13.199	3764	3766	3772	rVB5	1484	1154	0.09%	0.011%
79	13.382	3819	3823	3824	rBV3	1288	770	0.06%	0.008%
80	13.411	3827	3832	3834	rBV4	2342	1352	0.10%	0.013%
81	13.501	3856	3860	3863	rBV6	1528	1316	0.10%	0.013%
82	13.701	3919	3922	3926	rBV5	1812	1649	0.13%	0.016%
83	13.884	3976	3979	3984	rBV5	1839	1590	0.12%	0.016%
84	13.926	3989	3992	3997	rVV7	1374	1193	0.09%	0.012%
85	14.016	4018	4020	4023	rBV4	1016	721	0.05%	0.007%
86	14.048	4026	4030	4031	rBV2	1959	1191	0.09%	0.012%
87	14.103	4042	4047	4048	rBV4	1682	1190	0.09%	0.012%
88	14.164	4064	4066	4069	rBV4	1191	845	0.06%	0.008%
89	14.209	4074	4080	4084	rBV7	1624	1848	0.14%	0.018%
90	14.276	4099	4101	4105	rBV4	1342	923	0.07%	0.009%
91	14.350	4121	4124	4127	rVB5	1428	791	0.06%	0.008%
92	14.466	4157	4160	4162	rBV4	1547	856	0.07%	0.008%
93	14.643	4212	4215	4219	rBV4	1960	1332	0.10%	0.013%
94	14.697	4228	4232	4236	rVB6	1556	1124	0.09%	0.011%
95	14.717	4236	4238	4241	rBV4	1439	980	0.07%	0.010%
96	14.749	4246	4248	4252	rBV4	1505	1066	0.08%	0.010%
97	14.974	4316	4318	4321	rBV3	1427	964	0.07%	0.009%
98	15.032	4334	4336	4343	rVB6	2220	1872	0.14%	0.018%
99	15.090	4352	4354	4356	rBV2	1196	738	0.06%	0.007%
100	15.431	4456	4460	4462	rBV5	2143	1607	0.12%	0.016%


Sum of corrected areas: 10177786

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016864.D
Acq On : 12 Jun 2020 06:43
Operator : SY/MD
Sample : VV0611WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

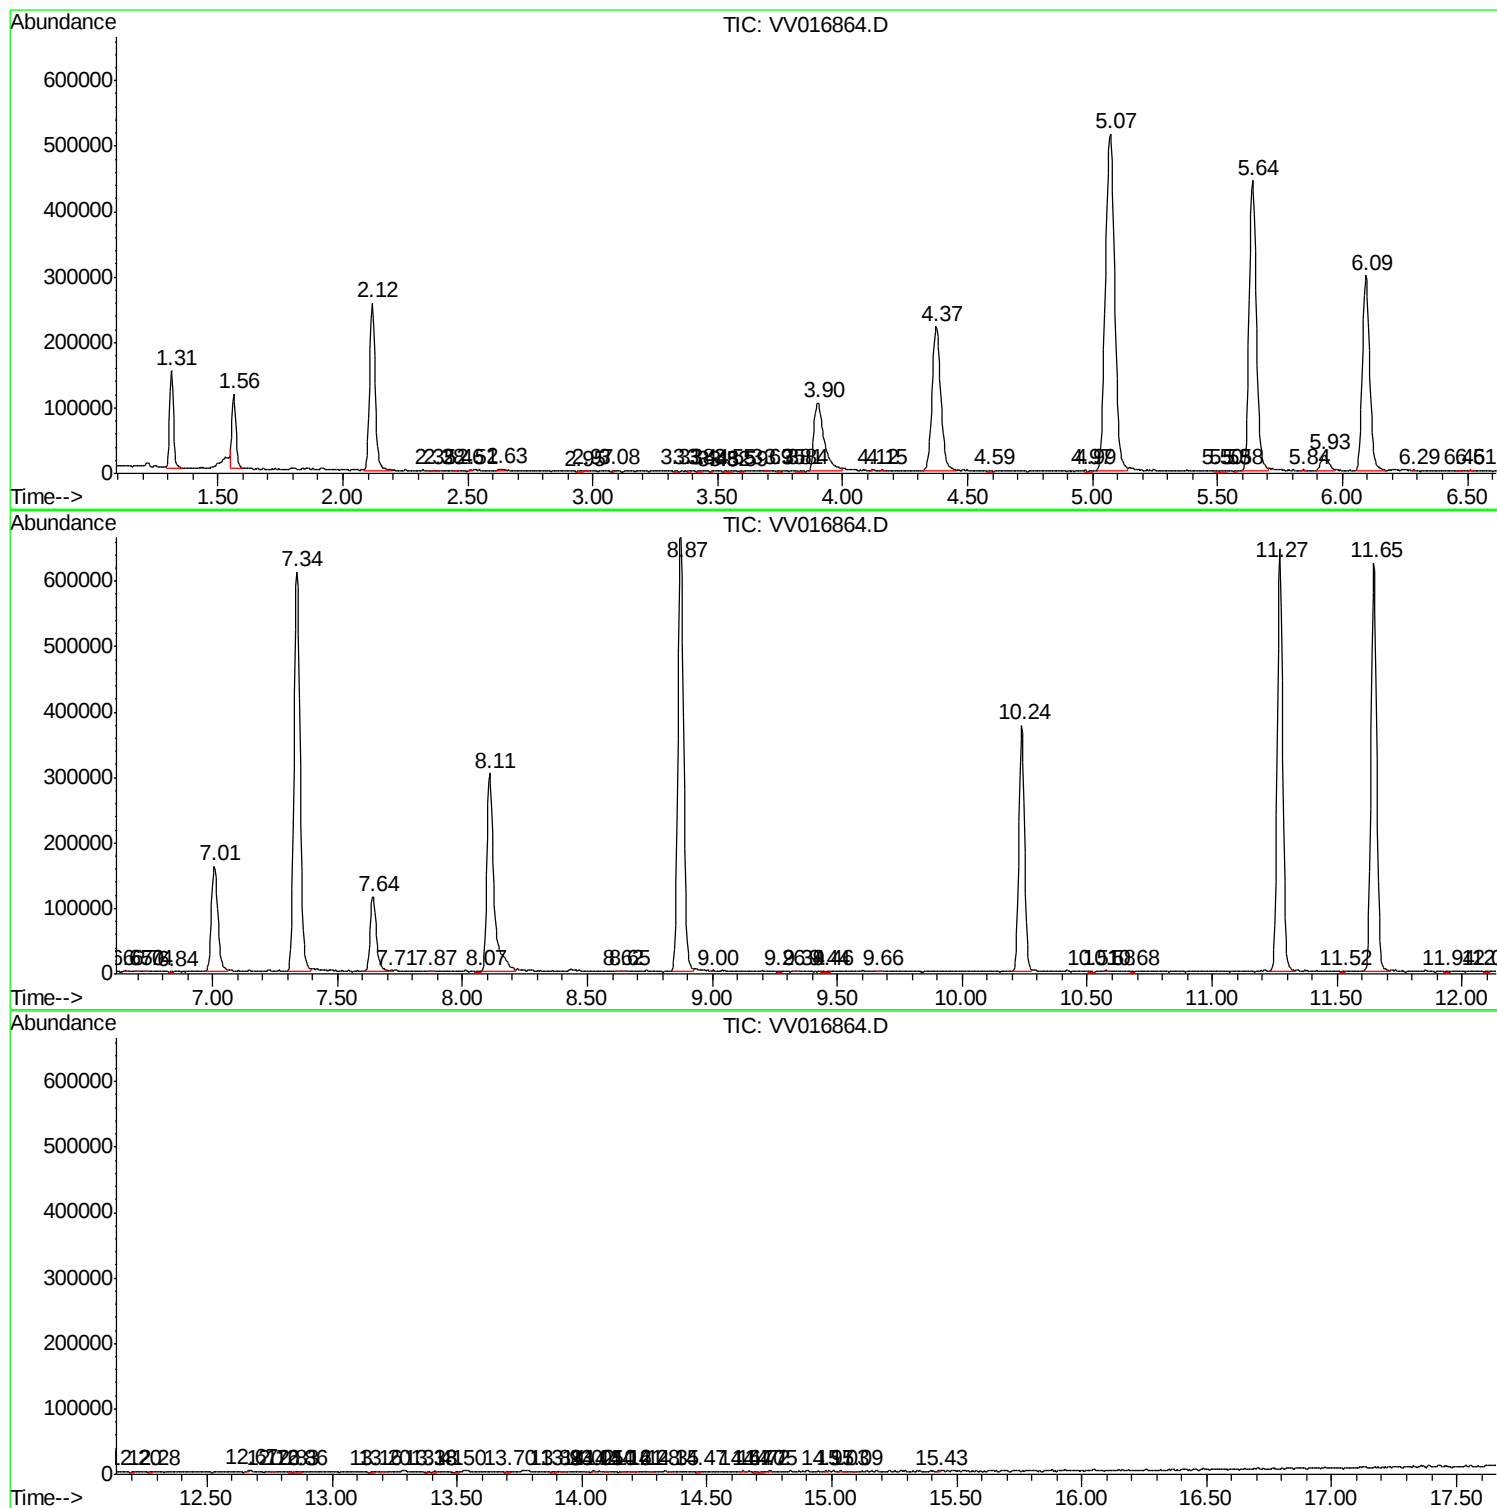

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016864.D
Acq On : 12 Jun 2020 06:43
Operator : SY/MD
Sample : VV0611WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016864.D
Acq On : 12 Jun 2020 06:43
Operator : SY/MD
Sample : VV0611WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK82

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc