

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016868.D
 Acq On : 12 Jun 2020 10:13
 Operator : SY/MD
 Sample : L2945-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	174851	178663	13.12%	1.729%
2	1.560	139	146	158	rVB	120367	144425	10.60%	1.398%
3	2.116	310	319	334	rVB	277361	411950	30.24%	3.988%
4	2.306	375	378	382	rBV6	1865	1945	0.14%	0.019%
5	2.495	434	437	438	rBV3	1320	766	0.06%	0.007%
6	2.592	465	467	470	rBV4	2098	1004	0.07%	0.010%
7	2.782	523	526	527	rBV3	1251	608	0.04%	0.006%
8	3.155	640	642	644	rVB3	1007	451	0.03%	0.004%
9	3.167	644	646	649	rBV3	1350	883	0.06%	0.009%
10	3.196	653	655	659	rVB4	1659	903	0.07%	0.009%
11	3.286	679	683	687	rBV5	1189	1101	0.08%	0.011%
12	3.319	691	693	695	rBV3	1702	815	0.06%	0.008%
13	3.331	695	697	699	rVB2	1439	603	0.04%	0.006%
14	3.367	705	708	712	rVB5	1056	884	0.06%	0.009%
15	3.563	765	769	770	rVV4	881	564	0.04%	0.005%
16	3.614	783	785	790	rVB6	1466	1031	0.08%	0.010%
17	3.679	803	805	808	rBV3	1818	1213	0.09%	0.012%
18	3.711	813	815	817	rBV3	976	454	0.03%	0.004%
19	3.727	817	820	824	rVB6	1622	1205	0.09%	0.012%
20	3.749	824	827	830	rBV4	1344	1095	0.08%	0.011%
21	3.798	840	842	846	rBV4	784	657	0.05%	0.006%
22	3.894	862	872	901	rBV2	106433	281682	20.68%	2.727%
23	4.373	1007	1021	1044	rVB	217970	532308	39.08%	5.153%
24	4.634	1099	1102	1104	rBV4	1372	888	0.07%	0.009%
25	4.981	1207	1210	1211	rBV2	1715	1185	0.09%	0.011%
26	5.068	1221	1237	1263	rBV2	529806	1362061	100.00%	13.185%
27	5.251	1293	1294	1296	rBV2	1685	873	0.06%	0.008%
28	5.322	1314	1316	1320	rVB4	1644	889	0.07%	0.009%
29	5.640	1400	1415	1435	rBV	405459	808816	59.38%	7.829%
30	6.093	1544	1556	1578	rVB	309027	613130	45.01%	5.935%
31	6.408	1650	1654	1656	rBV5	1319	926	0.07%	0.009%
32	6.611	1716	1717	1720	rBV3	814	433	0.03%	0.004%
33	6.672	1733	1736	1738	rBV4	2174	1496	0.11%	0.014%
34	6.701	1743	1745	1750	rVB5	2017	1279	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016868.D
 Acq On : 12 Jun 2020 10:13
 Operator : SY/MD
 Sample : L2945-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1830	1840	1865	rVV	180309	317664	23.32%	3.075%
36	7.106	1869	1871	1872	rBV2	1447	687	0.05%	0.007%
37	7.209	1900	1903	1904	rBV3	1306	784	0.06%	0.008%
38	7.338	1931	1943	1960	rBV	642185	1096797	80.52%	10.617%
39	7.601	2023	2025	2026	rBV2	1236	568	0.04%	0.005%
40	7.640	2028	2037	2055	rVB	127029	219595	16.12%	2.126%
41	8.106	2173	2182	2215	rBV2	307006	602524	44.24%	5.832%
42	8.373	2260	2265	2271	rBV6	2604	3307	0.24%	0.032%
43	8.402	2271	2274	2277	rBV5	1686	1294	0.10%	0.013%
44	8.434	2281	2284	2286	rBV4	3437	2131	0.16%	0.021%
45	8.871	2409	2420	2440	rBV	621889	997805	73.26%	9.659%
46	9.318	2554	2559	2561	rBV4	2334	1844	0.14%	0.018%
47	9.357	2568	2571	2575	rBV4	1265	614	0.05%	0.006%
48	9.383	2575	2579	2580	rBV4	1936	1271	0.09%	0.012%
49	9.505	2614	2617	2618	rBV3	1034	524	0.04%	0.005%
50	9.601	2644	2647	2649	rBV4	1116	788	0.06%	0.008%
51	9.649	2658	2662	2665	rBV6	1924	1839	0.14%	0.018%
52	9.807	2709	2711	2713	rBV3	881	514	0.04%	0.005%
53	9.936	2749	2751	2754	rVB4	1205	670	0.05%	0.006%
54	9.965	2758	2760	2764	rVV3	1088	677	0.05%	0.007%
55	10.003	2770	2772	2774	rBV3	931	458	0.03%	0.004%
56	10.096	2798	2801	2805	rVB4	2774	2125	0.16%	0.021%
57	10.112	2805	2806	2807	rBV	1530	583	0.04%	0.006%
58	10.154	2817	2819	2820	rBV2	1529	547	0.04%	0.005%
59	10.238	2832	2845	2859	rBV	387431	605781	44.48%	5.864%
60	10.402	2894	2896	2899	rBV4	1815	1362	0.10%	0.013%
61	10.582	2950	2952	2954	rBV3	1148	687	0.05%	0.007%
62	10.810	3017	3023	3025	rBV5	2534	2408	0.18%	0.023%
63	10.842	3029	3033	3036	rBV5	1624	1063	0.08%	0.010%
64	10.987	3073	3078	3080	rBV5	2363	1914	0.14%	0.019%
65	11.084	3106	3108	3110	rBV3	1237	588	0.04%	0.006%
66	11.270	3155	3166	3184	rBV	644926	979690	71.93%	9.483%
67	11.495	3234	3236	3238	rBV3	1078	444	0.03%	0.004%
68	11.518	3241	3243	3247	rVB5	1328	737	0.05%	0.007%
69	11.646	3272	3283	3301	rBV	706882	1091042	80.10%	10.561%
70	11.797	3328	3330	3333	rBV4	1806	1069	0.08%	0.010%
71	11.916	3364	3367	3371	rVB4	1985	1615	0.12%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
 Data File : VV016868.D
 Acq On : 12 Jun 2020 10:13
 Operator : SY/MD
 Sample : L2945-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.971	3380	3384	3385	rBV4	1506	976	0.07%	0.009%
73	12.141	3435	3437	3439	rBV3	917	447	0.03%	0.004%
74	12.254	3470	3472	3474	rBV3	1349	510	0.04%	0.005%
75	12.264	3474	3475	3479	rVB4	1444	754	0.06%	0.007%
76	12.292	3481	3484	3488	rVB4	2199	1382	0.10%	0.013%
77	12.321	3490	3493	3496	rBV4	1391	899	0.07%	0.009%
78	12.521	3553	3555	3557	rBV2	1157	519	0.04%	0.005%
79	12.646	3592	3594	3595	rBV2	1436	575	0.04%	0.006%
80	12.775	3630	3634	3636	rBV2	1315	1019	0.07%	0.010%
81	12.817	3642	3647	3648	rBV4	1549	1484	0.11%	0.014%
82	12.900	3671	3673	3675	rBV3	1343	611	0.04%	0.006%
83	12.990	3698	3701	3703	rBV4	1453	1078	0.08%	0.010%
84	13.125	3739	3743	3745	rBV3	965	751	0.06%	0.007%
85	13.148	3748	3750	3752	rBV3	1821	1080	0.08%	0.010%
86	13.328	3803	3806	3807	rBV3	1729	836	0.06%	0.008%
87	13.360	3812	3816	3818	rBV4	2392	1479	0.11%	0.014%
88	13.392	3823	3826	3828	rBV3	985	719	0.05%	0.007%
89	13.530	3867	3869	3871	rBV4	1466	570	0.04%	0.006%
90	13.614	3891	3895	3897	rBV4	1233	956	0.07%	0.009%
91	13.627	3897	3899	3903	rBV5	1422	951	0.07%	0.009%
92	13.681	3911	3916	3919	rBV7	1330	1313	0.10%	0.013%
93	13.752	3935	3938	3942	rBV5	2221	1835	0.13%	0.018%
94	13.791	3948	3950	3953	rBV3	1558	1095	0.08%	0.011%
95	13.807	3953	3955	3956	rBV2	1281	432	0.03%	0.004%
96	13.852	3967	3969	3972	rBV3	1294	569	0.04%	0.006%
97	14.006	4011	4017	4022	rVB10	1662	2192	0.16%	0.021%
98	14.386	4132	4135	4136	rBV2	1948	1111	0.08%	0.011%
99	14.681	4221	4227	4229	rBV4	1874	1886	0.14%	0.018%
100	15.292	4415	4417	4421	rBV5	2018	1465	0.11%	0.014%


Sum of corrected areas: 10330690

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016868.D
Acq On : 12 Jun 2020 10:13
Operator : SY/MD
Sample : L2945-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

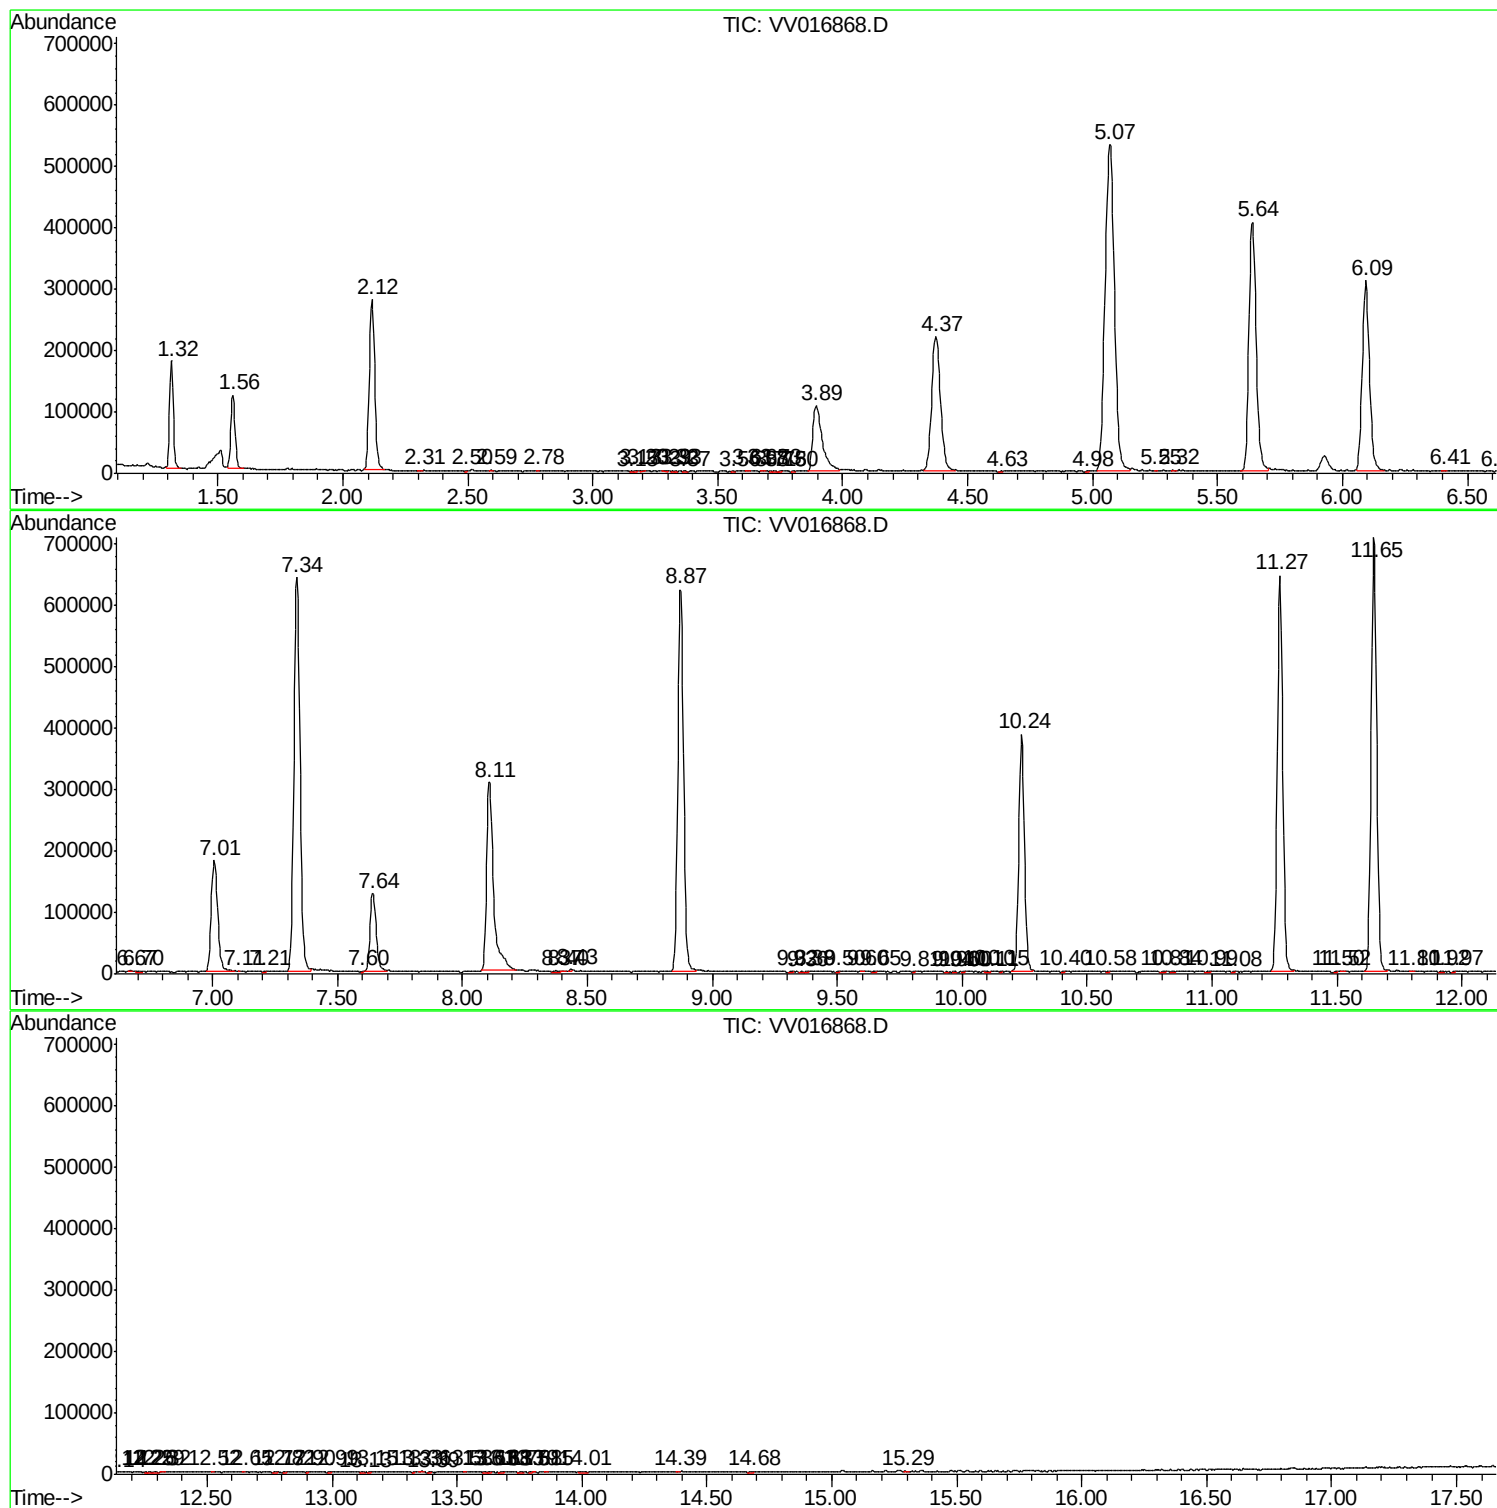

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016868.D
Acq On : 12 Jun 2020 10:13
Operator : SY/MD
Sample : L2945-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061120\
Data File : VV016868.D
Acq On : 12 Jun 2020 10:13
Operator : SY/MD
Sample : L2945-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc