


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061120\
 Data File : VV016811.D
 Acq On : 11 Jun 2020 08:44
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 12 05:55:11 2020

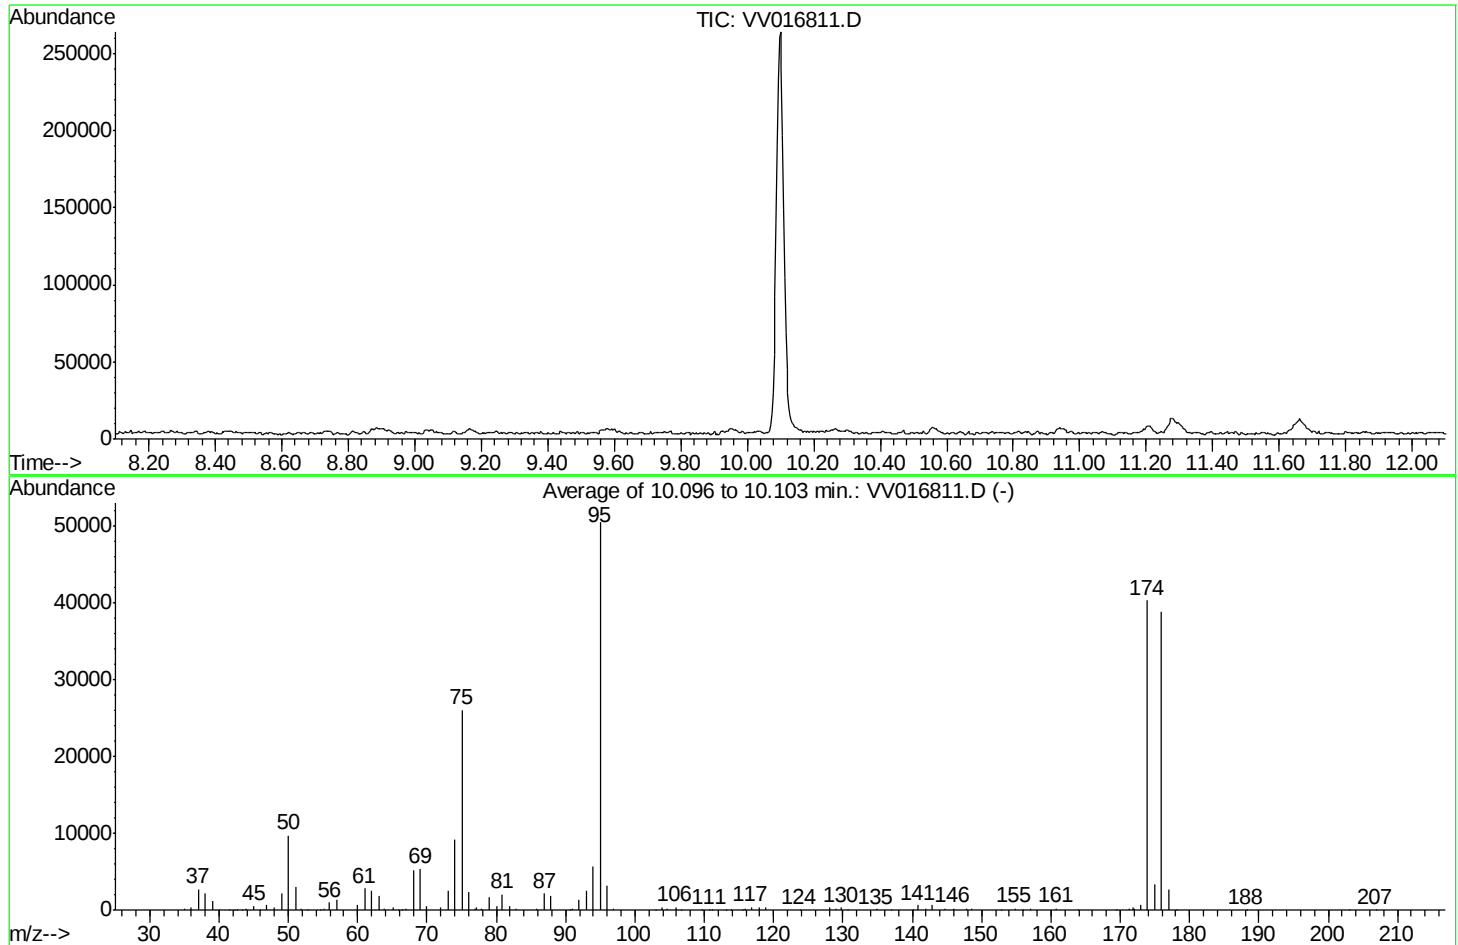

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	9686	PASS
75	95	30	80	51.5	26018	PASS
95	95	100	100	100.0	50482	PASS
96	95	5	9	6.4	3227	PASS
173	174	0.00	2	1.8	724	PASS
174	95	50	120	79.9	40328	PASS
175	174	5	9	8.1	3257	PASS
176	174	95	101	96.4	38874	PASS
177	176	5	9	7.0	2705	PASS

m/z	Abundance
35.00	145.0
36.00	600.0
37.00	3040.0
38.00	2414.0
39.00	1287.0
40.00	480.0
40.90	138.0
42.10	143.0
42.50	119.0
43.90	625.0
45.00	639.0
46.00	120.0
46.90	657.0
47.90	330.0
49.00	2339.0
50.00	10076.0
51.00	3435.0
51.90	270.0
55.00	208.0
55.90	1188.0
56.90	1230.0
60.00	573.0
61.00	2854.0
62.00	2773.0
63.00	2108.0
63.90	359.0
65.10	244.0
65.90	107.0
67.00	203.0
68.00	5555.0
69.00	5565.0
69.90	554.0
71.90	338.0
73.00	2448.0
74.00	9368.0
75.00	27080.0
76.00	2414.0
76.90	399.0
77.90	229.0
78.90	1878.0
80.00	573.0
80.90	2078.0
81.90	489.0
82.90	140.0
87.00	2153.0
87.90	1924.0
90.90	223.0
91.90	1478.0
93.00	2553.0
94.00	5869.0
95.00	52216.0
96.00	3581.0
96.90	189.0
98.40	111.0
103.00	107.0
103.90	294.0
104.70	227.0
105.90	367.0
111.10	107.0
113.10	137.0
115.60	183.0
116.00	175.0
116.80	381.0
117.90	265.0
118.80	337.0
128.00	292.0
129.00	208.0
129.80	241.0
130.70	129.0
134.90	124.0
140.90	637.0
141.90	208.0
142.90	665.0
144.70	130.0
145.90	145.0
147.70	107.0
148.60	107.0
154.90	168.0
160.90	222.0
171.90	337.0
173.00	679.0
173.90	39920.0
174.90	3258.0
175.90	39488.0
176.90	2821.0
178.20	110.0
206.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.00	123.0
36.00	559.0
37.00	3005.0
38.00	2295.0
39.00	1293.0
39.90	424.0
41.00	124.0
41.50	118.0
42.10	146.0
43.30	101.0
43.90	653.0
45.00	657.0
46.00	140.0
46.90	793.0
48.00	395.0
49.00	2322.0
50.00	10001.0
51.00	3157.0
51.90	254.0
52.70	104.0
54.60	116.0
55.10	213.0
56.00	987.0
56.90	1424.0
60.00	635.0
61.00	2882.0
62.00	2686.0
63.00	2066.0
63.80	348.0
65.10	283.0
67.00	205.0
68.00	5228.0
69.00	5605.0
70.00	590.0
71.90	392.0
73.00	2644.0
74.00	9625.0
75.00	26920.0
76.00	2433.0
77.10	405.0
77.90	245.0
79.00	1914.0
80.00	558.0
80.90	2114.0
81.90	483.0
82.90	149.0
85.80	132.0
86.90	2175.0
87.90	1800.0
91.00	184.0
91.90	1385.0
93.00	2459.0
94.00	5850.0
95.00	52408.0
96.00	3269.0
96.90	175.0
98.40	111.0
103.10	107.0
103.90	308.0
104.70	225.0
105.90	376.0
106.80	108.0
110.80	113.0
111.10	127.0
113.10	125.0
115.90	164.0
116.70	445.0
117.80	280.0
118.80	325.0
128.00	265.0
129.00	182.0
129.80	278.0
134.90	161.0
140.00	105.0
140.90	665.0
141.90	230.0
142.90	636.0
144.70	112.0
146.00	187.0
147.70	130.0
148.60	109.0
154.90	168.0
157.00	109.0
160.80	218.0
169.40	110.0
171.20	130.0
171.80	322.0
172.10	320.0
173.00	779.0
173.90	41784.0
174.90	3432.0
175.90	40168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

176.90

2823.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.10	103.0
36.00	476.0
37.00	2643.0
38.00	1935.0
39.00	1108.0
39.90	369.0
41.60	131.0
42.20	150.0
43.90	687.0
45.00	624.0
46.00	131.0
46.90	768.0
47.90	428.0
49.00	2066.0
50.00	8981.0
51.00	2591.0
51.90	199.0
53.00	105.0
54.60	106.0
55.10	176.0
56.00	739.0
57.00	1513.0
59.90	624.0
61.00	2562.0
62.00	2314.0
63.00	1842.0
63.80	286.0
65.10	286.0
66.40	101.0
67.00	173.0
68.00	4642.0
69.00	5211.0
70.00	492.0
71.90	374.0
73.00	2410.0
74.00	8612.0
75.00	24056.0
76.00	2191.0
77.10	439.0
77.90	220.0
79.00	1735.0
80.00	519.0
80.90	1848.0
81.90	492.0
82.90	136.0
85.80	164.0
86.90	2033.0
87.90	1597.0
90.60	133.0
91.00	135.0
92.00	1277.0
92.90	2349.0
94.00	5460.0
95.00	46824.0
96.00	2833.0
96.90	118.0
103.90	314.0
104.70	173.0
105.80	333.0
106.70	128.0
109.70	118.0
110.80	130.0
113.90	113.0
115.90	170.0
116.80	403.0
117.80	250.0
118.80	304.0
123.80	118.0
128.00	226.0
129.80	295.0
134.90	167.0
136.90	139.0
140.90	599.0
141.80	181.0
142.90	546.0
144.70	107.0
145.90	173.0
147.80	162.0
148.70	103.0
152.90	112.0
154.80	168.0
156.00	105.0
157.00	167.0
160.80	184.0
163.90	101.0
171.20	141.0
171.70	319.0
172.10	300.0
173.00	716.0
173.90	39280.0
174.90	3082.0
175.90	36968.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

177.00	2471.0
188.20	112.0
203.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.10	188.0
36.50	189.0
37.20	157.0
37.70	126.0
38.70	177.0
40.00	408.0
41.00	172.0
42.30	111.0
43.00	148.0
43.90	460.0
45.20	125.0
46.10	125.0
47.50	129.0
51.40	107.0
53.00	135.0
53.80	142.0
58.20	105.0
61.90	107.0
63.00	113.0
63.80	123.0
69.20	107.0
78.90	109.0
98.50	117.0
162.20	120.0
227.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86