

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061122\
 Data File : VW026132.D
 Acq On : 11 Jun 2022 16:08
 Operator : SY/MD
 Sample : N3312-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DX2

Quant Time: Jun 13 01:20:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 01:15:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.626	114	188797	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	182639	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73693	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	47344	4.272	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.581	69	55709	4.808	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%
11) 1,1-Dichloroethene-d2	2.121	63	79459	3.104	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%
20) 2-Butanone-d5	3.925	46	88895	54.232	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.460%
24) Chloroform-d	4.362	84	111191	4.734	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
26) 1,2-Dichloroethane-d4	5.044	65	47582	4.966	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.060	84	210235	4.764	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	6.076	67	66344	4.859	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.320	98	160632	4.119	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	7.629	79	14138	3.517	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.400%
46) 2-Hexanone-d5	8.092	63	71415	40.371	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.740%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42036	4.566	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	54070	4.796	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.000%
Target Compounds					Qvalue	
25) Chloroform	4.391	83	3255	0.122	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026132.D
Acq On : 11 Jun 2022 16:08
Operator : SY/MD
Sample : N3312-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DX2

Quant Time: Jun 13 01:20:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 01:15:38 2022
Response via : Initial Calibration

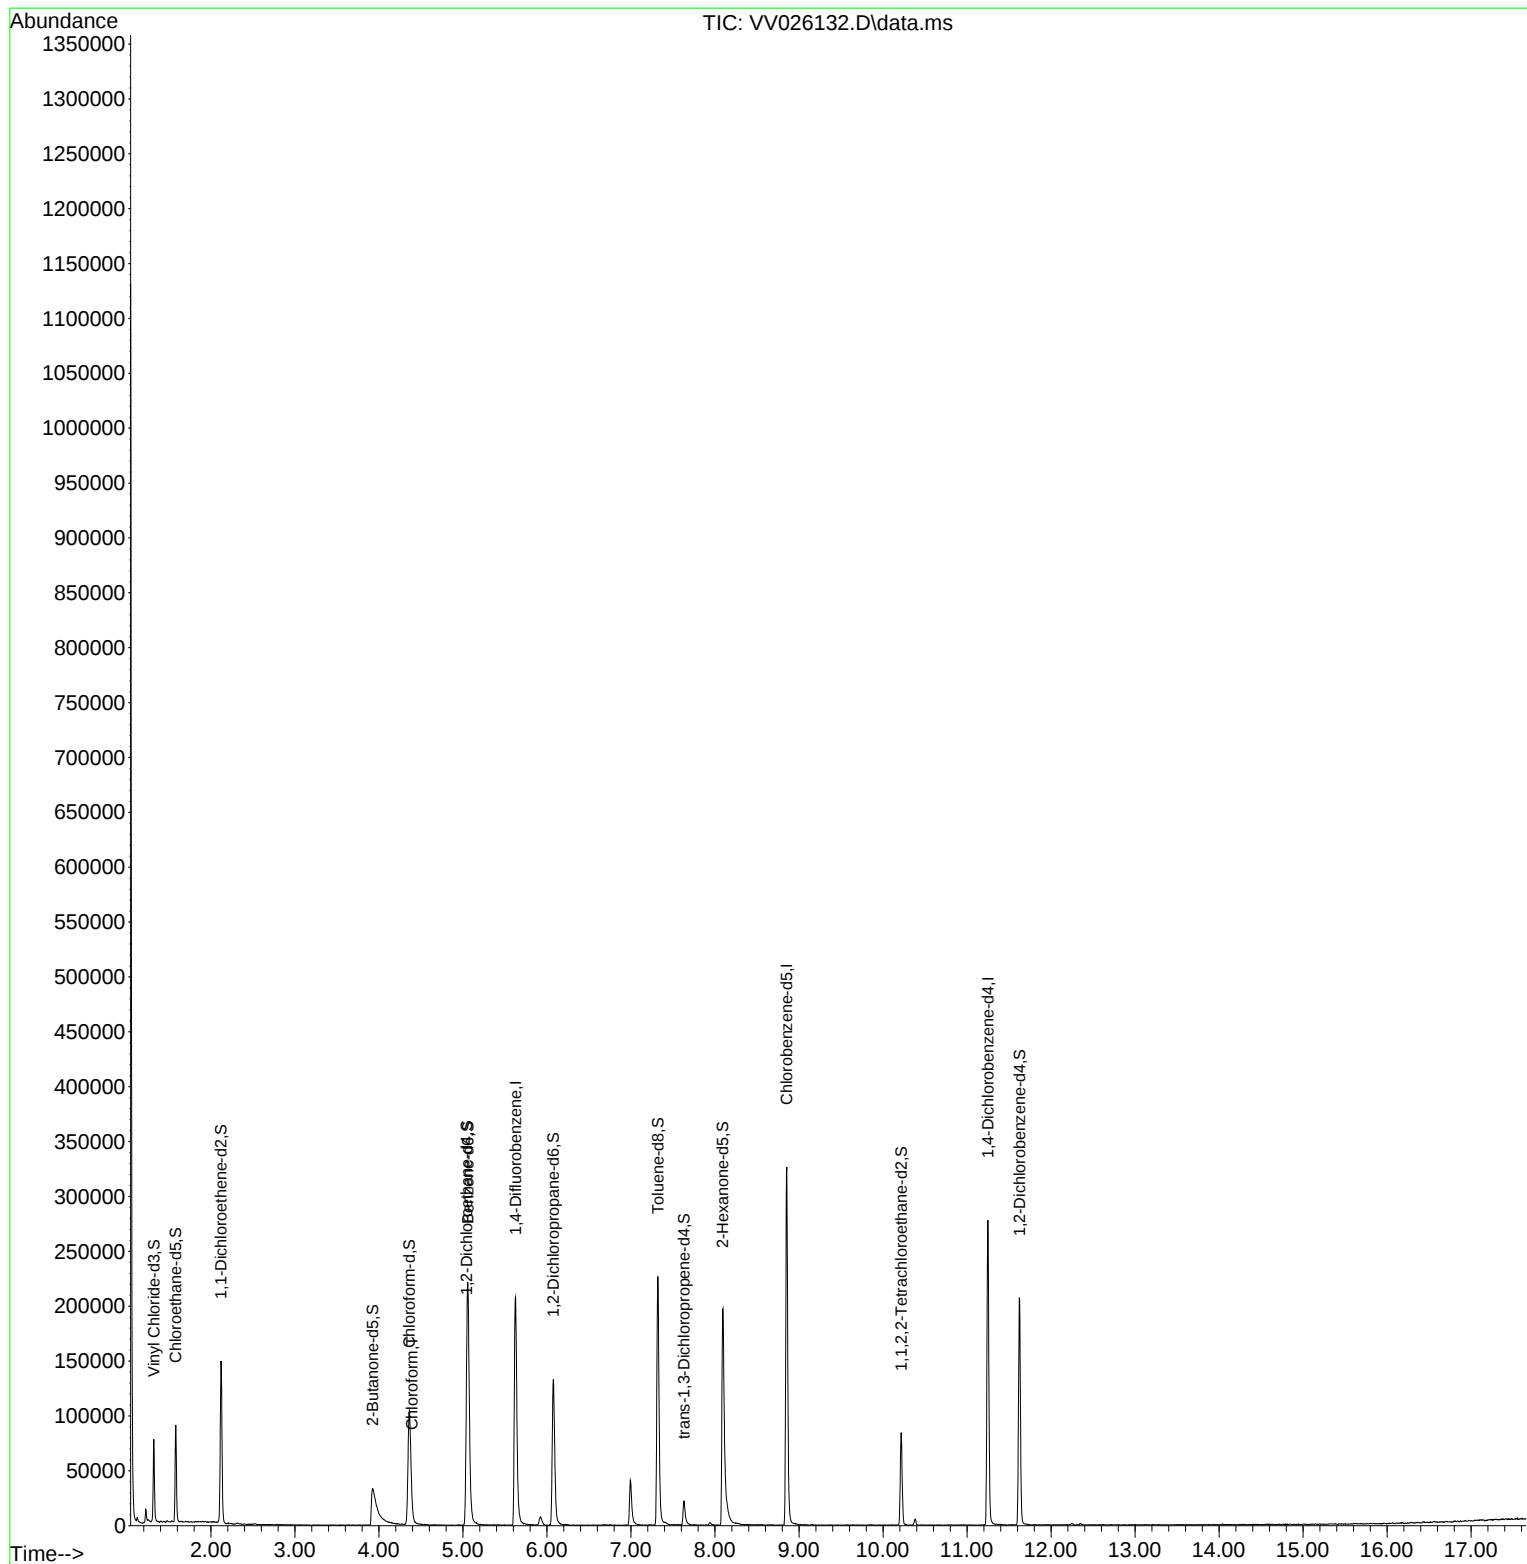

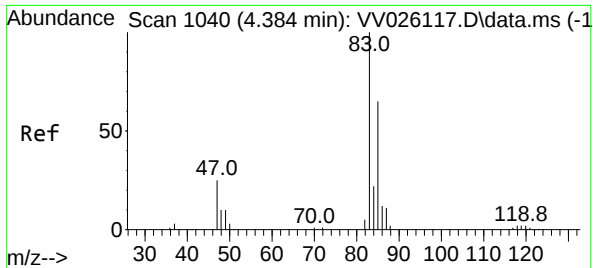

#25
 Chloroform
 Concen: 0.122 ug/L
 RT: 4.391 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VV026132.D
 Acq: 11 Jun 2022 16:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DX2

Tgt Ion: 83 Resp: 3255
 Ion Ratio Lower Upper
 83 100
 85 70.1 45.2 84.0

