

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061122\
 Data File : VW026137.D
 Acq On : 11 Jun 2022 18:07
 Operator : SY/MD
 Sample : N3312-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODY7

Quant Time: Jun 13 01:21:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 01:15:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	188127	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	184454	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74479	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	48609	4.402	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.000%	
7) Chloroethane-d5	1.581	69	55584	4.814	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2	2.121	63	79028	3.098	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.925	46	87547	53.600	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.200%	
24) Chloroform-d	4.362	84	111489	4.763	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	5.044	65	50277	5.266	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	5.060	84	210953	4.733	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.076	67	69518	5.041	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.800%	
41) Toluene-d8	7.320	98	160491	4.075	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.400%	
43) trans-1,3-Dichloroprop...	7.632	79	14534	3.580	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.600%	
46) 2-Hexanone-d5	8.092	63	72344	40.493	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.980%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43068	4.632	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	55610	4.880	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.600%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.253	50	1118	0.054	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026137.D
Acq On : 11 Jun 2022 18:07
Operator : SY/MD
Sample : N3312-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DY7

Quant Time: Jun 13 01:21:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 01:15:38 2022
Response via : Initial Calibration

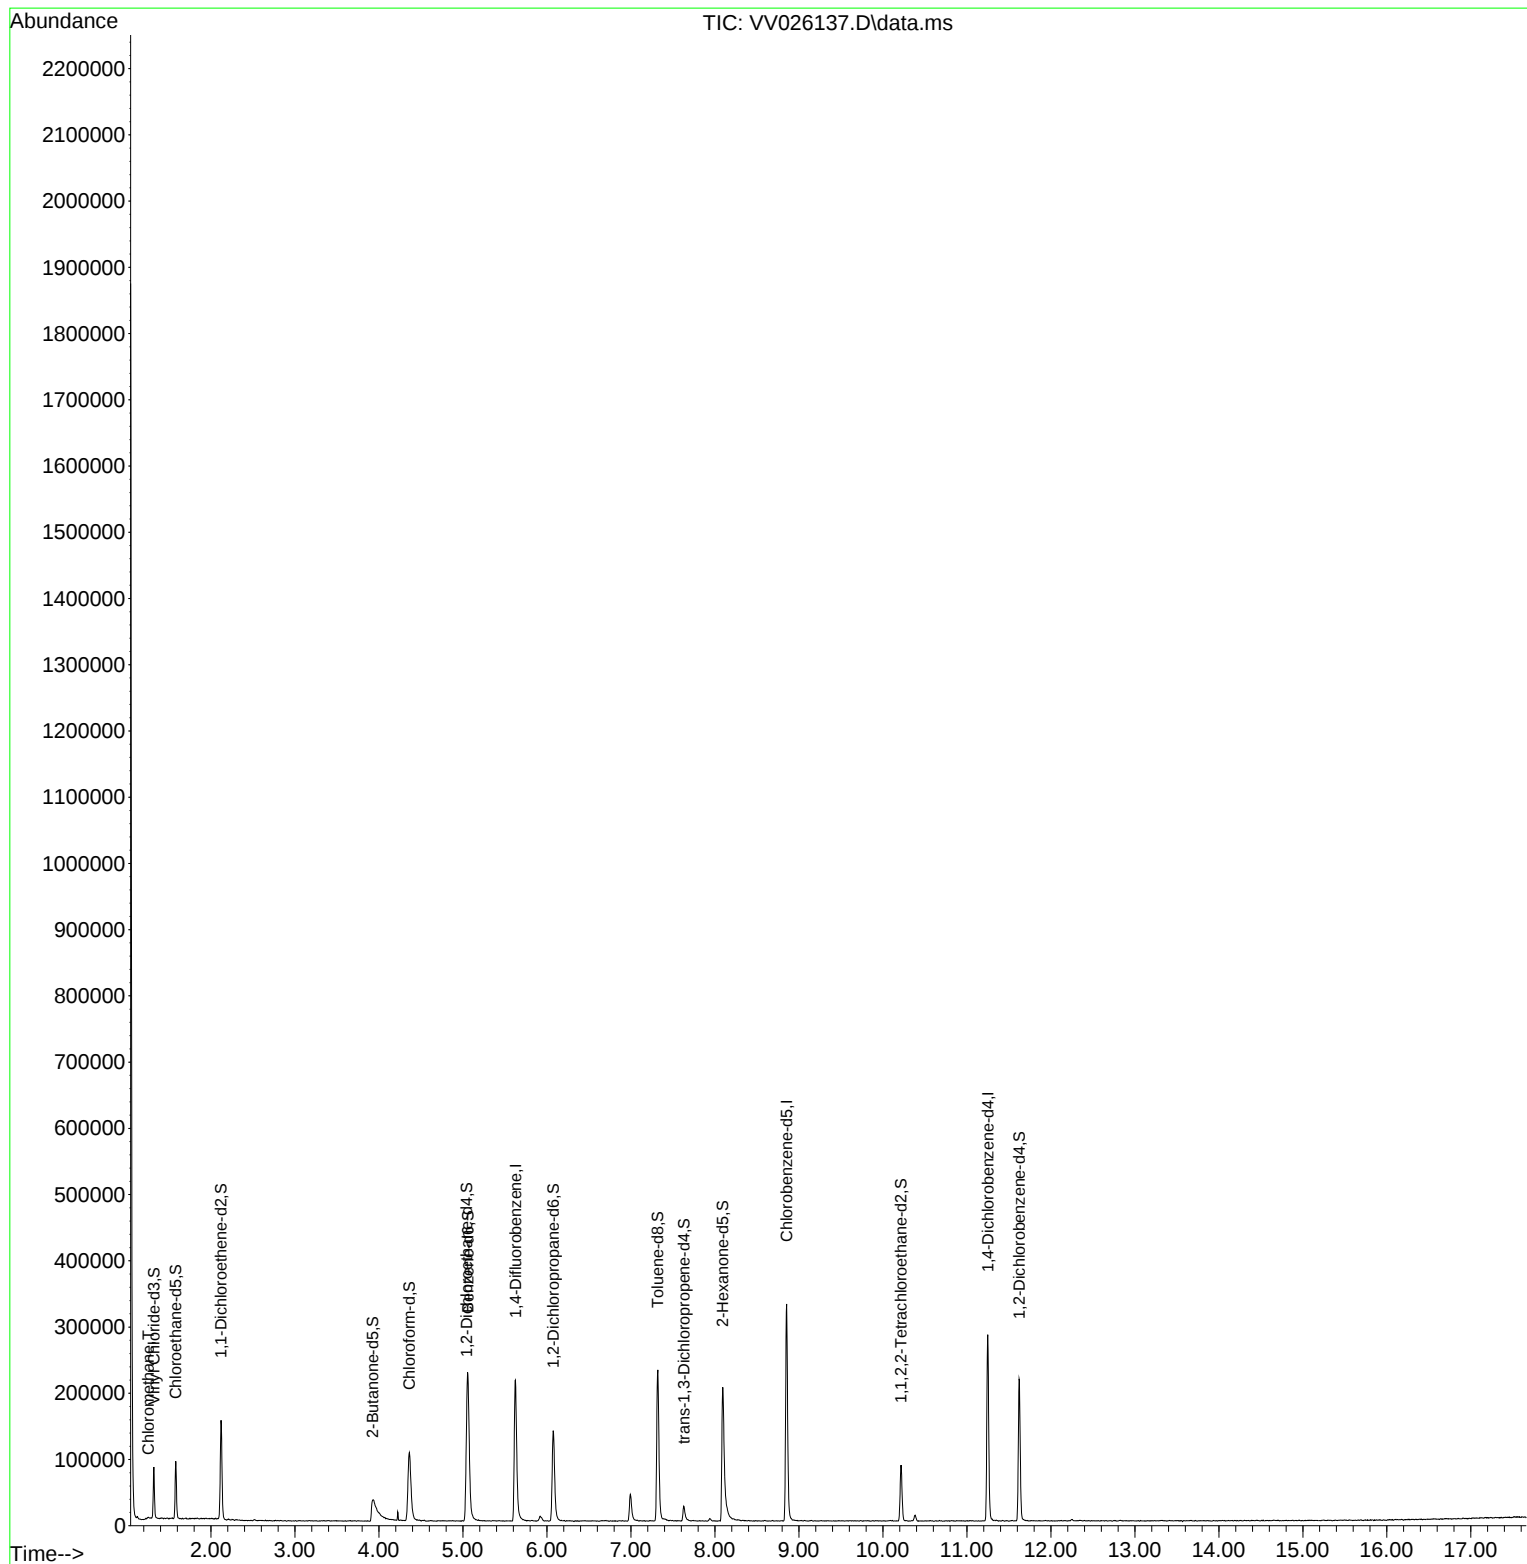

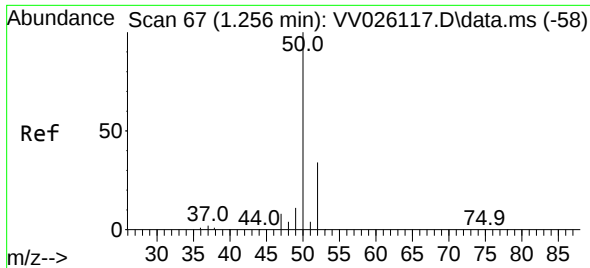

#3
 Chloromethane
 Concen: 0.054 ug/L
 RT: 1.253 min Scan# 60
 Delta R.T. -0.003 min
 Lab File: VV026137.D
 Acq: 11 Jun 2022 18:07

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DY7

Tgt Ion: 50 Resp: 1118
 Ion Ratio Lower Upper
 50 100
 52 50.7 23.0 42.6#

