

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061122\
 Data File : VW026155.D
 Acq On : 12 Jun 2022 02:13
 Operator : SY/MD
 Sample : N3289-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DS5

Quant Time: Jun 13 07:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 07:40:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	194078	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	189262	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	76669	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	46934	4.12	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.40%
7) Chloroethane-d5	1.581	69	57183	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.121	63	80229	3.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.00%
20) 2-Butanone-d5	3.921	46	77757	46.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.30%
24) Chloroform-d	4.362	84	114323	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.043	65	47882	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.056	84	216528	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
36) 1,2-Dichloropropane-d6	6.076	67	70488	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.320	98	164253	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.20%
43) trans-1,3-Dichloroprop...	7.629	79	14626	3.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.20%
46) 2-Hexanone-d5	8.092	63	67225	36.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.34%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40748	4.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.40%
66) 1,2-Dichlorobenzene-d4	11.622	152	55675	4.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.00%
Target Compounds						
25) Chloroform	4.391	83	10515	0.38	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026155.D
Acq On : 12 Jun 2022 02:13
Operator : SY/MD
Sample : N3289-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DS5

Quant Time: Jun 13 07:45:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 07:40:59 2022
Response via : Initial Calibration

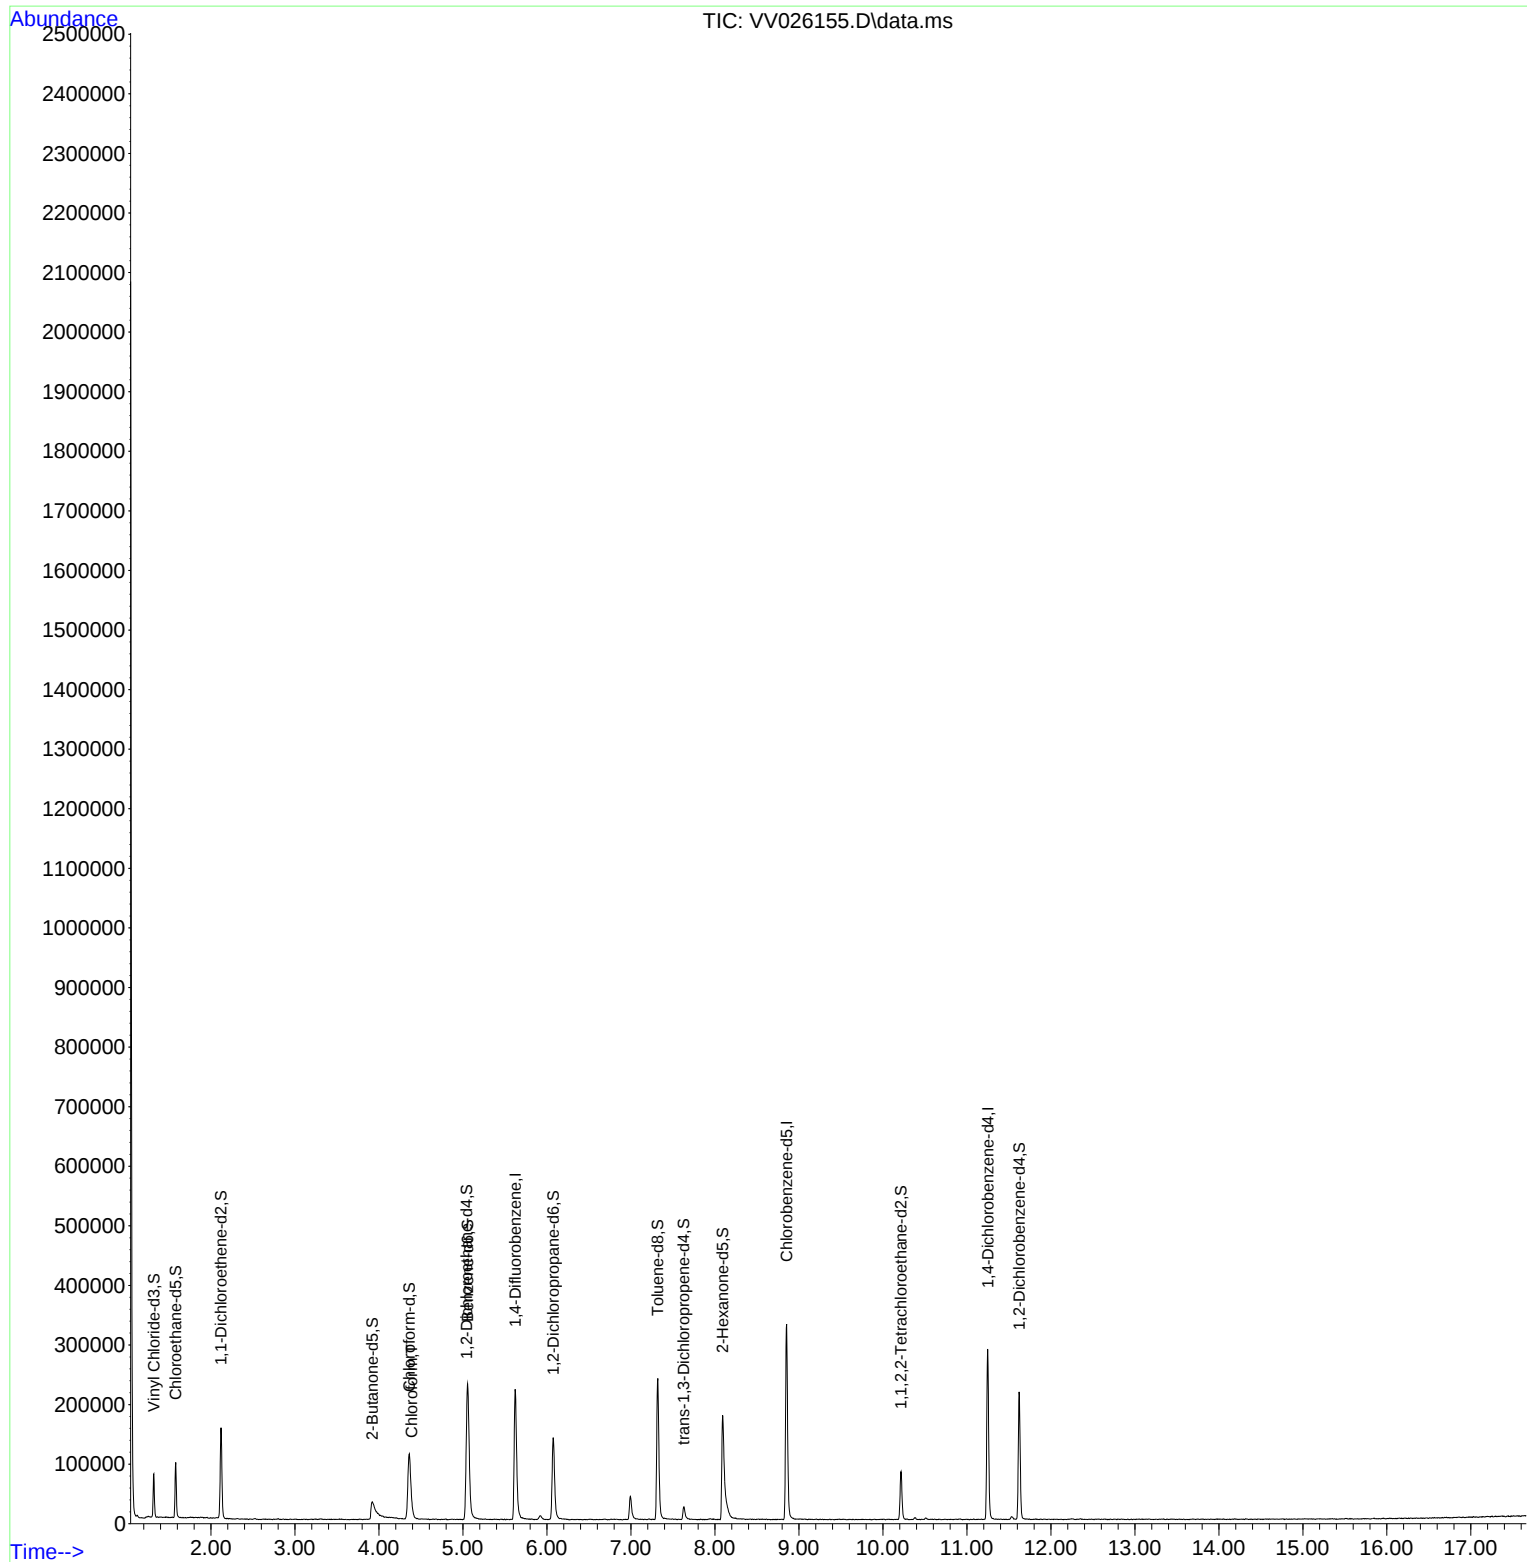

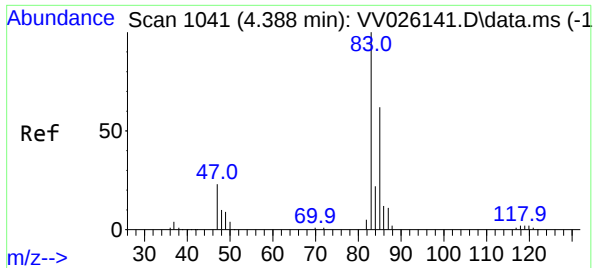

#25
 Chloroform
 Concen: 0.38 ug/L
 RT: 4.391 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV026155.D
 Acq: 12 Jun 2022 02:13

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DS5

Tgt Ion: 83 Resp: 10515
 Ion Ratio Lower Upper
 83 100
 85 60.3 45.2 84.0

