

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061122\
 Data File : VW026159.D
 Acq On : 12 Jun 2022 03:48
 Operator : SY/MD
 Sample : N3273-10 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80

Quant Time: Jun 13 07:46:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 07:40:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	177650	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	175398	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68324	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	42505	4.076	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.581	69	53527	4.910	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.200%
11) 1,1-Dichloroethene-d2	2.121	63	72999	3.031	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.600%
20) 2-Butanone-d5	3.915	46	62485	40.512	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.020%
24) Chloroform-d	4.359	84	108509	4.909	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.043	65	45374	5.033	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	5.059	84	202165	4.770	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.076	67	67076	5.115	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.400%
41) Toluene-d8	7.320	98	151974	4.057	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	7.629	79	12745	3.301	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.000%
46) 2-Hexanone-d5	8.092	63	54330	31.980	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	63.960%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38202	4.321	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	52543	5.027	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.979	164	4199	0.377	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026159.D
Acq On : 12 Jun 2022 03:48
Operator : SY/MD
Sample : N3273-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80


Quant Time: Jun 13 07:46:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 07:40:59 2022
Response via : Initial Calibration

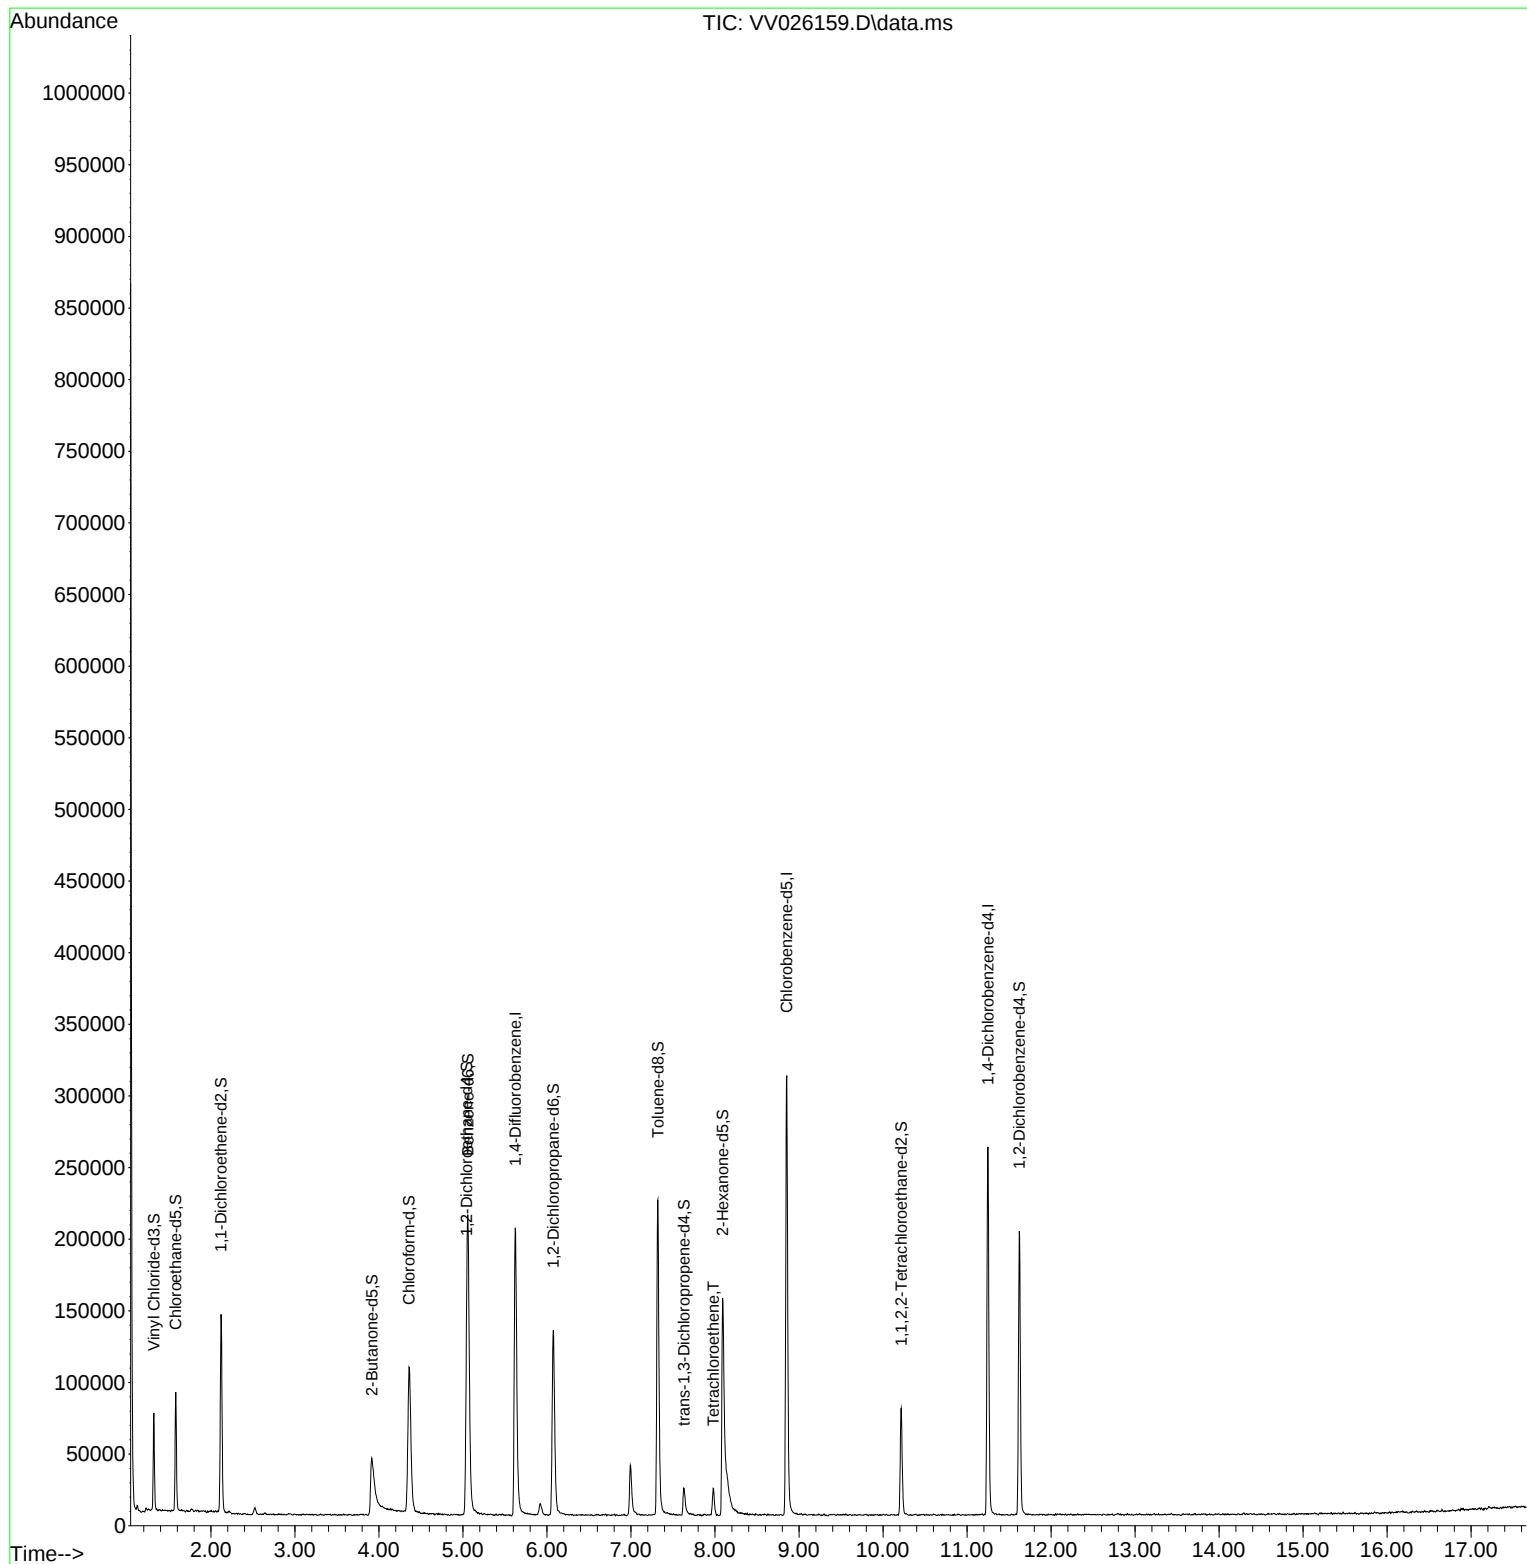

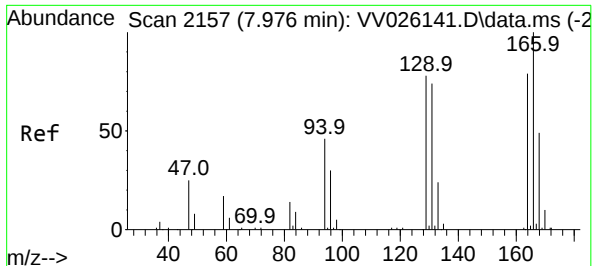

#47
 Tetrachloroethene
 Concen: 0.377 ug/L
 RT: 7.979 min Scan# 2158
 Delta R.T. 0.003 min
 Lab File: VV026159.D
 Acq: 12 Jun 2022 03:48

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80

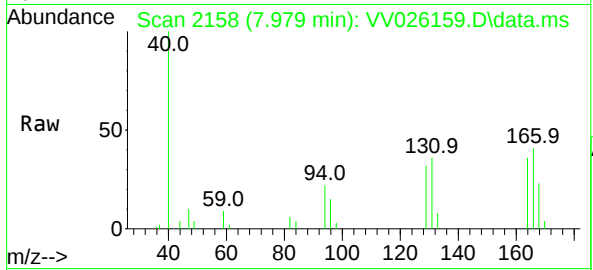

Tgt Ion:	164	Resp:	4199
Ion	Ratio	Lower	Upper
164	100		
129	88.7	68.3	126.9
131	101.6	66.5	123.5
166	116.3	88.1	163.7

