

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026120.D
 Acq On : 11 Jun 2022 11:22
 Operator : SY/MD
 Sample : N3272-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	97	rBV	78234	82339	14.57%	1.768%
2	1.580	160	168	181	rBV	91782	103889	18.38%	2.231%
3	2.121	325	336	351	rVB	156218	227920	40.32%	4.895%
4	3.921	884	896	941	rBV2	33748	152151	26.91%	3.268%
5	4.362	1017	1033	1057	rBV	108407	270721	47.89%	5.814%
6	5.056	1234	1249	1276	rBV2	227134	565318	100.00%	12.141%
7	5.622	1410	1425	1453	rBV	222207	454217	80.35%	9.755%
8	5.924	1507	1519	1536	rBV6	14880	35505	6.28%	0.763%
9	6.075	1553	1566	1595	rBV2	135806	285183	50.45%	6.125%
10	6.992	1838	1851	1878	rBV2	43604	86954	15.38%	1.867%
11	7.320	1940	1953	1973	rBV	247248	435134	76.97%	9.345%
12	7.628	2038	2049	2066	rBV	25295	45915	8.12%	0.986%
13	7.940	2135	2146	2150	rBV3	5403	8008	1.42%	0.172%
14	7.979	2151	2158	2173	rVB3	13651	24587	4.35%	0.528%
15	8.091	2180	2193	2227	rBV2	181711	397852	70.38%	8.544%
16	8.854	2419	2430	2452	rBV	339038	549819	97.26%	11.808%
17	10.217	2840	2854	2877	rVB	76405	122857	21.73%	2.639%
18	10.381	2894	2905	2917	rBV2	10161	16426	2.91%	0.353%
19	11.249	3163	3175	3196	rBV	288063	451379	79.85%	9.694%
20	11.622	3280	3291	3311	rBV	216656	340143	60.17%	7.305%




Sum of corrected areas: 4656317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026120.D
Acq On : 11 Jun 2022 11:22
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

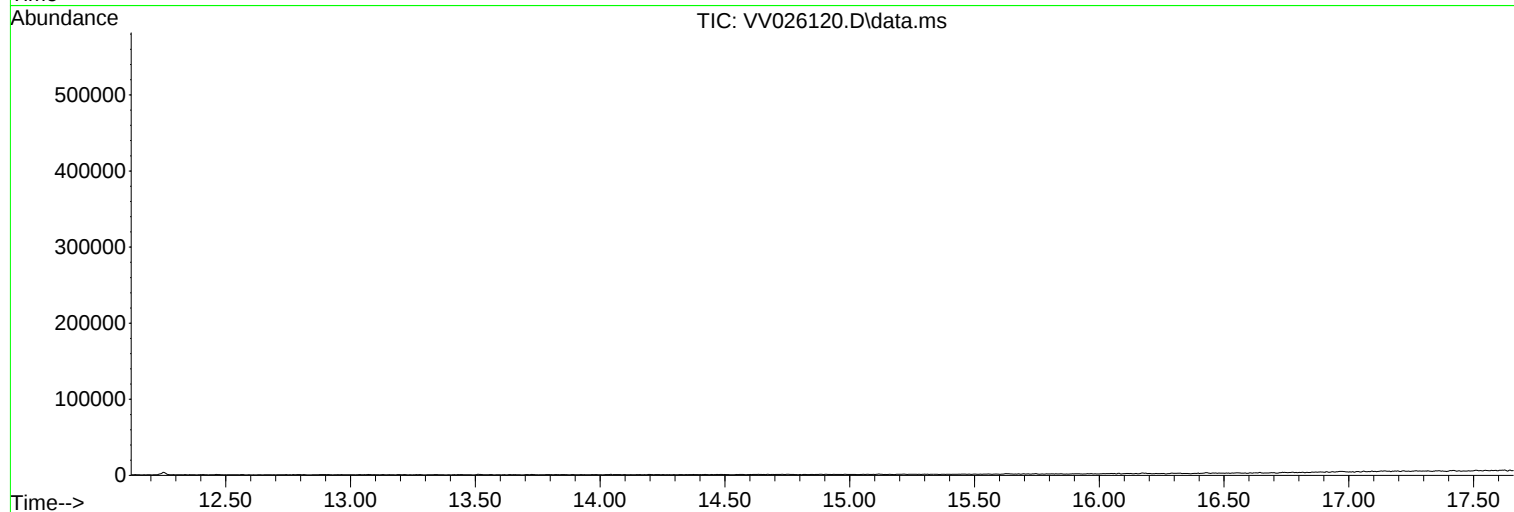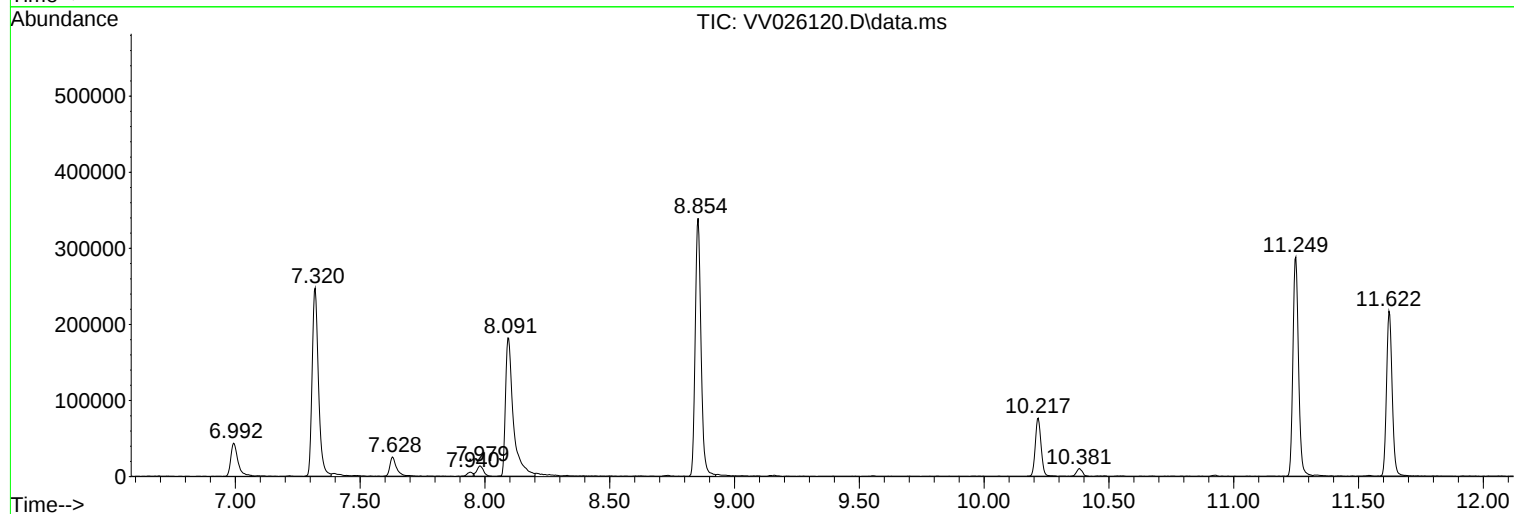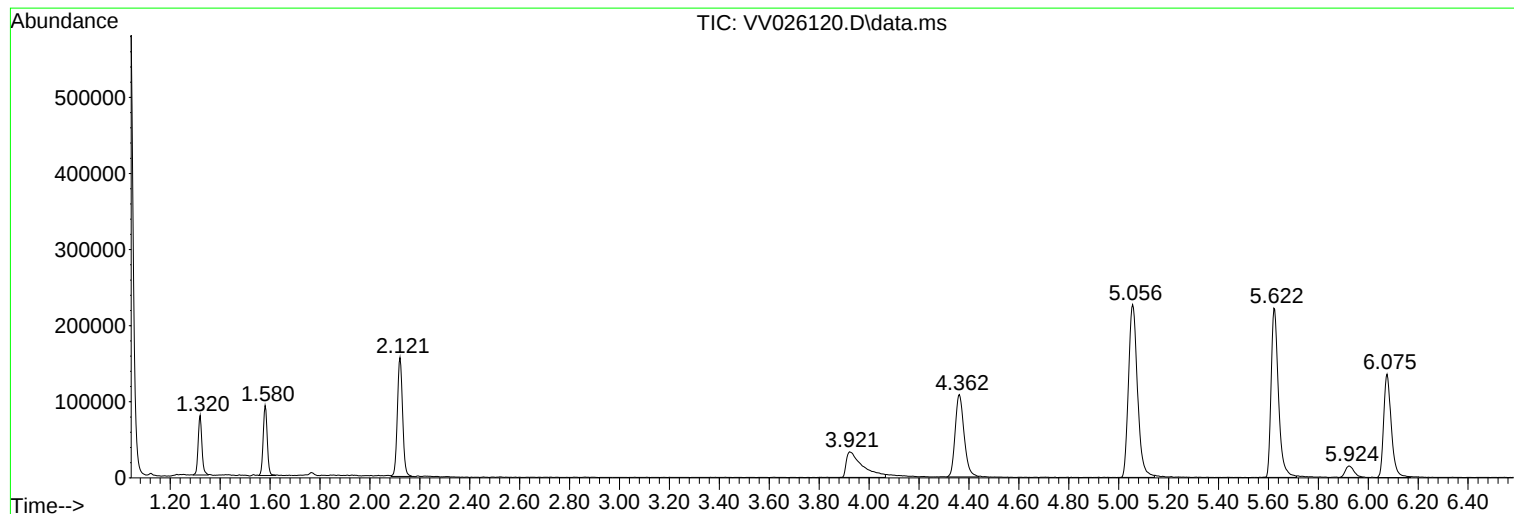

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026120.D
Acq On : 11 Jun 2022 11:22
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026120.D
Acq On : 11 Jun 2022 11:22
Operator : SY/MD
Sample : N3272-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc