

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026121.D
 Acq On : 11 Jun 2022 11:45
 Operator : SY/MD
 Sample : N3273-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	38	rVB2	13277	14293	2.50%	0.289%
2	1.317	77	86	97	rBV	88341	103228	18.02%	2.091%
3	1.429	114	121	126	rVB3	6267	6884	1.20%	0.139%
4	1.581	160	168	178	rBV	90654	102998	17.98%	2.086%
5	1.719	202	211	222	rBV	133812	163461	28.54%	3.311%
6	2.121	325	336	354	rVB	155858	233204	40.71%	4.723%
7	2.217	356	366	384	rVB	22860	37219	6.50%	0.754%
8	3.831	859	868	884	rBV4	3077	7829	1.37%	0.159%
9	3.925	885	897	949	rBV3	56602	218352	38.12%	4.422%
10	4.362	1017	1033	1055	rBV	106322	265189	46.30%	5.371%
11	5.056	1233	1249	1285	rBV2	229525	572801	100.00%	11.601%
12	5.622	1414	1425	1450	rBV	220745	453455	79.16%	9.184%
13	5.928	1502	1520	1533	rBV9	7786	19508	3.41%	0.395%
14	6.076	1551	1566	1598	rBV	133197	283470	49.49%	5.741%
15	6.992	1837	1851	1874	rBV	43078	83206	14.53%	1.685%
16	7.320	1941	1953	1971	rBV	245971	432639	75.53%	8.762%
17	7.629	2038	2049	2071	rBV	23250	44559	7.78%	0.902%
18	7.940	2134	2146	2153	rBV4	8117	14527	2.54%	0.294%
19	7.982	2153	2159	2177	rVB5	6442	11069	1.93%	0.224%
20	8.095	2183	2194	2233	rBV3	175068	385575	67.31%	7.809%
21	8.854	2418	2430	2452	rBV	326532	545445	95.22%	11.047%
22	10.214	2843	2853	2878	rBV	80536	129623	22.63%	2.625%
23	10.381	2894	2905	2917	rBV3	14752	23438	4.09%	0.475%
24	11.246	3163	3174	3197	rBV	282836	445022	77.69%	9.013%
25	11.622	3280	3291	3310	rBV	214388	334605	58.42%	6.777%
26	12.249	3476	3486	3496	rBV2	3391	5799	1.01%	0.117%




Sum of corrected areas: 4937398

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026121.D
Acq On : 11 Jun 2022 11:45
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

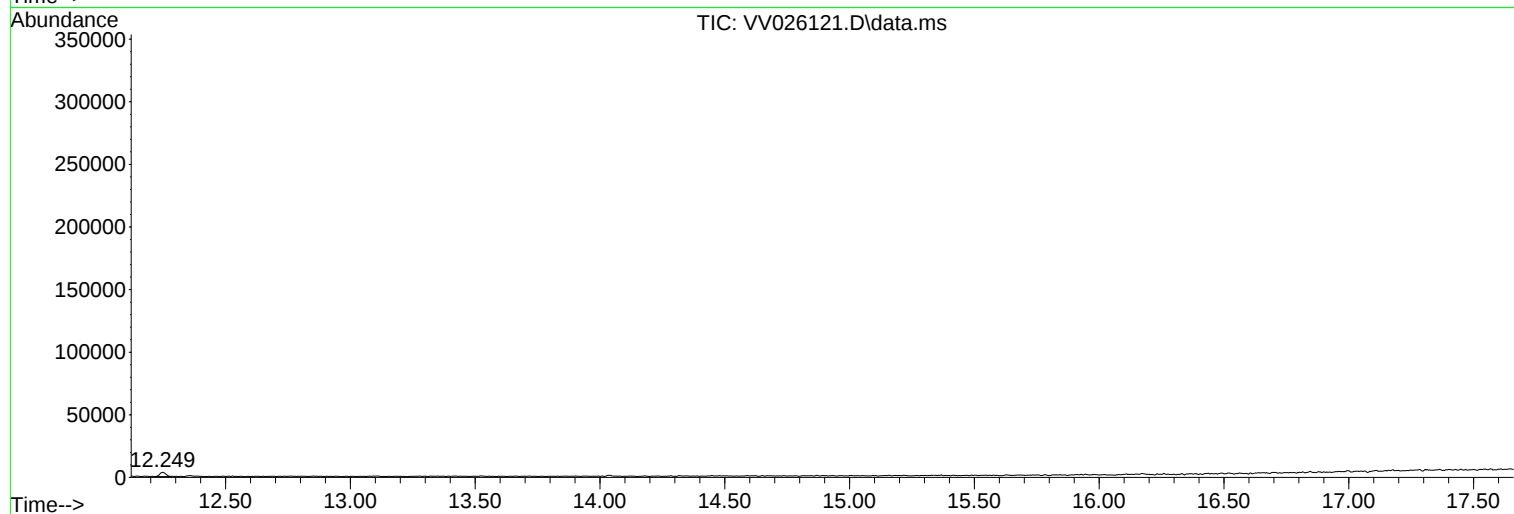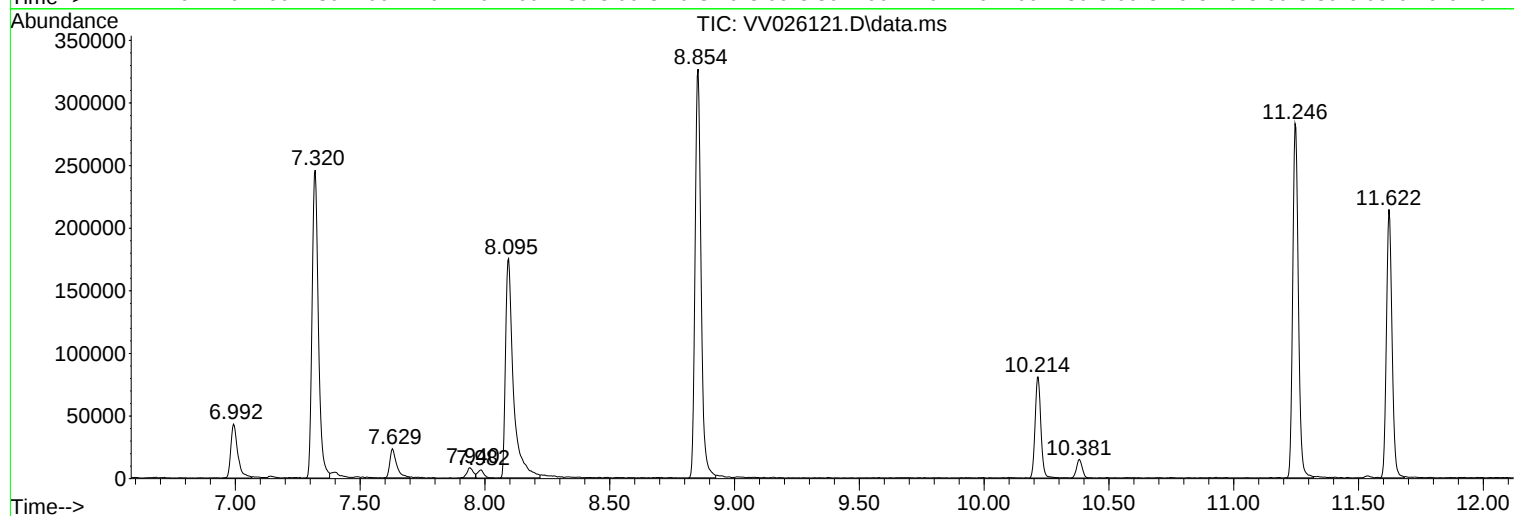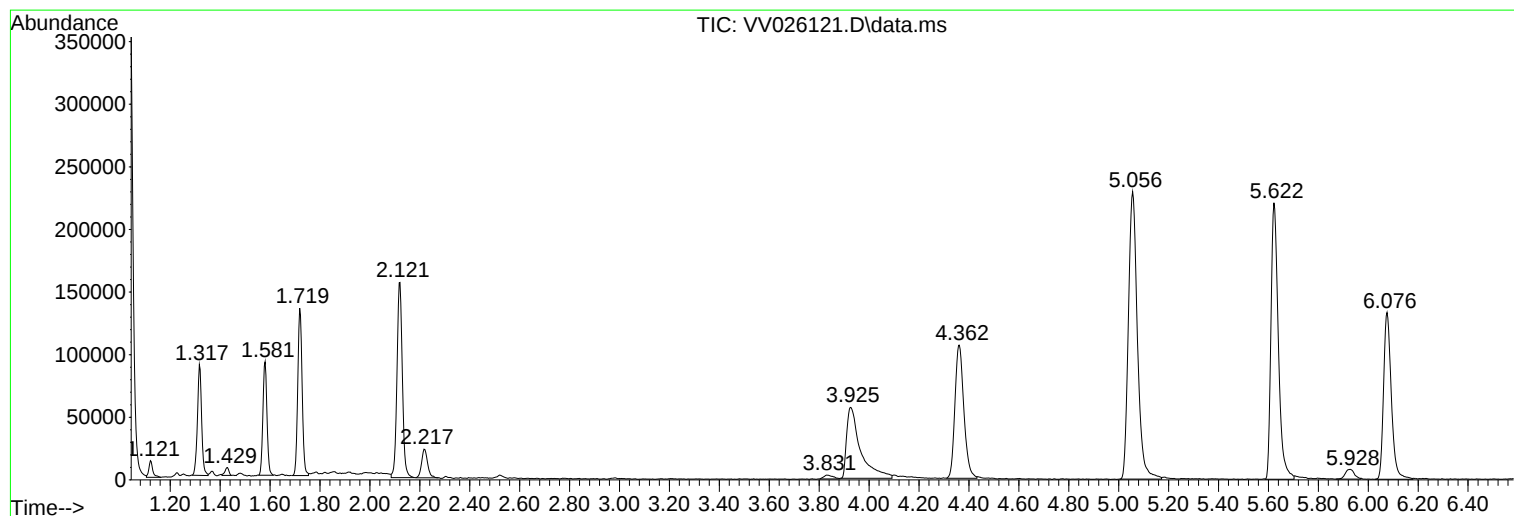

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026121.D
Acq On : 11 Jun 2022 11:45
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.719	1.80 ug/L	163461	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Hexyne	82	C6H10	000693-02-7	7
5			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7

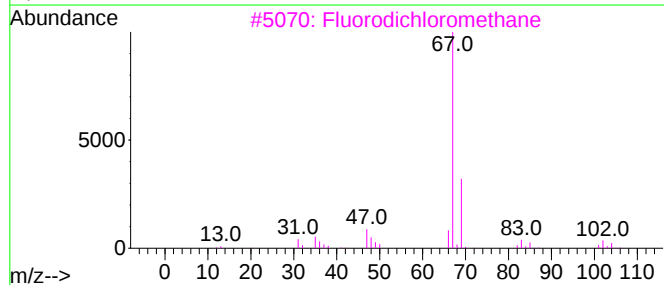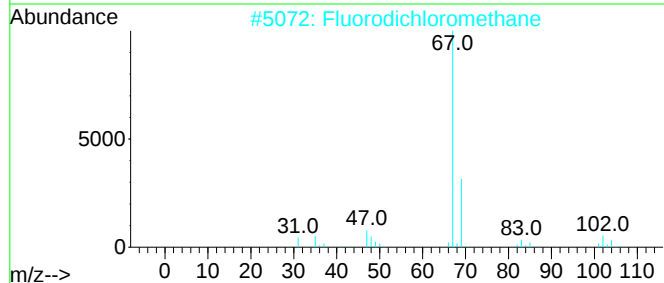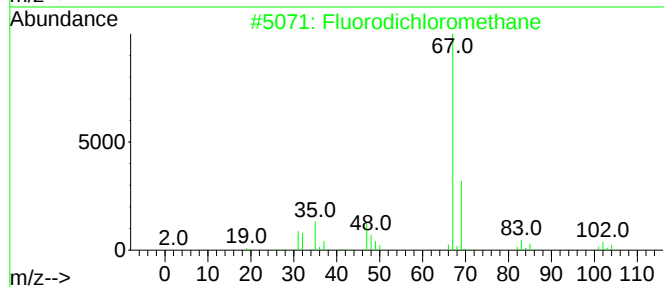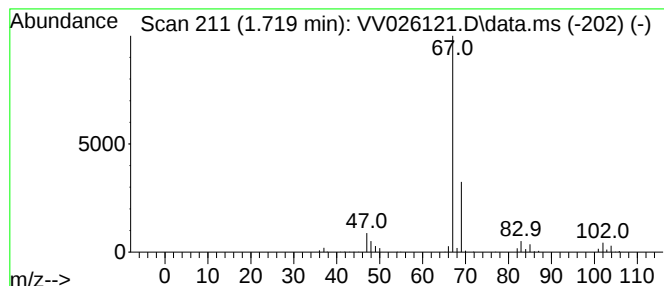

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026121.D
Acq On : 11 Jun 2022 11:45
Operator : SY/MD
Sample : N3273-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	1.719	1.8	ug/L	163461	1	5.622	453455	5.0