

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026124.D
 Acq On : 11 Jun 2022 12:57
 Operator : SY/MD
 Sample : N3273-05DL 40X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	78	88	102	rBV2	297635	332065	57.30%	6.661%
2	1.584	161	169	181	rVB	92459	106538	18.39%	2.137%
3	2.124	326	337	351	rVB	157255	231117	39.88%	4.636%
4	2.526	450	462	472	rBV2	7849	13529	2.33%	0.271%
5	3.925	881	897	947	rBV3	59484	267994	46.25%	5.376%
6	4.362	1016	1033	1065	rBV	108637	273566	47.21%	5.488%
7	5.060	1233	1250	1285	rBV3	229236	579471	100.00%	11.624%
8	5.625	1414	1426	1454	rBV	191629	398242	68.73%	7.989%
9	5.921	1503	1518	1541	rBV3	70368	151102	26.08%	3.031%
10	6.076	1553	1566	1588	rBV	137754	286785	49.49%	5.753%
11	6.992	1842	1851	1878	rBV	37930	75489	13.03%	1.514%
12	7.320	1941	1953	1973	rBV	240796	428374	73.93%	8.593%
13	7.629	2040	2049	2076	rBV	20214	40059	6.91%	0.804%
14	7.982	2150	2159	2173	rVB3	13388	23659	4.08%	0.475%
15	8.092	2184	2193	2224	rBV2	197663	426606	73.62%	8.557%
16	8.854	2417	2430	2456	rBV	293042	487115	84.06%	9.771%
17	10.217	2840	2854	2869	rBV	85064	134975	23.29%	2.708%
18	11.249	3163	3175	3197	rBV	253945	395724	68.29%	7.938%
19	11.622	3279	3291	3307	rBV	208659	332769	57.43%	6.675%




Sum of corrected areas: 4985179

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026124.D
Acq On : 11 Jun 2022 12:57
Operator : SY/MD
Sample : N3273-05DL 40X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

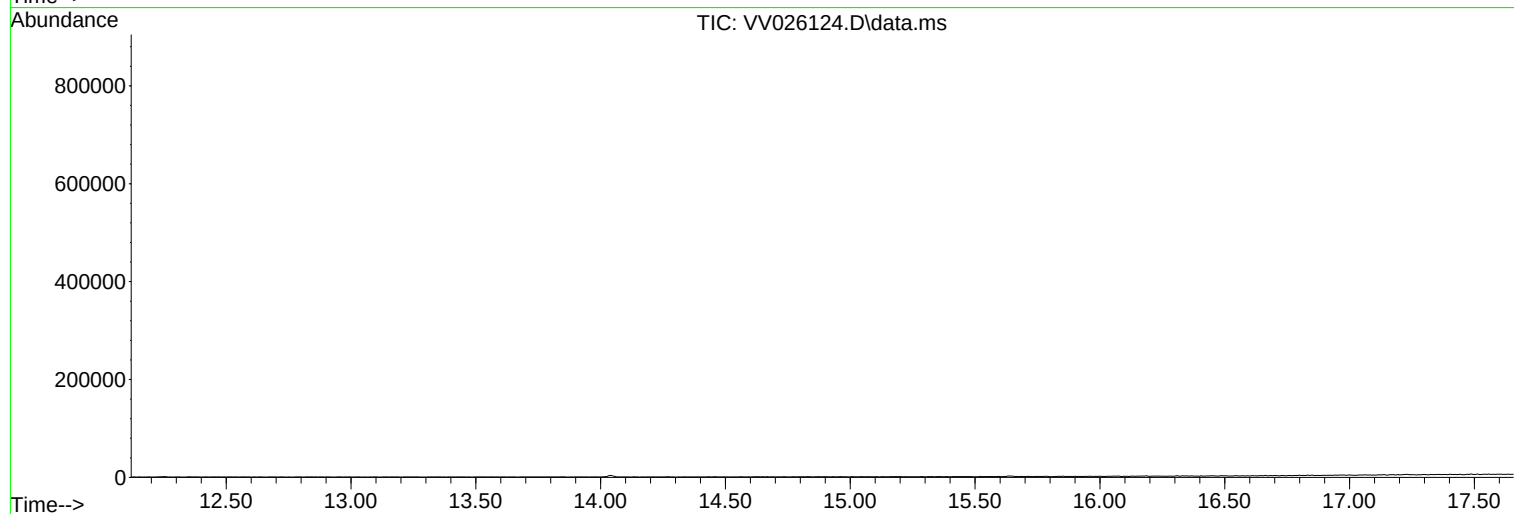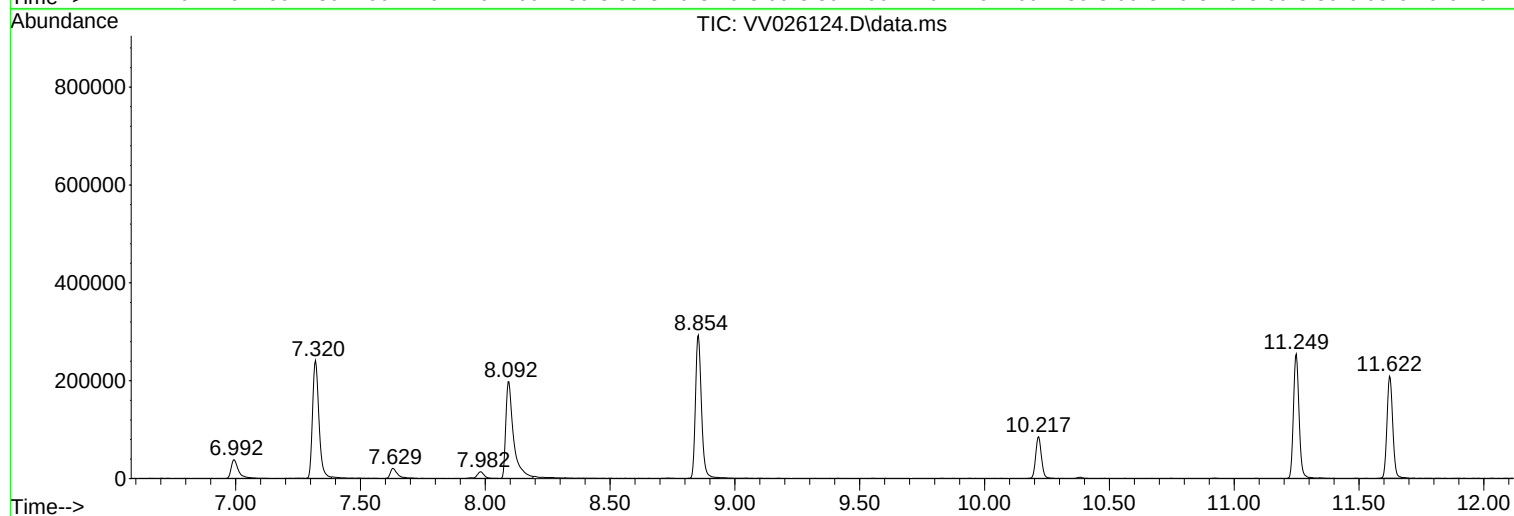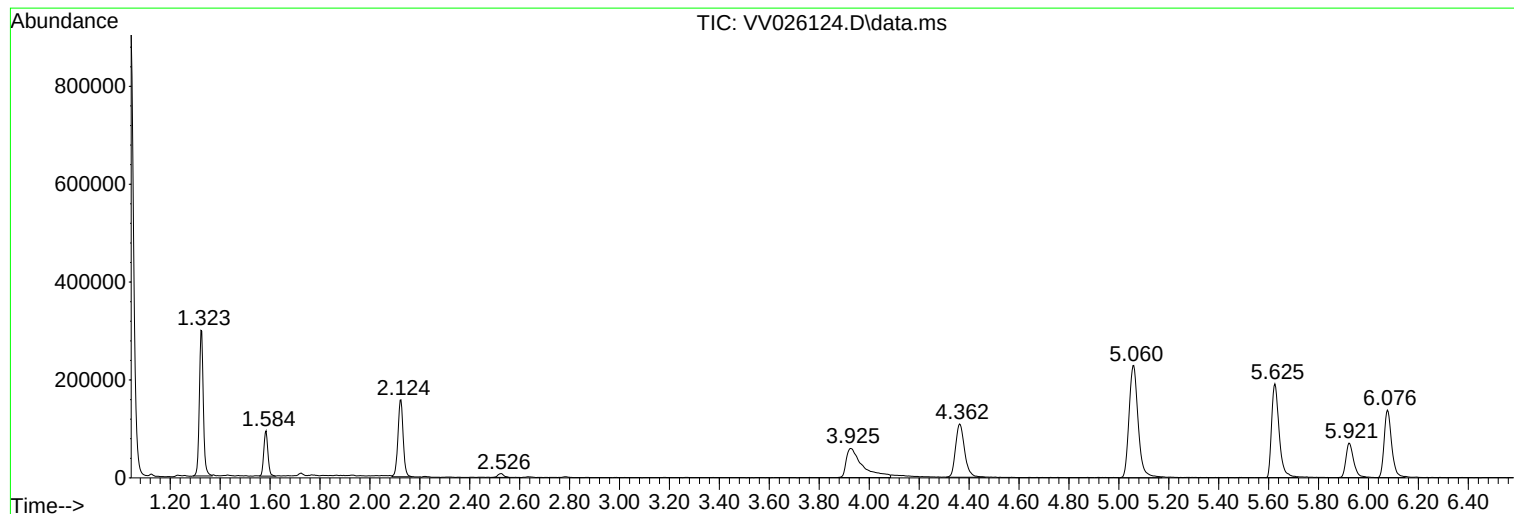

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026124.D
Acq On : 11 Jun 2022 12:57
Operator : SY/MD
Sample : N3273-05DL 40X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026124.D
Acq On : 11 Jun 2022 12:57
Operator : SY/MD
Sample : N3273-05DL 40X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc