

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026127.D
 Acq On : 11 Jun 2022 14:09
 Operator : SY/MD
 Sample : N3272-14DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B58DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	79	88	100	rBV	71364	78404	14.61%	1.826%
2	1.481	130	137	146	rBV	7802	11161	2.08%	0.260%
3	1.584	161	169	184	rVB	87477	101981	19.00%	2.375%
4	1.767	219	226	235	rVB	21454	27773	5.17%	0.647%
5	2.124	326	337	350	rVB	134717	195677	36.46%	4.556%
6	2.523	453	461	475	rVB2	8875	15317	2.85%	0.357%
7	3.931	882	899	954	rBV3	54394	270105	50.33%	6.289%
8	4.362	1017	1033	1058	rBV	102034	259378	48.33%	6.040%
9	5.060	1232	1250	1277	rBV2	215037	536681	100.00%	12.497%
10	5.625	1415	1426	1452	rBV	154795	320082	59.64%	7.453%
11	5.924	1506	1519	1542	rBV	102013	212406	39.58%	4.946%
12	6.076	1553	1566	1587	rBV	130693	274306	51.11%	6.387%
13	6.995	1842	1852	1871	rBV	37767	74477	13.88%	1.734%
14	7.320	1942	1953	1973	rBV	208333	365057	68.02%	8.500%
15	7.629	2040	2049	2068	rBV	22034	40334	7.52%	0.939%
16	8.095	2183	2194	2226	rBV	203819	430969	80.30%	10.035%
17	8.854	2419	2430	2454	rBV	229553	374214	69.73%	8.714%
18	10.217	2839	2854	2870	rBV2	81912	132706	24.73%	3.090%
19	11.249	3163	3175	3197	rBV	185988	287941	53.65%	6.705%
20	11.622	3280	3291	3312	rBV	181221	285674	53.23%	6.652%




Sum of corrected areas: 4294643

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026127.D
Acq On : 11 Jun 2022 14:09
Operator : SY/MD
Sample : N3272-14DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

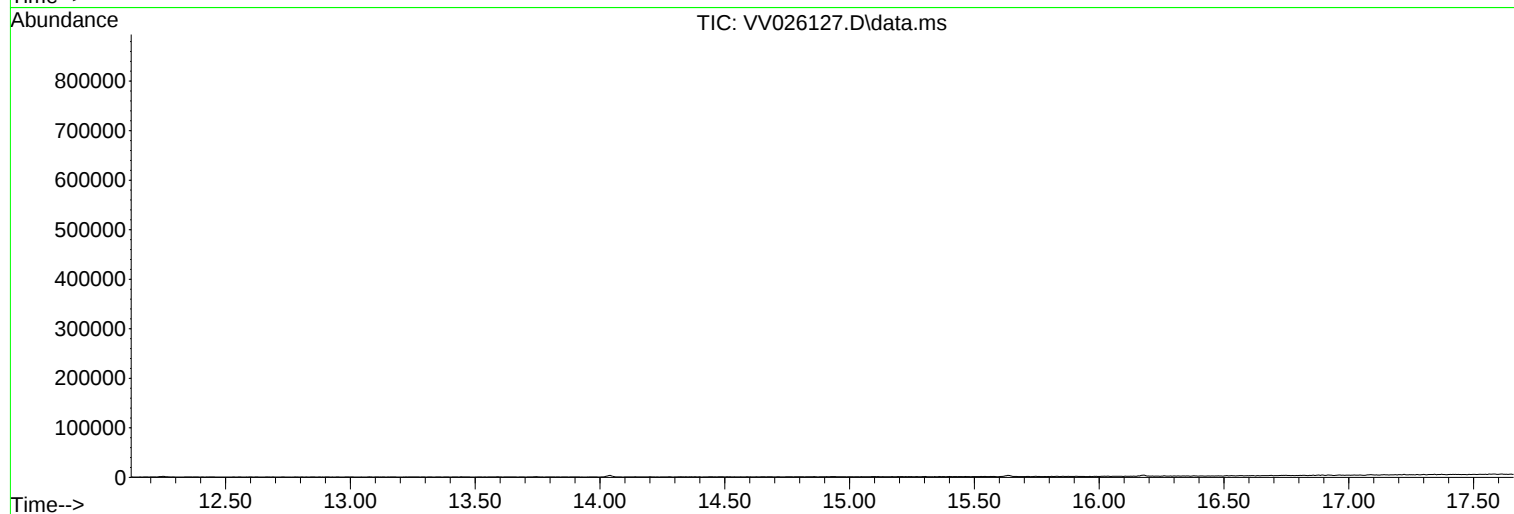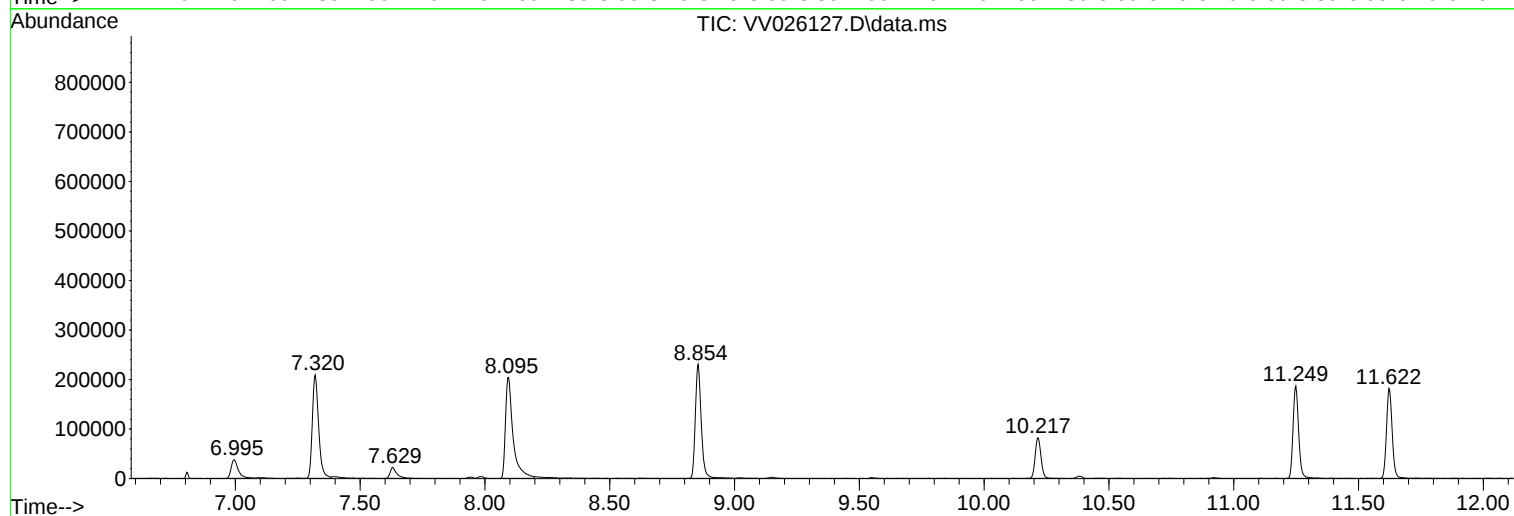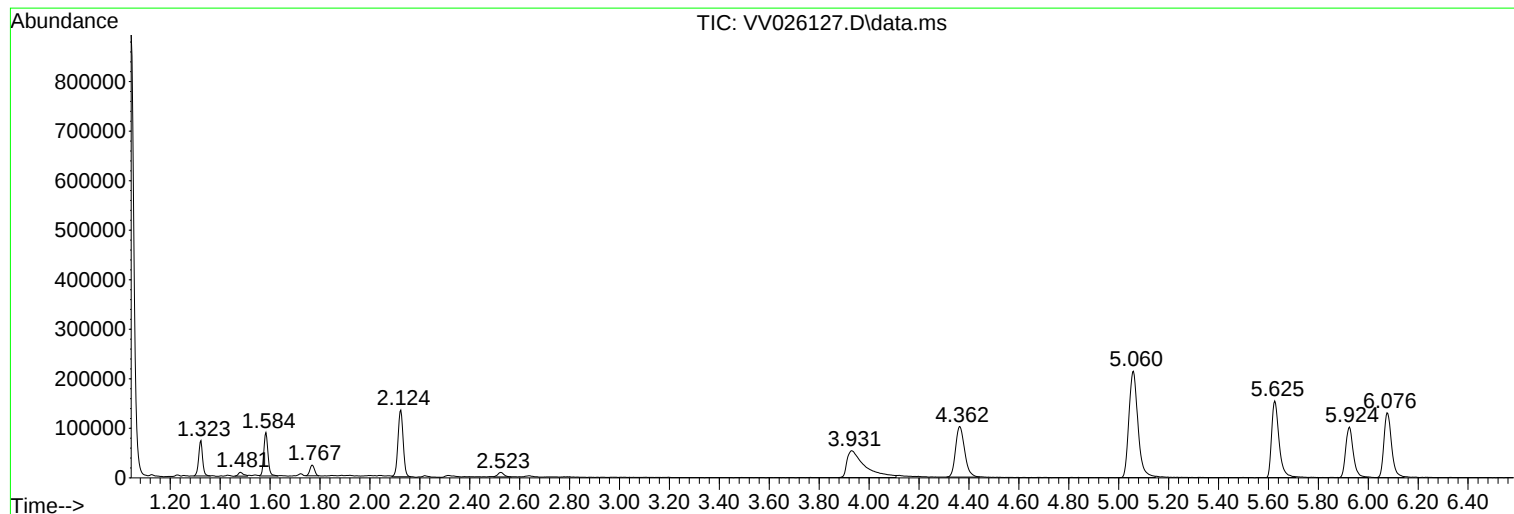

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026127.D
Acq On : 11 Jun 2022 14:09
Operator : SY/MD
Sample : N3272-14DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026127.D
Acq On : 11 Jun 2022 14:09
Operator : SY/MD
Sample : N3272-14DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B58DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------