

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026128.D
 Acq On : 11 Jun 2022 14:32
 Operator : SY/MD
 Sample : N3272-15DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	99	rBV	76979	81213	15.28%	1.756%
2	1.584	160	169	181	rBV	87349	101426	19.08%	2.193%
3	1.767	218	226	237	rBV	30354	40783	7.67%	0.882%
4	2.121	327	336	354	rVB	142203	209999	39.50%	4.541%
5	2.523	452	461	471	rBV3	6908	11609	2.18%	0.251%
6	3.934	883	900	959	rBV3	48913	255549	48.07%	5.526%
7	4.362	1018	1033	1057	rBV	101695	255861	48.13%	5.532%
8	5.056	1234	1249	1276	rBV3	212327	531584	100.00%	11.494%
9	5.626	1414	1426	1457	rBV	164686	337535	63.50%	7.298%
10	5.921	1505	1518	1547	rBV	202688	410274	77.18%	8.871%
11	6.076	1554	1566	1592	rBV	130176	268530	50.52%	5.806%
12	6.995	1841	1852	1876	rBV2	35443	71559	13.46%	1.547%
13	7.320	1941	1953	1975	rBV	207077	366610	68.97%	7.927%
14	7.632	2041	2050	2072	rBV2	19359	37357	7.03%	0.808%
15	7.979	2147	2158	2176	rVB2	85274	143588	27.01%	3.105%
16	8.095	2184	2194	2229	rBV2	195070	414232	77.92%	8.957%
17	8.854	2419	2430	2455	rBV	234602	385182	72.46%	8.329%
18	10.217	2843	2854	2874	rBV	79686	128808	24.23%	2.785%
19	11.249	3164	3175	3197	rBV	192274	293891	55.29%	6.355%
20	11.622	3280	3291	3318	rBV	174543	279248	52.53%	6.038%




Sum of corrected areas: 4624838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026128.D
Acq On : 11 Jun 2022 14:32
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

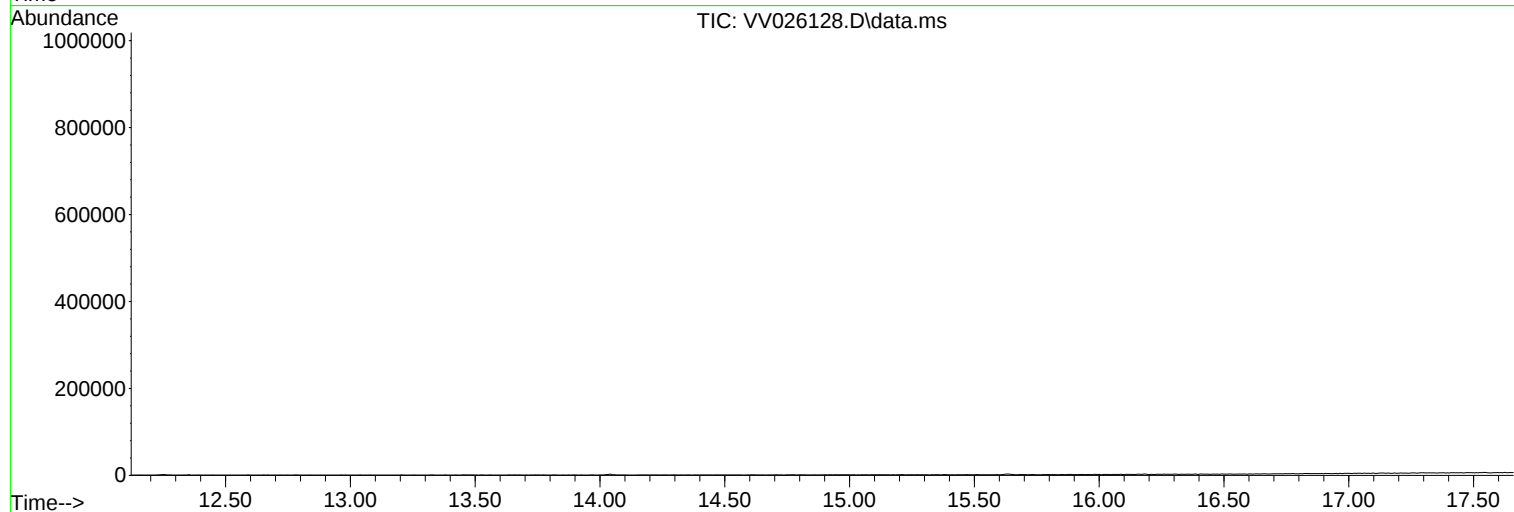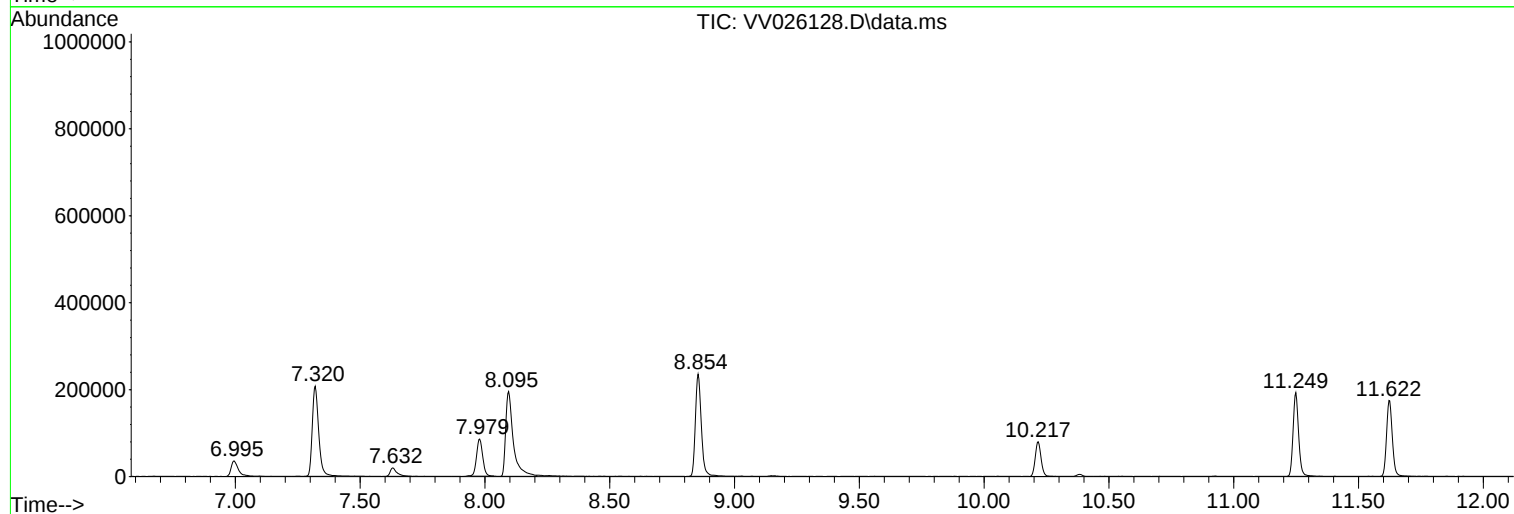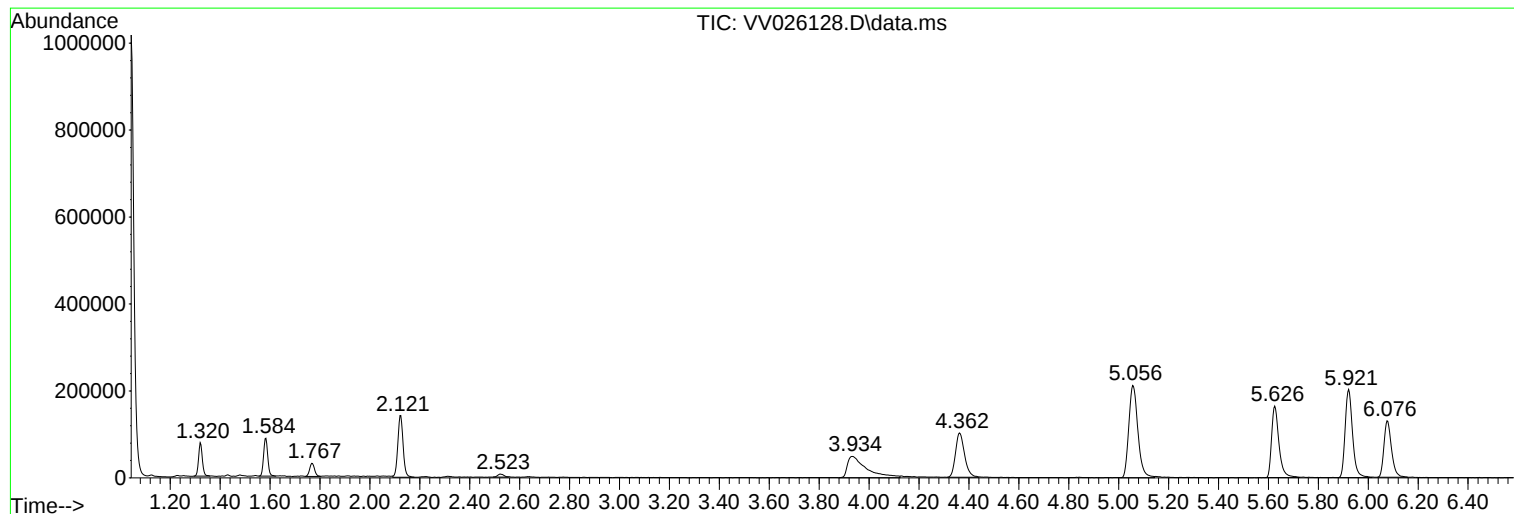

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026128.D
Acq On : 11 Jun 2022 14:32
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026128.D
Acq On : 11 Jun 2022 14:32
Operator : SY/MD
Sample : N3272-15DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------