

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026130.D
 Acq On : 11 Jun 2022 15:20
 Operator : SY/MD
 Sample : N3272-05DL 400X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B49DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	104	rVB	75922	81159	5.50%	1.401%
2	1.580	160	168	179	rBV	89409	99904	6.77%	1.724%
3	1.767	218	226	235	rVB	11927	16137	1.09%	0.278%
4	2.121	322	336	353	rVB	147752	219160	14.86%	3.782%
5	2.523	452	461	474	rBV2	11795	19013	1.29%	0.328%
6	3.928	881	898	940	rBV4	51595	249521	16.91%	4.306%
7	4.362	1017	1033	1053	rBV2	102113	255503	17.32%	4.409%
8	5.056	1233	1249	1273	rBV2	219404	540902	36.66%	9.334%
9	5.625	1414	1426	1453	rBV	179127	365512	24.78%	6.308%
10	5.918	1503	1517	1553	rBV	744993	1475311	100.00%	25.459%
11	6.075	1553	1566	1594	rVB	131938	276775	18.76%	4.776%
12	6.992	1842	1851	1867	rBV	35859	69087	4.68%	1.192%
13	7.320	1942	1953	1970	rBV	220836	395216	26.79%	6.820%
14	7.632	2040	2050	2065	rBV2	19315	37211	2.52%	0.642%
15	7.979	2151	2158	2170	rVB4	8920	15958	1.08%	0.275%
16	8.091	2183	2193	2232	rBV	197617	425976	28.87%	7.351%
17	8.419	2284	2295	2309	rBV2	13360	23125	1.57%	0.399%
18	8.853	2419	2430	2455	rBV	262830	434706	29.47%	7.502%
19	10.217	2843	2854	2876	rBV	80527	129234	8.76%	2.230%
20	11.249	3163	3175	3196	rBV	227941	355875	24.12%	6.141%
21	11.625	3280	3292	3309	rBV	196578	309506	20.98%	5.341%




Sum of corrected areas: 5794791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026130.D
Acq On : 11 Jun 2022 15:20
Operator : SY/MD
Sample : N3272-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

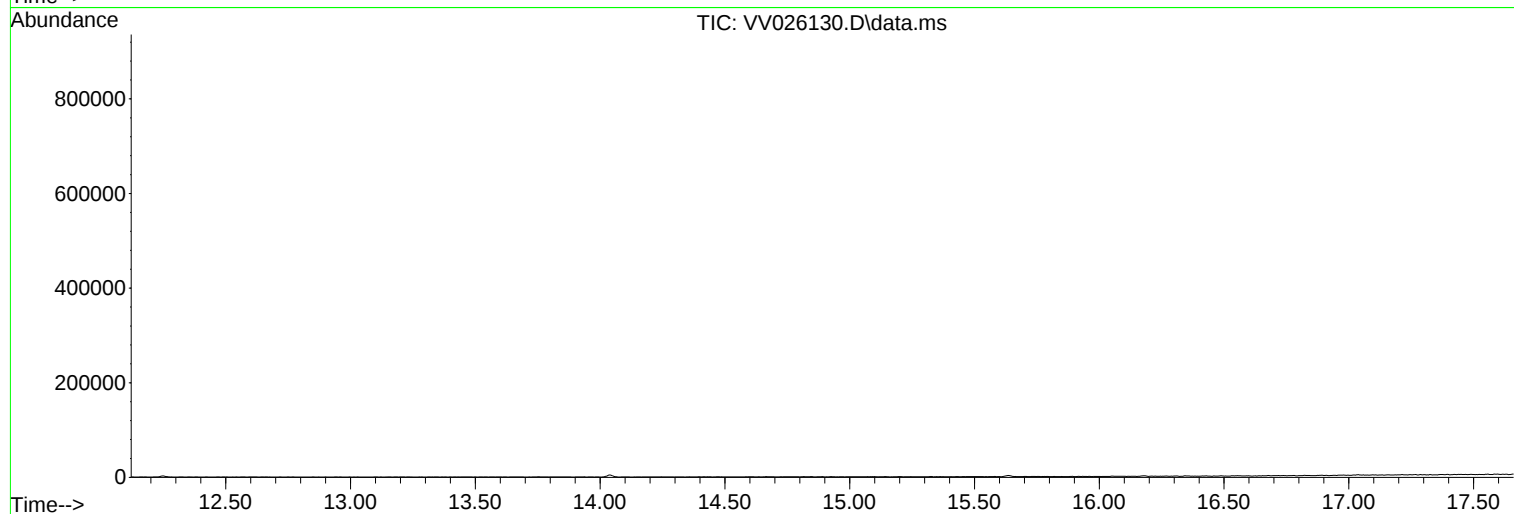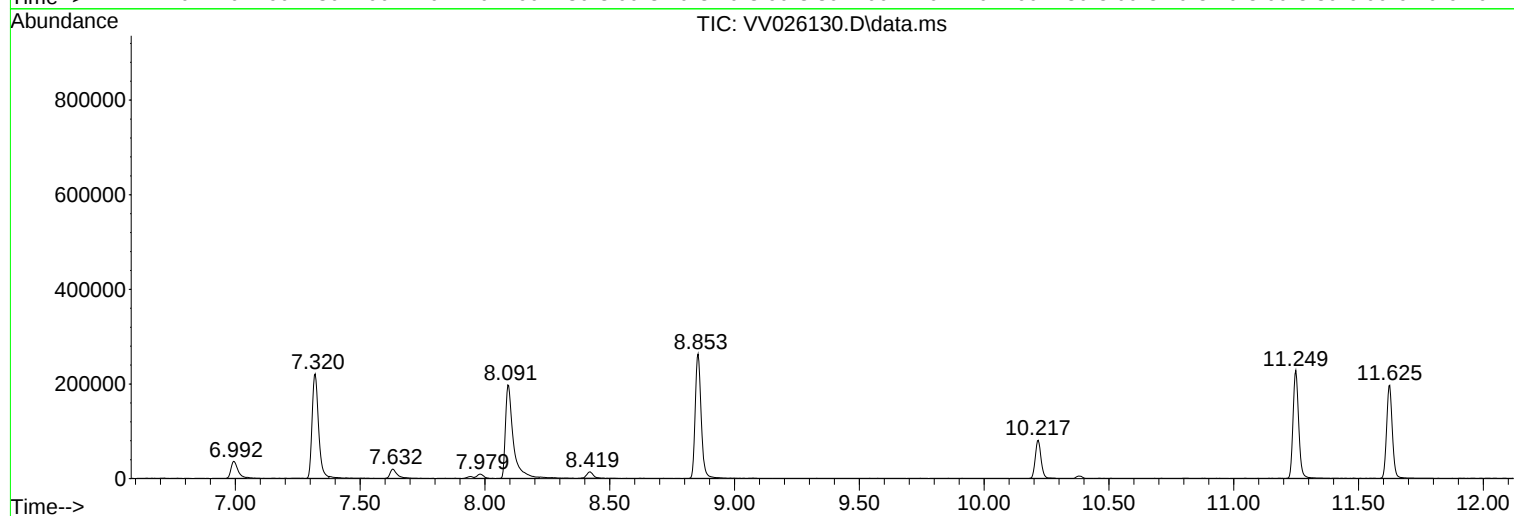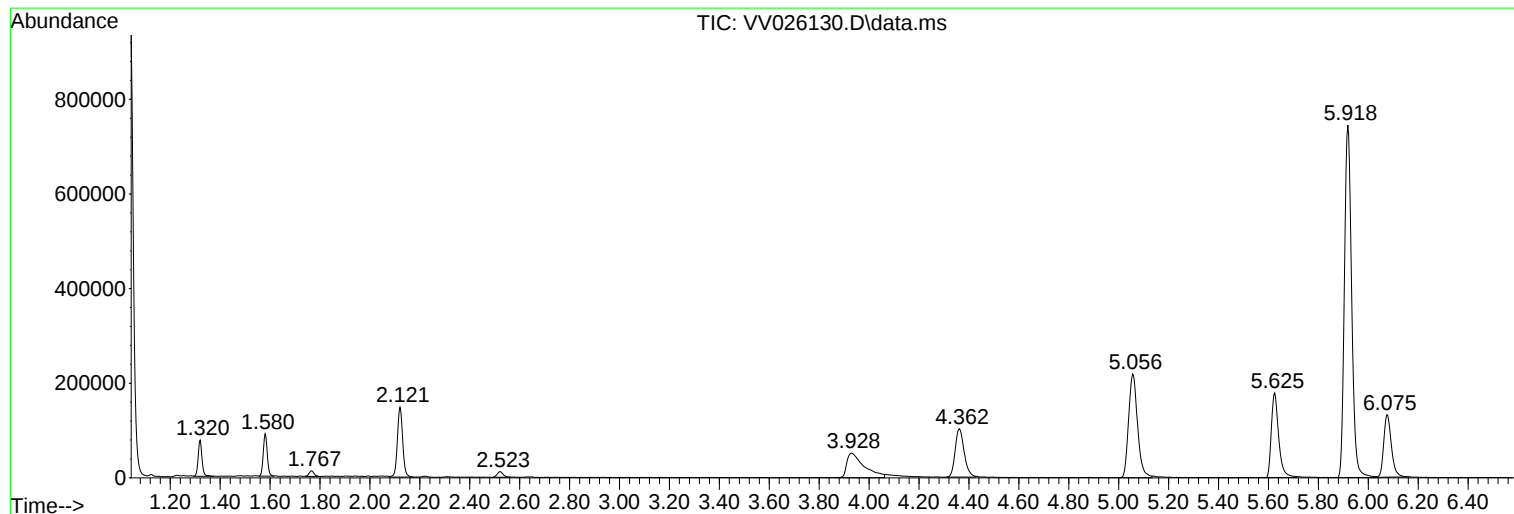

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026130.D
Acq On : 11 Jun 2022 15:20
Operator : SY/MD
Sample : N3272-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026130.D
Acq On : 11 Jun 2022 15:20
Operator : SY/MD
Sample : N3272-05DL 400X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------