

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026131.D
 Acq On : 11 Jun 2022 15:44
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK253

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	77	87	103	rVB	84093	90743	16.02%	2.037%
2	1.581	161	168	179	rVB	93506	105401	18.60%	2.366%
3	2.121	326	336	352	rVB	163134	237078	41.84%	5.322%
4	2.523	452	461	472	rBV2	9453	16035	2.83%	0.360%
5	3.925	880	897	947	rBV2	48224	237682	41.95%	5.336%
6	4.362	1017	1033	1060	rBV	107037	271391	47.90%	6.093%
7	5.056	1233	1249	1272	rBV2	230599	566573	100.00%	12.719%
8	5.625	1414	1426	1449	rBV	178678	372634	65.77%	8.365%
9	5.921	1507	1518	1535	rVB8	8675	19932	3.52%	0.447%
10	6.076	1551	1566	1593	rBV	136157	285004	50.30%	6.398%
11	6.995	1842	1852	1871	rBV2	34718	69965	12.35%	1.571%
12	7.320	1941	1953	1973	rBV	238783	420096	74.15%	9.431%
13	7.632	2040	2050	2070	rBV2	20037	38032	6.71%	0.854%
14	8.092	2178	2193	2227	rBV	196994	418764	73.91%	9.401%
15	8.420	2285	2295	2308	rBV2	16414	27014	4.77%	0.606%
16	8.854	2419	2430	2448	rBV	273073	449690	79.37%	10.095%
17	10.217	2843	2854	2871	rBV	84454	133284	23.52%	2.992%
18	11.249	3164	3175	3197	rBV	234579	368142	64.98%	8.264%
19	11.622	3280	3291	3312	rBV	203294	327039	57.72%	7.342%




Sum of corrected areas: 4454499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026131.D
Acq On : 11 Jun 2022 15:44
Operator : SY/MD
Sample : VIBLK
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

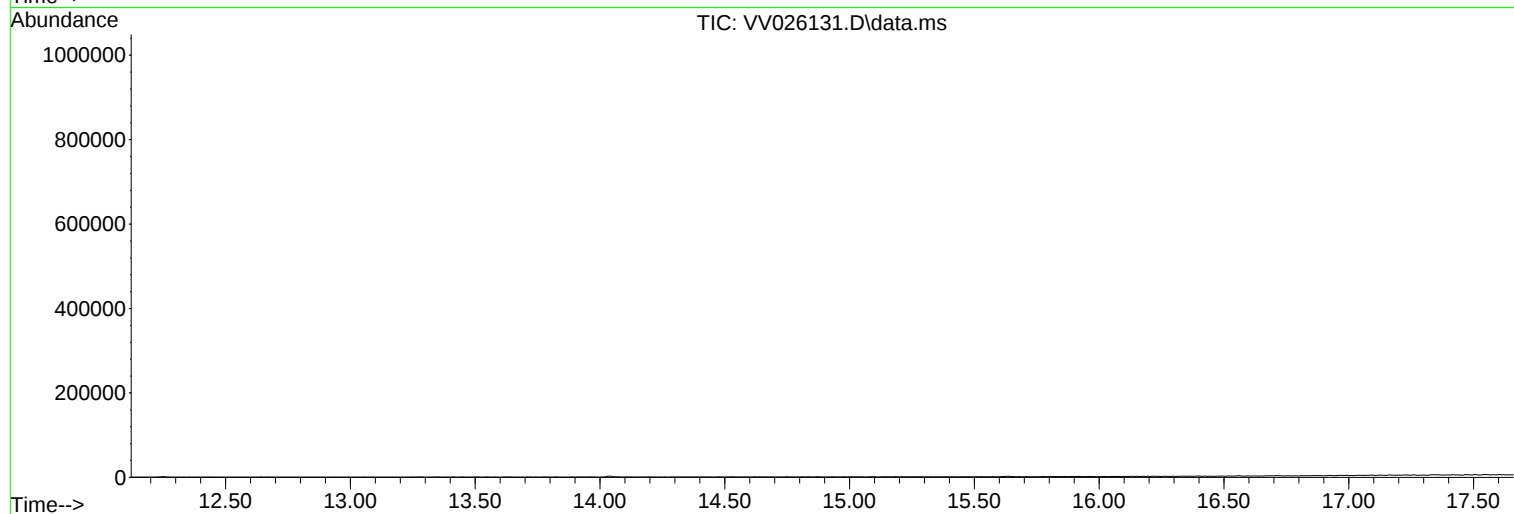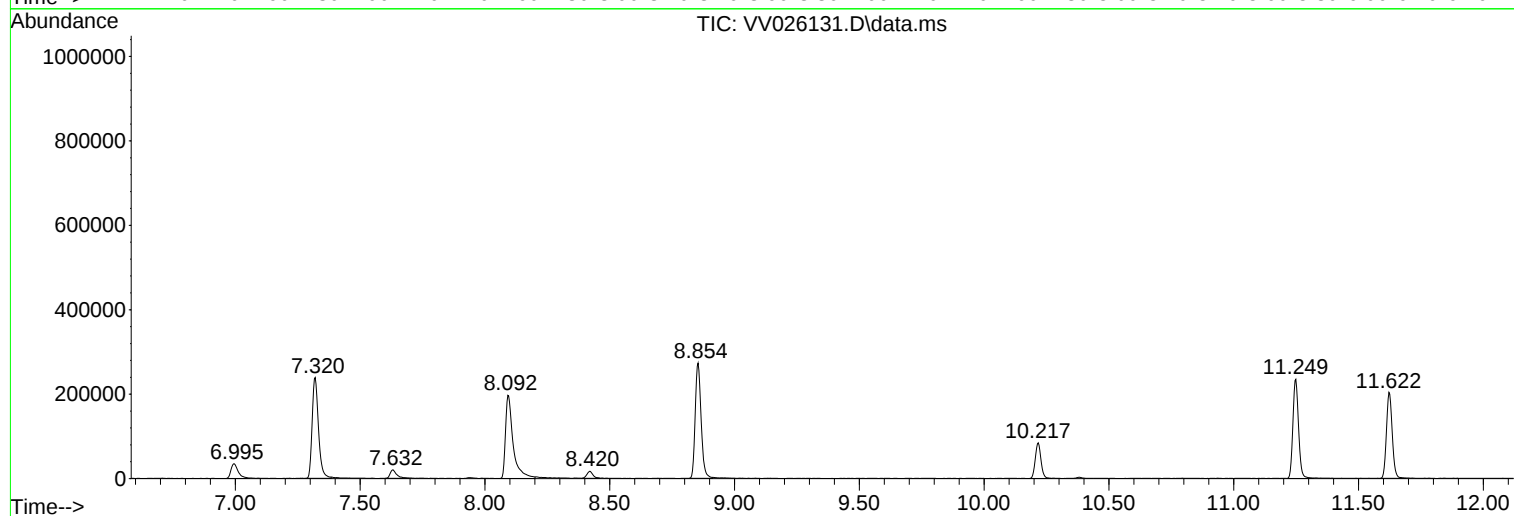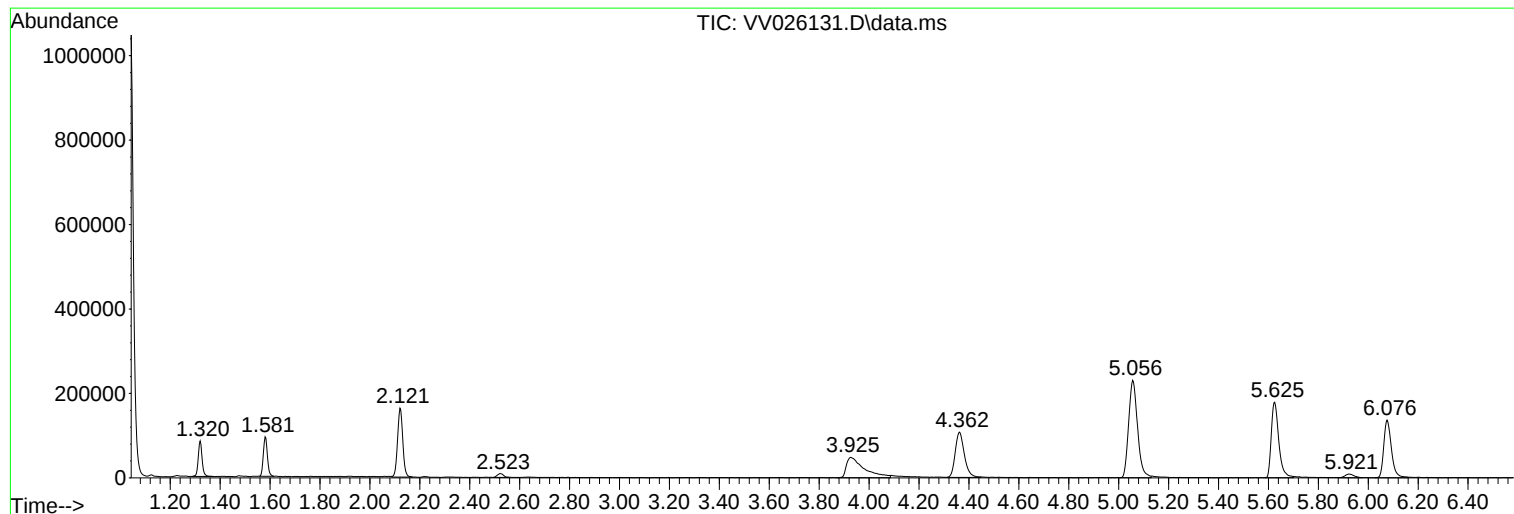

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026131.D
Acq On : 11 Jun 2022 15:44
Operator : SY/MD
Sample : VIBLK
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026131.D
Acq On : 11 Jun 2022 15:44
Operator : SY/MD
Sample : VIBLK
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK253

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc