

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061122\  
 Data File : VV026150.D  
 Acq On : 12 Jun 2022 00:14  
 Operator : SY/MD  
 Sample : N3312-17  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 38 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0E09

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.1 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026150.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.320       | 80            | 87          | 104          | rVB      | 73153          | 79599         | 14.56%          | 1.781%        |
| 2         | 1.580       | 160           | 168         | 178          | rBV      | 85981          | 98047         | 17.94%          | 2.194%        |
| 3         | 2.121       | 326           | 336         | 351          | rVB2     | 150757         | 234366        | 42.88%          | 5.244%        |
| 4         | 3.915       | 884           | 894         | 921          | rBV3     | 38536          | 136656        | 25.00%          | 3.058%        |
| 5         | 4.362       | 1016          | 1033        | 1059         | rBV2     | 106524         | 288428        | 52.77%          | 6.454%        |
| 6         | 5.056       | 1232          | 1249        | 1276         | rBV3     | 219601         | 546582        | 100.00%         | 12.231%       |
| 7         | 5.625       | 1414          | 1426        | 1449         | rBV      | 205964         | 423240        | 77.43%          | 9.471%        |
| 8         | 6.075       | 1553          | 1566        | 1588         | rBV      | 133208         | 275532        | 50.41%          | 6.166%        |
| 9         | 6.992       | 1842          | 1851        | 1874         | rBV      | 41682          | 81521         | 14.91%          | 1.824%        |
| 10        | 7.320       | 1939          | 1953        | 1975         | rBV      | 219250         | 397583        | 72.74%          | 8.897%        |
| 11        | 7.628       | 2040          | 2049        | 2064         | rBV      | 22613          | 41269         | 7.55%           | 0.923%        |
| 12        | 8.091       | 2181          | 2193        | 2238         | rBV2     | 180472         | 456556        | 83.53%          | 10.216%       |
| 13        | 8.854       | 2419          | 2430        | 2454         | rBV      | 316834         | 519786        | 95.10%          | 11.631%       |
| 14        | 10.217      | 2840          | 2854        | 2876         | rBV      | 86374          | 141777        | 25.94%          | 3.173%        |
| 15        | 11.249      | 3164          | 3175        | 3194         | rBV      | 271613         | 419138        | 76.68%          | 9.379%        |
| 16        | 11.622      | 3277          | 3291        | 3313         | rBV      | 206741         | 328840        | 60.16%          | 7.358%        |




Sum of corrected areas: 4468920

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061122\  
Data File : VV026150.D  
Acq On : 12 Jun 2022 00:14  
Operator : SY/MD  
Sample : N3312-17  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0E09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

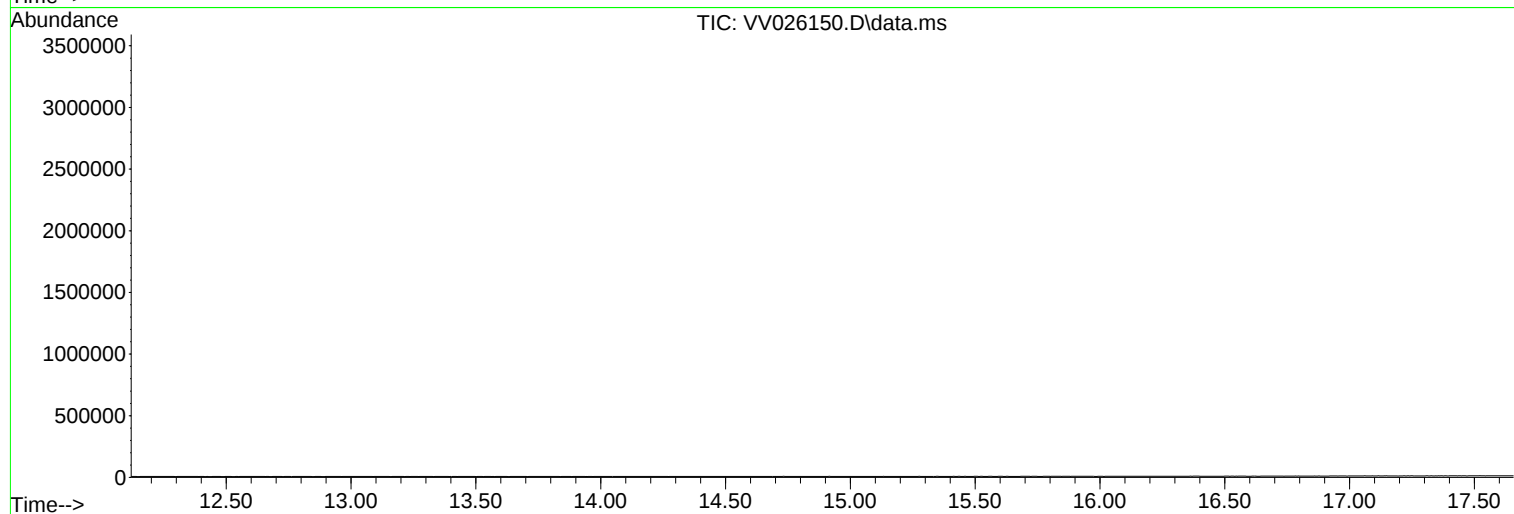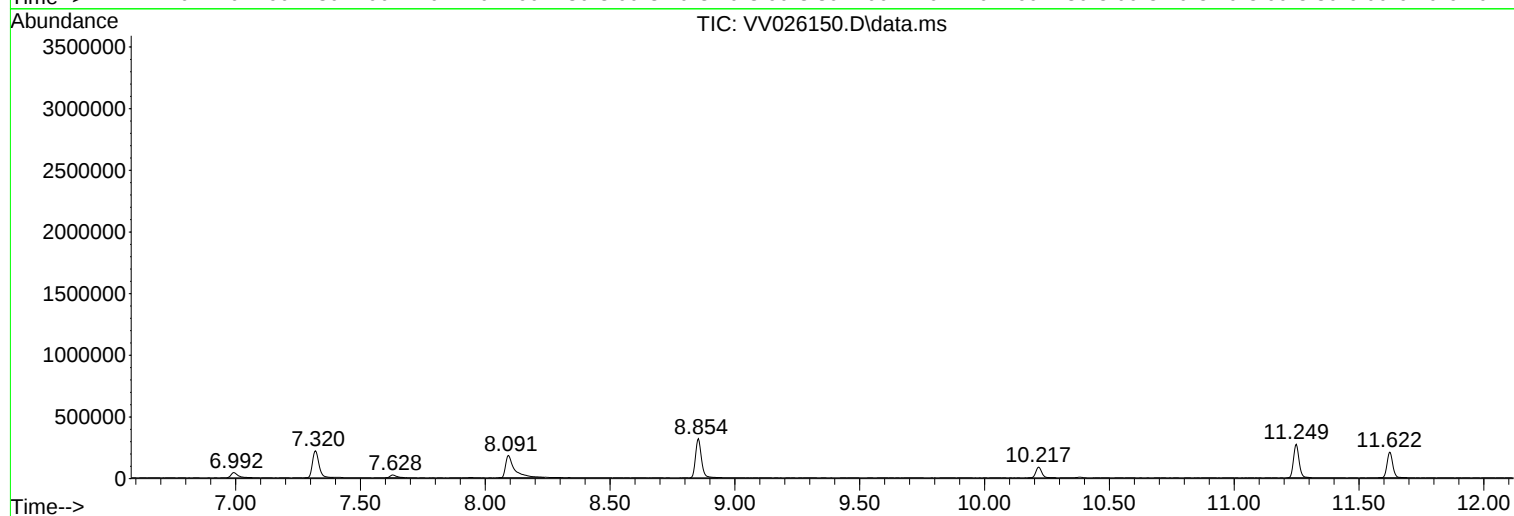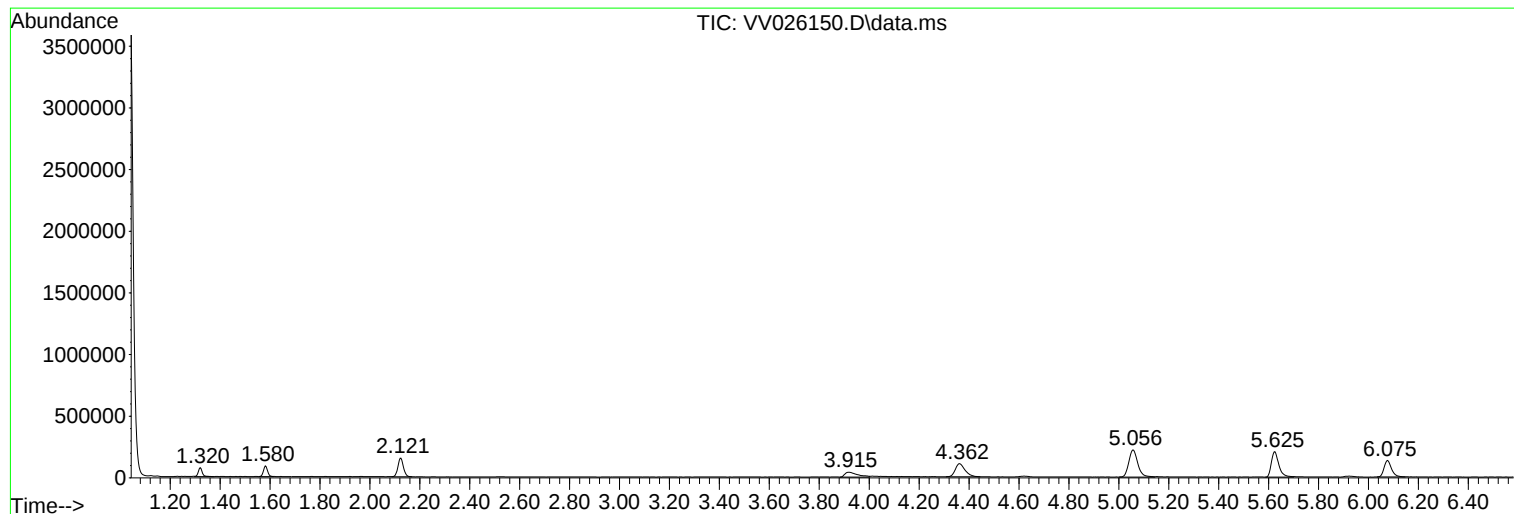

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061122\  
Data File : VV026150.D  
Acq On : 12 Jun 2022 00:14  
Operator : SY/MD  
Sample : N3312-17  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0E09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV061122\  
Data File : VV026150.D  
Acq On : 12 Jun 2022 00:14  
Operator : SY/MD  
Sample : N3312-17  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0E09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060822WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |