

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026158.D
 Acq On : 12 Jun 2022 03:24
 Operator : SY/MD
 Sample : N3273-09 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B79

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026158.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	96	rBV	69230	73958	13.87%	1.670%
2	1.580	160	168	183	rVB	83860	98578	18.49%	2.225%
3	2.121	325	336	350	rVB	140927	205126	38.47%	4.631%
4	2.519	452	460	471	rVB4	5150	9168	1.72%	0.207%
5	3.931	884	899	942	rBV3	36958	196562	36.86%	4.438%
6	4.362	1016	1033	1060	rVB	101620	255311	47.88%	5.764%
7	5.056	1234	1249	1274	rBV2	212957	533278	100.00%	12.039%
8	5.625	1414	1426	1454	rBV	210973	438232	82.18%	9.893%
9	5.928	1507	1520	1534	rVB7	11637	27104	5.08%	0.612%
10	6.075	1553	1566	1590	rBV2	126868	268877	50.42%	6.070%
11	6.992	1841	1851	1874	rBV2	37044	73158	13.72%	1.652%
12	7.320	1936	1953	1978	rBV	218095	393526	73.79%	8.884%
13	7.628	2040	2049	2079	rBV3	18817	40311	7.56%	0.910%
14	7.979	2146	2158	2169	rBV2	25107	41862	7.85%	0.945%
15	8.095	2182	2194	2229	rBV2	172530	394689	74.01%	8.910%
16	8.853	2418	2430	2450	rBV	315125	523541	98.17%	11.819%
17	10.217	2842	2854	2873	rBV	78107	123648	23.19%	2.791%
18	11.249	3161	3175	3196	rBV	271639	419771	78.72%	9.477%
19	11.622	3277	3291	3311	rBV	198912	312856	58.67%	7.063%




Sum of corrected areas: 4429556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026158.D
Acq On : 12 Jun 2022 03:24
Operator : SY/MD
Sample : N3273-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

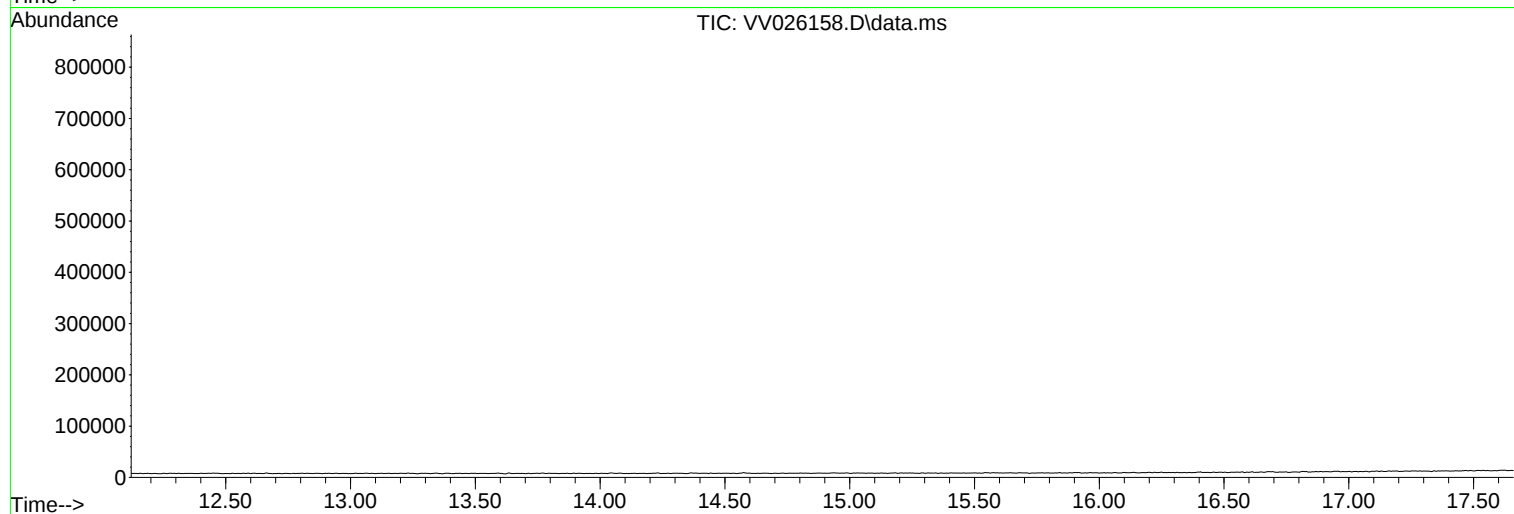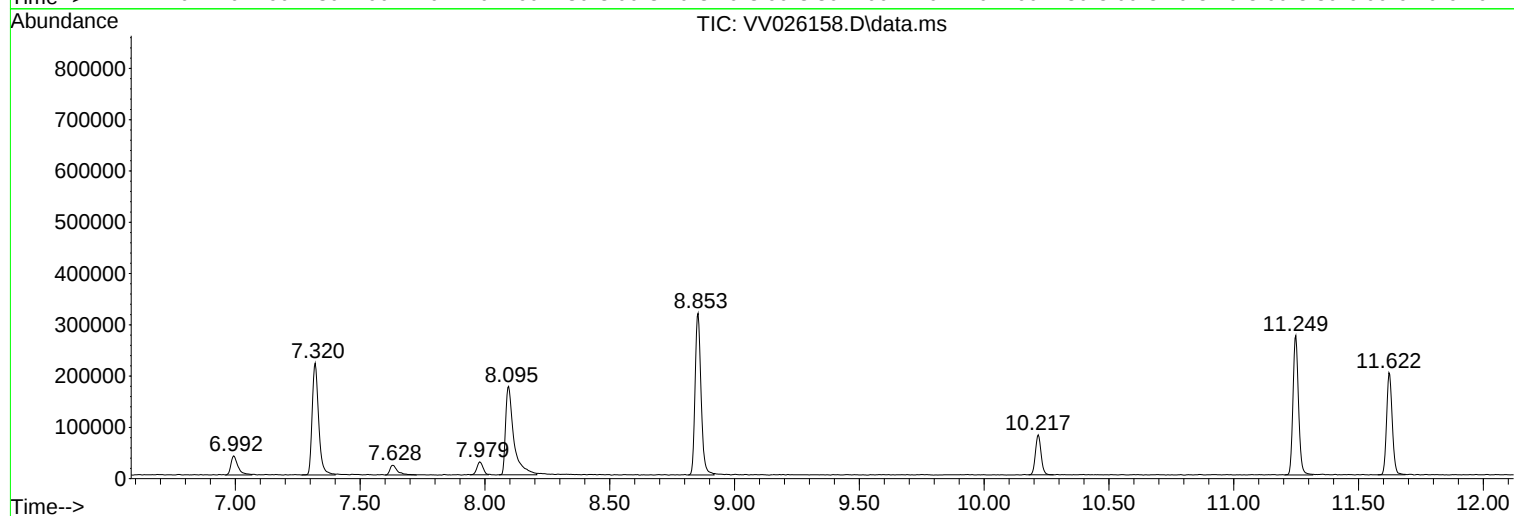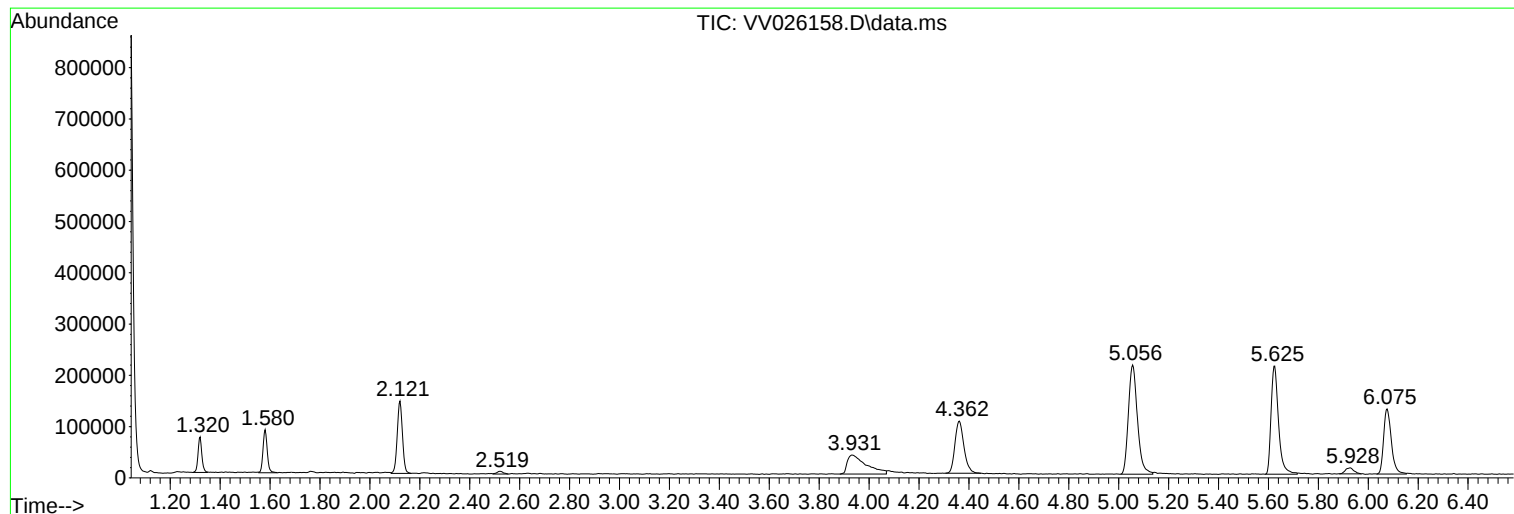

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026158.D
Acq On : 12 Jun 2022 03:24
Operator : SY/MD
Sample : N3273-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026158.D
Acq On : 12 Jun 2022 03:24
Operator : SY/MD
Sample : N3273-09 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
