

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026159.D
 Acq On : 12 Jun 2022 03:48
 Operator : SY/MD
 Sample : N3273-10 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B80

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	96	rVB	67401	69045	13.20%	1.619%
2	1.581	160	168	181	rVB	82495	93978	17.97%	2.204%
3	2.121	326	336	350	rVB	138041	200535	38.34%	4.702%
4	2.523	447	461	469	rBV4	5057	9525	1.82%	0.223%
5	3.915	880	894	926	rBV2	39989	149798	28.64%	3.512%
6	4.359	1018	1032	1057	rVB	100852	251894	48.16%	5.906%
7	5.056	1233	1249	1273	rBV2	209157	522998	100.00%	12.263%
8	5.622	1410	1425	1450	rBV	201122	417579	79.84%	9.791%
9	5.918	1507	1517	1535	rVB7	7929	18165	3.47%	0.426%
10	6.076	1553	1566	1594	rBV	128792	267035	51.06%	6.261%
11	6.992	1837	1851	1877	rBV2	35395	72747	13.91%	1.706%
12	7.320	1939	1953	1976	rBV	219691	387360	74.07%	9.083%
13	7.629	2041	2049	2068	rBV3	18980	37584	7.19%	0.881%
14	7.979	2149	2158	2170	rVB3	18699	30736	5.88%	0.721%
15	8.092	2178	2193	2233	rBV3	151911	386286	73.86%	9.057%
16	8.854	2415	2430	2461	rBV	306946	510635	97.64%	11.973%
17	10.217	2843	2854	2870	rBV	74699	123816	23.67%	2.903%
18	11.249	3164	3175	3192	rBV	256697	401950	76.85%	9.425%
19	11.622	3281	3291	3316	rVB	197895	313211	59.89%	7.344%




Sum of corrected areas: 4264877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026159.D
Acq On : 12 Jun 2022 03:48
Operator : SY/MD
Sample : N3273-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

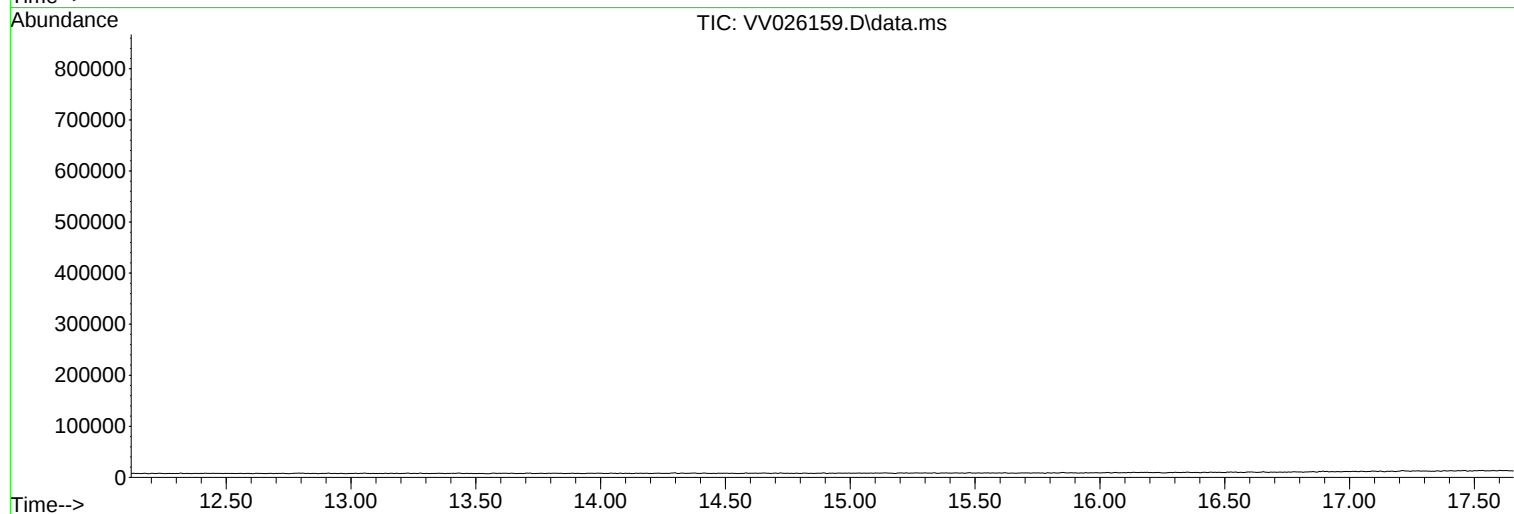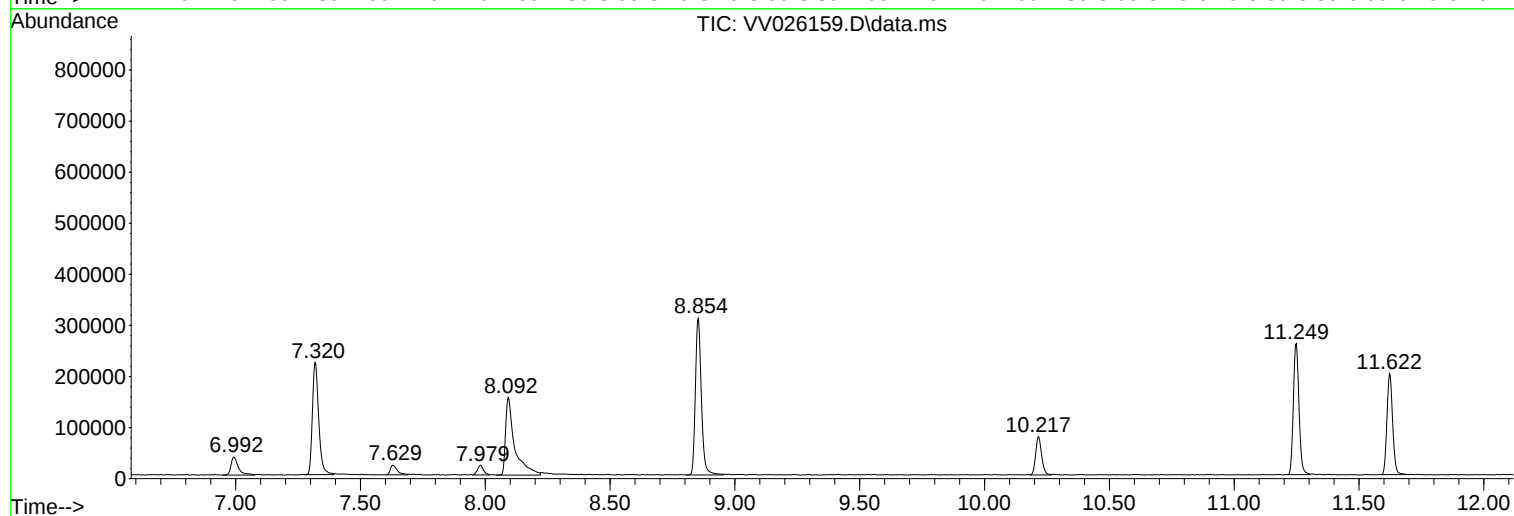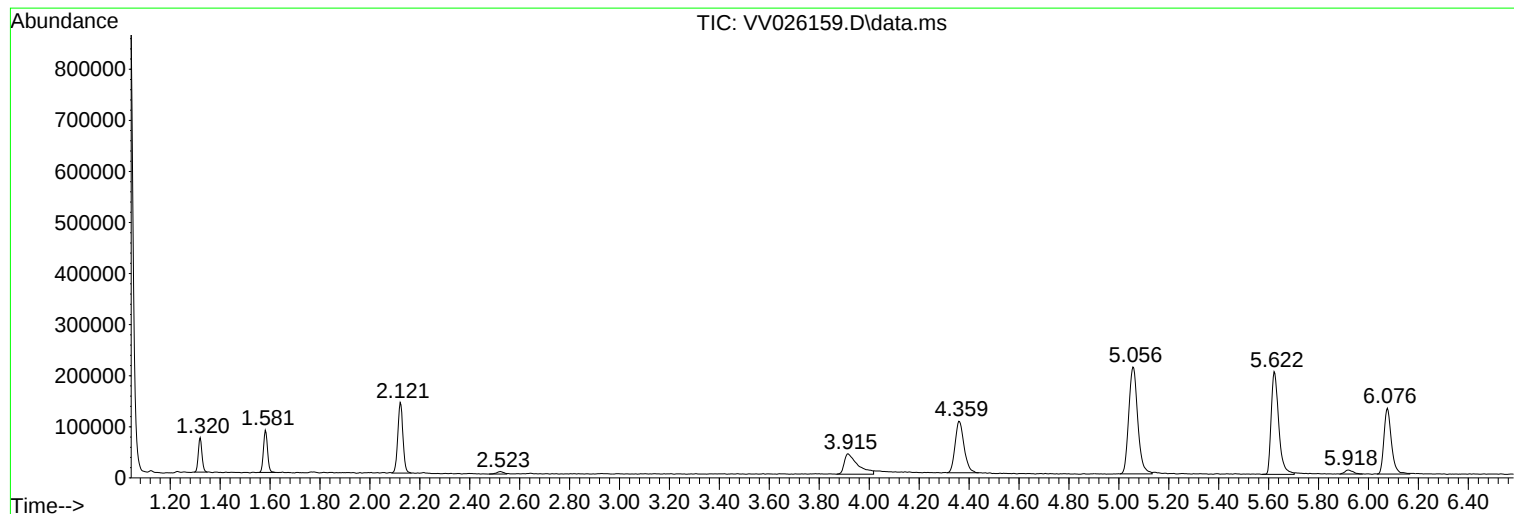

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026159.D
Acq On : 12 Jun 2022 03:48
Operator : SY/MD
Sample : N3273-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026159.D
Acq On : 12 Jun 2022 03:48
Operator : SY/MD
Sample : N3273-10 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc