

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026164.D
 Acq On : 12 Jun 2022 05:47
 Operator : SY/MD
 Sample : N3273-15 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	101	rVB	68430	71290	13.35%	1.661%
2	1.581	161	168	177	rBV	81360	92765	17.37%	2.161%
3	2.121	326	336	352	rVB	137995	201933	37.81%	4.704%
4	2.526	453	462	469	rBV5	4971	8920	1.67%	0.208%
5	3.915	879	894	926	rBV2	37367	148715	27.85%	3.464%
6	4.362	1018	1033	1054	rBV	101727	257359	48.19%	5.995%
7	5.056	1233	1249	1277	rBV2	215233	534048	100.00%	12.440%
8	5.626	1413	1426	1458	rBV	194133	408916	76.57%	9.525%
9	5.921	1508	1518	1531	rBV7	7983	20289	3.80%	0.473%
10	6.076	1551	1566	1589	rBV	130465	274951	51.48%	6.405%
11	6.992	1839	1851	1878	rBV2	35749	74106	13.88%	1.726%
12	7.320	1942	1953	1971	rBV	221110	389973	73.02%	9.084%
13	7.629	2038	2049	2062	rBV3	20433	38698	7.25%	0.901%
14	7.979	2146	2158	2172	rVB2	28802	50853	9.52%	1.185%
15	8.092	2182	2193	2234	rBV	159984	402355	75.34%	9.372%
16	8.854	2417	2430	2455	rBV	295638	492152	92.16%	11.464%
17	10.217	2843	2854	2867	rBV	77010	122297	22.90%	2.849%
18	11.249	3161	3175	3195	rBV	244942	389268	72.89%	9.068%
19	11.622	3280	3291	3310	rBV	198283	314059	58.81%	7.316%




Sum of corrected areas: 4292947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026164.D
Acq On : 12 Jun 2022 05:47
Operator : SY/MD
Sample : N3273-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

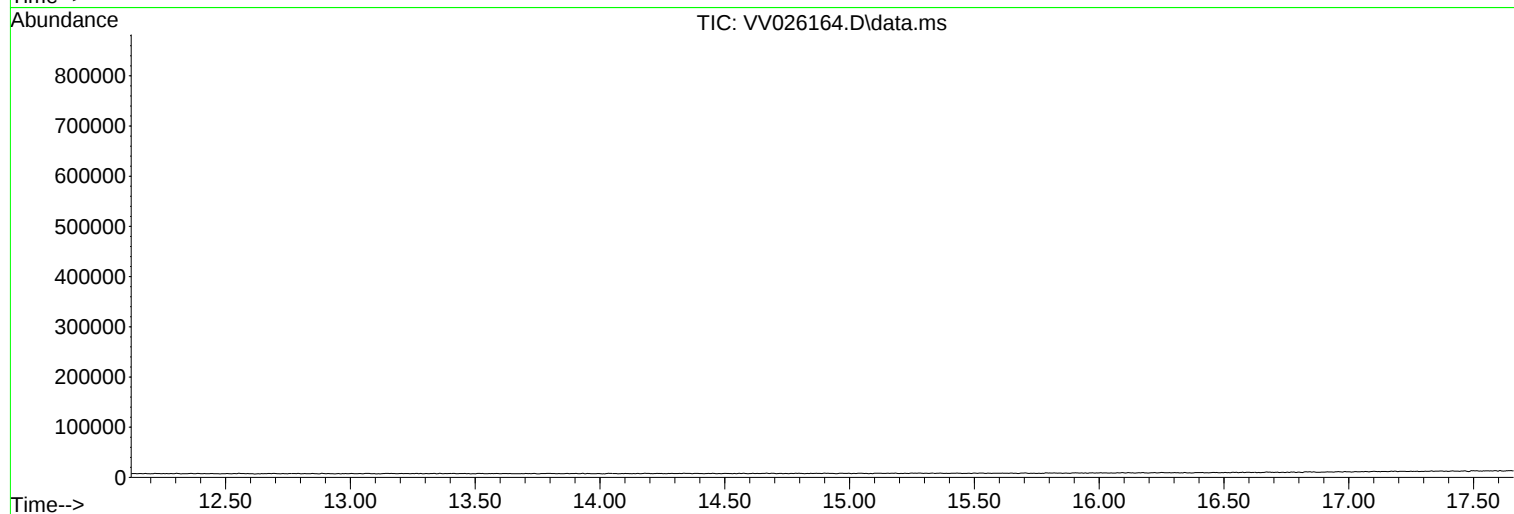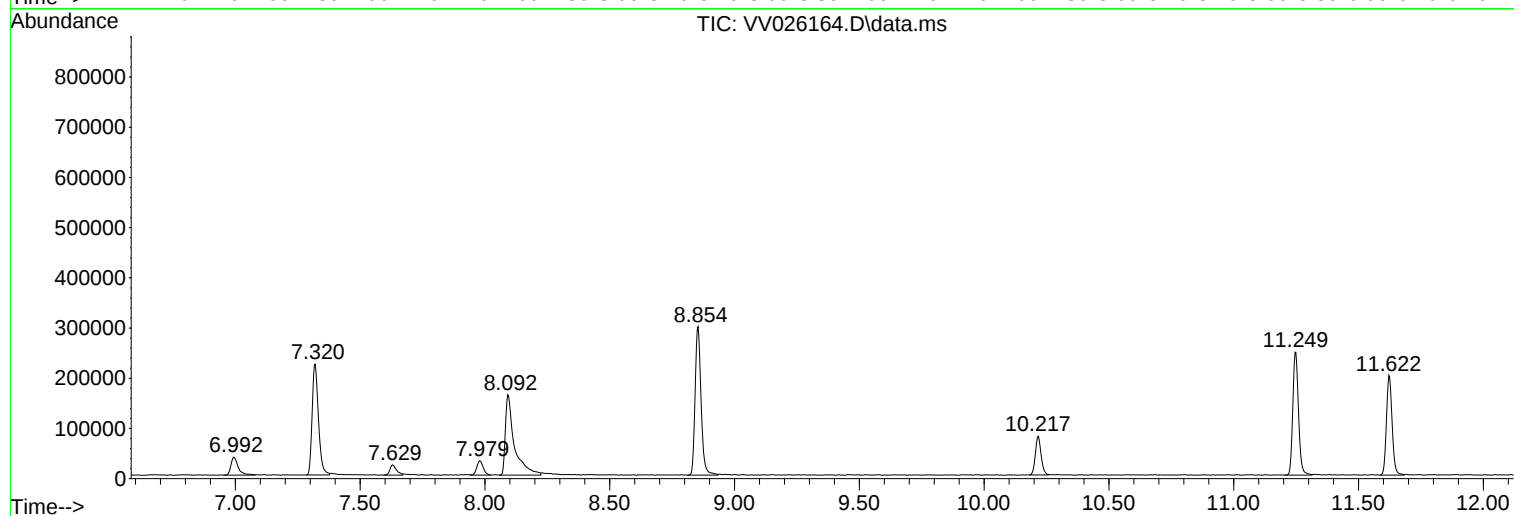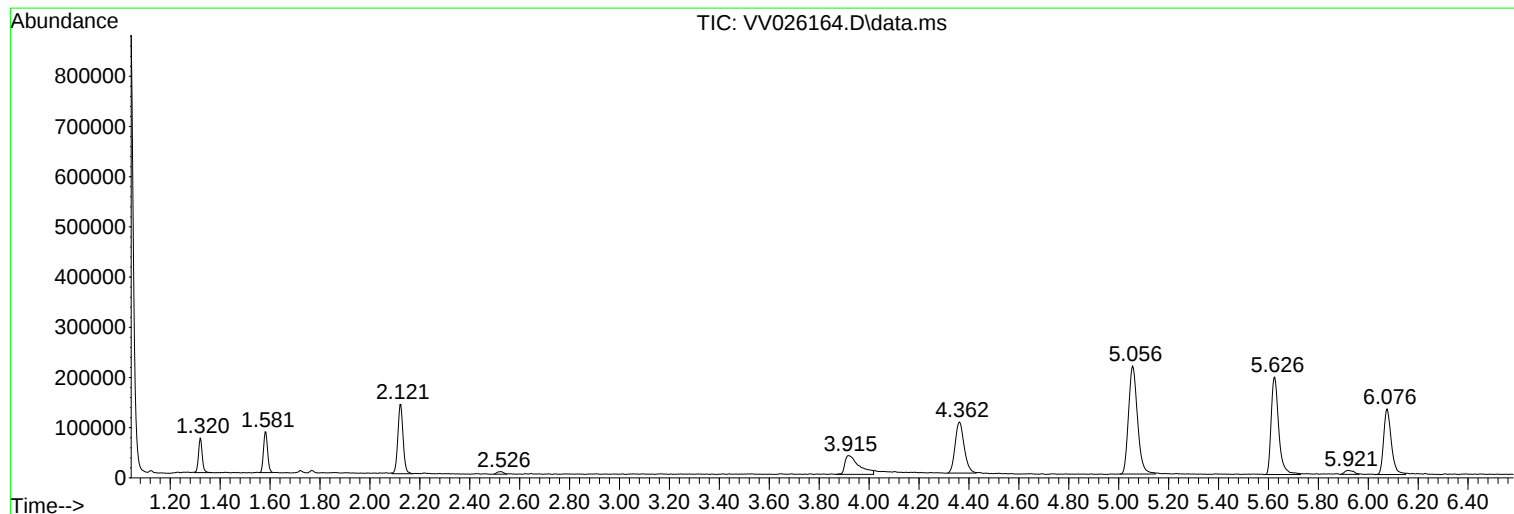

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026164.D
Acq On : 12 Jun 2022 05:47
Operator : SY/MD
Sample : N3273-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
Data File : VV026164.D
Acq On : 12 Jun 2022 05:47
Operator : SY/MD
Sample : N3273-15 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc