


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061122\
 Data File : VV026116.D
 Acq On : 11 Jun 2022 08:59
 Operator : SY/MD
 Sample : BFB325
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB325

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 13 07:40:59 2022

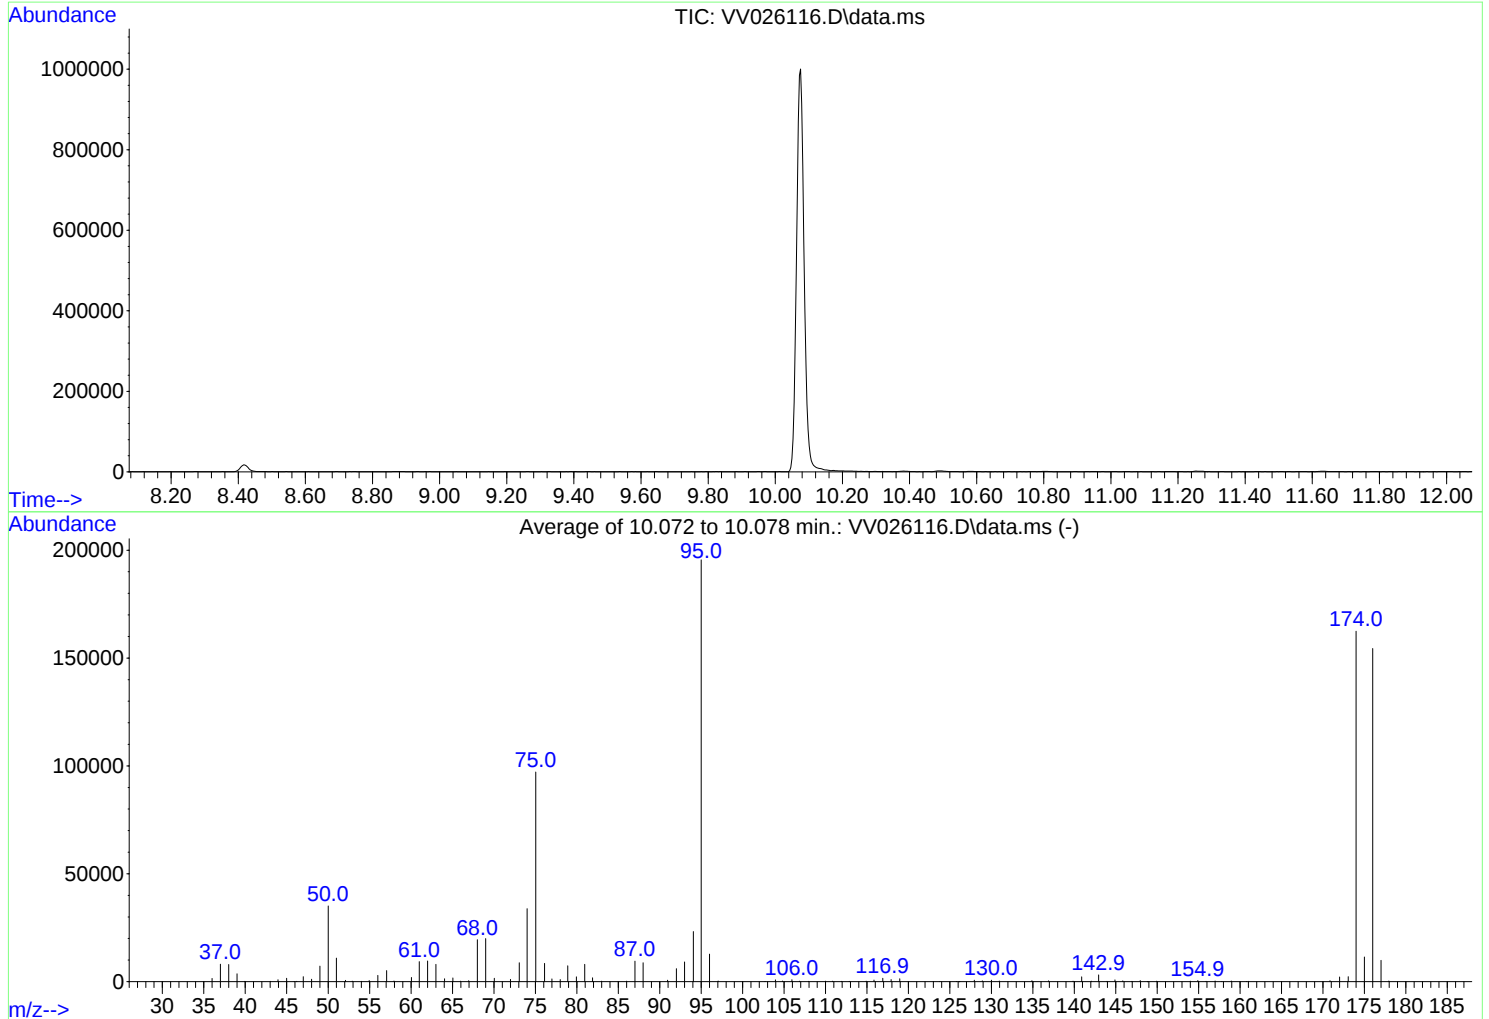

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	35072	PASS
75	95	30	80	49.7	97147	PASS
95	95	100	100	100.0	195541	PASS
96	95	5	9	6.5	12760	PASS
173	174	0.00	2	1.4	2312	PASS
174	95	50	120	83.1	162411	PASS
175	174	5	9	7.0	11397	PASS
176	174	95	105	95.1	154411	PASS
177	176	5	10	6.4	9881	PASS

Scan 2796 (10.030 min): VV026116.D\data.ms
BFB325

m/z	Abundance
39.90	264.0
44.00	316.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

m/z	Abundance
36.00	1519.0
37.00	8454.0
38.00	8512.0
39.00	3663.0
40.00	460.0
43.00	177.0
43.90	1182.0
45.00	1678.0
45.90	158.0
47.00	2342.0
48.00	1155.0
49.00	7639.0
50.00	35800.0
51.00	11667.0
52.10	659.0
52.90	191.0
54.10	138.0
55.00	602.0
56.00	2919.0
57.00	5424.0
57.90	293.0
60.00	2074.0
61.00	9854.0
62.00	10042.0
63.00	8438.0
64.00	1415.0
65.10	1908.0
66.00	198.0
66.90	454.0
68.00	20016.0
69.00	20208.0
70.00	1600.0
72.00	1142.0
73.00	9007.0
74.00	34072.0
75.00	99800.0
76.10	9037.0
77.00	1310.0
78.00	1004.0
78.90	7672.0
79.90	2140.0
81.00	8422.0
81.90	1795.0
83.00	275.0
86.10	273.0
87.00	9824.0
88.00	8801.0
90.90	727.0
92.00	6243.0
93.00	9402.0
94.00	23704.0
95.00	200128.0
96.00	13337.0
97.00	354.0
102.70	108.0
104.00	862.0
104.80	249.0
105.90	982.0
106.80	201.0
107.90	195.0
110.00	207.0
110.80	220.0
111.90	173.0
112.90	185.0
114.90	201.0
115.90	730.0
116.90	1634.0
117.90	972.0
119.00	1358.0
123.80	132.0
125.80	134.0
128.00	686.0
128.90	341.0
130.10	604.0
130.90	282.0
134.90	433.0
136.90	365.0
139.80	138.0
140.90	2273.0
142.10	218.0
142.90	3115.0
143.90	167.0
144.90	937.0
145.90	382.0
146.90	182.0
147.90	449.0
148.80	113.0
150.00	253.0
154.10	197.0
154.90	503.0
155.90	150.0
157.00	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

157.80	135.0
158.90	255.0
160.80	232.0
170.80	482.0
172.00	2044.0
173.10	2396.0
174.00	162496.0
175.00	11799.0
176.00	154304.0
177.00	10129.0
178.00	321.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

m/z	Abundance
36.00	1549.0
37.00	8328.0
38.00	8249.0
39.00	3774.0
40.00	461.0
43.00	171.0
44.00	1227.0
45.00	1625.0
45.90	174.0
46.20	172.0
47.00	2402.0
48.00	1143.0
49.00	7453.0
50.00	36464.0
51.00	11266.0
52.10	627.0
52.90	237.0
54.10	163.0
55.00	541.0
56.00	2983.0
57.10	5220.0
57.90	295.0
60.00	1981.0
61.00	9624.0
62.00	9854.0
63.00	8384.0
64.00	1342.0
65.10	1758.0
66.00	210.0
67.00	483.0
68.00	20120.0
69.00	20720.0
70.10	1665.0
72.00	1073.0
73.10	9047.0
74.00	35128.0
75.10	100328.0
76.10	8737.0
77.00	1275.0
78.00	1016.0
78.90	7591.0
79.90	2325.0
81.00	8281.0
81.90	1835.0
83.00	291.0
86.00	279.0
87.00	9855.0
88.00	9072.0
90.90	674.0
92.00	6224.0
93.00	9427.0
94.00	23976.0
95.00	202368.0
96.00	13200.0
97.00	326.0
102.70	110.0
103.90	867.0
104.80	300.0
105.90	944.0
106.80	250.0
108.00	158.0
110.00	225.0
110.80	239.0
111.90	180.0
112.80	169.0
114.90	232.0
115.80	760.0
116.90	1549.0
117.90	1019.0
118.90	1437.0
123.00	108.0
123.80	130.0
128.00	693.0
128.90	407.0
130.00	704.0
131.00	309.0
134.90	436.0
136.90	371.0
139.80	196.0
140.90	2283.0
142.10	273.0
143.00	3264.0
144.00	173.0
144.90	865.0
145.90	370.0
146.90	177.0
147.90	522.0
150.00	226.0
154.00	207.0
154.90	565.0
155.90	143.0
157.00	337.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

157.80	117.0
158.90	324.0
161.00	265.0
170.80	467.0
172.00	2217.0
173.10	2355.0
174.00	168192.0
175.00	11721.0
176.00	159872.0
177.00	10179.0
178.00	358.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

m/z	Abundance
36.00	1375.0
37.00	7453.0
38.00	6961.0
39.00	3428.0
40.00	407.0
43.10	150.0
44.00	1219.0
45.00	1406.0
46.20	256.0
47.00	2207.0
48.00	1009.0
49.00	6612.0
50.00	32952.0
51.00	9892.0
52.10	504.0
52.90	265.0
54.00	142.0
54.90	441.0
56.00	2784.0
57.10	4655.0
58.00	211.0
60.10	1692.0
61.00	8422.0
62.00	8900.0
63.00	7147.0
64.10	1234.0
65.00	1558.0
65.90	194.0
66.90	479.0
68.00	18240.0
69.00	18944.0
70.10	1504.0
72.00	993.0
73.00	8301.0
74.00	32296.0
75.10	91312.0
76.10	7642.0
77.00	1148.0
78.00	890.0
78.90	6818.0
80.00	2211.0
80.90	7326.0
81.90	1696.0
83.00	215.0
85.90	237.0
87.00	8843.0
88.00	8438.0
91.00	598.0
92.00	5631.0
93.00	8514.0
94.10	22008.0
95.00	184128.0
96.00	11743.0
97.10	320.0
102.70	105.0
103.90	776.0
104.80	317.0
106.00	825.0
106.90	270.0
108.00	120.0
110.00	179.0
110.90	218.0
111.90	158.0
112.80	149.0
114.90	214.0
115.90	717.0
116.90	1444.0
117.90	896.0
119.00	1297.0
123.00	105.0
126.10	104.0
127.90	676.0
128.90	421.0
129.90	807.0
131.00	300.0
134.90	392.0
136.90	404.0
139.90	255.0
140.90	2079.0
142.00	265.0
143.00	2997.0
144.00	131.0
144.90	719.0
145.80	346.0
147.00	144.0
148.00	526.0
149.90	160.0
153.90	192.0
154.90	527.0
155.90	110.0
157.00	327.0
159.00	338.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325

161.00	267.0
170.90	415.0
172.00	2117.0
173.00	2185.0
174.00	156544.0
175.00	10670.0
176.00	149056.0
177.00	9334.0
177.90	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB325