
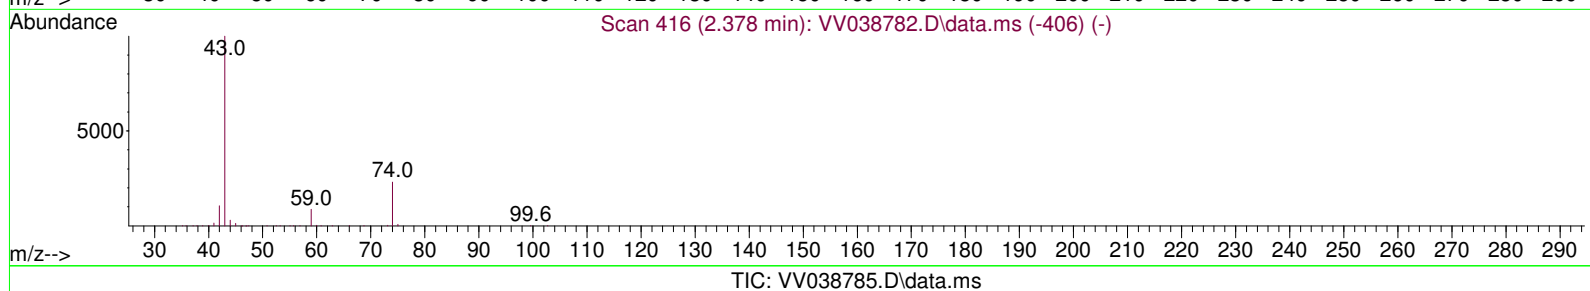
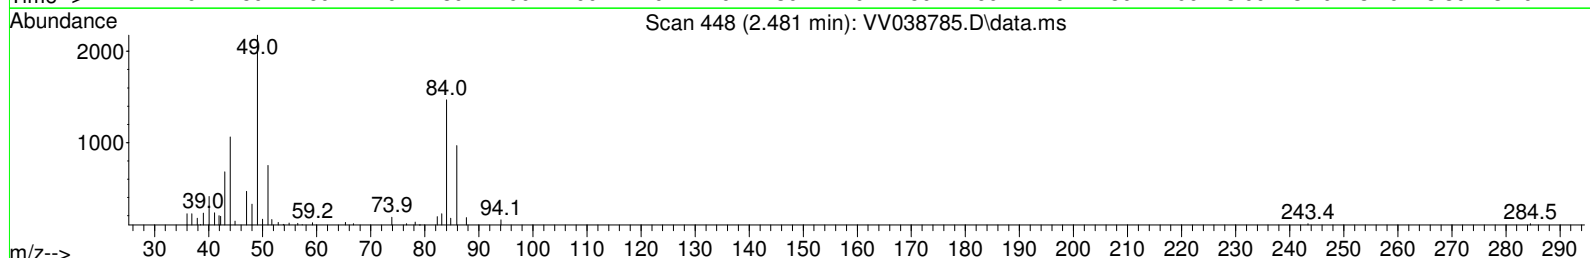


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

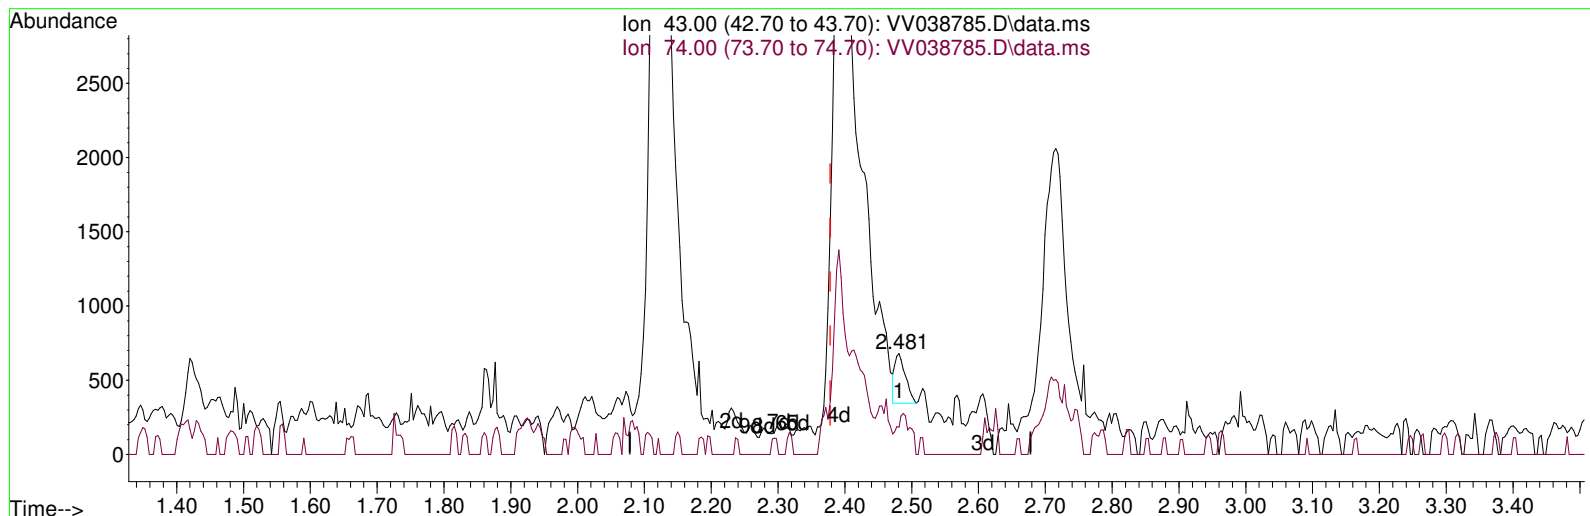

(15) Methyl Acetate (T)




2.481min (+ 0.103) 0.06 ug/L

response 372

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	26.88
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

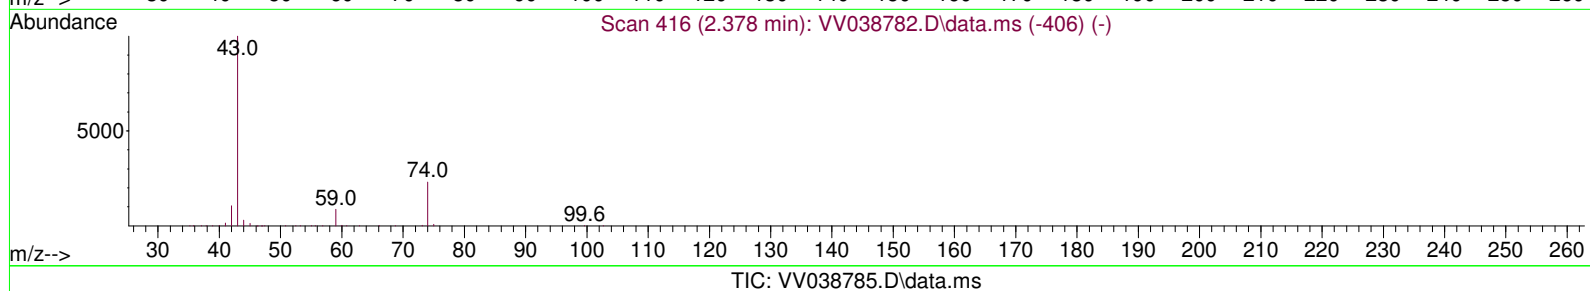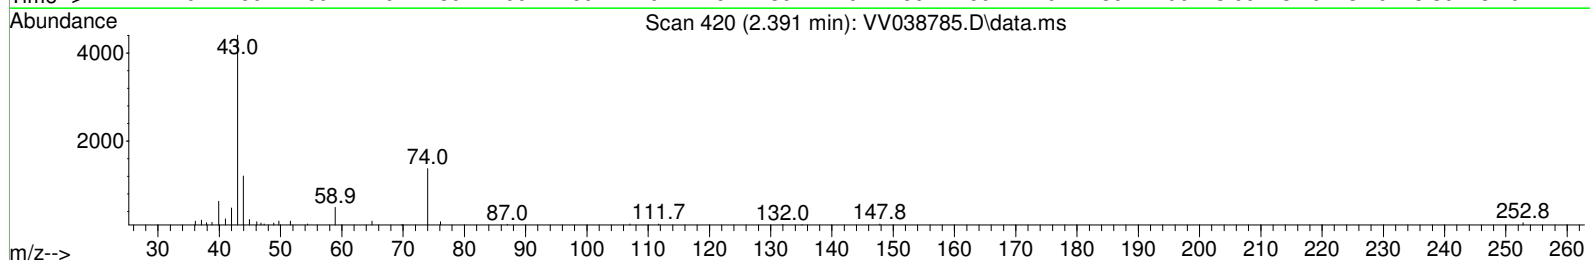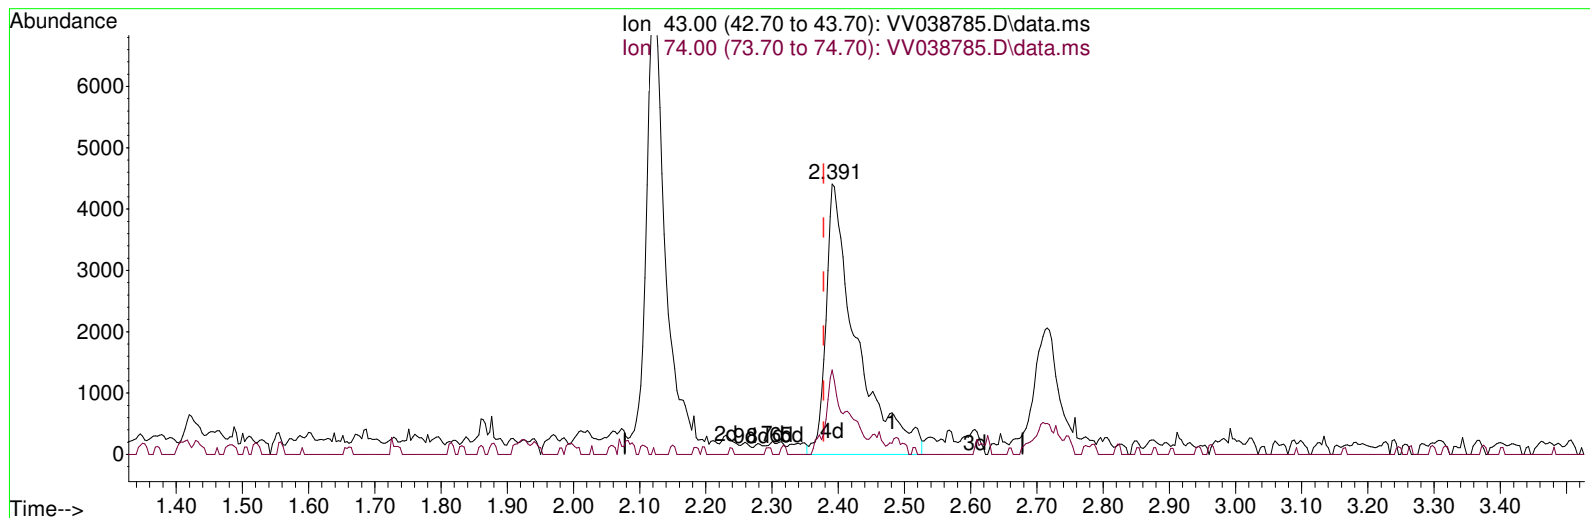

(15) Methyl Acetate (T)




2.391min (+ 0.013) 2.29 ug/L m

response 14021

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	0.71#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

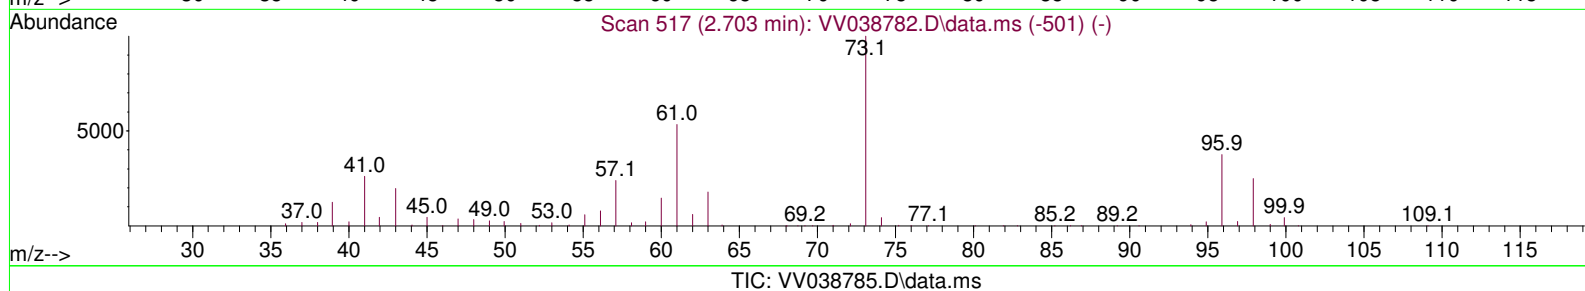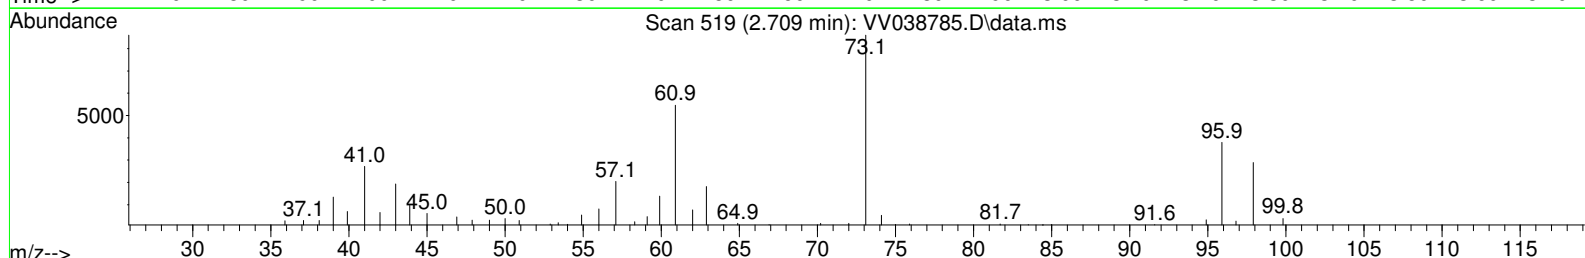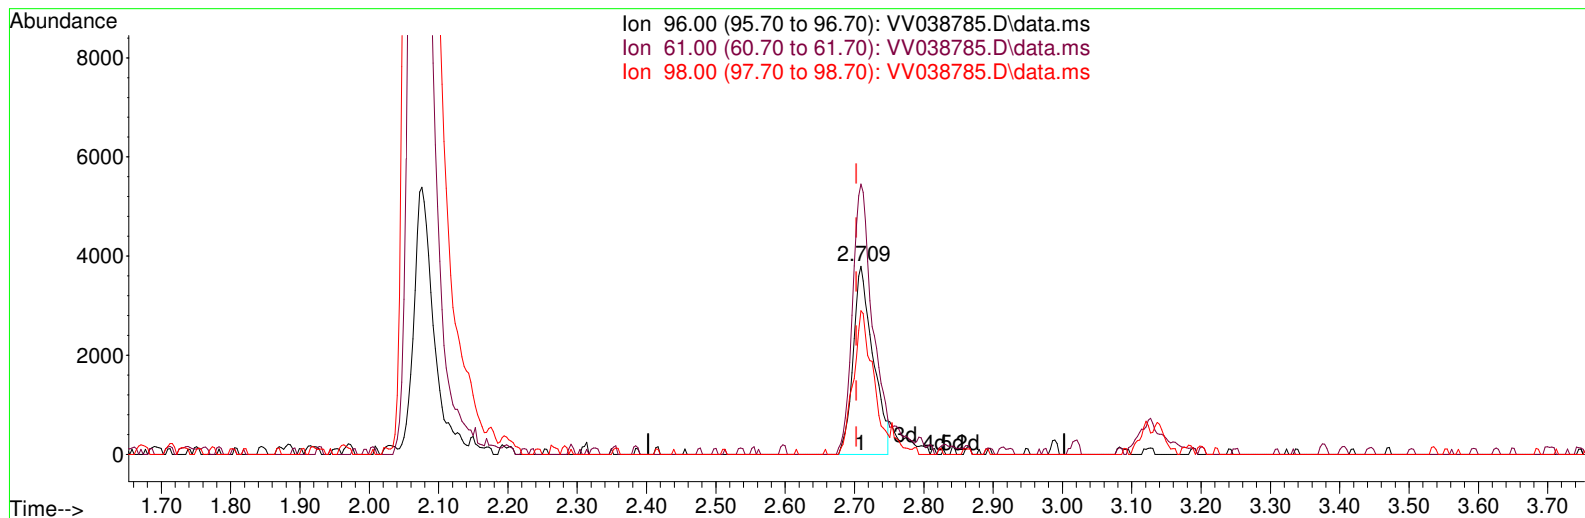

(17) trans-1,2-Dichloroethene (T)




2.709min (+ 0.006) 1.64 ug/L

response 7506

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	136.70	143.69
98.00	66.30	76.36
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

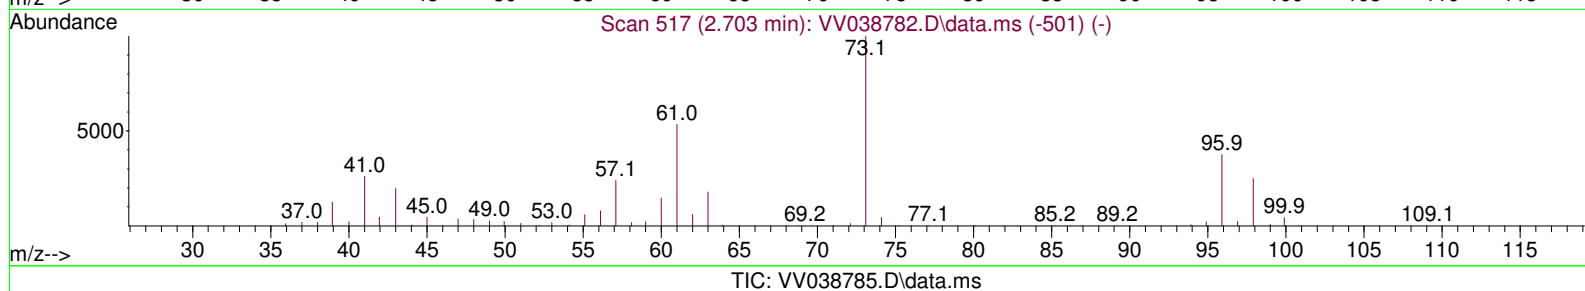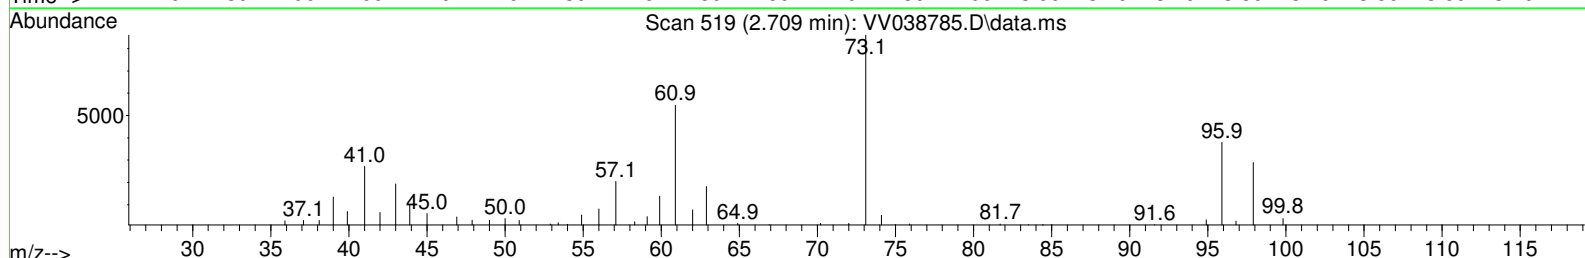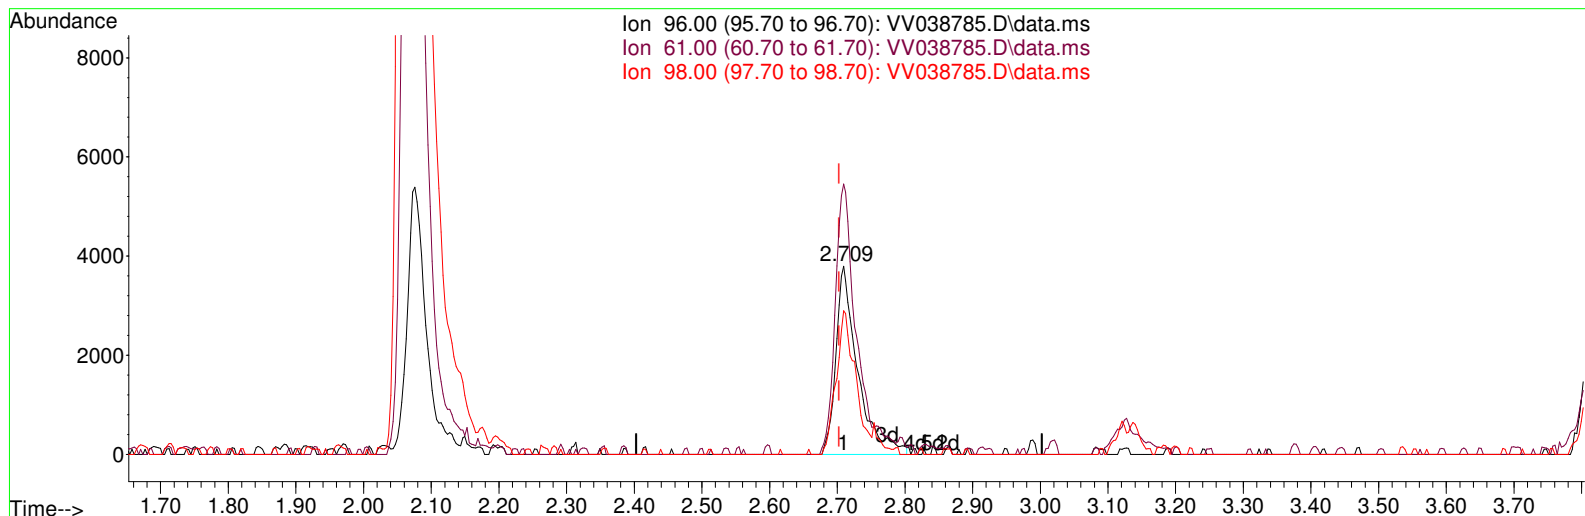

(17) trans-1,2-Dichloroethene (T)




2.709min (+ 0.006) 1.86 ug/L m

response 8497

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	136.70	143.69
98.00	66.30	76.36
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

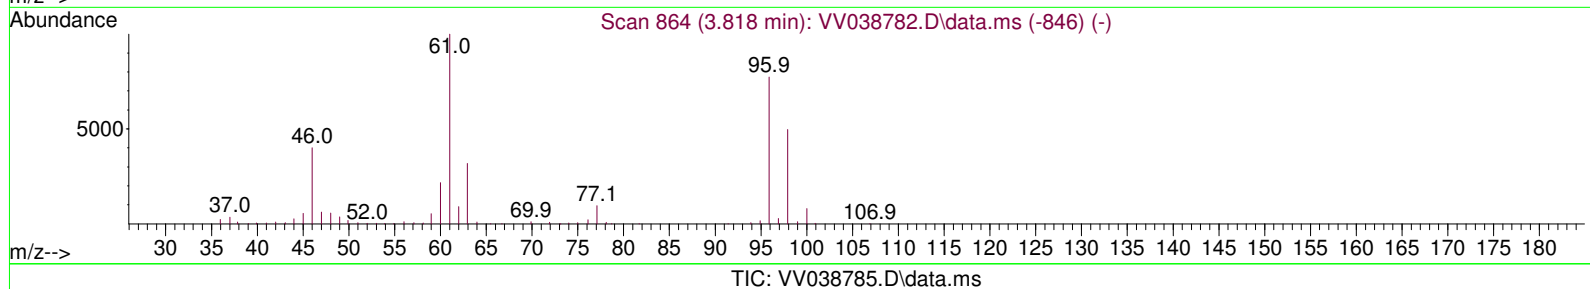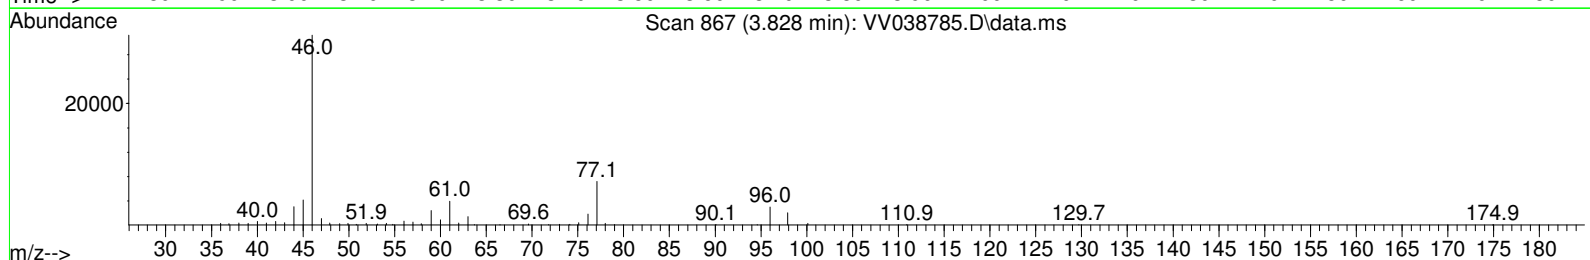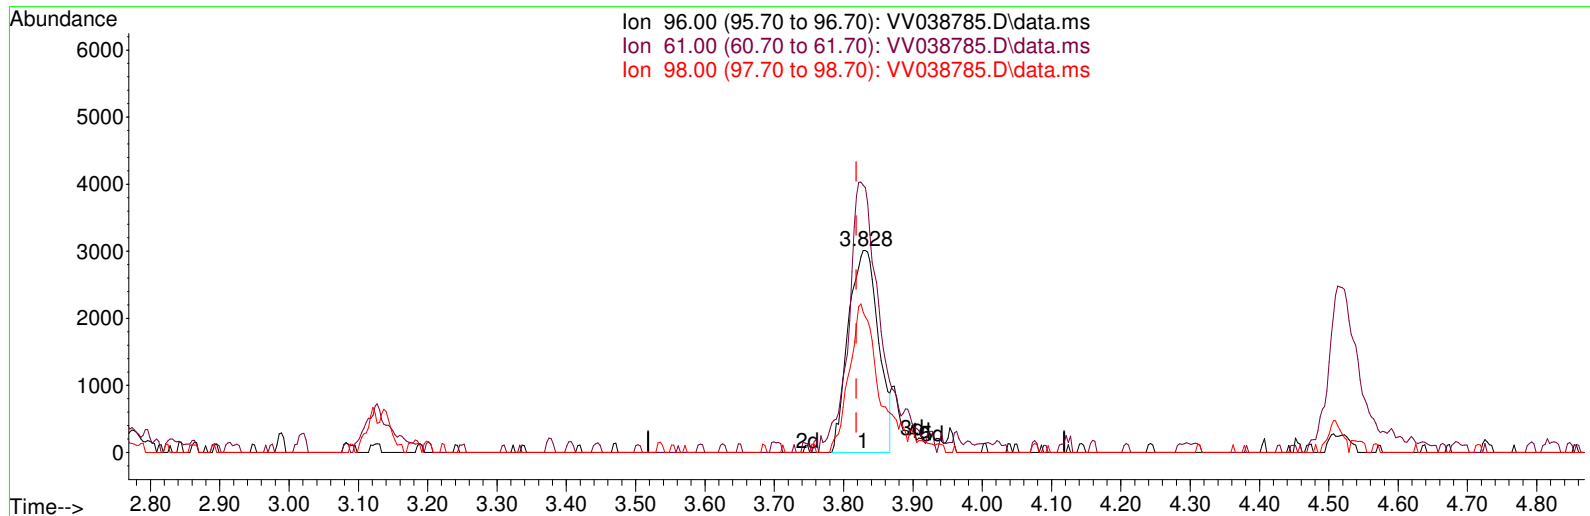

(20) cis-1,2-Dichloroethene (T)




3.828min (+ 0.010) 1.85 ug/L

response 9097

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	119.30	132.33
98.00	63.70	69.50
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

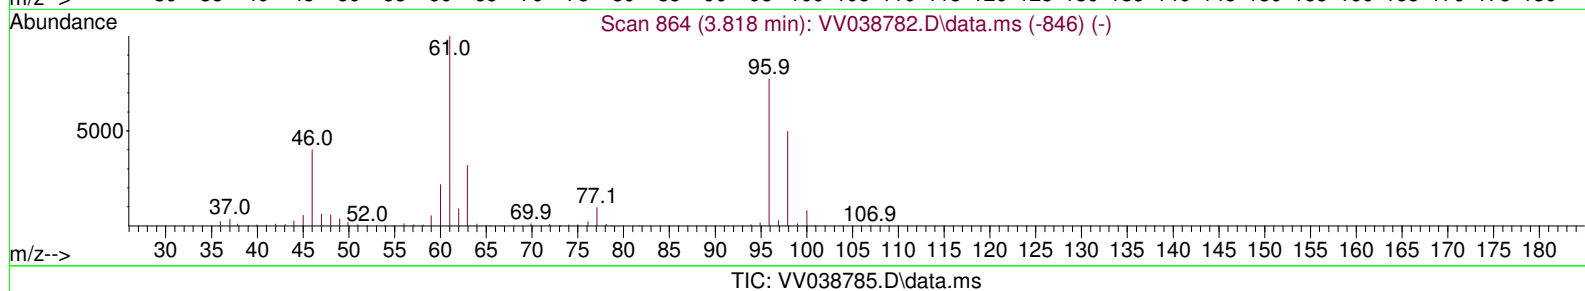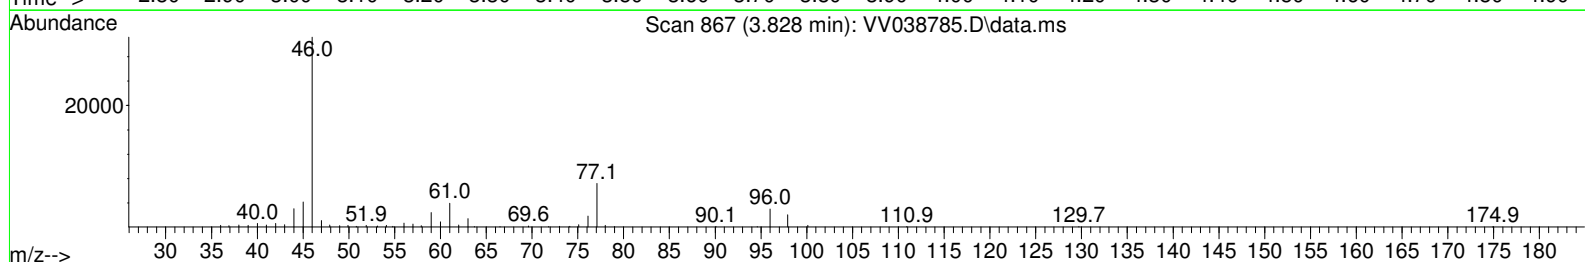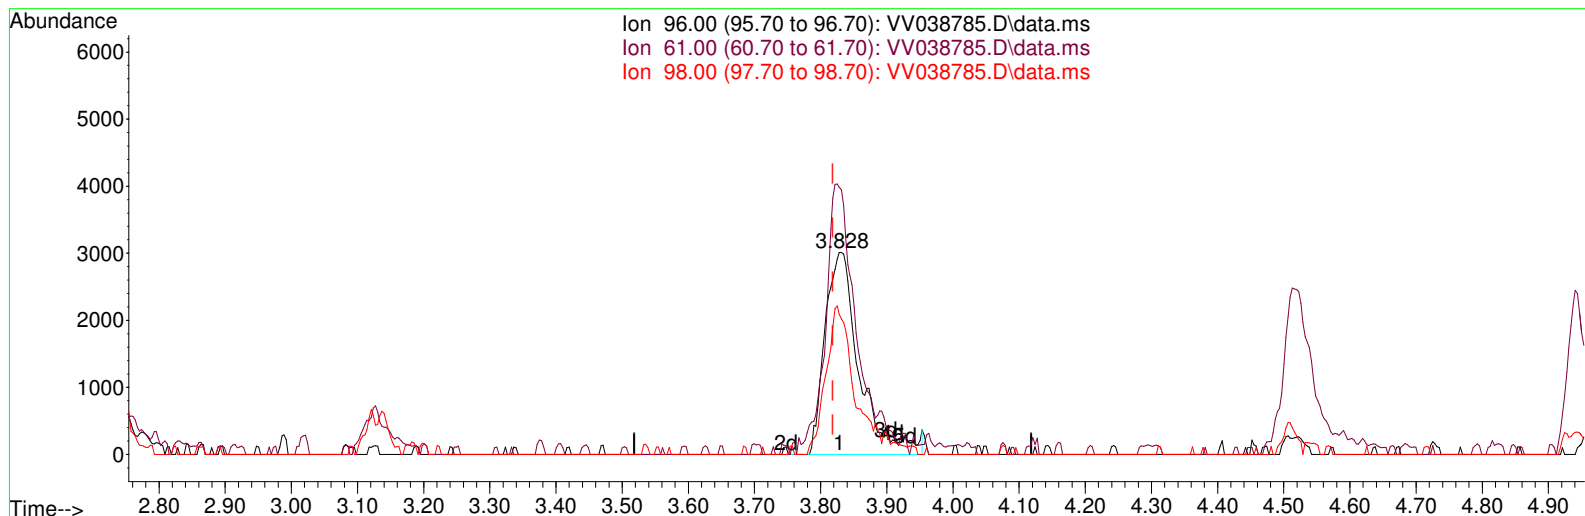

(20) cis-1,2-Dichloroethene (T)




3.828min (+ 0.010) 2.21 ug/L m

response 10862

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	119.30	132.33
98.00	63.70	69.50
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

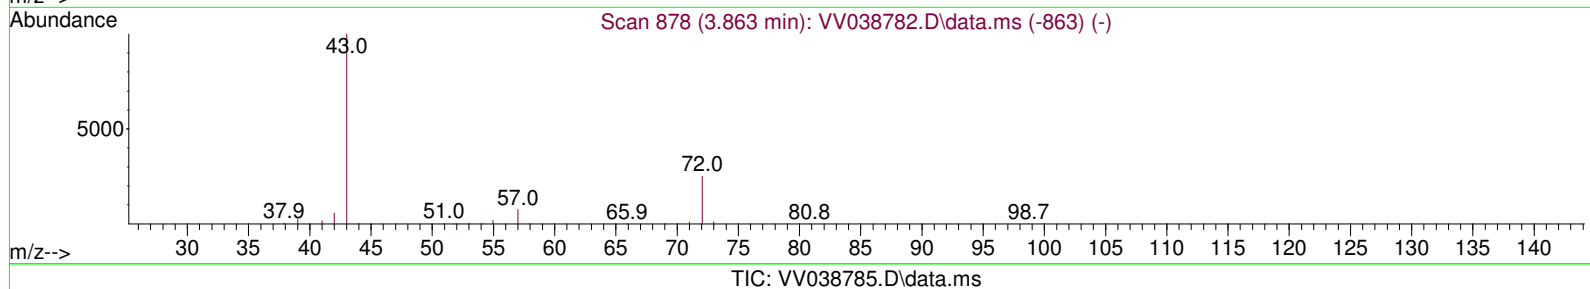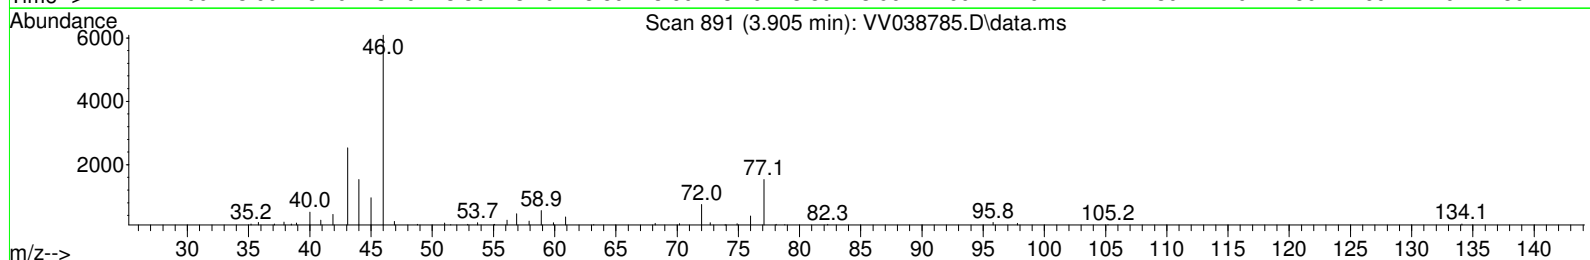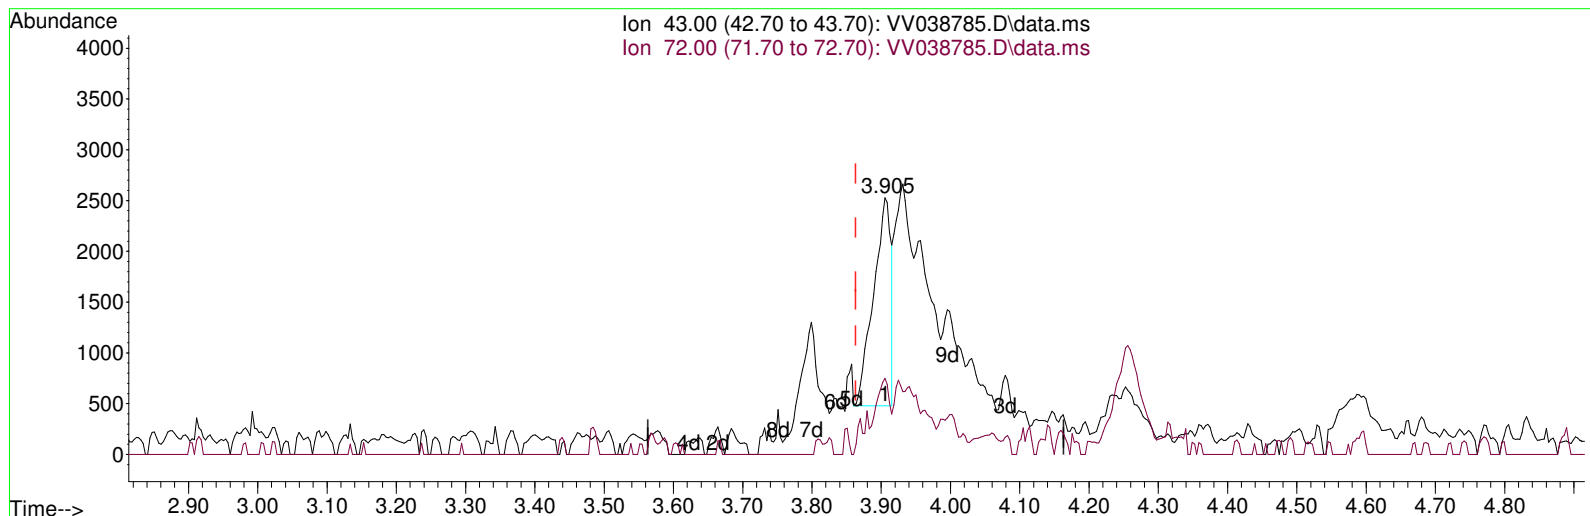

(22) 2-Butanone (T)


3.905min (+ 0.042) 0.98 ug/L

response 3536

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	15.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

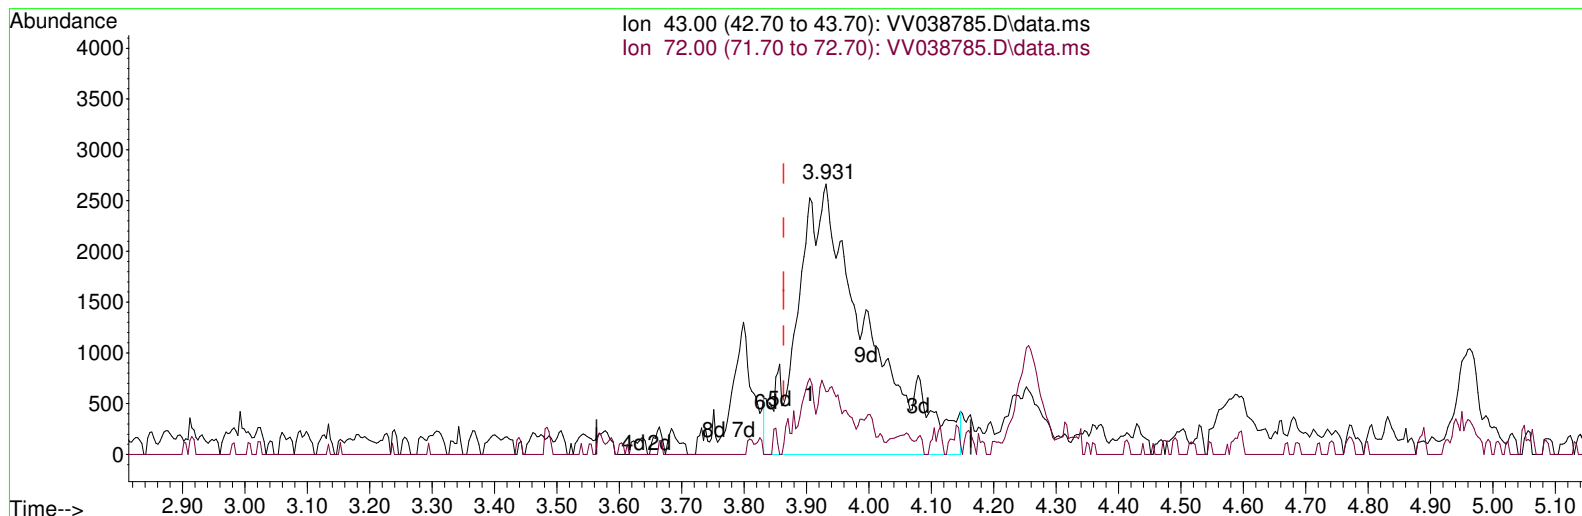

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

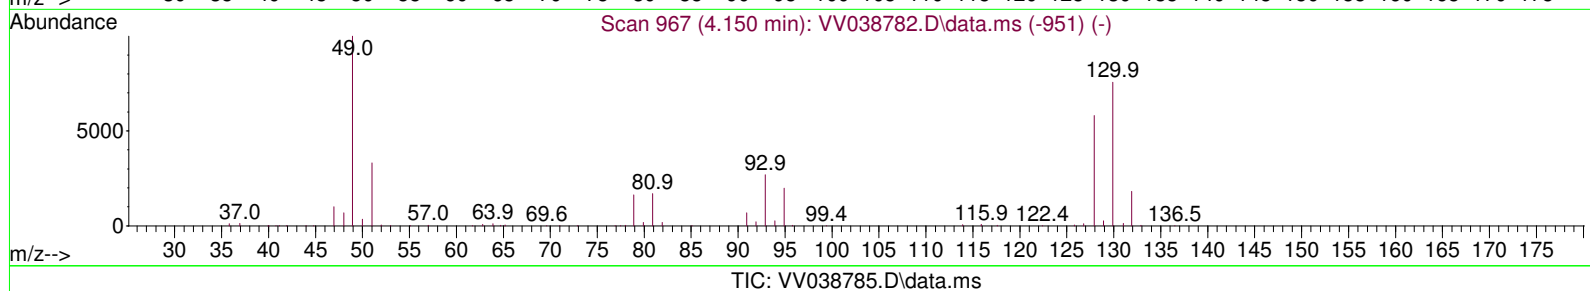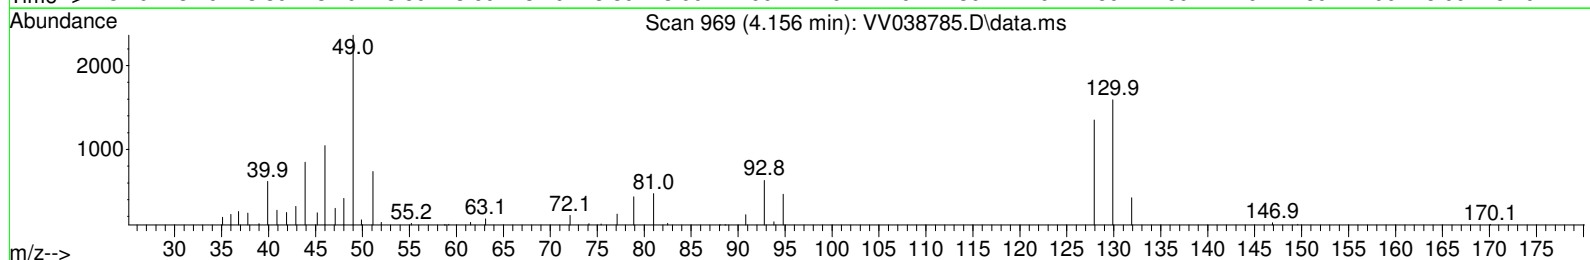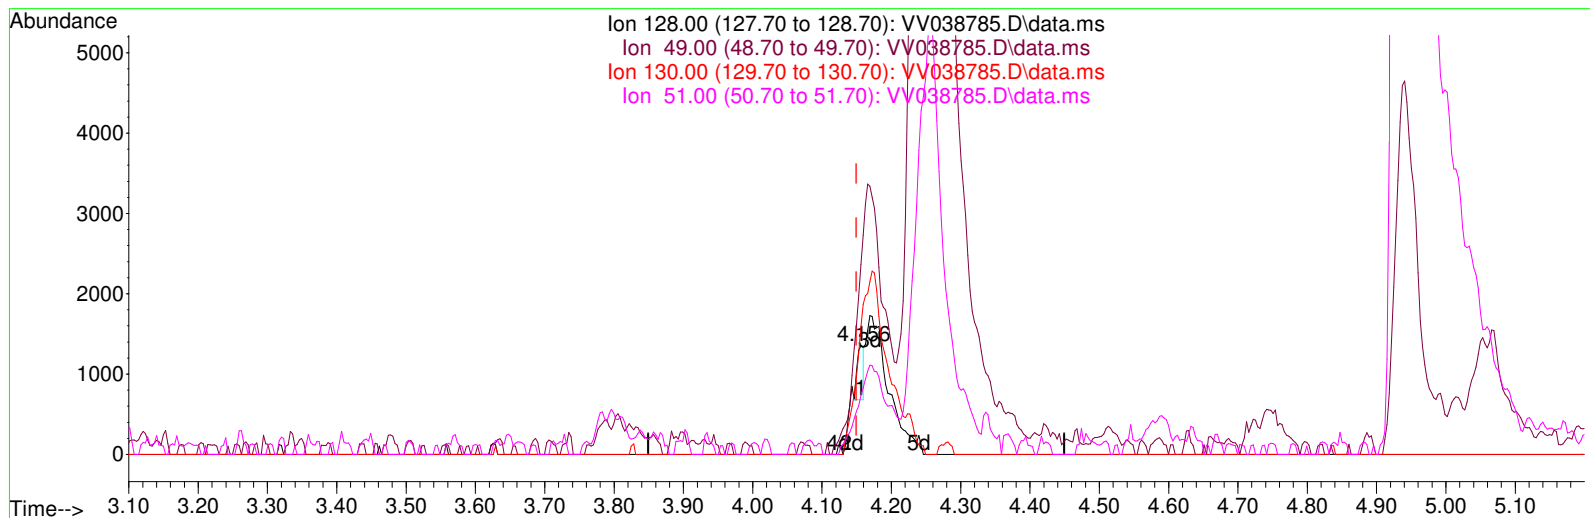

(23) Bromochloromethane (T)




4.156min (+ 0.006) 0.17 ug/L

response 442

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	174.93
130.00	133.20	117.75
51.00	50.30	54.36

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

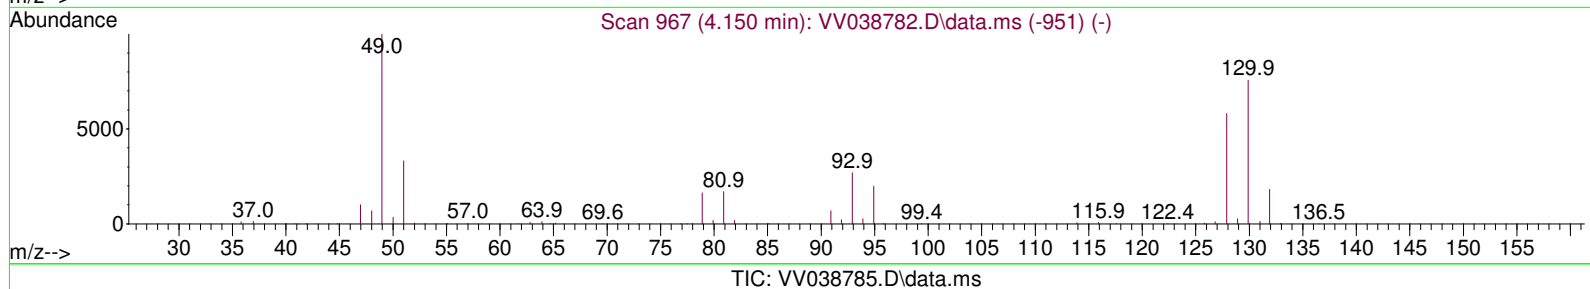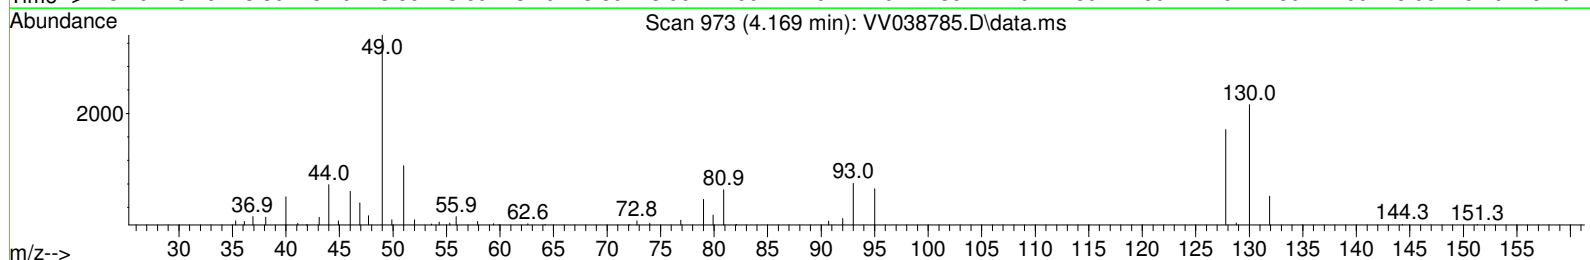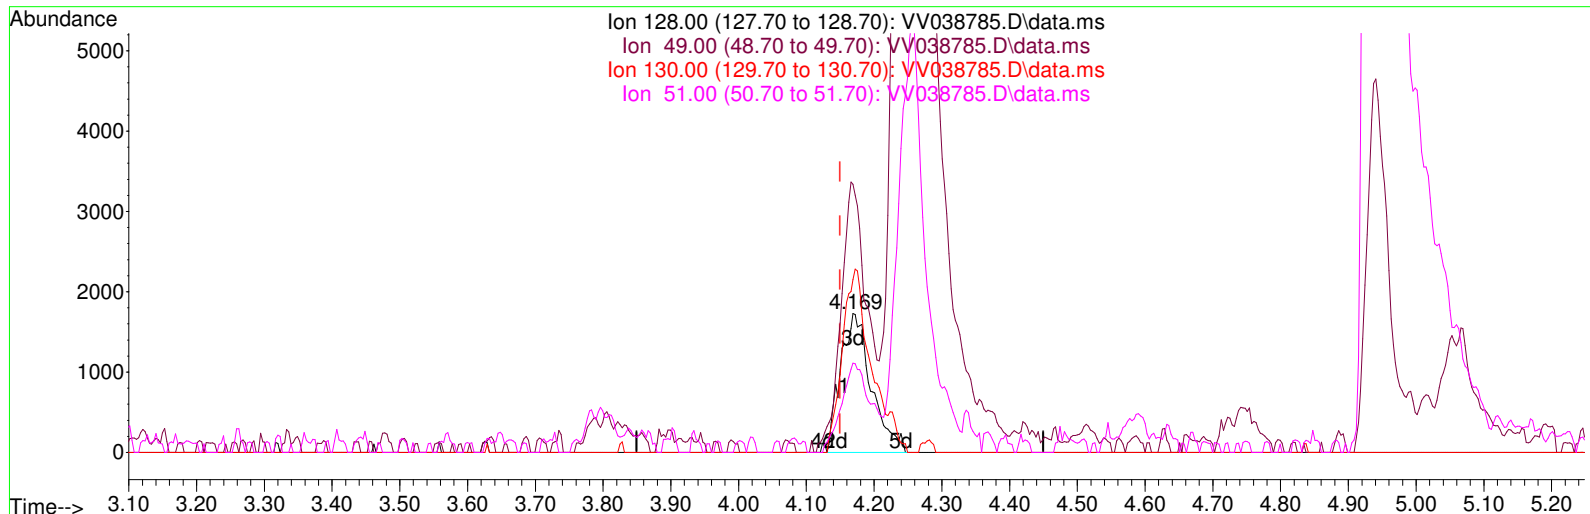

(23) Bromochloromethane (T)

4.169min (+ 0.019) 2.10 ug/L m

response 5494

Ion	Exp%	Act%
-----	------	------

128.00	100.00	100.00
--------	--------	--------




49.00	152.50	193.11
-------	--------	--------

130.00	133.20	124.59
--------	--------	--------

51.00	50.30	64.35#
-------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

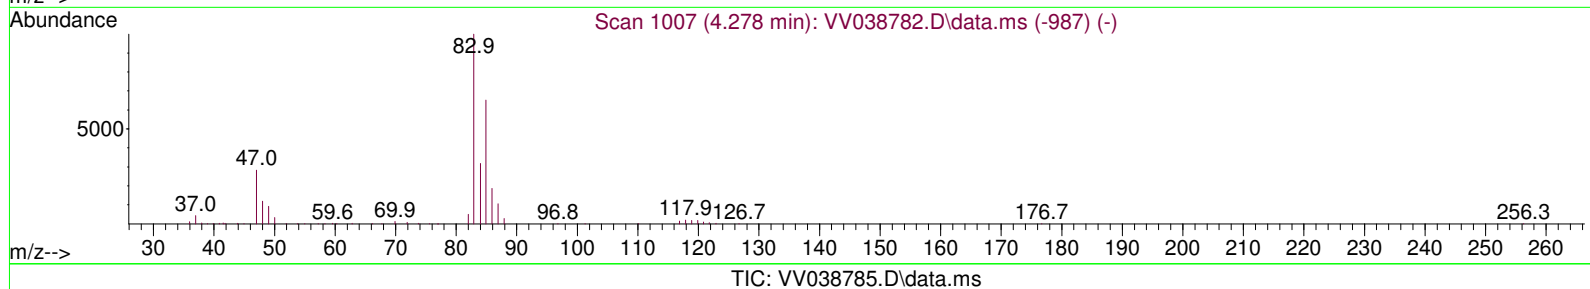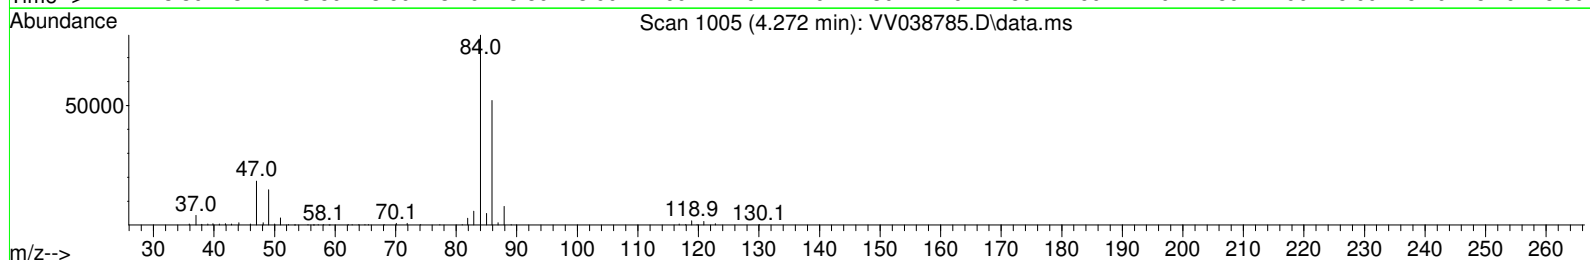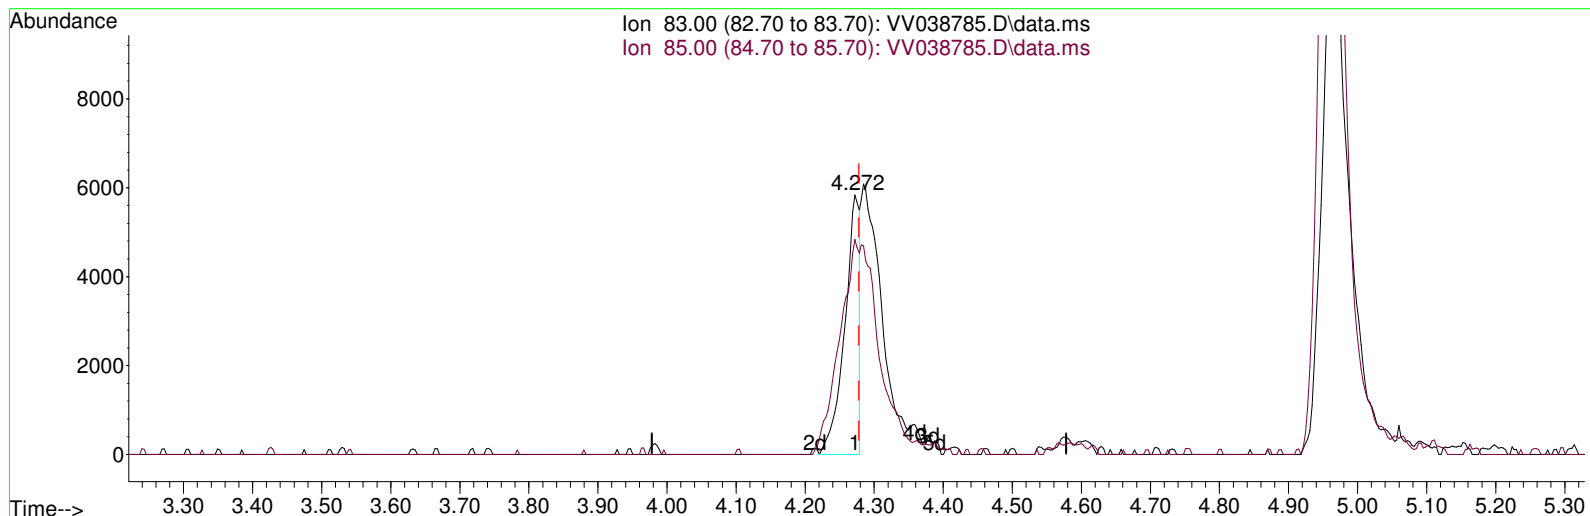

(25) Chloroform (T)




4.272min (-0.006) 0.92 ug/L

response 8616

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.60	82.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

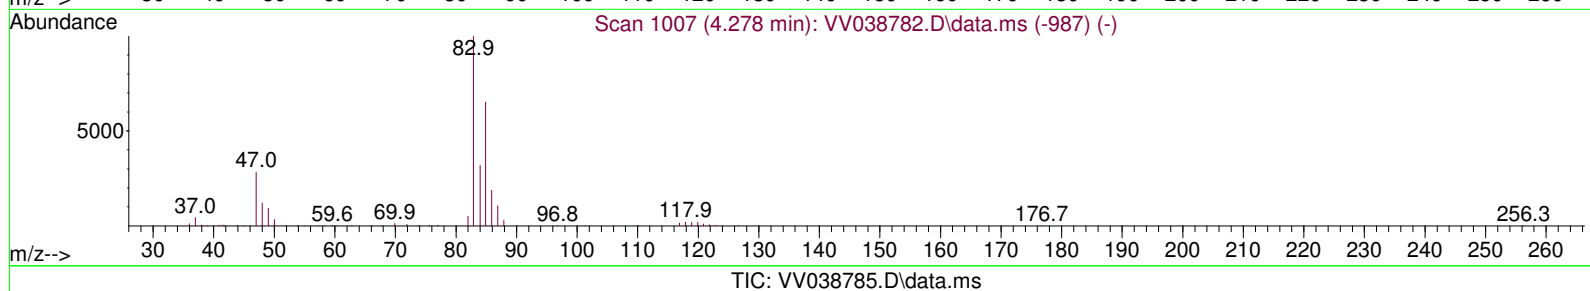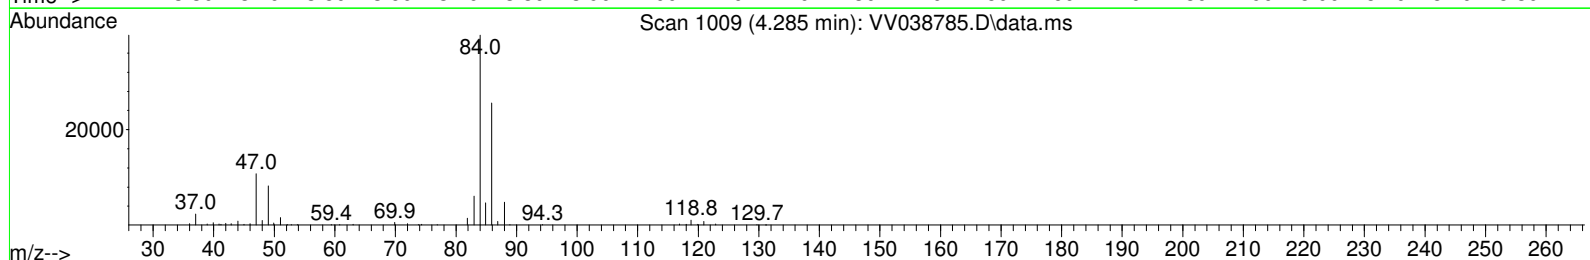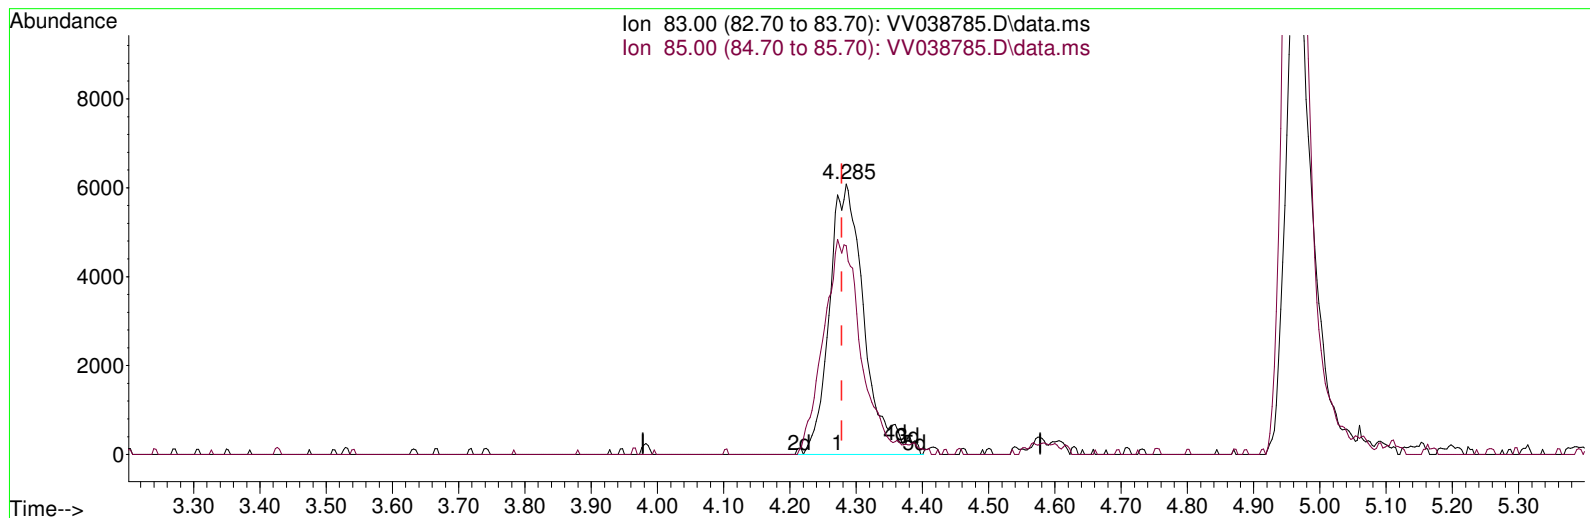

(25) Chloroform (T)




4.285min (+ 0.006) 2.39 ug/L m

response 22380

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.60	77.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

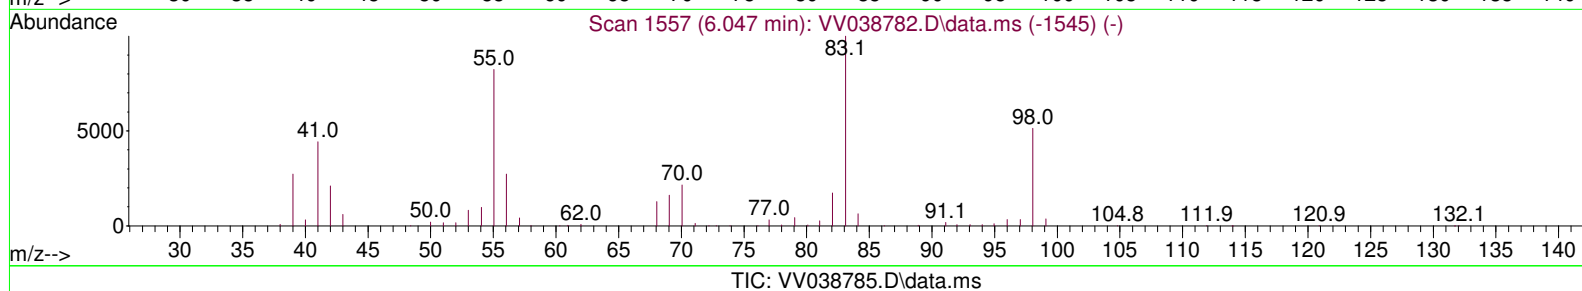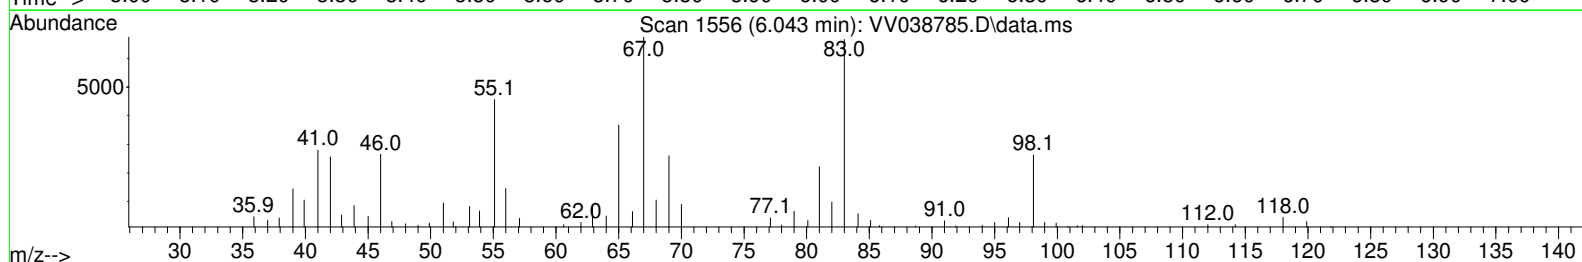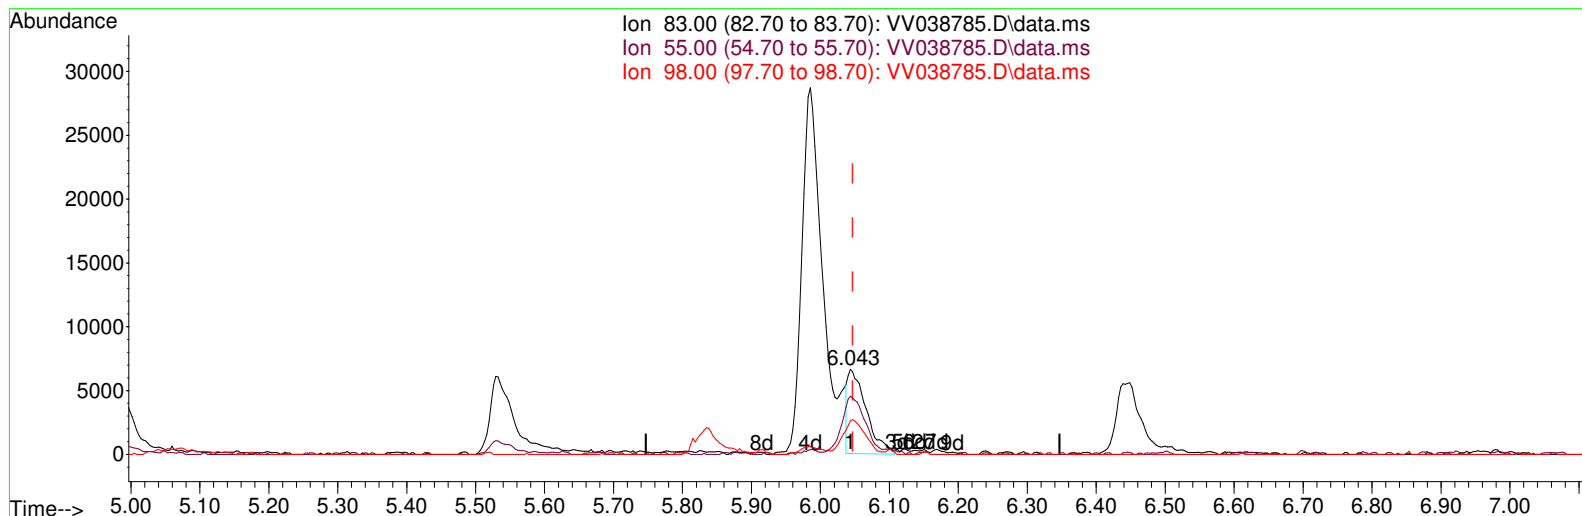

(35) Methylcyclohexane (T)




6.043min (-0.003) 1.52 ug/L

response 12215

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	73.80	84.62
98.00	49.40	50.13
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

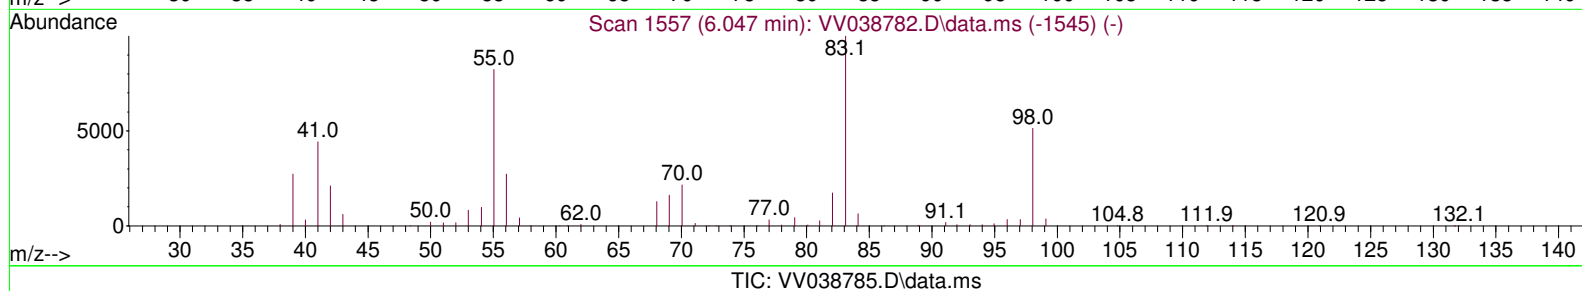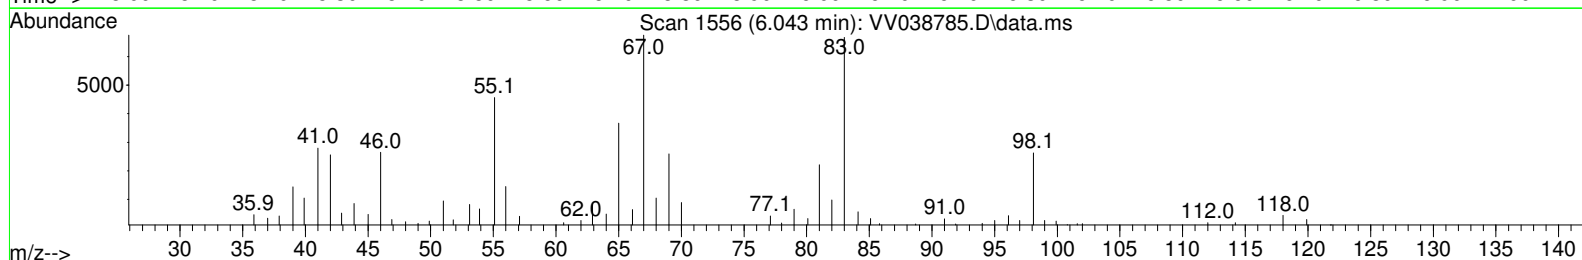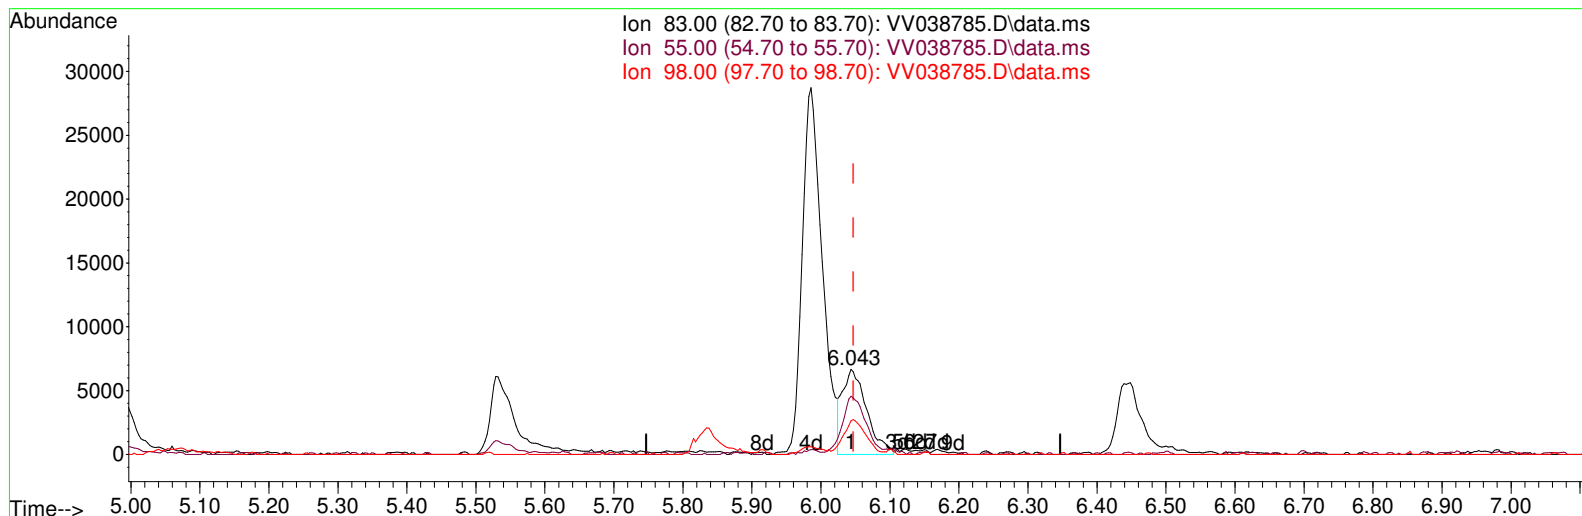

(35) Methylcyclohexane (T)




6.043min (-0.003) 2.02 ug/L m

response 16279

Ion	Exp%	Act%
83.00	100.00	100.00
55.00	73.80	63.49
98.00	49.40	37.61#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

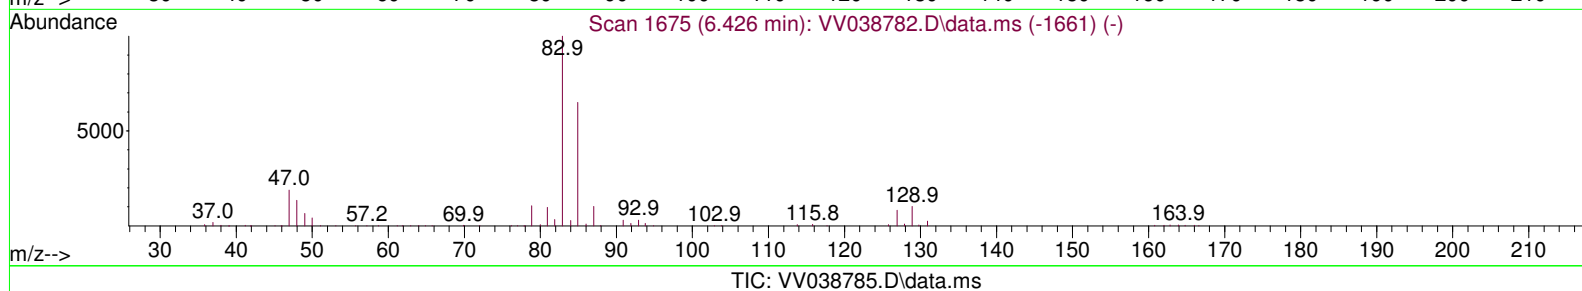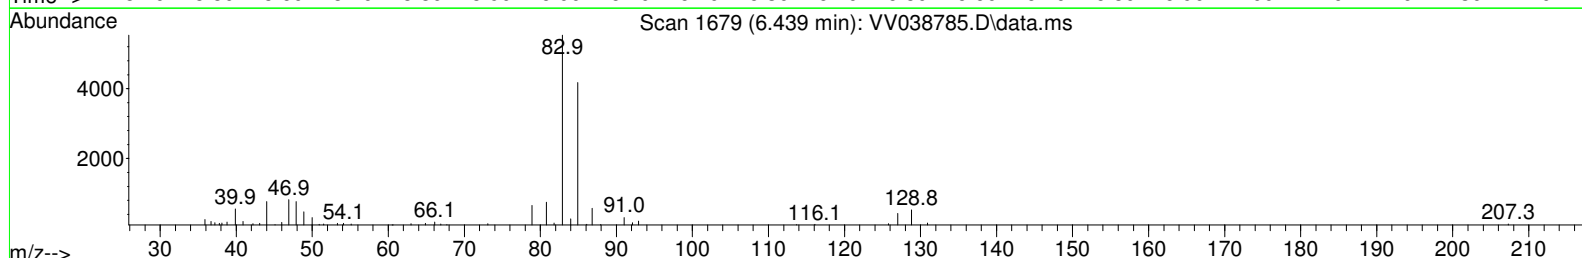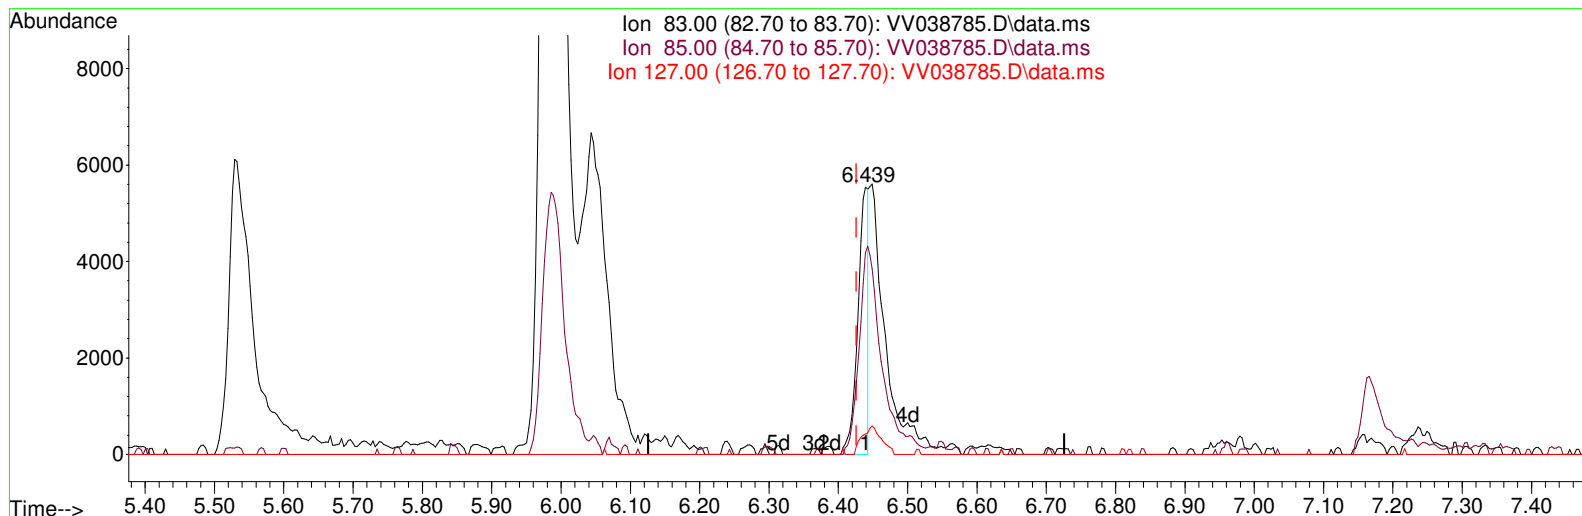

(38) Bromodichloromethane (T)




6.439min (+ 0.013) 0.79 ug/L

response 5691

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.20	75.46
127.00	8.50	7.68
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

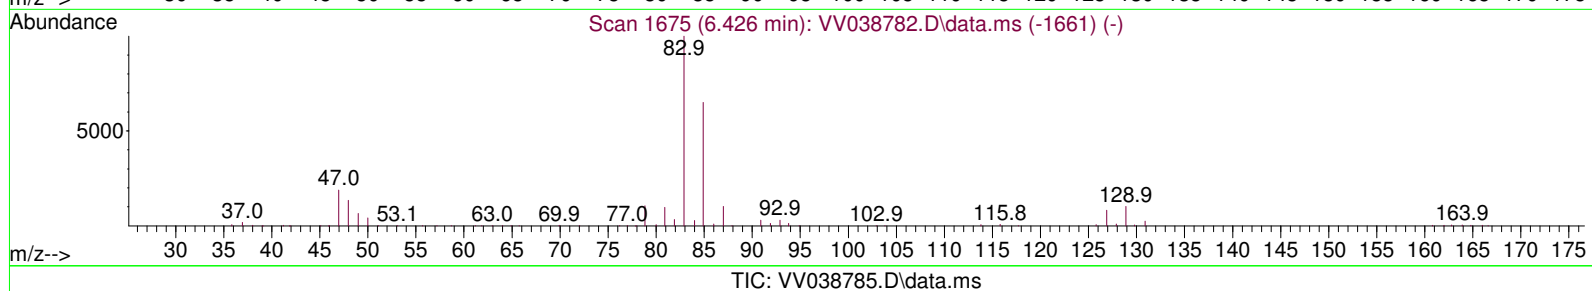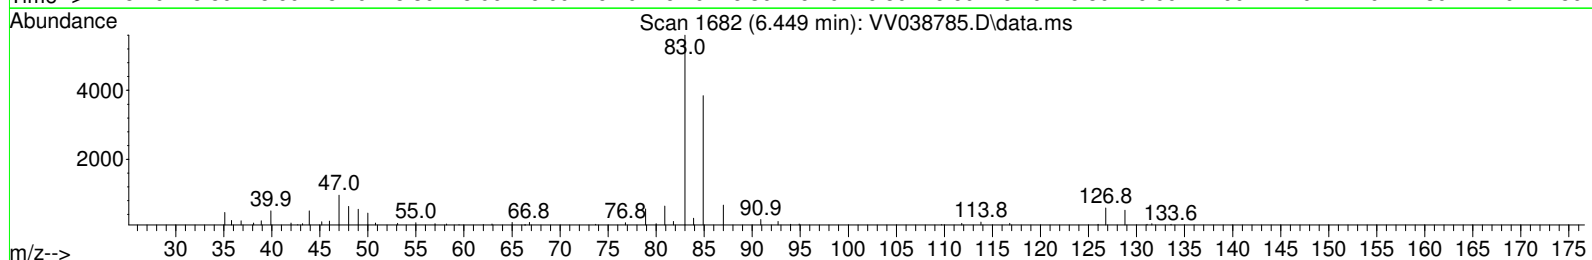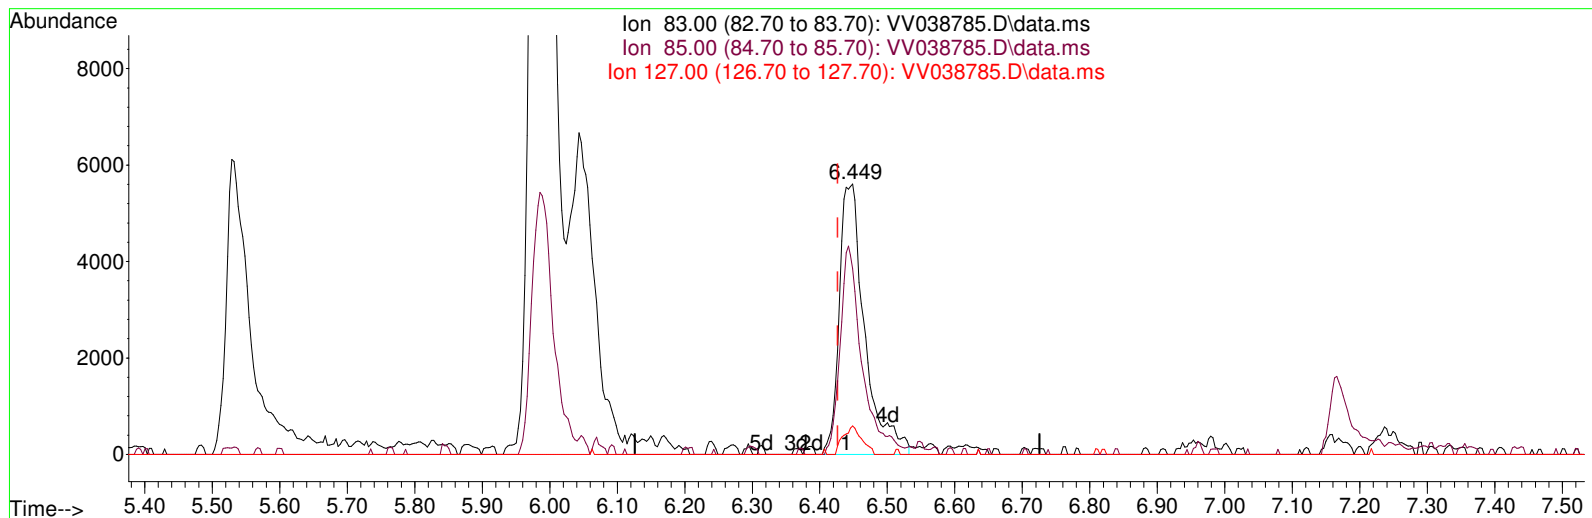

(38) Bromodichloromethane (T)




6.449min (+ 0.022) 2.03 ug/L m

response 14652

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	64.20	68.64
127.00	8.50	10.49#
0.00	0.00	0.00

```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VW061125\
Data File : VW038785.D
Acq On    : 11 Jun 2025  15:54
Operator  : SY/MD
Sample    : Q2117-02
Misc      : 5.0mL/MSVOA_V/WATER
ALS Vial  : 5   Sample Multiplier: 1
```

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

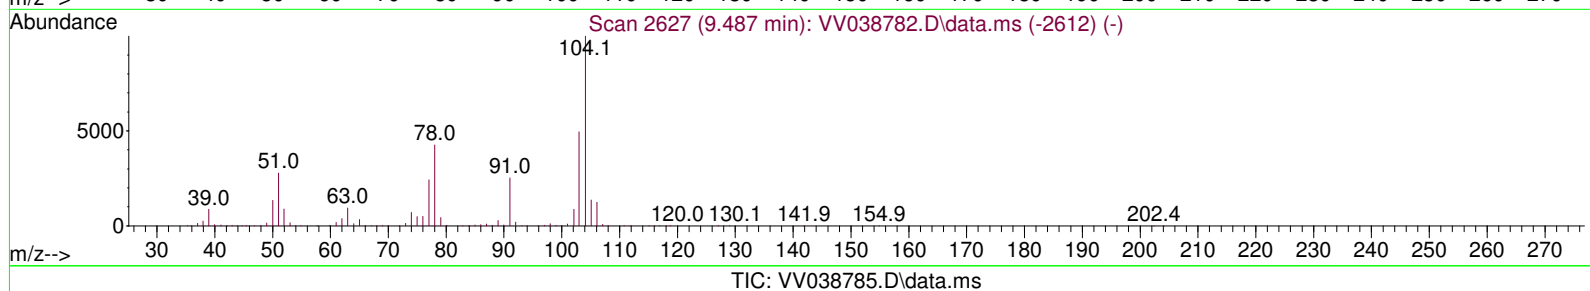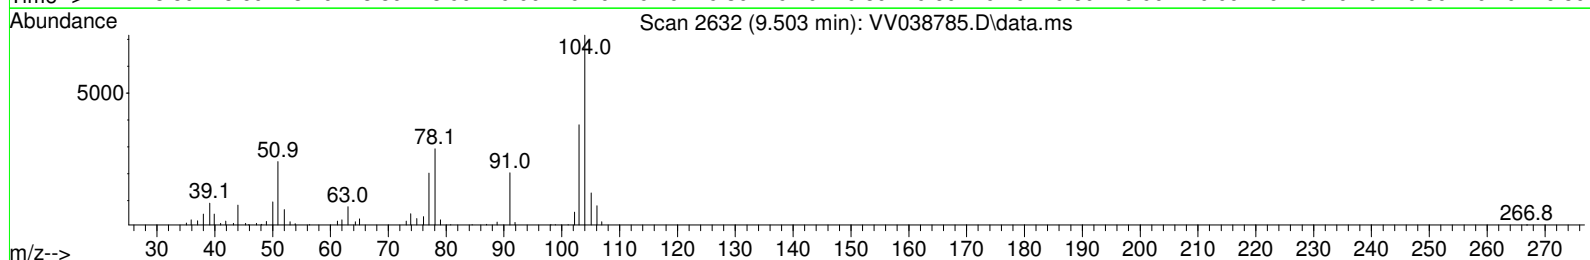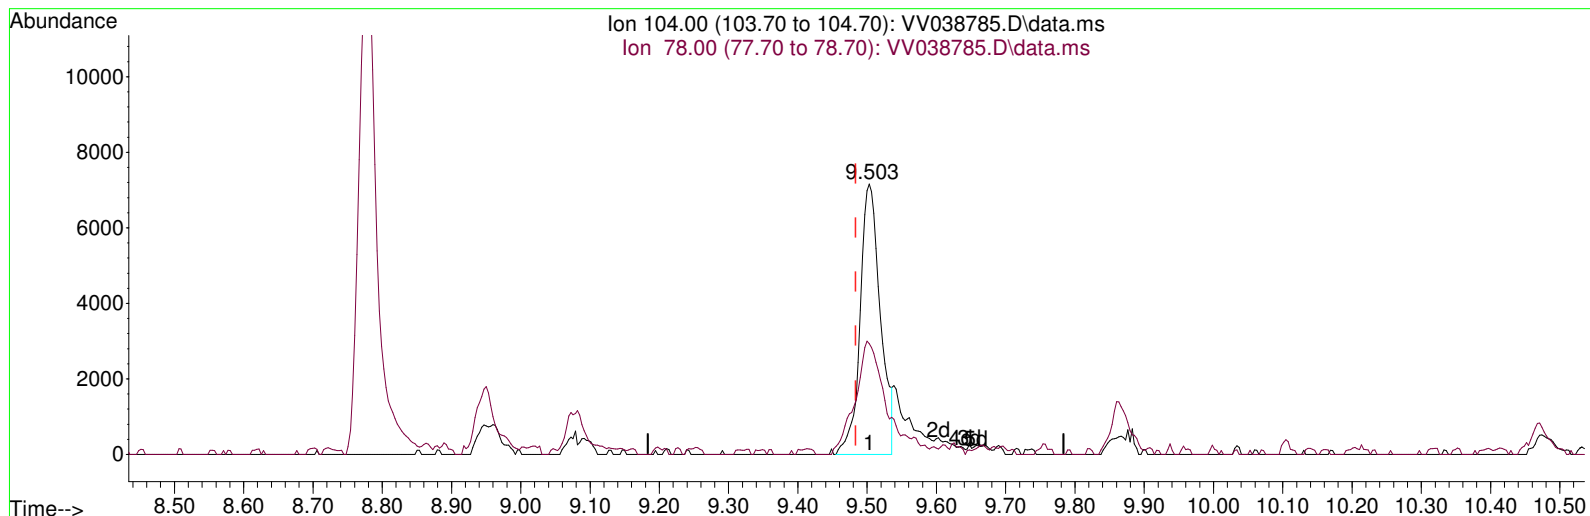

(55) Styrene (T)




9.503min (+ 0.019) 1.09 ug/L

```
response      14522
```

Ion	Exp%	Act%
104.00	100.00	100.00
78.00	42.40	40.90
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038785.D
Acq On : 11 Jun 2025 15:54
Operator : SY/MD
Sample : Q2117-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 11 16:14:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 14:44:52 2025
Response via : Initial Calibration

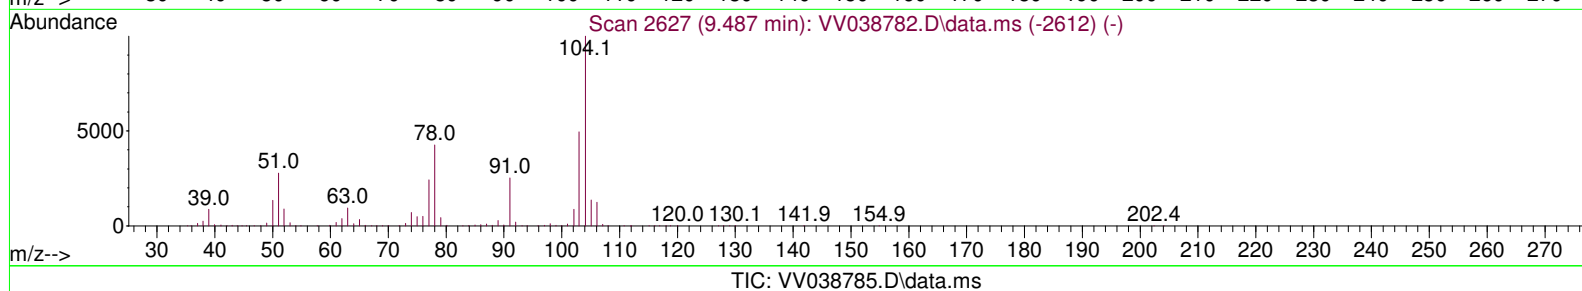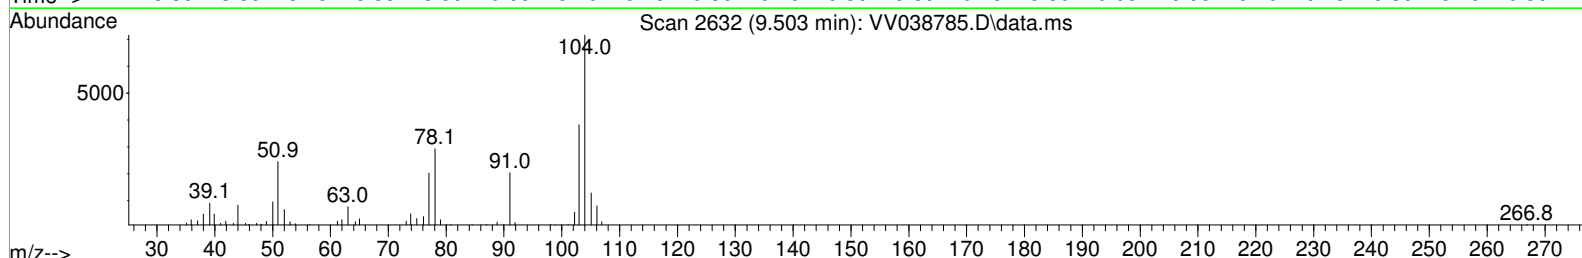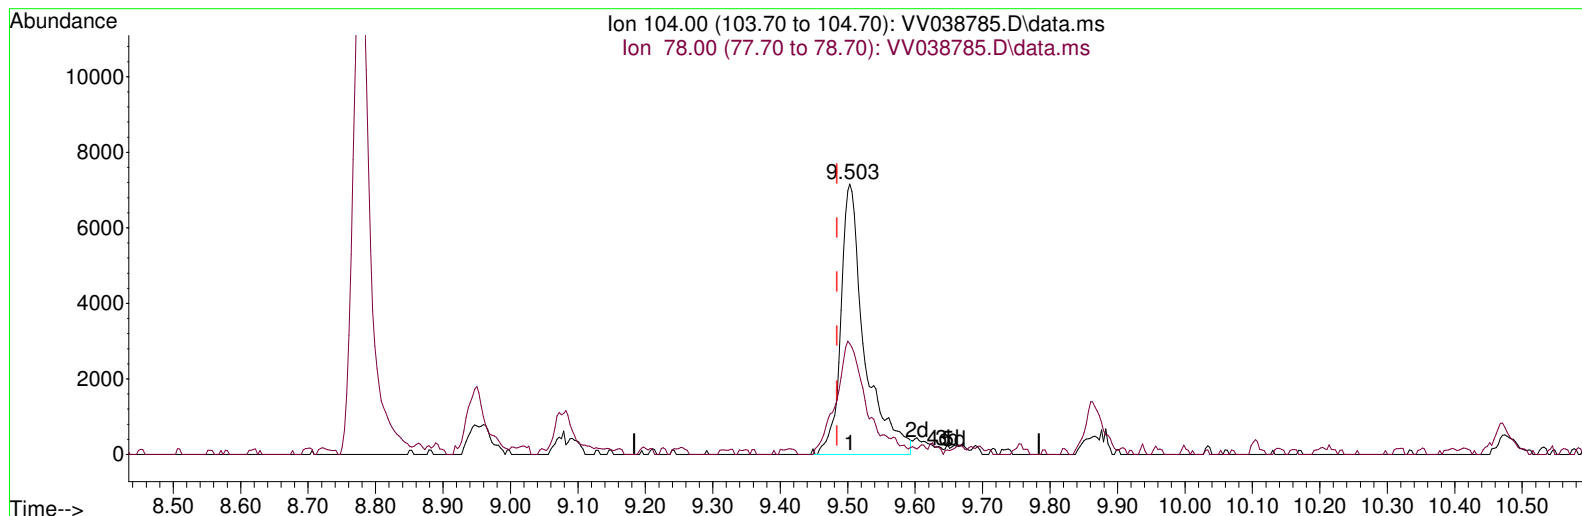

(55) Styrene (T)

9.503min (+ 0.019) 1.32 ug/L m

response 17526

Ion	Exp%	Act%
104.00	100.00	100.00
78.00	42.40	40.90
0.00	0.00	0.00
0.00	0.00	0.00