
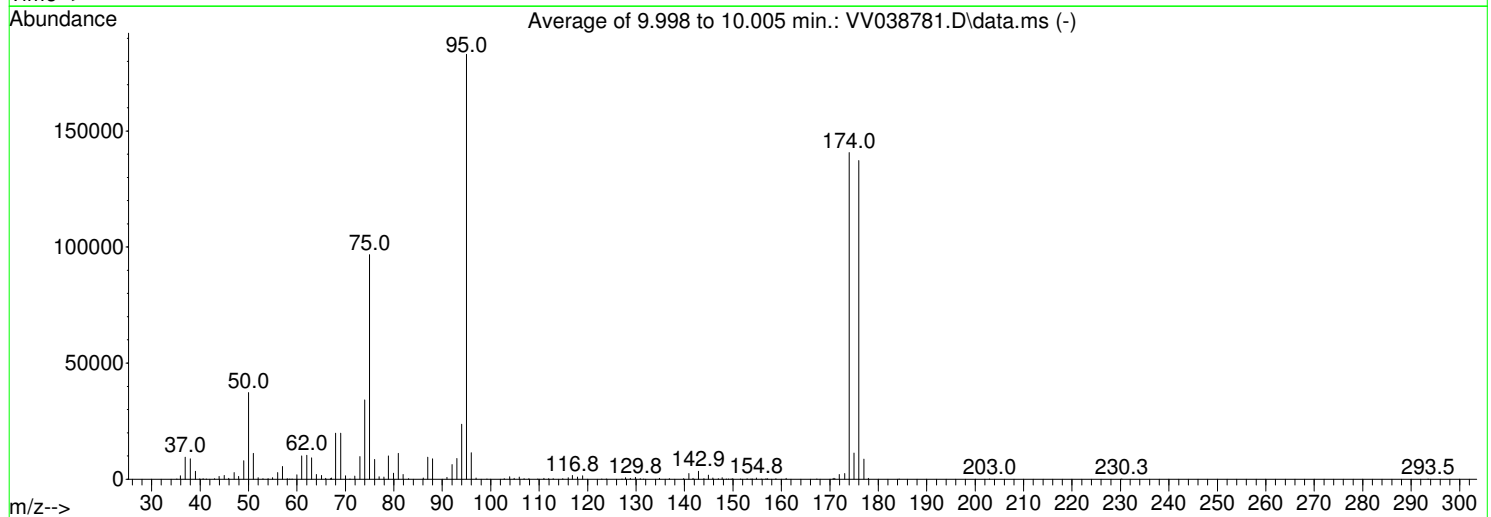


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061125\
Data File : VV038781.D
Acq On : 11 Jun 2025 14:13
Operator : SY/MD
Sample : BFB204
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB204

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Title : VOC Analysis
Last Update : Tue Jun 10 14:44:52 2025

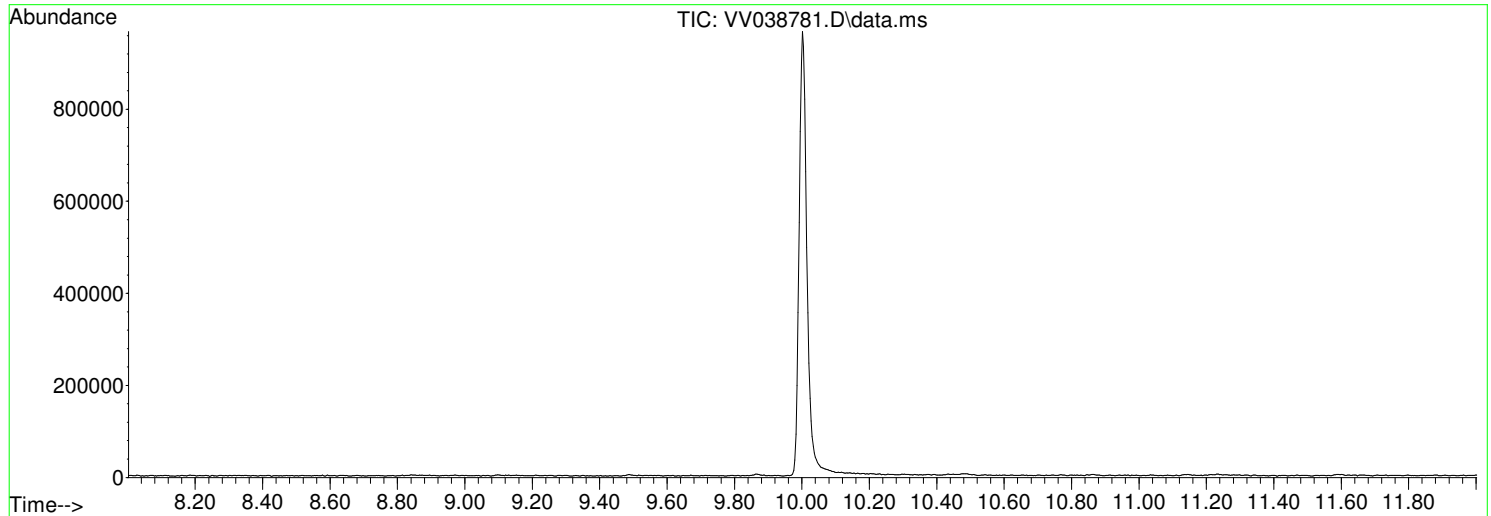

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	37248	PASS
75	95	30	80	52.9	96773	PASS
95	95	100	100	100.0	183104	PASS
96	95	5	9	6.3	11449	PASS
173	174	0.00	2	1.7	2361	PASS
174	95	50	120	76.8	140715	PASS
175	174	5	9	8.0	11192	PASS
176	174	95	105	97.5	137240	PASS
177	176	5	10	6.3	8684	PASS

m/z	Abundance
35.90	144.0
36.90	160.0
37.90	233.0
39.20	118.0
40.00	502.0
41.40	102.0
41.80	106.0
43.90	1040.0
45.00	124.0
50.40	137.0
53.10	191.0
53.90	119.0
55.30	108.0
56.50	105.0
59.70	154.0
63.40	106.0
66.30	113.0
69.60	112.0
77.10	193.0
202.10	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	1617.0
37.00	9724.0
38.00	9051.0
39.10	3294.0
39.90	694.0
41.30	133.0
43.00	170.0
44.00	2291.0
45.00	1772.0
45.90	256.0
47.10	2672.0
47.90	1266.0
49.00	7695.0
50.00	36880.0
51.00	11268.0
52.00	492.0
52.90	414.0
54.00	229.0
55.00	666.0
56.00	2856.0
57.00	5357.0
58.00	231.0
58.50	134.0
60.00	1788.0
61.00	9962.0
62.00	10076.0
63.00	9022.0
64.00	1982.0
65.10	1623.0
65.90	318.0
66.90	513.0
68.00	19064.0
69.00	19632.0
70.00	1489.0
71.00	139.0
72.00	1214.0
73.00	9412.0
74.00	33880.0
75.00	93824.0
76.00	8820.0
77.00	1214.0
78.00	925.0
78.90	9938.0
79.90	2701.0
80.90	11158.0
81.90	1840.0
83.10	162.0
86.10	408.0
87.00	9016.0
88.00	8723.0
91.00	721.0
92.00	6248.0
93.00	8884.0
94.00	23160.0
95.00	176448.0
96.00	11349.0
97.00	480.0
99.20	103.0
102.80	216.0
103.90	1042.0
104.90	324.0
105.90	870.0
106.80	264.0
107.80	330.0
109.70	142.0
111.00	363.0
112.00	186.0
112.90	186.0
114.90	305.0
116.00	662.0
116.90	1676.0
117.90	875.0
118.90	1503.0
123.80	115.0
127.80	663.0
128.80	409.0
129.90	592.0
130.80	191.0
131.60	108.0
134.80	318.0
136.80	187.0
139.80	176.0
140.90	2173.0
141.80	330.0
142.90	3249.0
144.10	271.0
144.90	1638.0
145.80	424.0
147.00	140.0
147.80	598.0
149.60	188.0
150.00	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

151.60	120.0
152.80	129.0
154.00	127.0
154.80	426.0
155.80	145.0
156.80	160.0
157.20	260.0
158.90	253.0
161.00	316.0
170.70	476.0
172.00	1671.0
173.00	2211.0
174.00	132928.0
175.00	10831.0
176.00	128328.0
177.00	8116.0
177.90	293.0
184.30	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	1646.0
37.00	9924.0
38.00	9258.0
39.00	3664.0
39.90	640.0
40.60	386.0
41.30	161.0
43.00	154.0
44.00	2232.0
45.00	1772.0
45.90	293.0
47.00	2925.0
47.90	1195.0
49.00	8132.0
50.00	38408.0
51.00	11509.0
52.00	597.0
52.90	433.0
54.00	266.0
54.90	616.0
56.00	2964.0
57.00	5769.0
58.00	266.0
59.00	126.0
60.00	1851.0
61.00	10208.0
62.00	10479.0
63.00	9580.0
64.00	2013.0
65.00	1672.0
65.90	326.0
67.10	669.0
68.00	20760.0
69.00	20584.0
70.00	1514.0
70.90	138.0
71.90	1267.0
73.00	10128.0
74.00	35512.0
75.00	100704.0
76.00	8884.0
76.90	1313.0
77.90	979.0
78.90	10334.0
79.90	2697.0
80.90	11415.0
81.90	2141.0
83.10	219.0
86.10	447.0
87.00	9740.0
88.00	9089.0
91.00	742.0
92.00	6612.0
93.00	9232.0
94.00	24408.0
95.00	189440.0
96.00	11802.0
97.00	452.0
99.20	101.0
102.80	207.0
103.90	1045.0
104.90	331.0
105.90	957.0
106.90	270.0
107.90	290.0
111.00	399.0
111.90	215.0
112.90	216.0
114.90	283.0
116.00	654.0
116.90	1605.0
117.90	962.0
118.90	1514.0
122.90	130.0
123.90	121.0
127.10	145.0
127.90	704.0
128.80	433.0
129.80	714.0
130.80	276.0
131.60	120.0
134.80	387.0
136.80	316.0
139.80	166.0
140.90	2451.0
141.80	310.0
142.90	3554.0
144.00	251.0
144.90	1786.0
145.80	446.0
146.90	164.0
147.80	569.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

149.10	110.0
150.00	240.0
151.60	115.0
152.90	130.0
153.70	147.0
154.80	425.0
155.80	139.0
156.80	164.0
157.20	239.0
158.80	294.0
161.00	421.0
170.70	446.0
171.10	447.0
172.00	1992.0
173.00	2446.0
174.00	145408.0
175.00	11724.0
176.00	141696.0
177.00	9016.0
178.00	304.0
230.30	123.0
293.50	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.20	159.0
36.00	1584.0
37.00	9002.0
38.00	8624.0
39.00	3704.0
39.90	568.0
40.70	419.0
41.30	135.0
42.00	125.0
43.00	171.0
44.00	1956.0
45.00	1636.0
45.90	374.0
47.00	2709.0
48.00	1079.0
49.00	7798.0
50.00	36456.0
51.00	10567.0
52.00	609.0
53.00	394.0
54.10	301.0
54.90	540.0
56.00	2846.0
57.00	5434.0
58.00	298.0
59.00	126.0
60.00	1832.0
61.00	9878.0
62.00	10117.0
63.00	9065.0
64.00	1947.0
65.00	1671.0
66.00	291.0
67.10	759.0
68.00	19768.0
69.00	19336.0
70.00	1417.0
70.90	143.0
71.90	1274.0
73.00	9496.0
74.00	33016.0
75.00	95792.0
76.00	7941.0
76.90	1306.0
77.90	915.0
78.90	9624.0
79.90	2414.0
80.90	10629.0
81.90	2135.0
83.00	241.0
86.10	462.0
87.00	9546.0
88.00	8338.0
90.90	730.0
92.00	6018.0
93.00	8709.0
94.00	23592.0
95.00	183424.0
96.00	11195.0
97.00	359.0
102.80	188.0
103.90	878.0
104.80	317.0
105.90	930.0
106.90	239.0
108.00	217.0
110.90	380.0
111.90	251.0
112.90	191.0
114.90	226.0
116.00	545.0
116.80	1458.0
117.90	920.0
119.00	1524.0
122.90	153.0
123.90	128.0
127.10	166.0
127.90	652.0
128.80	372.0
129.80	818.0
130.90	311.0
134.90	439.0
136.90	352.0
139.80	163.0
140.90	2432.0
141.70	280.0
142.90	3377.0
143.90	286.0
144.90	1677.0
145.90	546.0
146.90	140.0
147.80	545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

148.60	135.0
149.10	137.0
149.80	215.0
151.60	106.0
153.00	176.0
153.70	132.0
154.90	438.0
155.80	126.0
156.80	211.0
157.10	169.0
158.80	297.0
161.00	346.0
167.30	108.0
170.90	517.0
171.90	2294.0
173.10	2427.0
174.00	143808.0
175.00	11021.0
176.00	141696.0
177.00	8921.0
178.00	280.0
203.00	101.0
230.30	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204